

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011620\
 Data File : P0065551.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Jan 2020 14:28
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 14:42:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.154	3.433	423358	458308	23.185	20.835
2)	SA Decachlor...	9.657	8.336	679542	897340	20.056	21.638
Target Compounds							
38)	L8 AR-1262-3	0.000	7.340	0	19508	N.D.	11.591 #
39)	L8 AR-1262-4	0.000	7.340	0	19508	N.D.	5.673 #
40)	L8 AR-1262-5	0.000	7.831	0	50652	N.D.	29.704 #
41)	L9 AR-1268-1	0.000	7.340	0	19508	N.D.	3.673 #
42)	L9 AR-1268-2	0.000	7.340	0	19508	N.D.	3.841 #
43)	L9 AR-1268-3	0.000	7.547	0	24671	N.D.	5.808 #
44)	L9 AR-1268-4	0.000	7.831	0	50652	N.D.	25.592 #
45)	L9 AR-1268-5	0.000	8.105	0	21506	N.D.	1.496 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011620\
Data File : P0065551.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jan 2020 14:28
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 14:42:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

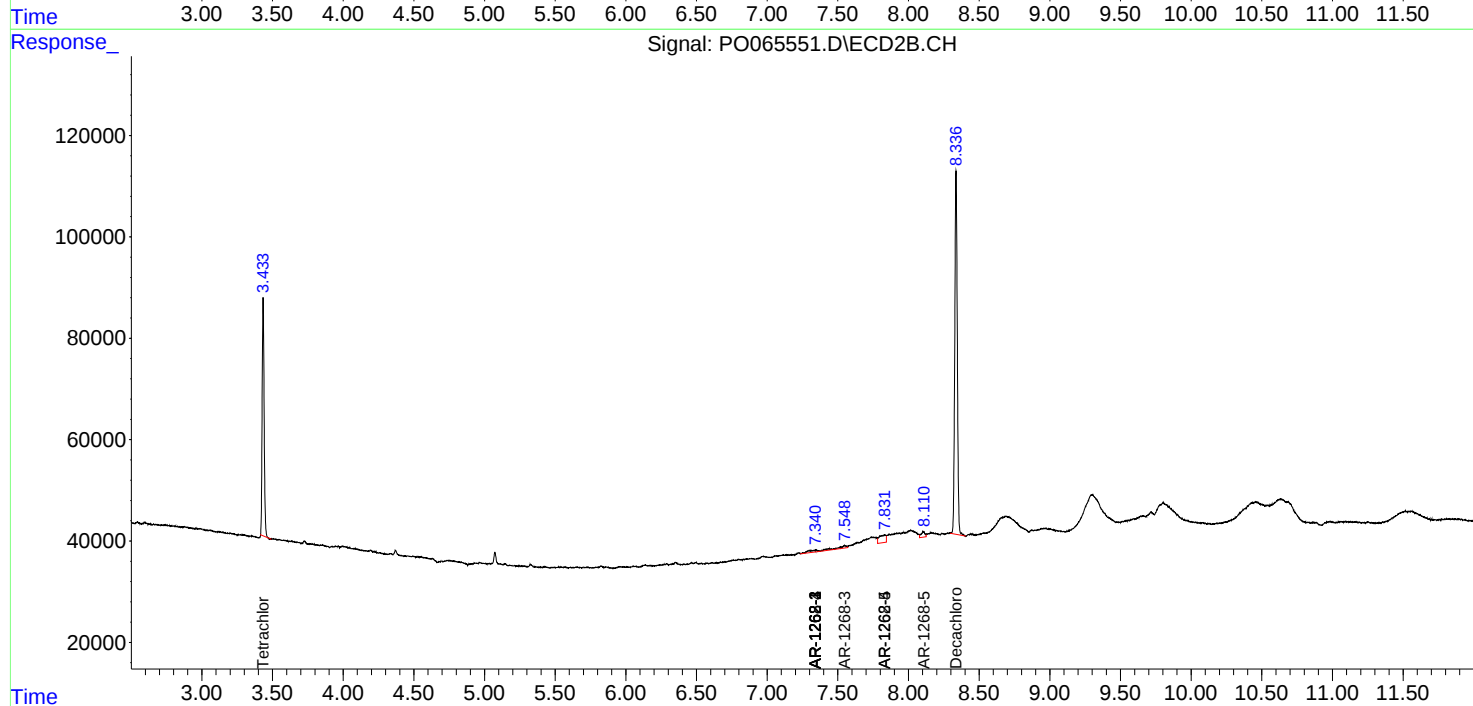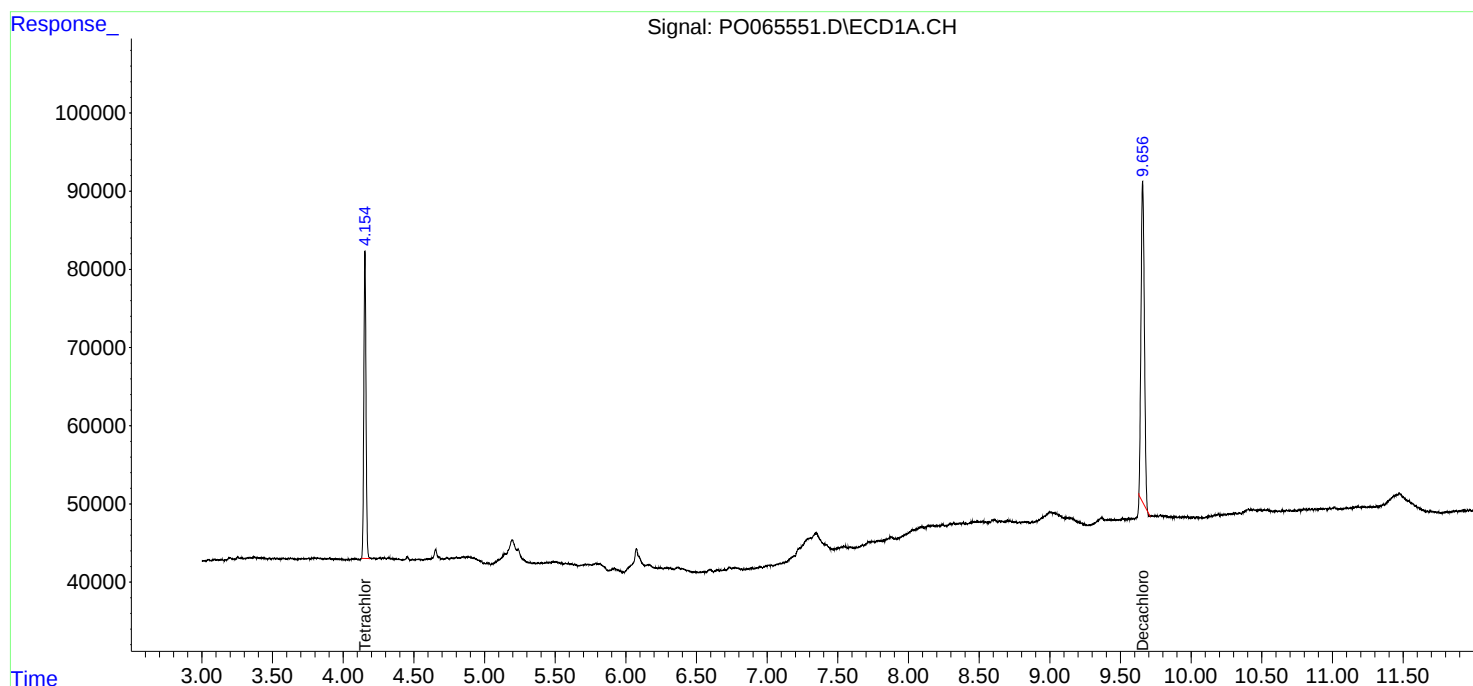


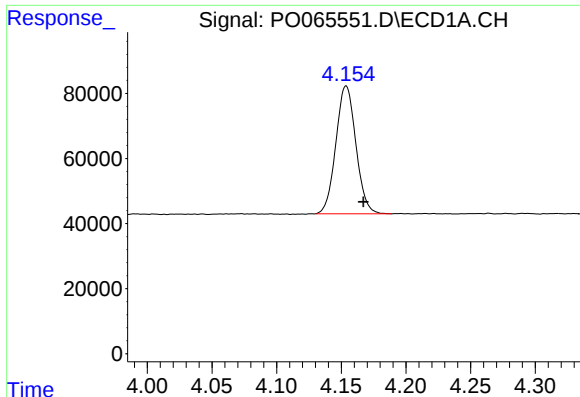

#1 Tetrachloro-m-xylene


R.T.: 4.154 min
Delta R.T.: -0.013 min
Response: 423358
Conc: 23.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

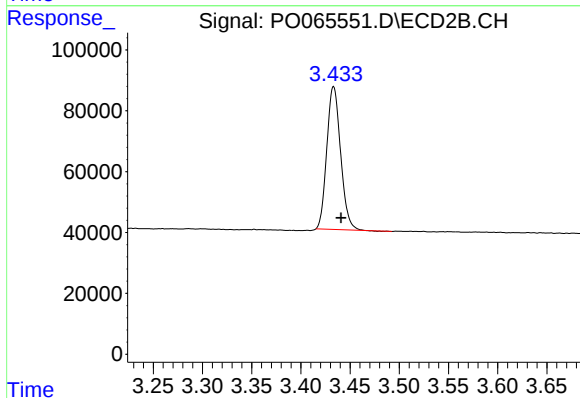


#1 Tetrachloro-m-xylene

R.T.: 3.433 min
Delta R.T.: -0.008 min
Response: 458308
Conc: 20.83 ng/ml

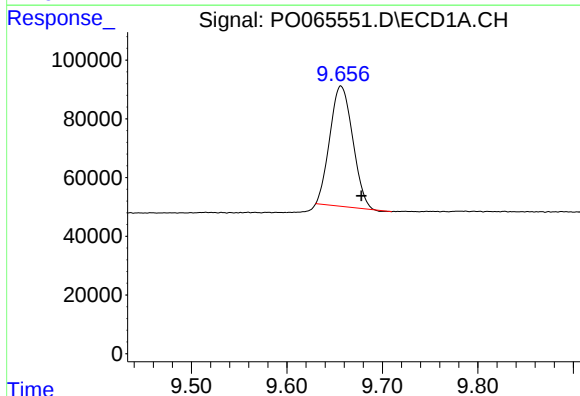


#2 Decachlorobiphenyl

R.T.: 9.657 min
Delta R.T.: -0.022 min
Response: 679542
Conc: 20.06 ng/ml

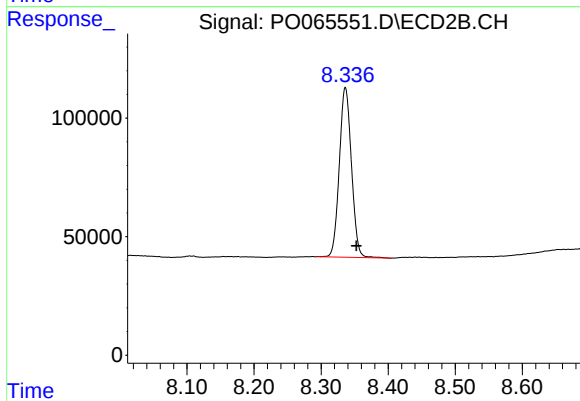

#2 Decachlorobiphenyl


R.T.: 8.336 min
Delta R.T.: -0.016 min
Response: 897340
Conc: 21.64 ng/ml

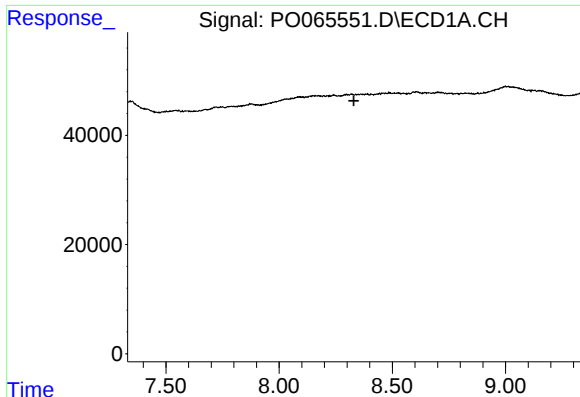

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.330 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

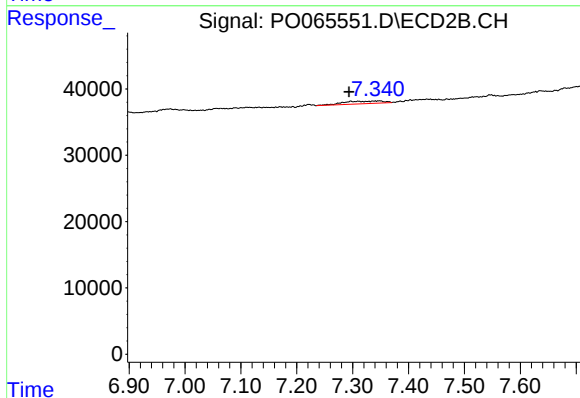


#38 AR-1262-3

R.T.: 7.340 min
Delta R.T.: 0.047 min
Response: 19508
Conc: 11.59 ng/ml

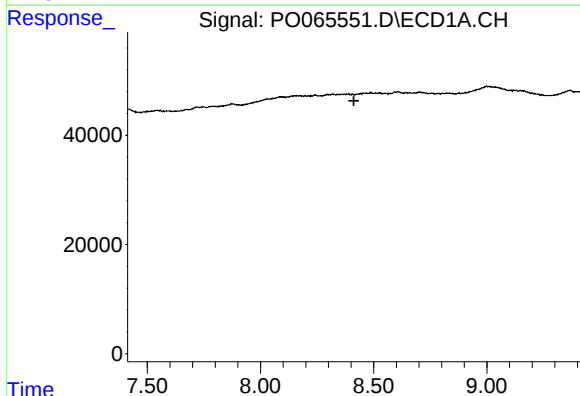


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 8.413 min
Response: 0
Conc: N.D.

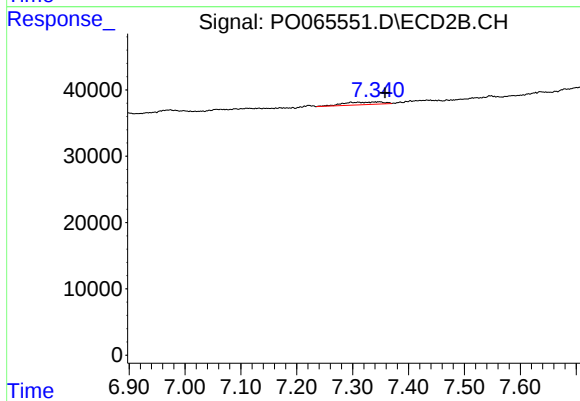

#39 AR-1262-4


R.T.: 7.340 min
Delta R.T.: -0.018 min
Response: 19508
Conc: 5.67 ng/ml

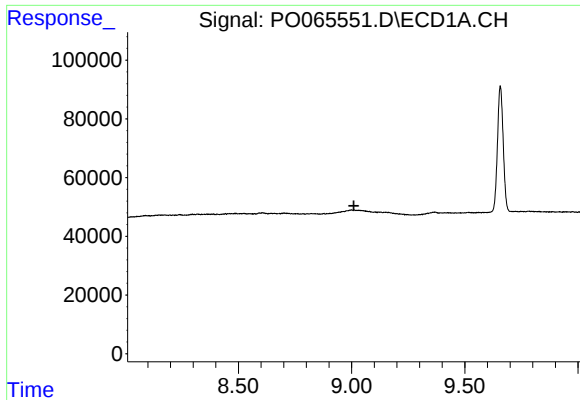

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 9.010 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

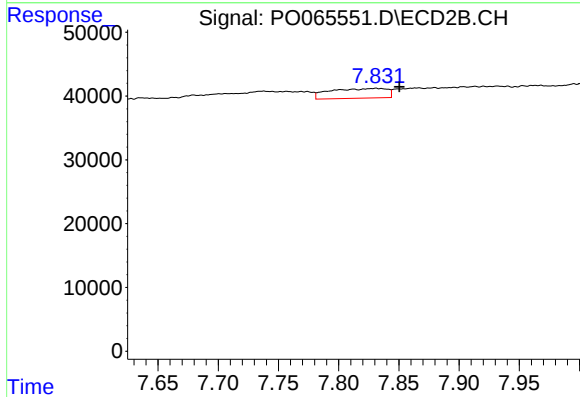


#40 AR-1262-5

R.T.: 7.831 min
Delta R.T.: -0.019 min
Response: 50652
Conc: 29.70 ng/ml

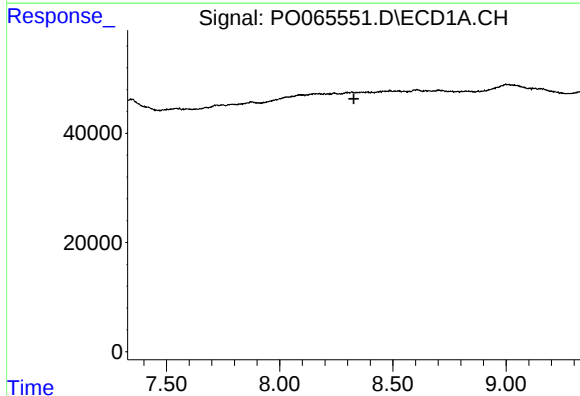


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.327 min
Response: 0
Conc: N.D.

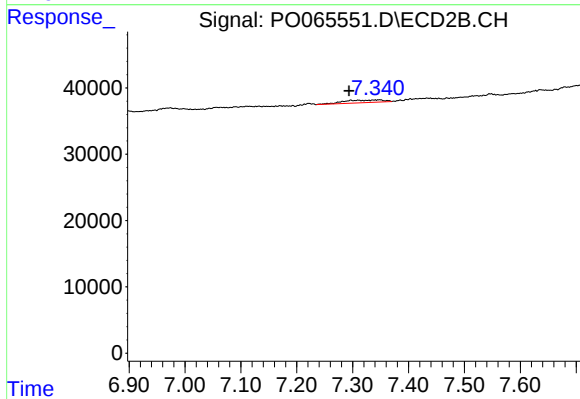

#41 AR-1268-1


R.T.: 7.340 min
Delta R.T.: 0.047 min
Response: 19508
Conc: 3.67 ng/ml

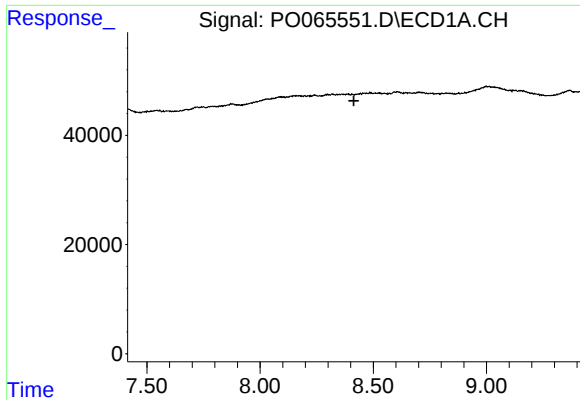

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 8.414 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

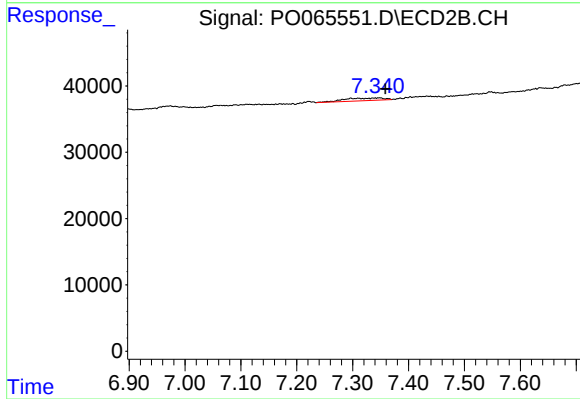


#42 AR-1268-2

R.T.: 7.340 min
Delta R.T.: -0.018 min
Response: 19508
Conc: 3.84 ng/ml

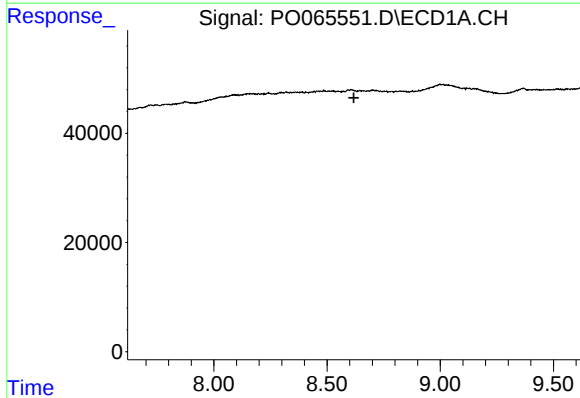


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 8.619 min
Response: 0
Conc: N.D.

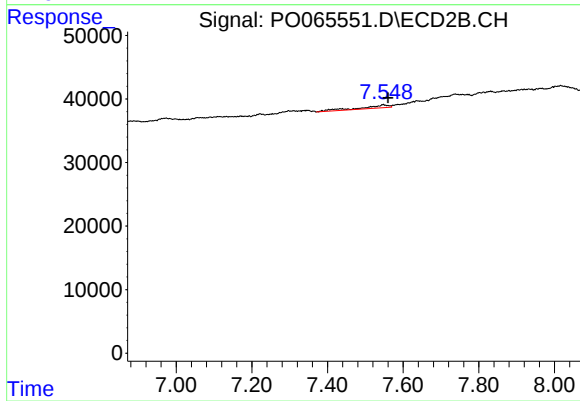

#43 AR-1268-3


R.T.: 7.547 min
Delta R.T.: -0.013 min
Response: 24671
Conc: 5.81 ng/ml

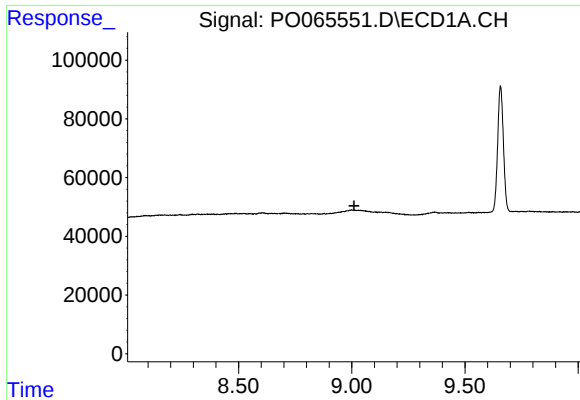

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 9.010 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

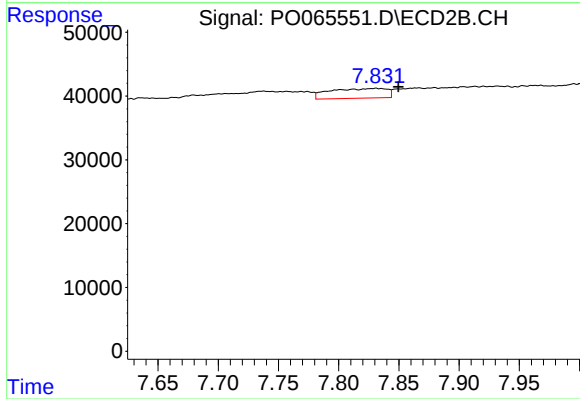


#44 AR-1268-4

R.T.: 7.831 min
Delta R.T.: -0.018 min
Response: 50652
Conc: 25.59 ng/ml

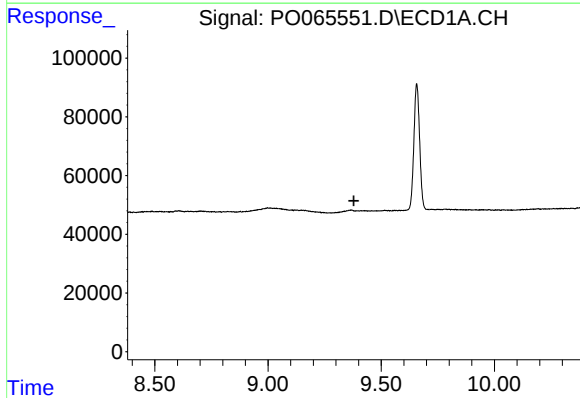

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.380 min
Response: 0
Conc: N.D.

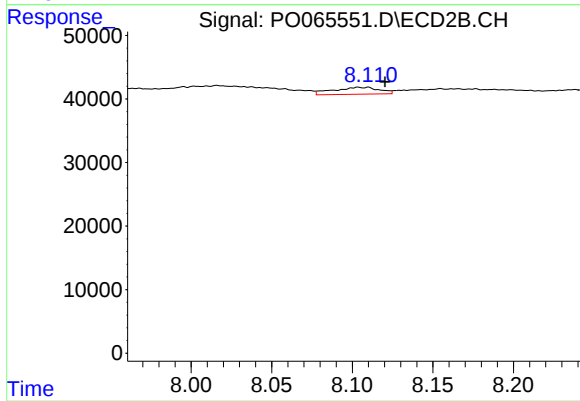

#45 AR-1268-5

R.T.: 8.105 min
Delta R.T.: -0.015 min
Response: 21506
Conc: 1.50 ng/ml