

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011620\
 Data File : P0065576.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Jan 2020 21:43
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 03:20:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.159	3.434	615235	748820	33.692	34.041
2)	SA Decachlor...	9.662	8.338	566842	649187	16.730	15.654
Target Compounds							
9)	L2 AR-1221-2	0.000	3.727	0	9594	N.D.	48.655 #
28)	L6 AR-1254-3	0.000	5.825	0	10009	N.D.	4.441 #
29)	L6 AR-1254-4	0.000	6.129	0	89574	N.D.	59.416 #
30)	L6 AR-1254-5	0.000	6.462	0	46129	N.D.	20.723 #
32)	L7 AR-1260-2	0.000	6.129	0	89574	N.D.	36.870 #
40)	L8 AR-1262-5	0.000	7.822	0	45514	N.D.	26.691 #
44)	L9 AR-1268-4	0.000	7.822	0	45514	N.D.	22.996 #
45)	L9 AR-1268-5	0.000	8.106	0	15578	N.D.	1.083 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011620\
Data File : P0065576.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jan 2020 21:43
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 03:20:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

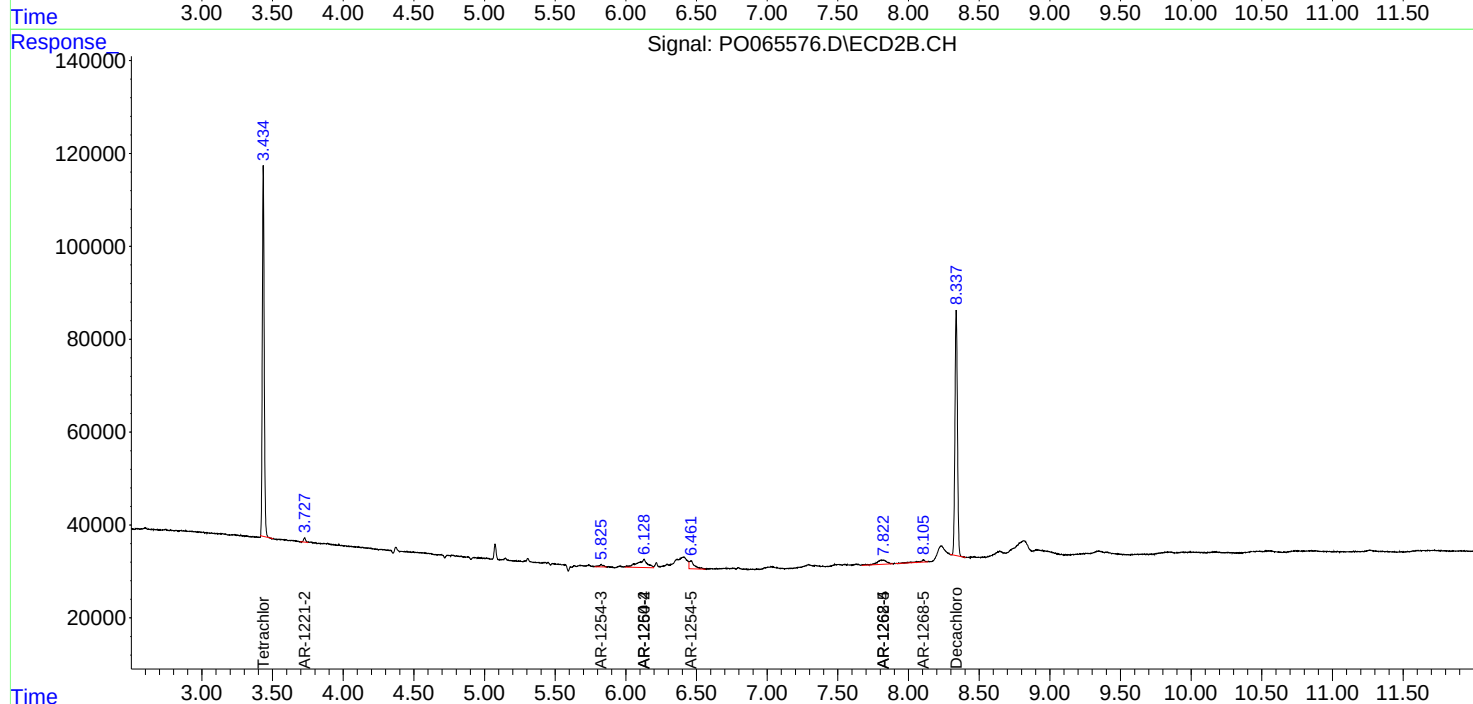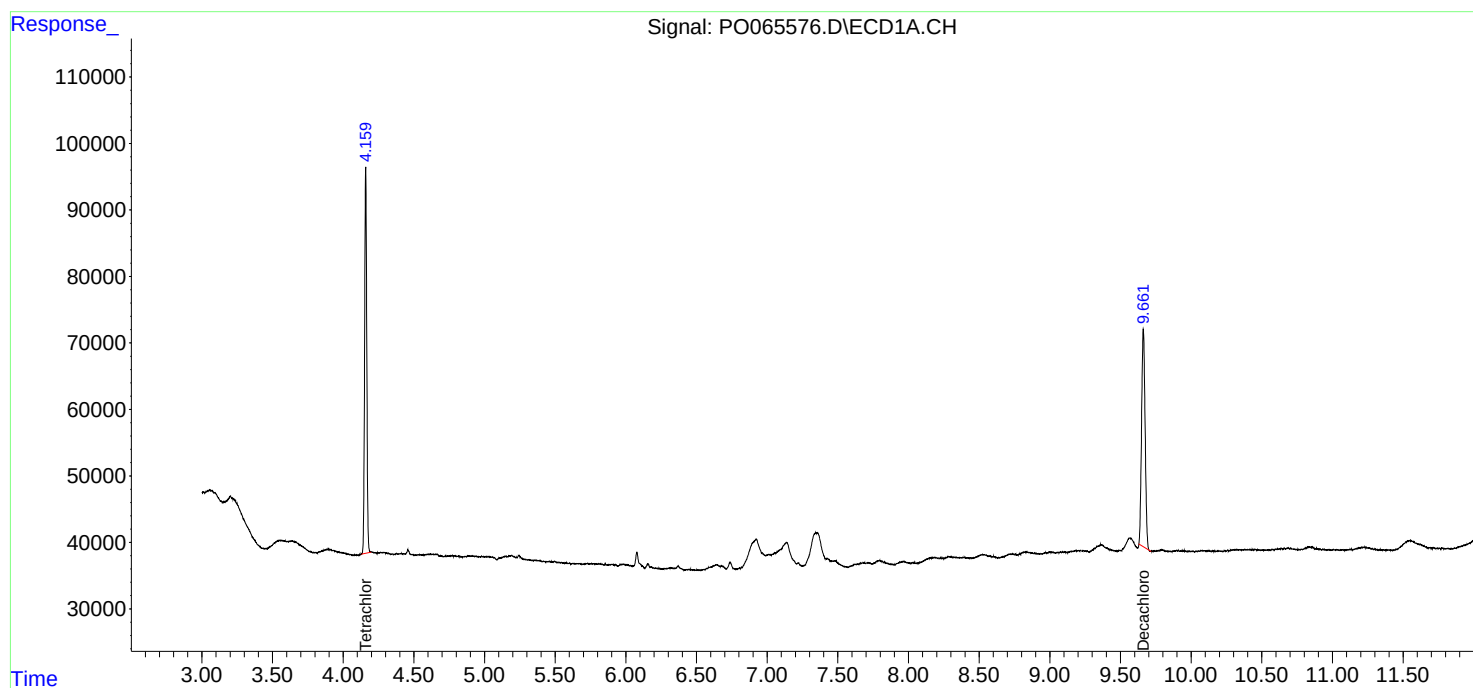


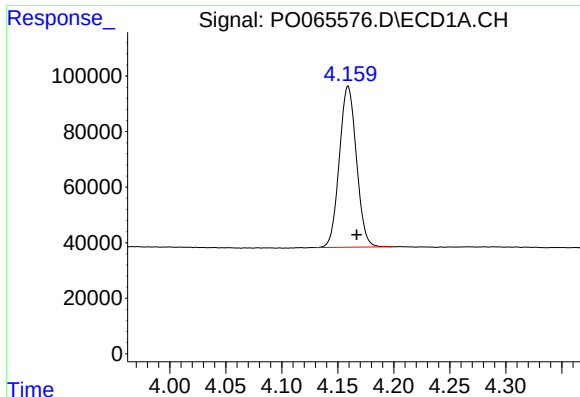

#1 Tetrachloro-m-xylene


R.T.: 4.159 min
Delta R.T.: -0.008 min
Response: 615235
Conc: 33.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

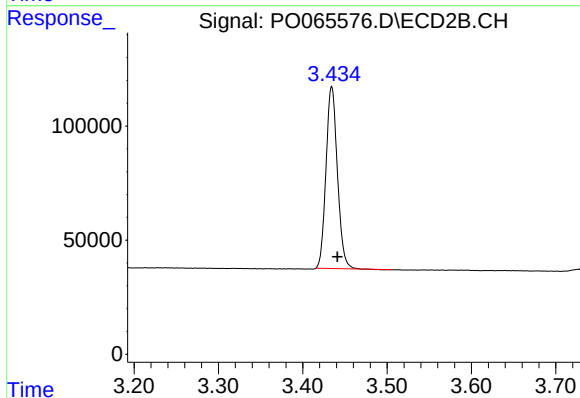


#1 Tetrachloro-m-xylene

R.T.: 3.434 min
Delta R.T.: -0.007 min
Response: 748820
Conc: 34.04 ng/ml

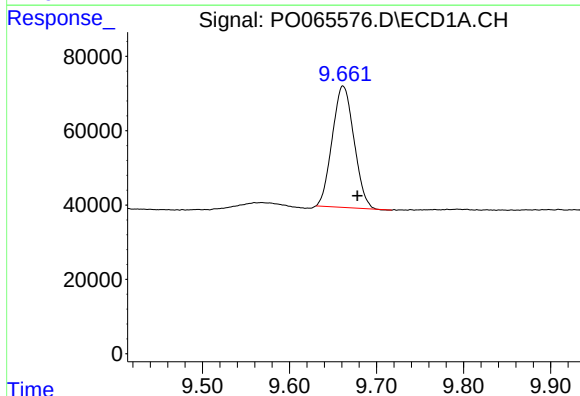


#2 Decachlorobiphenyl

R.T.: 9.662 min
Delta R.T.: -0.017 min
Response: 566842
Conc: 16.73 ng/ml

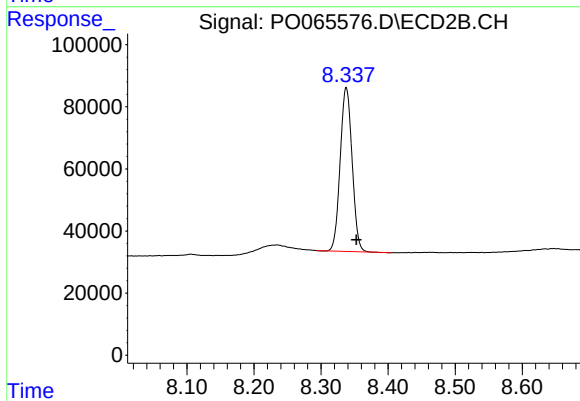

#2 Decachlorobiphenyl


R.T.: 8.338 min
Delta R.T.: -0.015 min
Response: 649187
Conc: 15.65 ng/ml

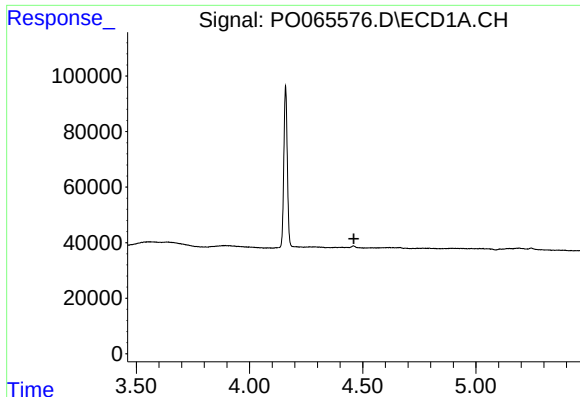

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.461 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

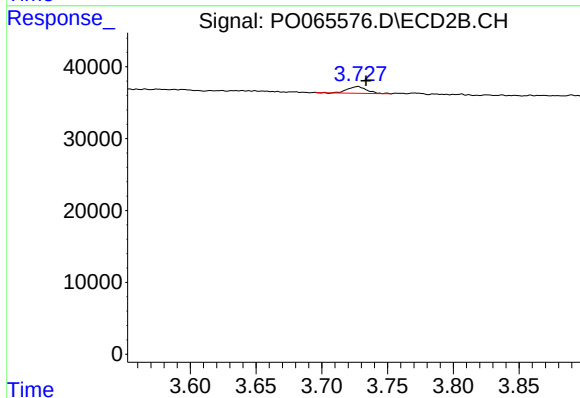


#9 AR-1221-2

R.T.: 3.727 min
Delta R.T.: -0.006 min
Response: 9594
Conc: 48.66 ng/ml

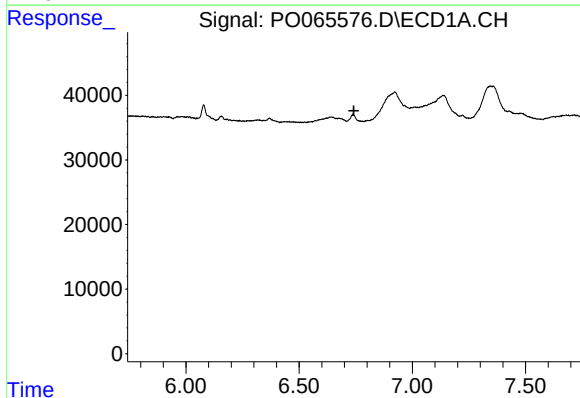


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T.: 6.742 min
Response: 0
Conc: N.D.

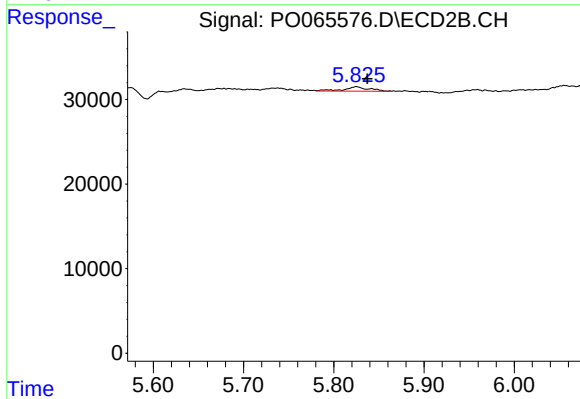

#28 AR-1254-3


R.T.: 5.825 min
Delta R.T.: -0.012 min
Response: 10009
Conc: 4.44 ng/ml

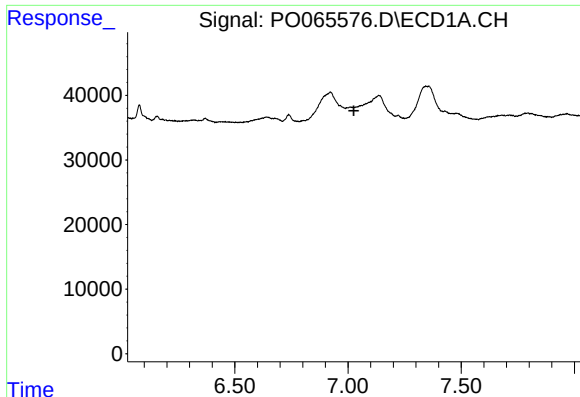

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.026 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

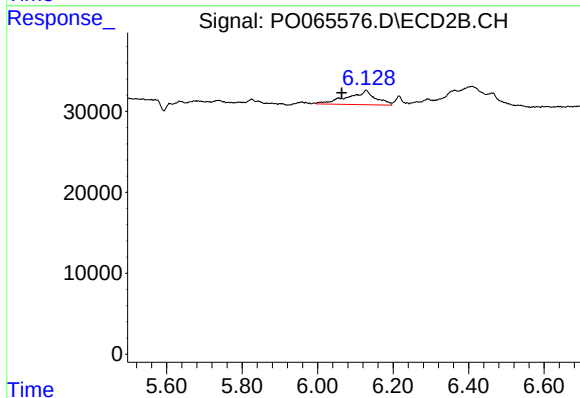


#29 AR-1254-4

R.T.: 6.129 min
Delta R.T.: 0.064 min
Response: 89574
Conc: 59.42 ng/ml

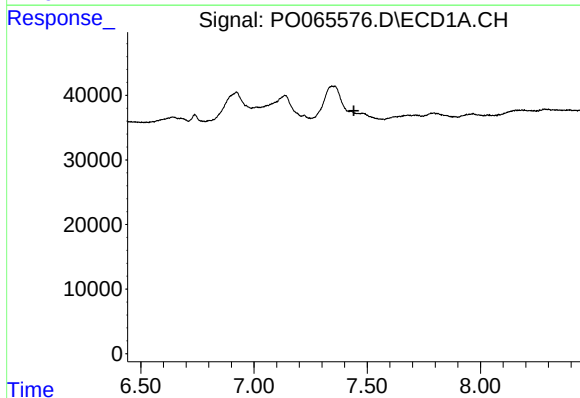


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 7.441 min
Response: 0
Conc: N.D.

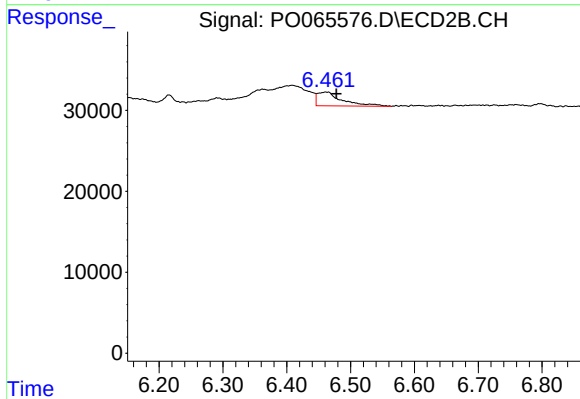

#30 AR-1254-5


R.T.: 6.462 min
Delta R.T.: -0.016 min
Response: 46129
Conc: 20.72 ng/ml

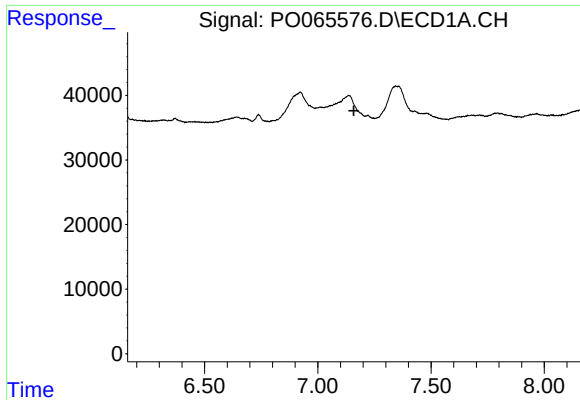

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.160 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

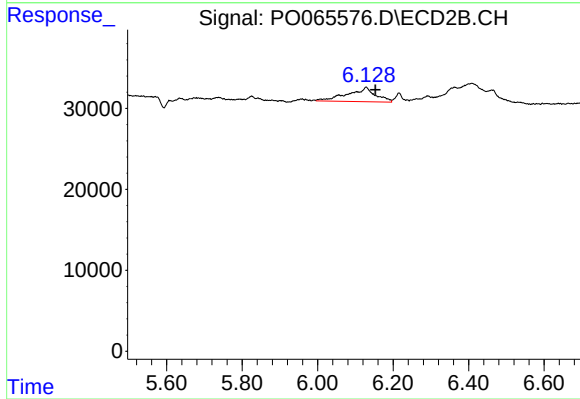


#32 AR-1260-2

R.T.: 6.129 min
Delta R.T.: -0.024 min
Response: 89574
Conc: 36.87 ng/ml

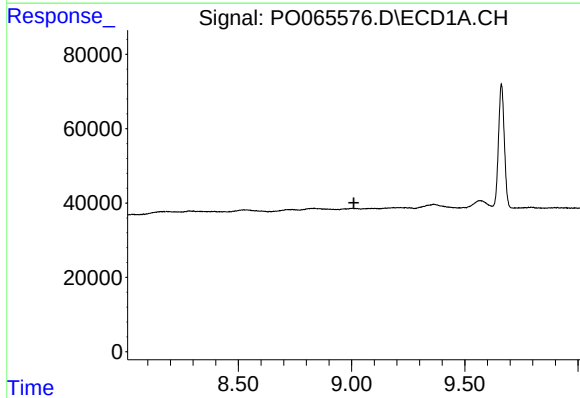


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.010 min
Response: 0
Conc: N.D.

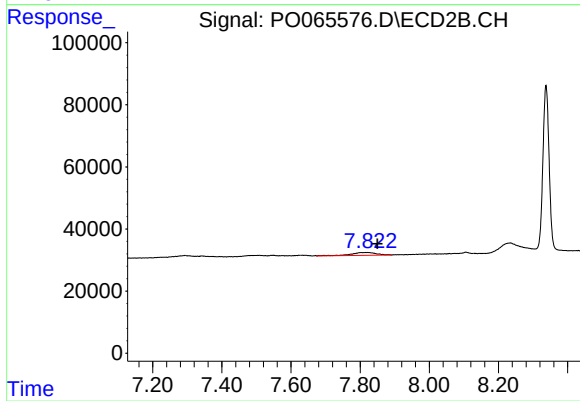

#40 AR-1262-5


R.T.: 7.822 min
Delta R.T.: -0.029 min
Response: 45514
Conc: 26.69 ng/ml

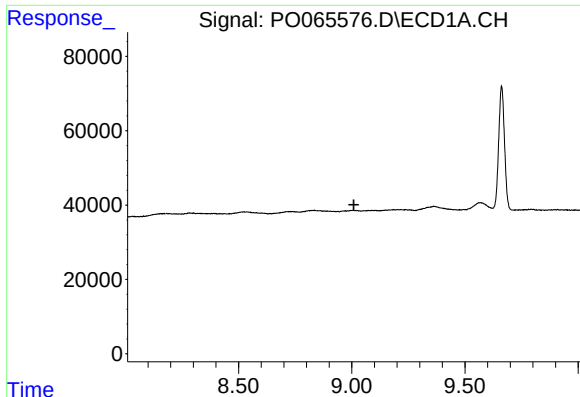

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 9.010 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

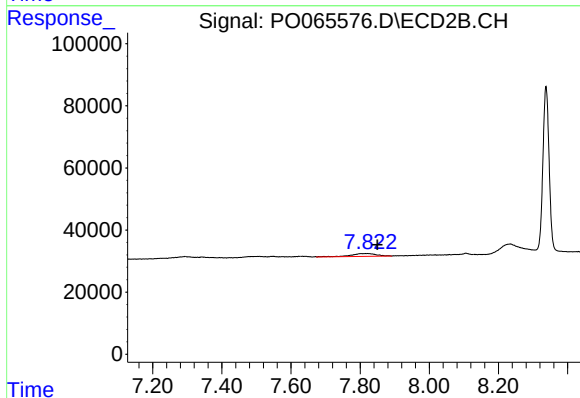


#44 AR-1268-4

R.T.: 7.822 min
Delta R.T.: -0.028 min
Response: 45514
Conc: 23.00 ng/ml

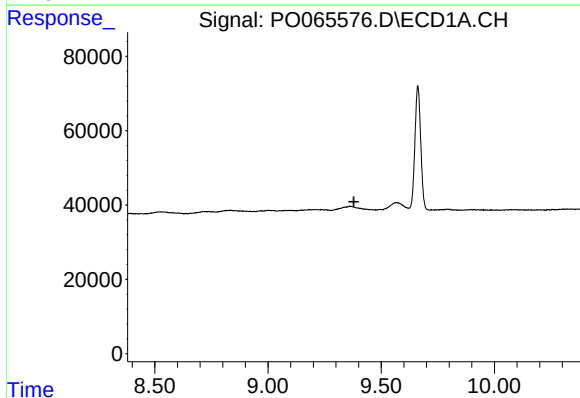

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.380 min
Response: 0
Conc: N.D.

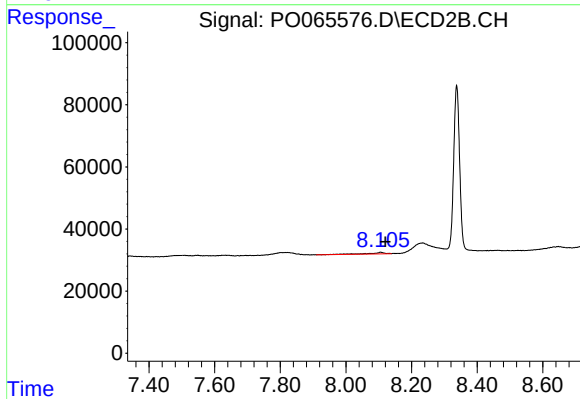

#45 AR-1268-5

R.T.: 8.106 min
Delta R.T.: -0.014 min
Response: 15578
Conc: 1.08 ng/ml