

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011620\
 Data File : P0065545.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Jan 2020 12:03
 Operator : DD\AJ
 Sample : L1126-02RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BW-2-45.0RE

Manual Integrations
 APPROVED

mohammad
 1/17/2020 11:27:09 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 13:10:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.162	3.435	490793	596770	26.877	27.129
2) SA Decachlor...	9.667	8.341	892293	1059366	26.335m	25.545

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011620\
Data File : P0065545.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jan 2020 12:03
Operator : DD\AJ
Sample : L1126-02RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BW-2-45.0RE


Manual Integrations
APPROVED

mohammad
1/17/2020 11:27:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 13:10:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

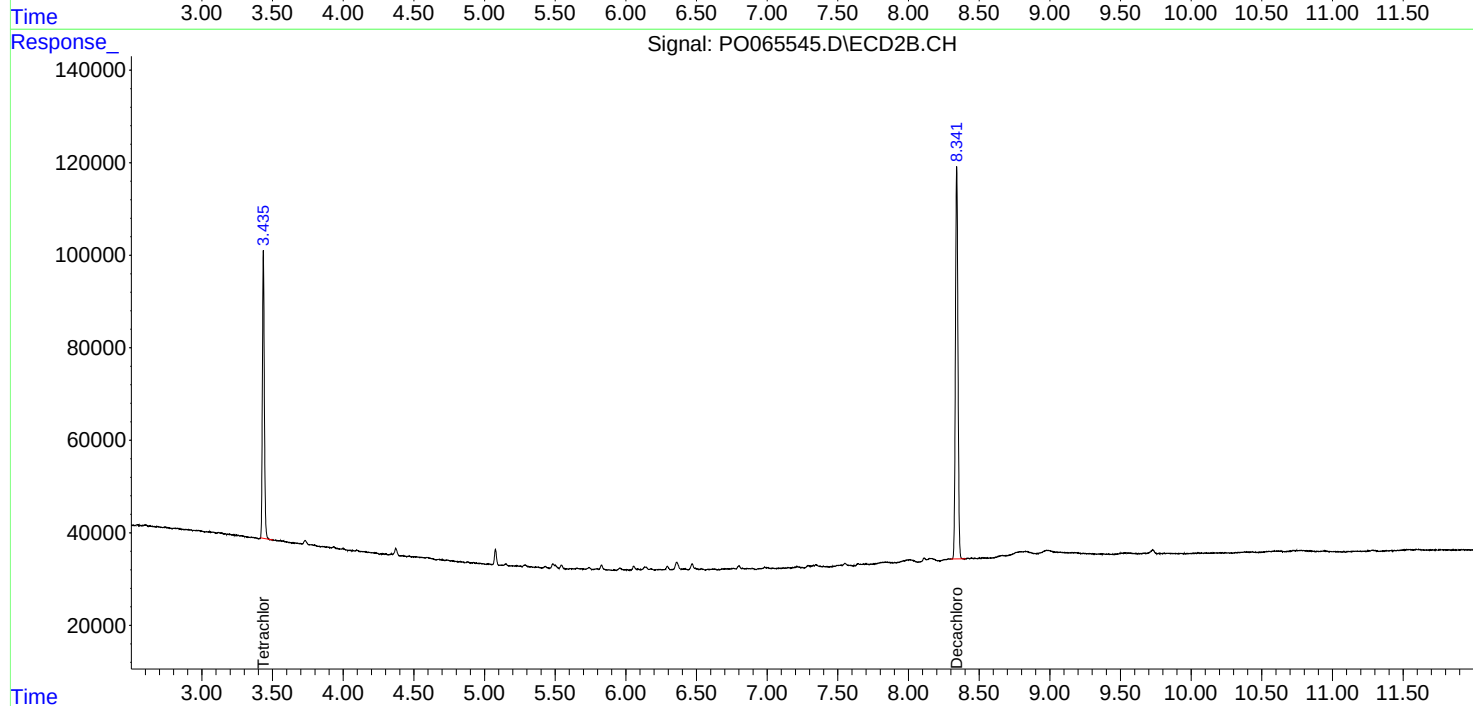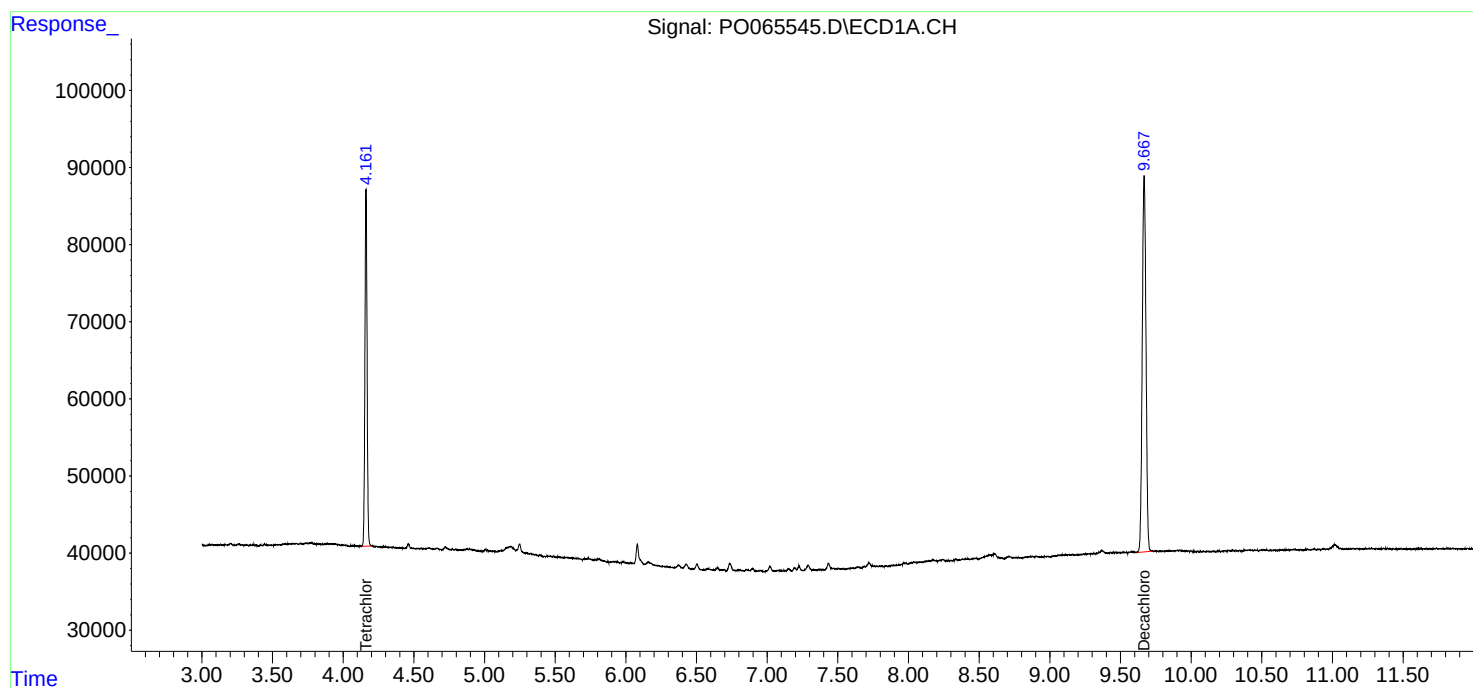

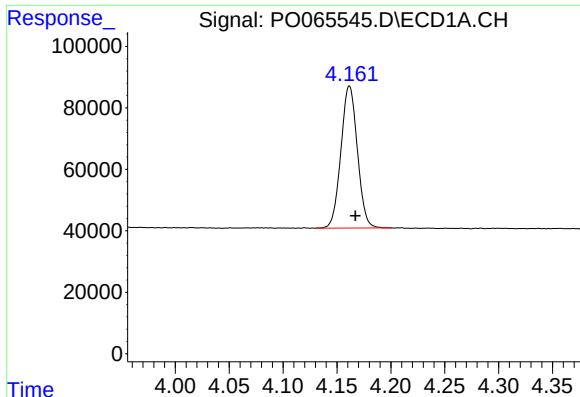


#1 Tetrachloro-m-xylene

R.T.: 4.162 min
Delta R.T.: -0.005 min
Response: 490793
Conc: 26.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
BW-2-45.0RE


Manual Integrations
APPROVED

mohammad
1/17/2020 11:27:09 AM

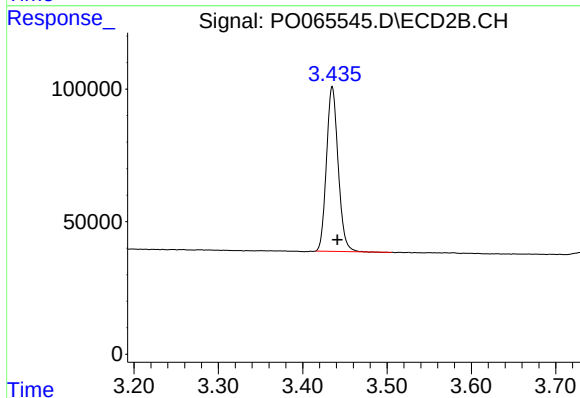


#1 Tetrachloro-m-xylene

R.T.: 3.435 min
Delta R.T.: -0.006 min
Response: 596770
Conc: 27.13 ng/ml

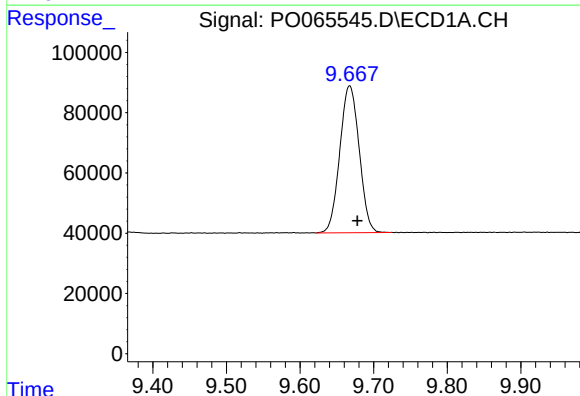

#2 Decachlorobiphenyl

R.T.: 9.667 min
Delta R.T.: -0.011 min
Response: 892293
Conc: 26.33 ng/ml m

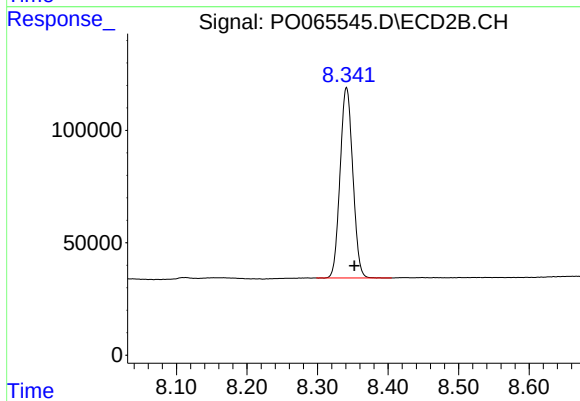

#2 Decachlorobiphenyl

R.T.: 8.341 min
Delta R.T.: -0.011 min
Response: 1059366
Conc: 25.55 ng/ml