

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011620\
 Data File : P0065561.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Jan 2020 17:15
 Operator : DD\AJ
 Sample : PB126146BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB126146BL

Manual Integrations
 APPROVED

Ankita
 1/17/2020 1:07:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 17:50:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.158	3.433	350031	419729	19.169	19.081m
2) SA Decachlor...	9.660	8.338	682009	834193	20.129m	20.115

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011620\
Data File : P0065561.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jan 2020 17:15
Operator : DD\AJ
Sample : PB126146BL
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB126146BL


Manual Integrations
APPROVED

Ankita
1/17/2020 1:07:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 17:50:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

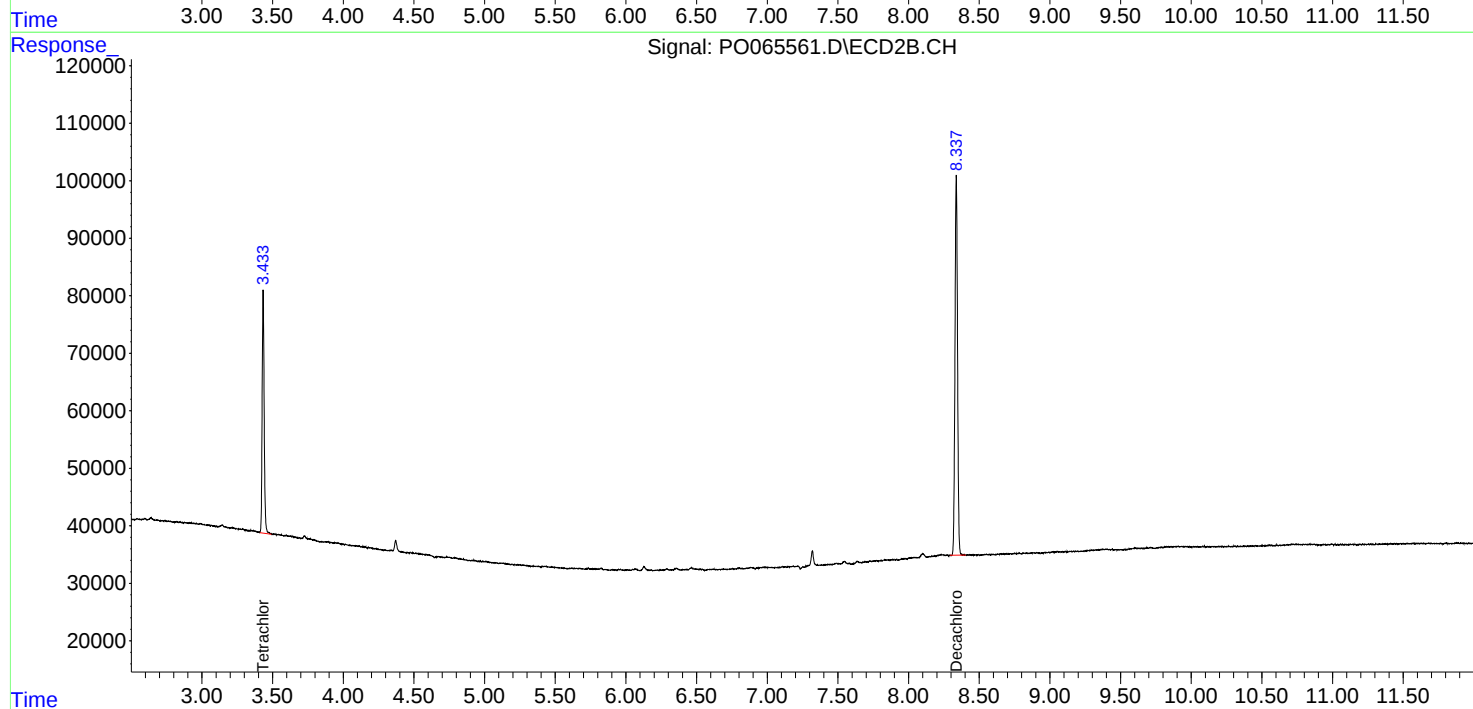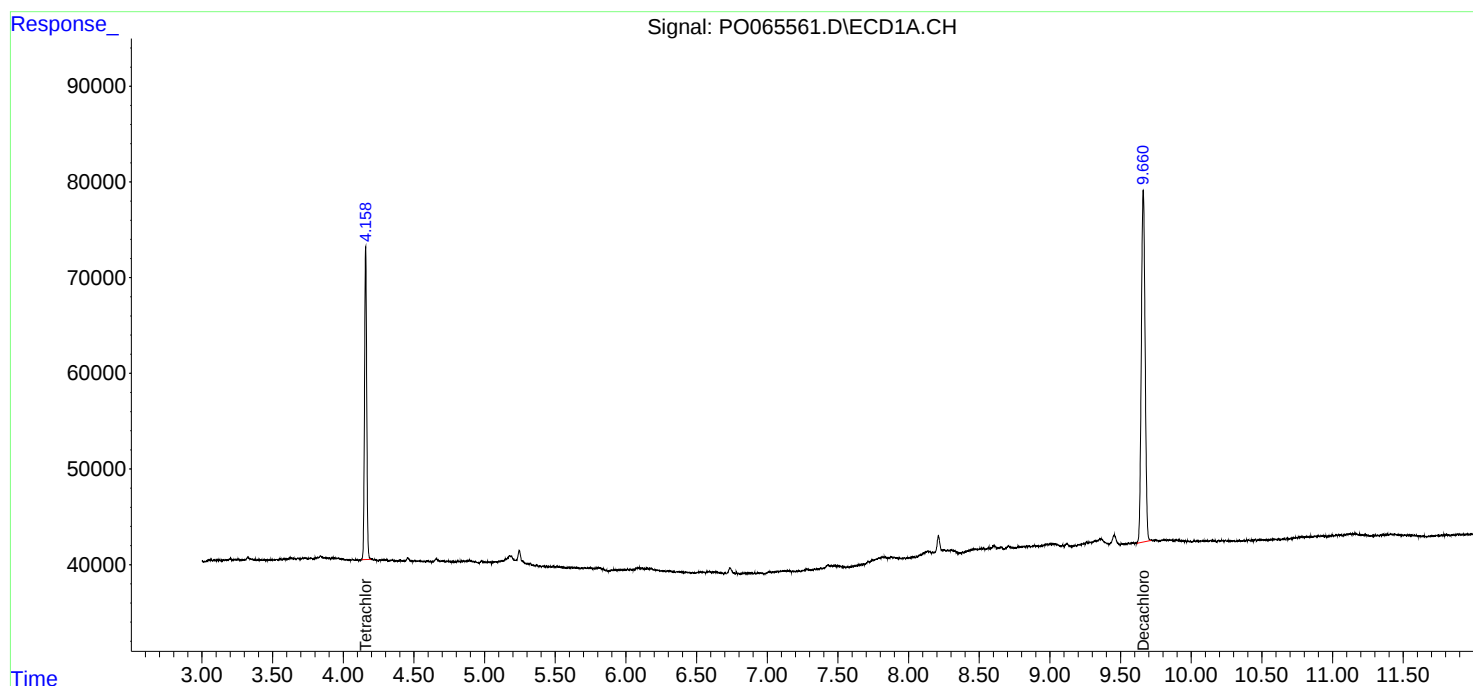

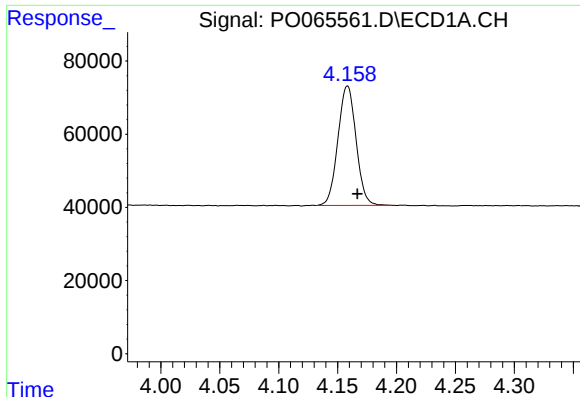


#1 Tetrachloro-m-xylene

R.T.: 4.158 min
Delta R.T.: -0.009 min
Response: 350031
Conc: 19.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB126146BL


Manual Integrations
APPROVED

Ankita
1/17/2020 1:07:43 PM

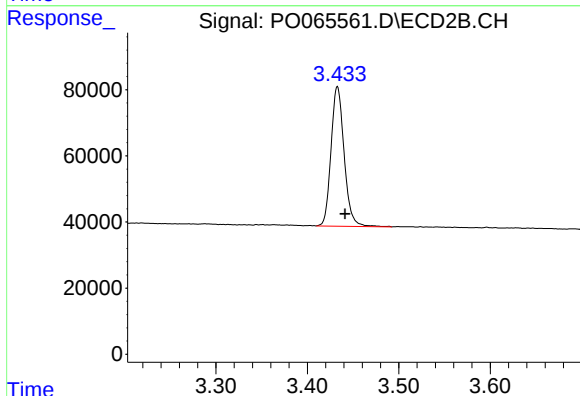


#1 Tetrachloro-m-xylene

R.T.: 3.433 min
Delta R.T.: -0.009 min
Response: 419729
Conc: 19.08 ng/ml m

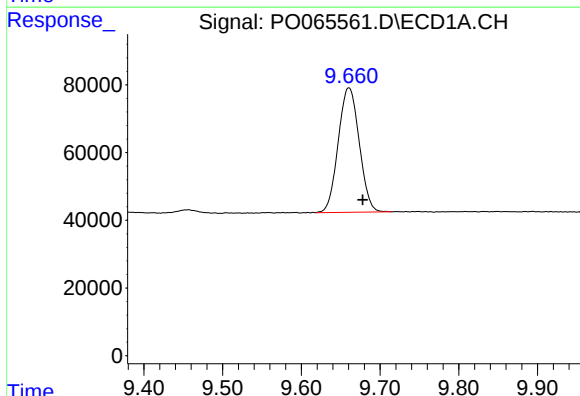

#2 Decachlorobiphenyl

R.T.: 9.660 min
Delta R.T.: -0.018 min
Response: 682009
Conc: 20.13 ng/ml m

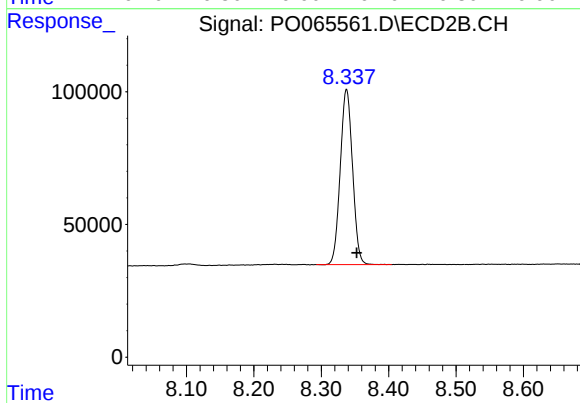

#2 Decachlorobiphenyl

R.T.: 8.338 min
Delta R.T.: -0.015 min
Response: 834193
Conc: 20.12 ng/ml