

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011620\
 Data File : P0065586.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jan 2020 1:54
 Operator : DD\AJ
 Sample : L1153-06
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 06-A-06-B-06-C

Manual Integrations
 APPROVED

mohammad
 1/17/2020 11:33:38 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 03:24:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.158	3.434	546817	633482	29.946	28.798
2) SA Decachlor...	9.659	8.336	594278	685642	17.539m	16.533

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011620\
Data File : PO065586.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jan 2020 1:54
Operator : DD\AJ
Sample : L1153-06
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
06-A-06-B-06-C


Manual Integrations
APPROVED

mohammad
1/17/2020 11:33:38 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 03:24:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

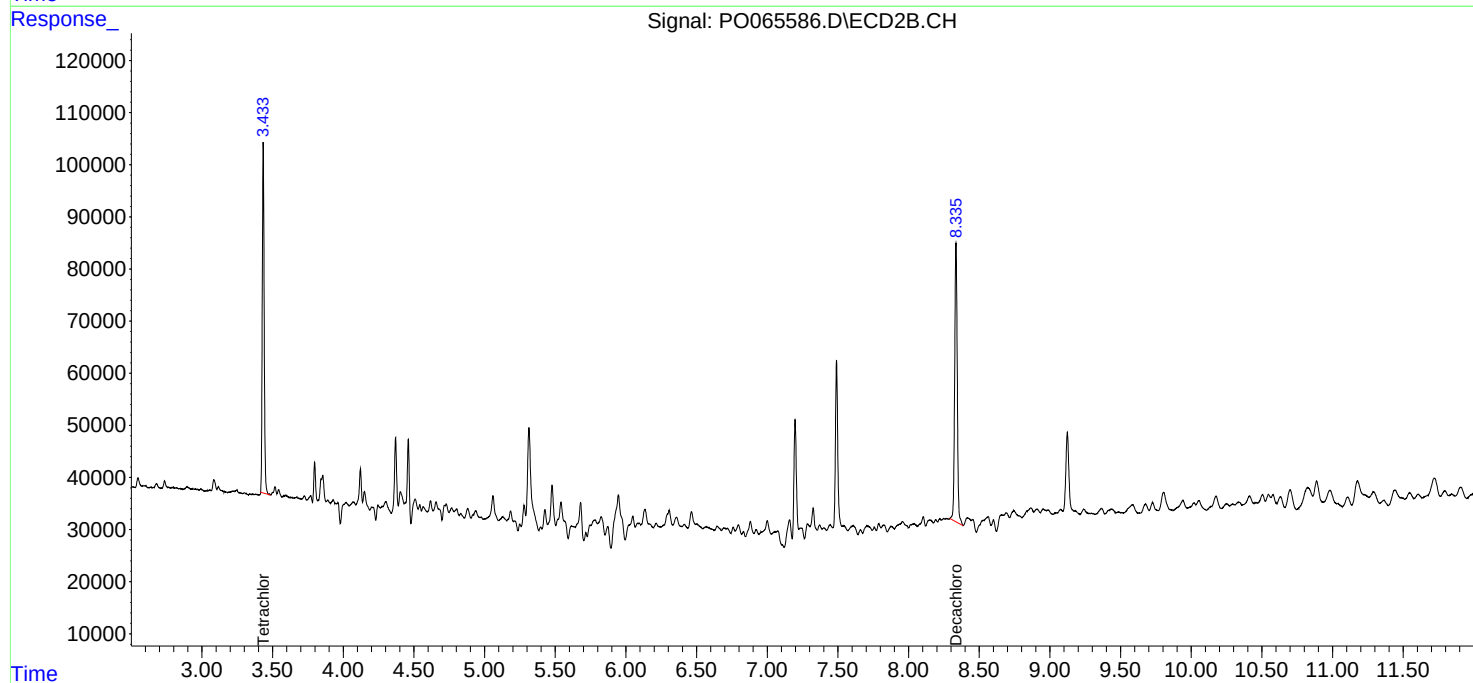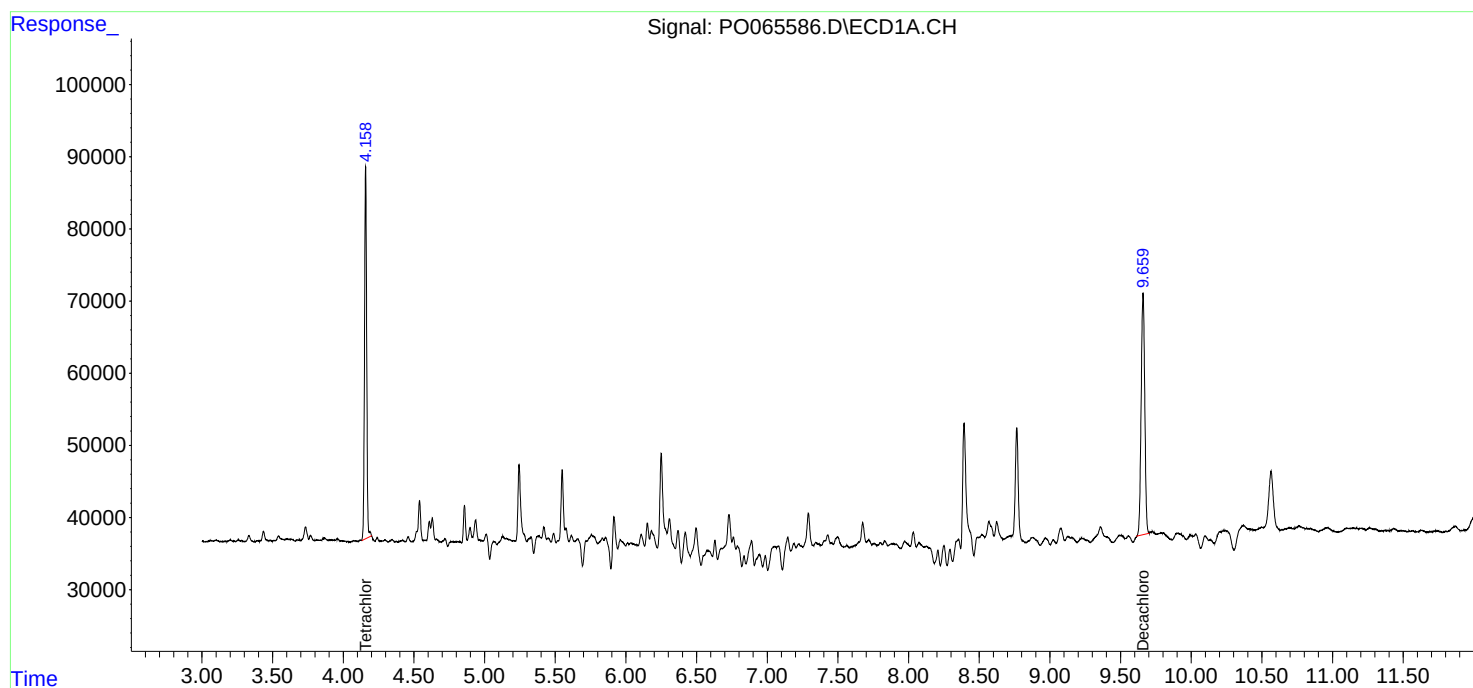

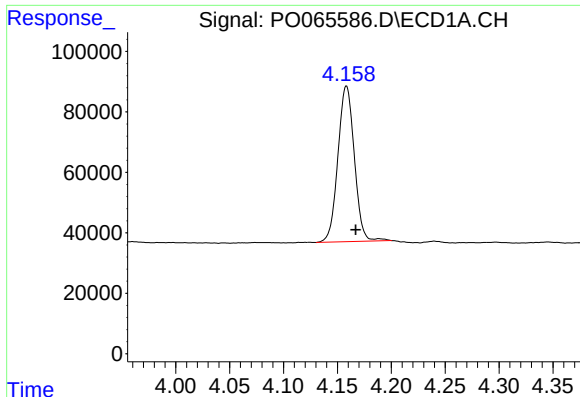


#1 Tetrachloro-m-xylene

R.T.: 4.158 min
Delta R.T.: -0.009 min
Response: 546817
Conc: 29.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
06-A-06-B-06-C


Manual Integrations
APPROVED

mohammad
1/17/2020 11:33:38 AM

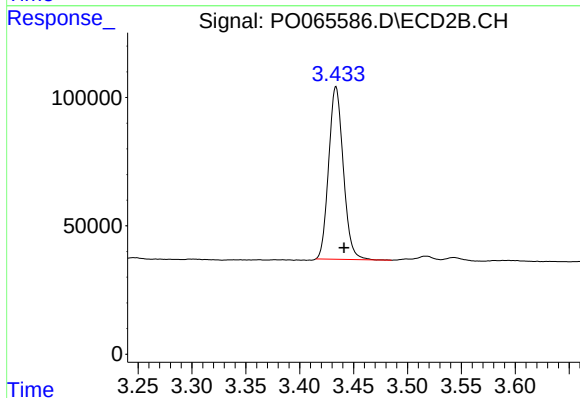


#1 Tetrachloro-m-xylene

R.T.: 3.434 min
Delta R.T.: -0.007 min
Response: 633482
Conc: 28.80 ng/ml

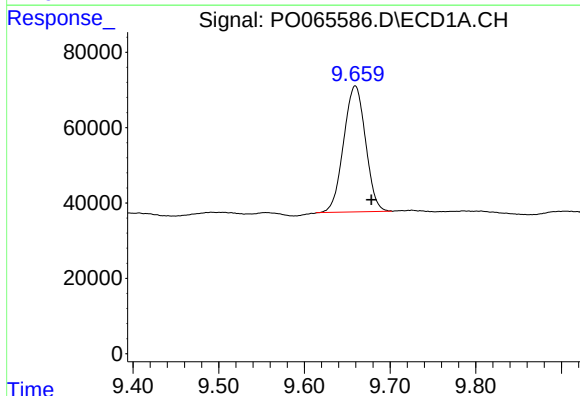

#2 Decachlorobiphenyl

R.T.: 9.659 min
Delta R.T.: -0.019 min
Response: 594278
Conc: 17.54 ng/ml m

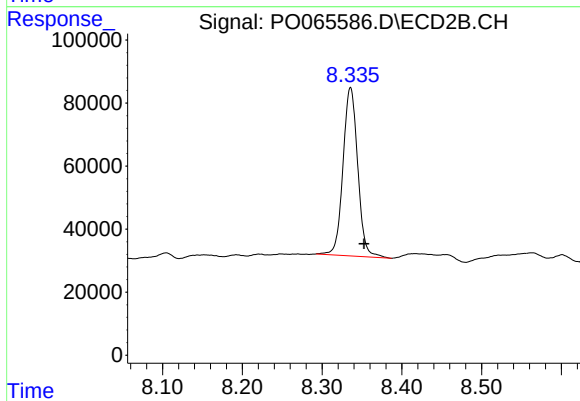

#2 Decachlorobiphenyl

R.T.: 8.336 min
Delta R.T.: -0.017 min
Response: 685642
Conc: 16.53 ng/ml