

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011620\
 Data File : P0065592.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jan 2020 3:34
 Operator : DD\AJ
 Sample : L1153-07 5X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 07-A-07-B-07-C

Manual Integrations
 APPROVED

mohammad
 1/17/2020 11:36:02 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 06:01:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.155	3.437	102283	246267	5.601m	11.195 #
2) SA Decachlor...	9.657	8.335	107527	131401	3.174m	3.169

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011620\
Data File : P0065592.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jan 2020 3:34
Operator : DD\AJ
Sample : L1153-07 5X
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
07-A-07-B-07-C


Manual Integrations
APPROVED

mohammad
1/17/2020 11:36:02 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 06:01:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

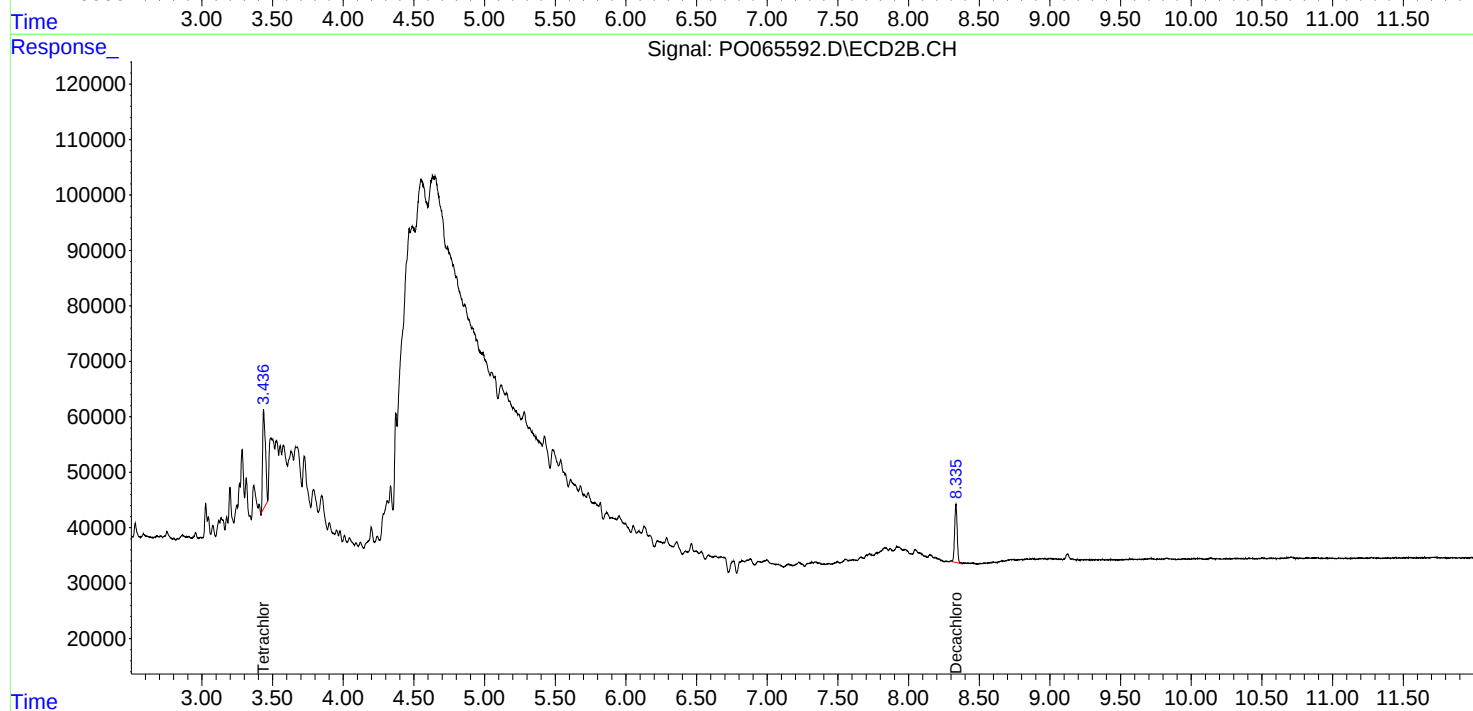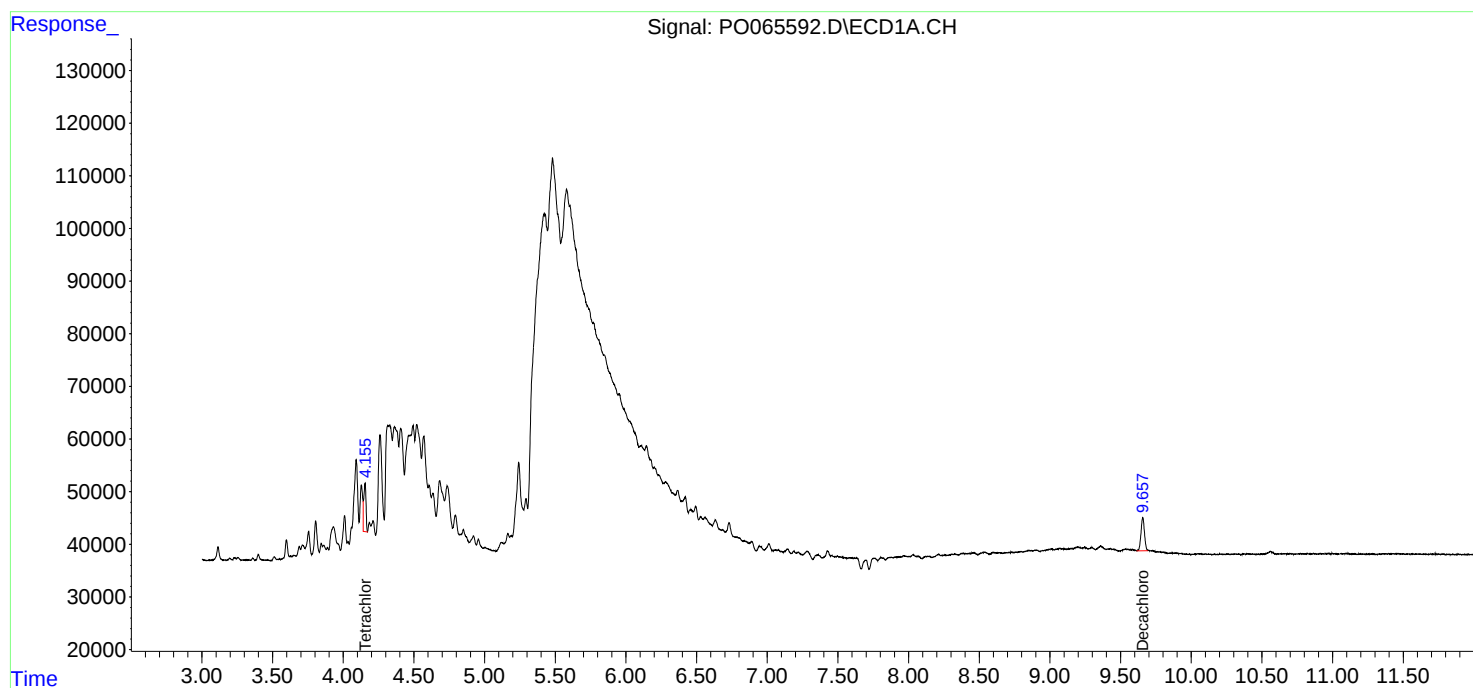

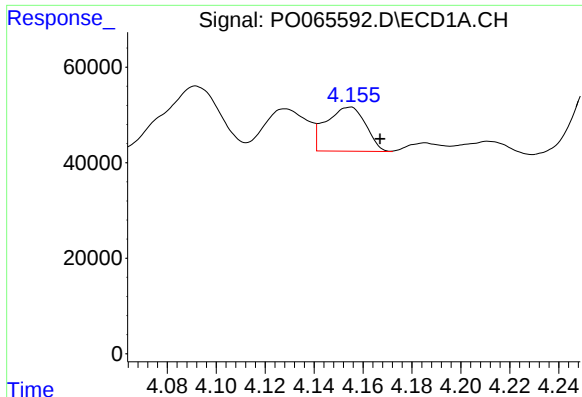


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: -0.012 min
Response: 102283
Conc: 5.60 ng/ml m

Instrument :
ECD_O
ClientSampleId :
07-A-07-B-07-C


Manual Integrations
APPROVED

mohammad
1/17/2020 11:36:02 AM

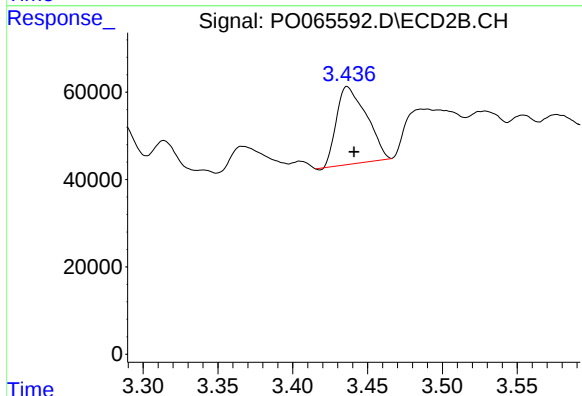


#1 Tetrachloro-m-xylene

R.T.: 3.437 min
Delta R.T.: -0.005 min
Response: 246267
Conc: 11.20 ng/ml

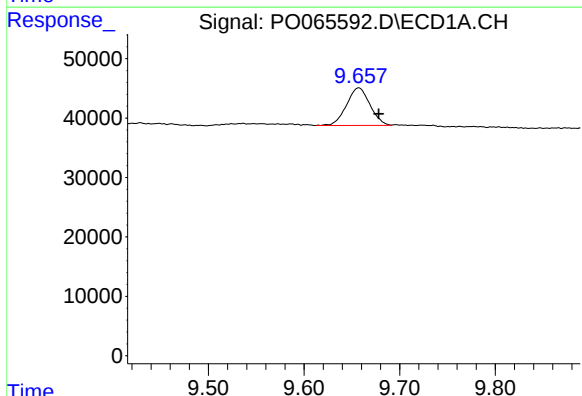

#2 Decachlorobiphenyl

R.T.: 9.657 min
Delta R.T.: -0.021 min
Response: 107527
Conc: 3.17 ng/ml m

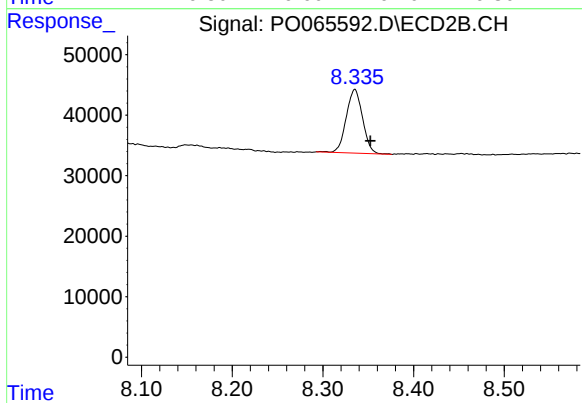

#2 Decachlorobiphenyl

R.T.: 8.335 min
Delta R.T.: -0.017 min
Response: 131401
Conc: 3.17 ng/ml