

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011623\
 Data File : P0092042.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jan 2023 14:45
 Operator : YP/AJ
 Sample : 01157-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TR-4-011323

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/17/2023
 Supervised By :Ankita Jodhani 01/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 20:49:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 11 04:41:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.461	3.647	48283074	26627860	17.311m	19.179
2) SA Decachlor...	10.376	8.702	30597688	15286240	15.629m	17.240

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011623\
Data File : PO092042.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jan 2023 14:45
Operator : YP/AJ
Sample : 01157-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TR-4-011323


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/17/2023
Supervised By :Ankita Jodhani 01/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 20:49:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 11 04:41:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

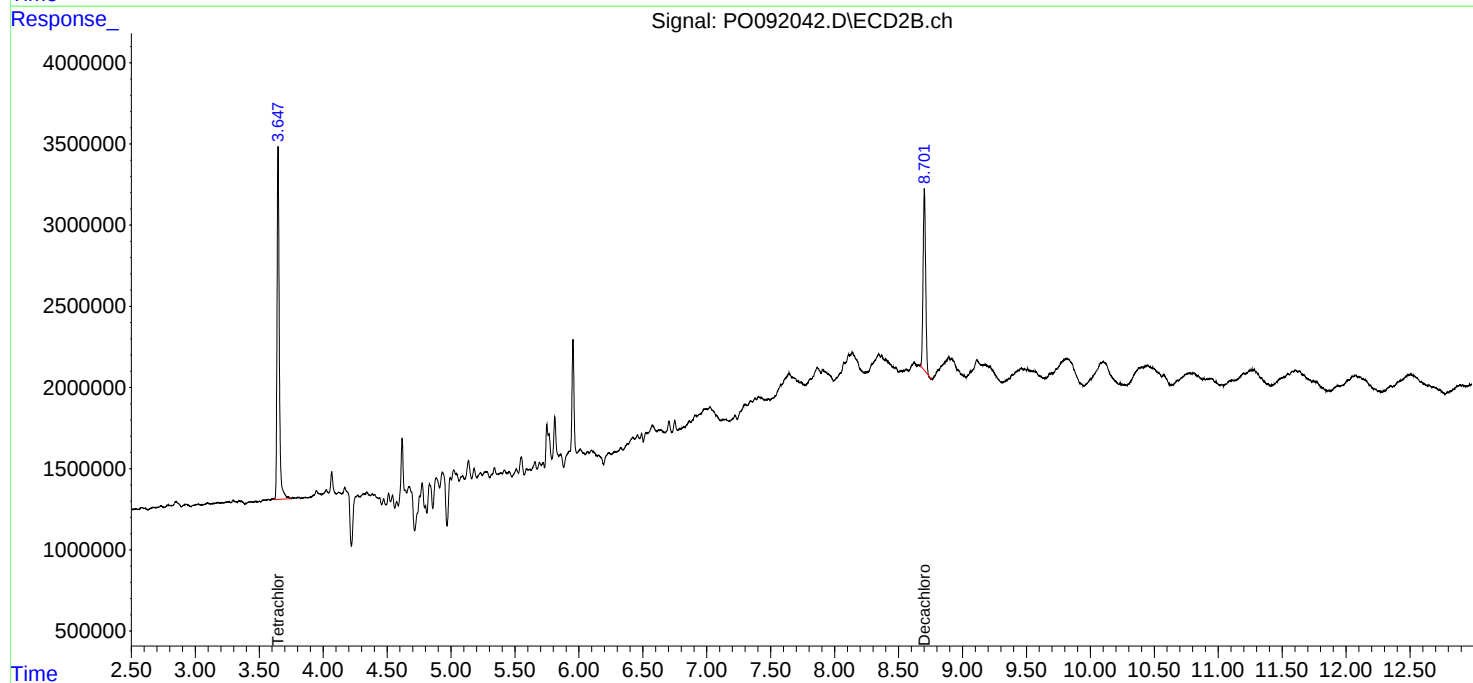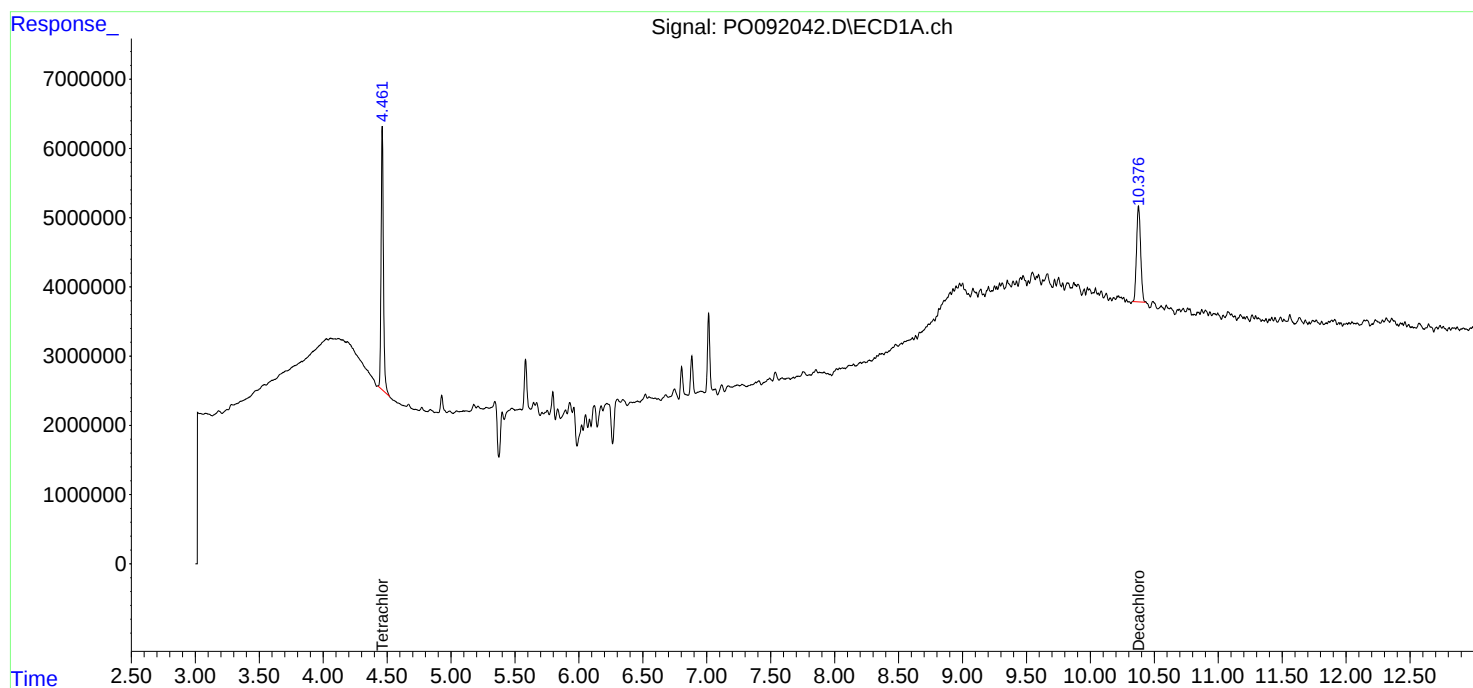

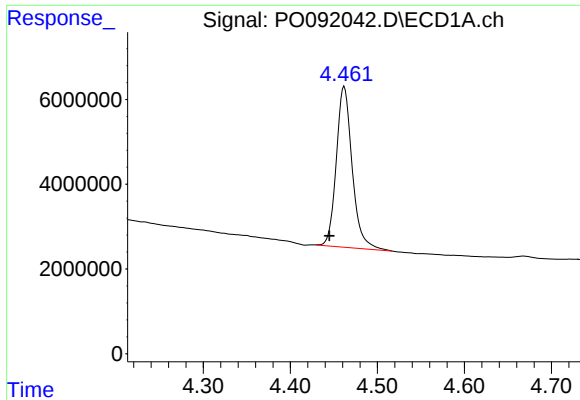


#1 Tetrachloro-m-xylene

R.T.: 4.461 min
Delta R.T.: 0.016 min
Response: 48283074
Conc: 17.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
TR-4-011323


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/17/2023
Supervised By :Ankita Jodhani 01/17/2023

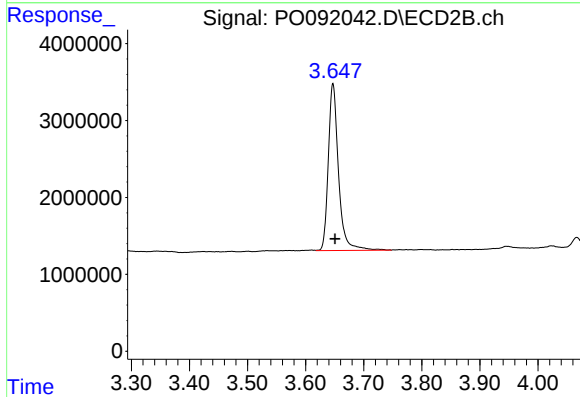


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: -0.004 min
Response: 26627860
Conc: 19.18 ng/ml

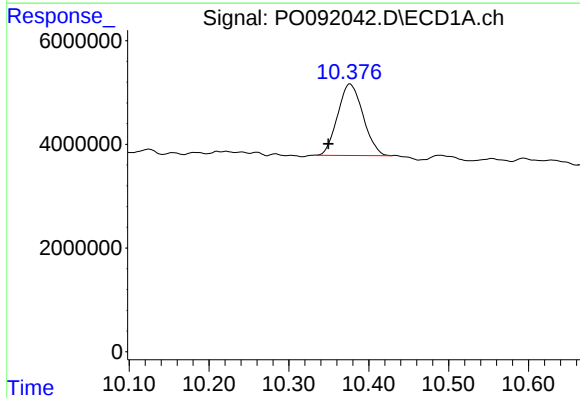

#2 Decachlorobiphenyl

R.T.: 10.376 min
Delta R.T.: 0.026 min
Response: 30597688
Conc: 15.63 ng/ml m

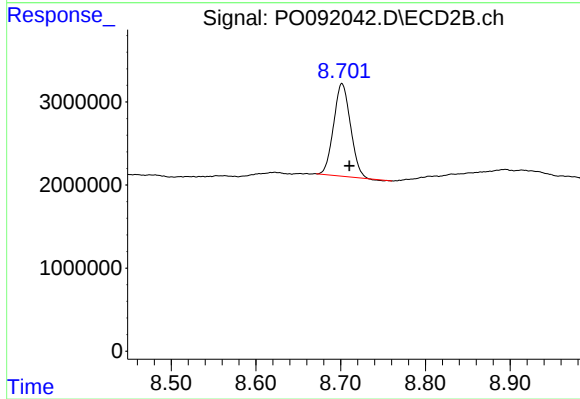

#2 Decachlorobiphenyl

R.T.: 8.702 min
Delta R.T.: -0.009 min
Response: 15286240
Conc: 17.24 ng/ml