

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011623\
 Data File : P0092057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jan 2023 20:37
 Operator : YP/AJ
 Sample : 01161-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20230113-H4-STOCKPILE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/17/2023
 Supervised By :Ankita Jodhani 01/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 02:39:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 11 04:41:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.445	3.646	42500174	22136959	15.237	15.945m
2) SA Decachlor...	10.361	8.700	38144182	19150741	19.484	21.598

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011623\
Data File : PO092057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jan 2023 20:37
Operator : YP/AJ
Sample : 01161-01
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
20230113-H4-STOCKPILE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/17/2023
Supervised By :Ankita Jodhani 01/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 02:39:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 11 04:41:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

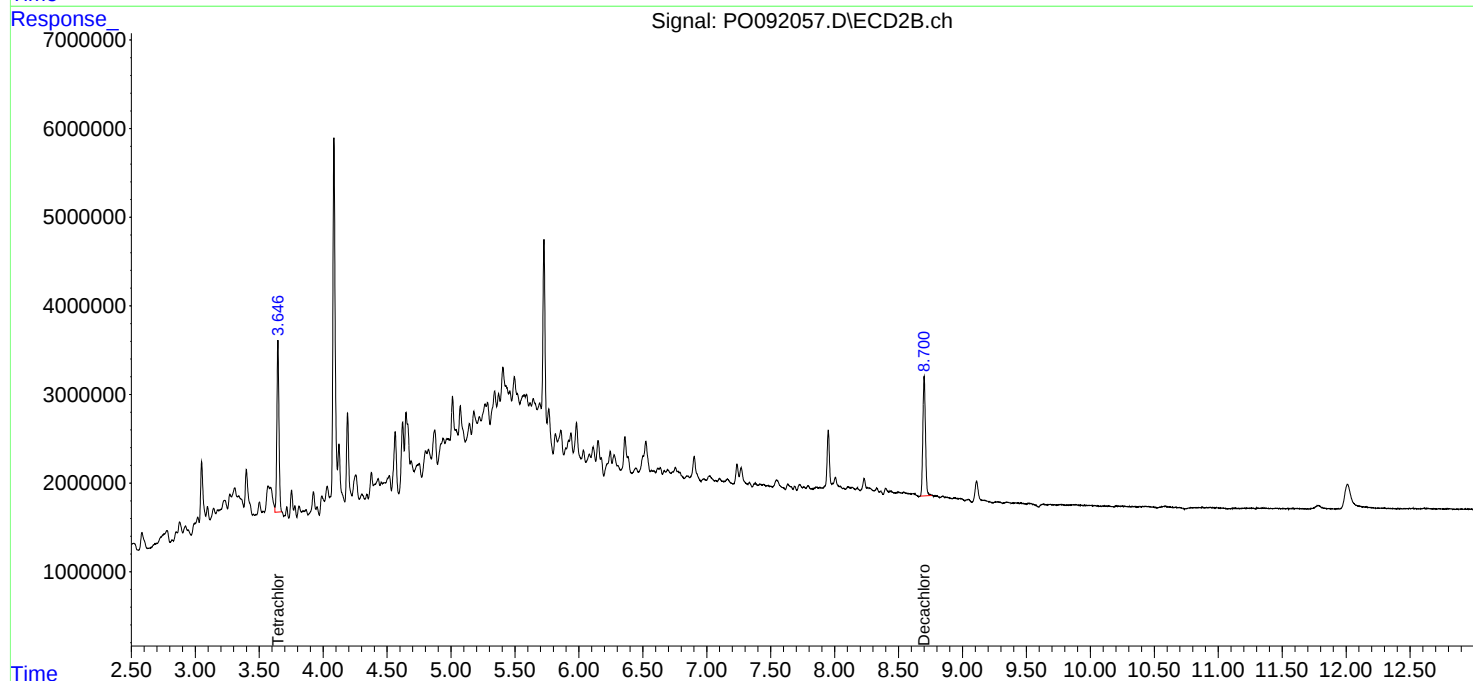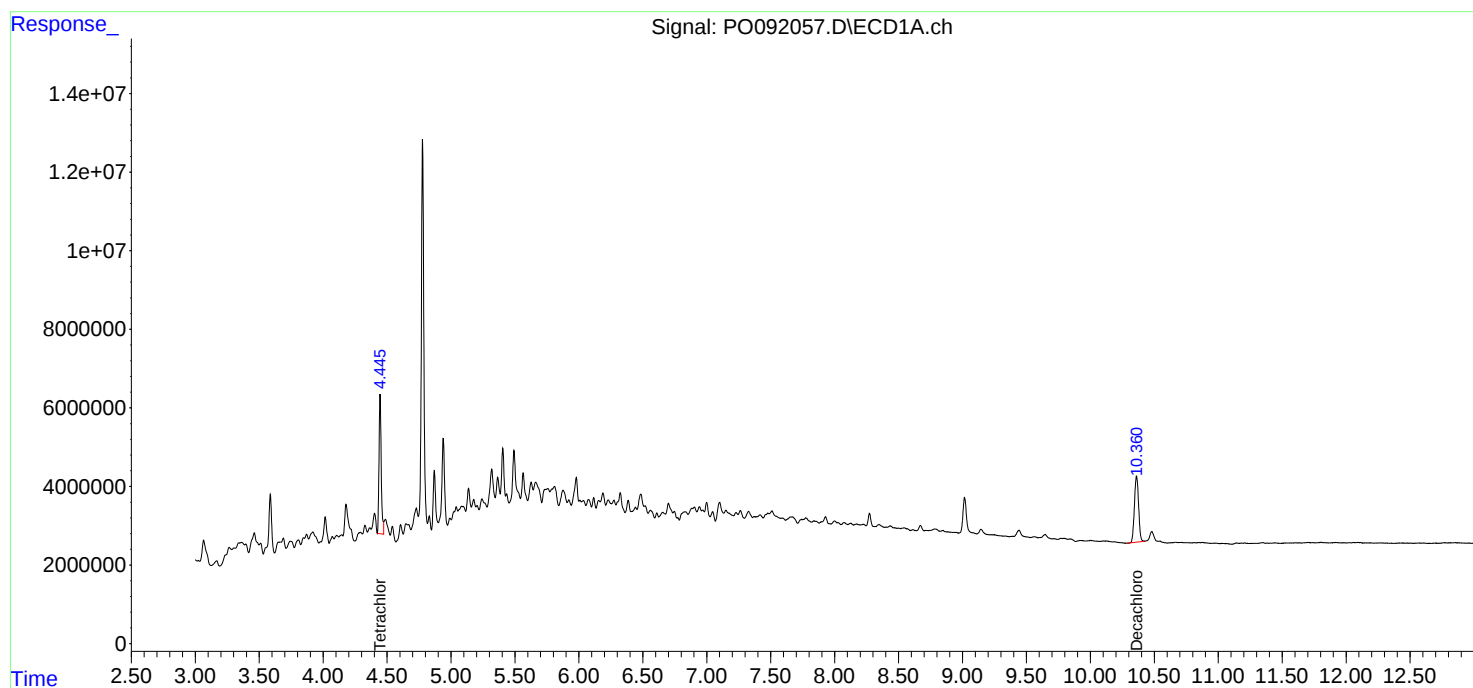

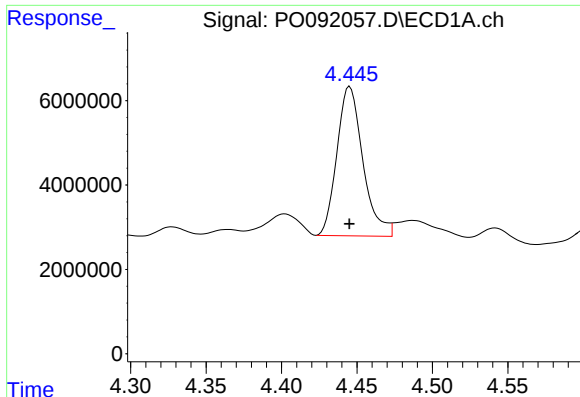


#1 Tetrachloro-m-xylene

R.T.: 4.445 min
Delta R.T.: 0.000 min
Response: 42500174
Conc: 15.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
20230113-H4-STOCKPILE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/17/2023
Supervised By :Ankita Jodhani 01/17/2023

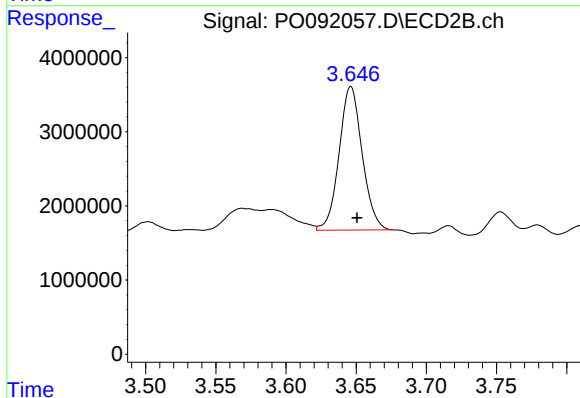


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: -0.005 min
Response: 22136959
Conc: 15.94 ng/ml m

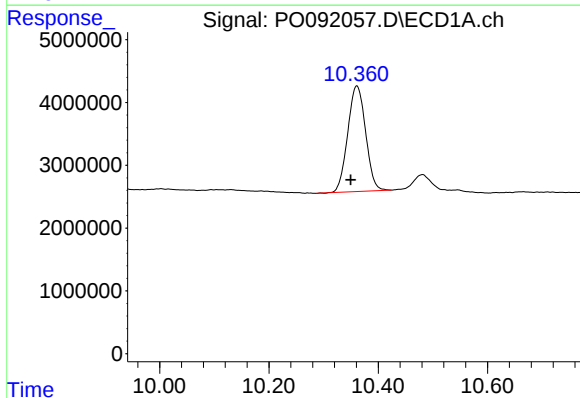

#2 Decachlorobiphenyl

R.T.: 10.361 min
Delta R.T.: 0.012 min
Response: 38144182
Conc: 19.48 ng/ml

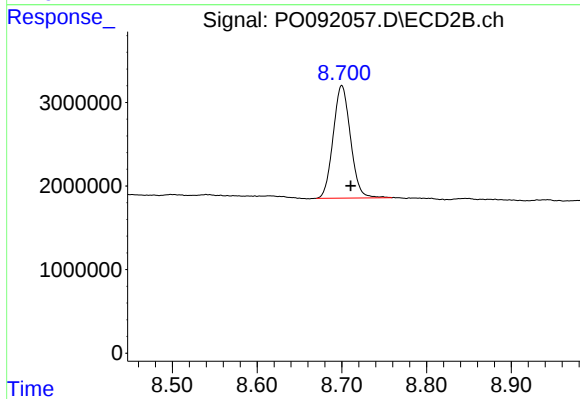

#2 Decachlorobiphenyl

R.T.: 8.700 min
Delta R.T.: -0.010 min
Response: 19150741
Conc: 21.60 ng/ml