

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011623\
 Data File : P0092067.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jan 2023 00:14
 Operator : YP/AJ
 Sample : 01142-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-011023-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/17/2023
 Supervised By :Ankita Jodhani 01/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 02:52:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 11 04:41:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.445	3.647	84330879	29132858	30.235m	20.984 #
2) SA Decachlor...	10.363	8.700	49952461	24249876	25.516	27.349

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011623\
Data File : PO092067.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jan 2023 00:14
Operator : YP/AJ
Sample : 01142-01
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PCB-011023-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/17/2023
Supervised By :Ankita Jodhani 01/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 02:52:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 11 04:41:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

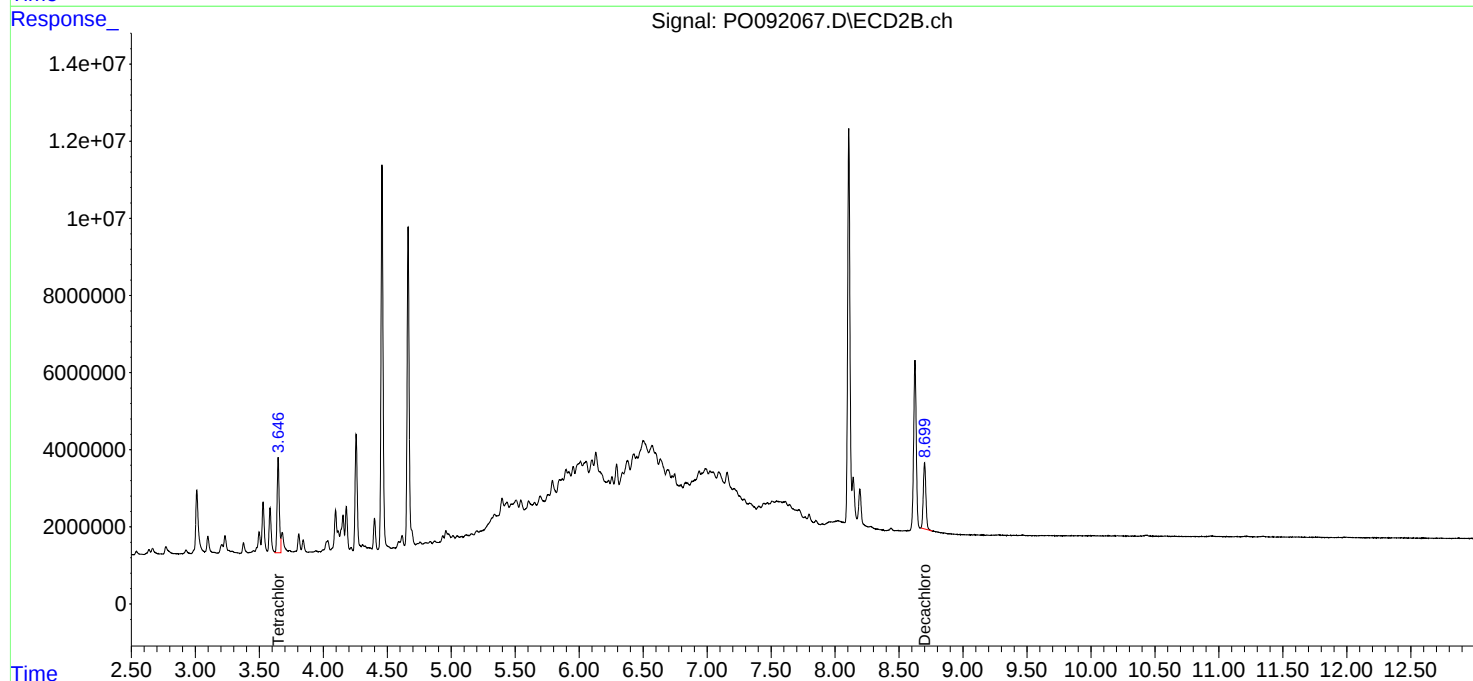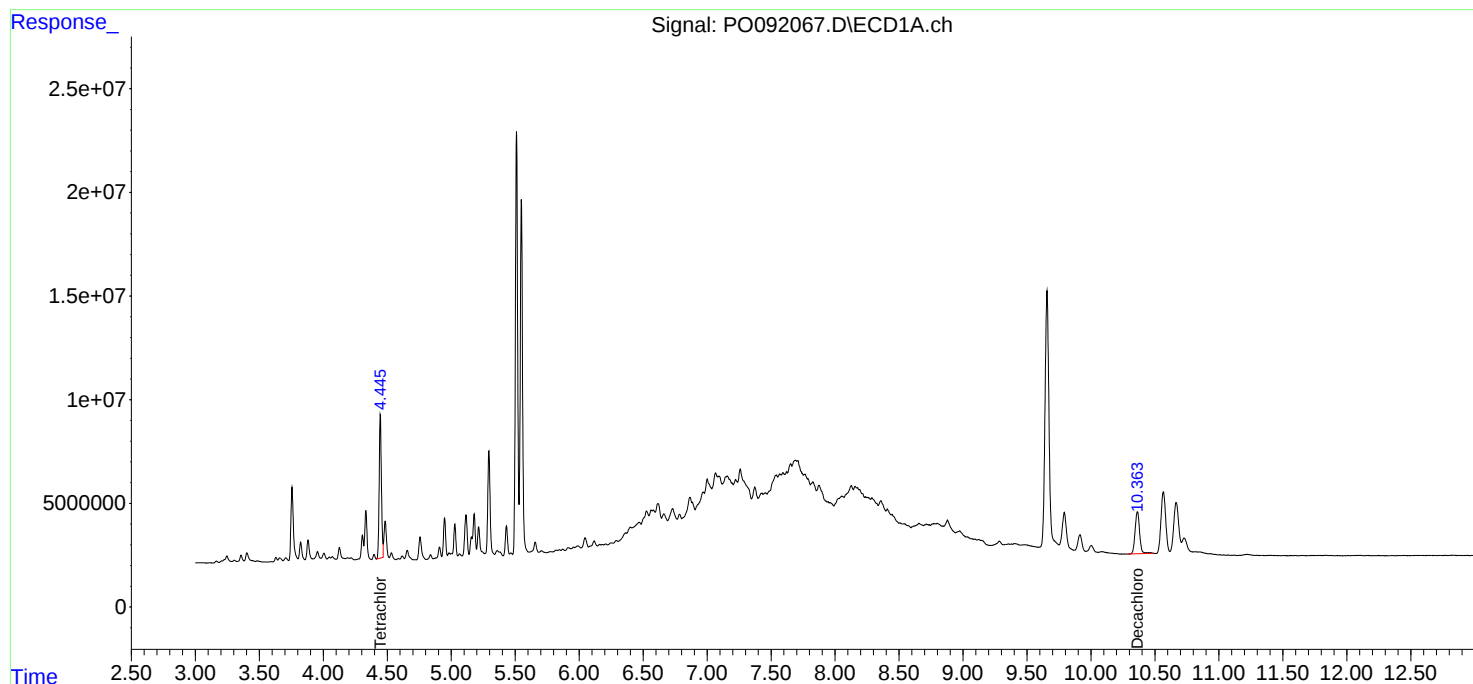

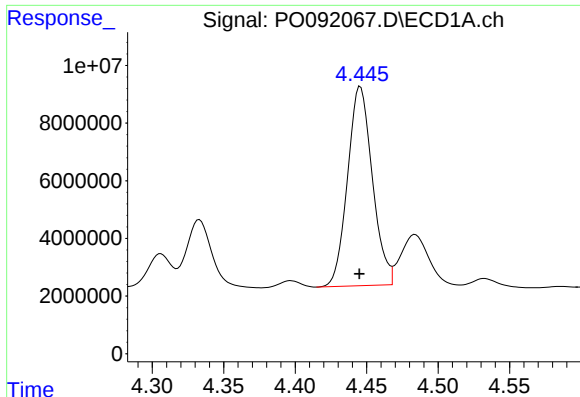


#1 Tetrachloro-m-xylene

R.T.: 4.445 min
Delta R.T.: 0.000 min
Response: 84330879
Conc: 30.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-011023-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/17/2023
Supervised By :Ankita Jodhani 01/17/2023

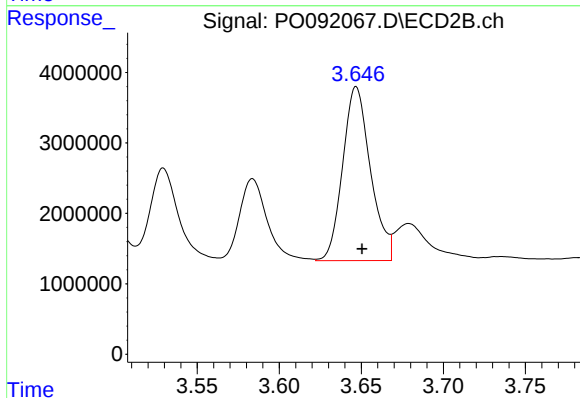


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: -0.004 min
Response: 29132858
Conc: 20.98 ng/ml

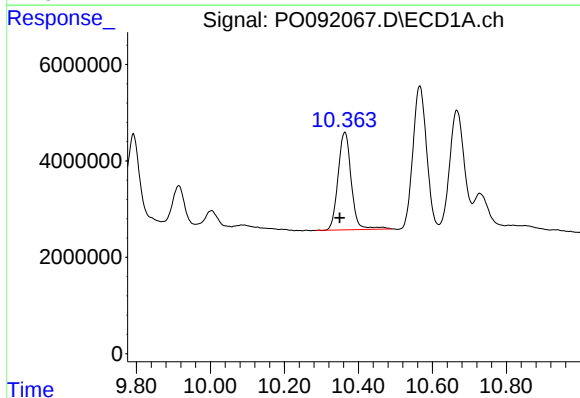

#2 Decachlorobiphenyl

R.T.: 10.363 min
Delta R.T.: 0.014 min
Response: 49952461
Conc: 25.52 ng/ml

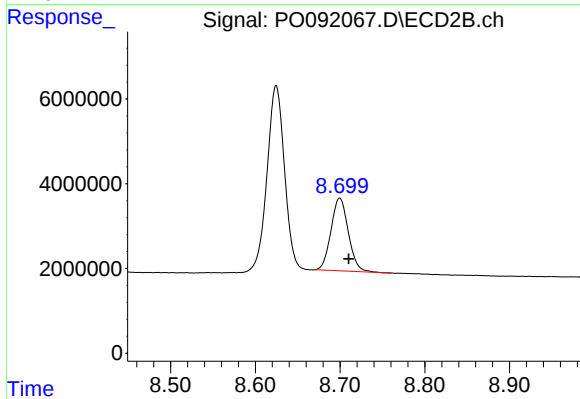

#2 Decachlorobiphenyl

R.T.: 8.700 min
Delta R.T.: -0.011 min
Response: 24249876
Conc: 27.35 ng/ml