

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011719\
 Data File : P0053482.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jan 2019 17:31
 Operator : SM/SJ
 Sample : K1164-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 011519-BLST-E-D-B

Manual Integrations
 APPROVED

Sohil
 1/18/2019 9:08:53 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 23:50:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 09 03:34:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.153	3.197	24268548	4466335	18.162m	17.862m
2) SA Decachlor...	9.596	7.834	14997614	4407020	18.988	19.244

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011719\
Data File : P0053482.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jan 2019 17:31
Operator : SM/SJ
Sample : K1164-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
011519-BLST-E-D-B


Manual Integrations
APPROVED

Sohil
1/18/2019 9:08:53 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 23:50:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010819.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 09 03:34:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

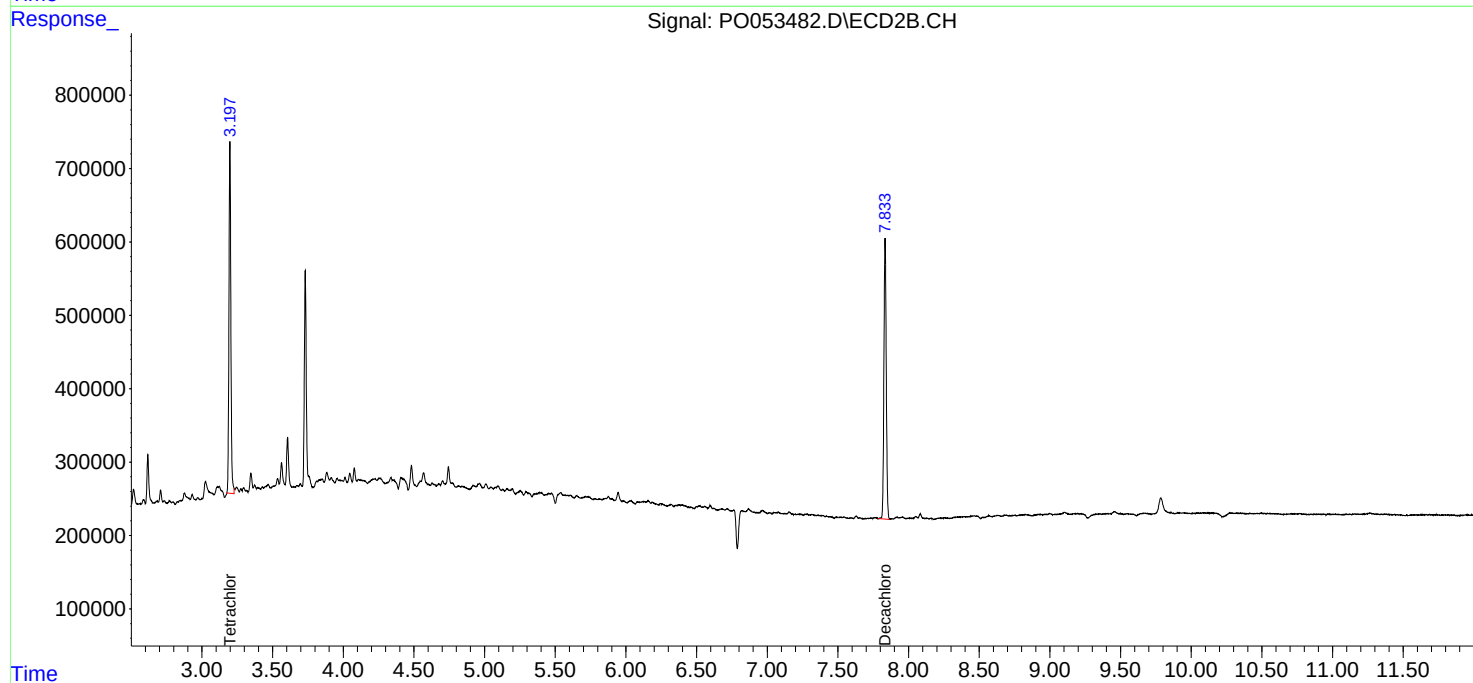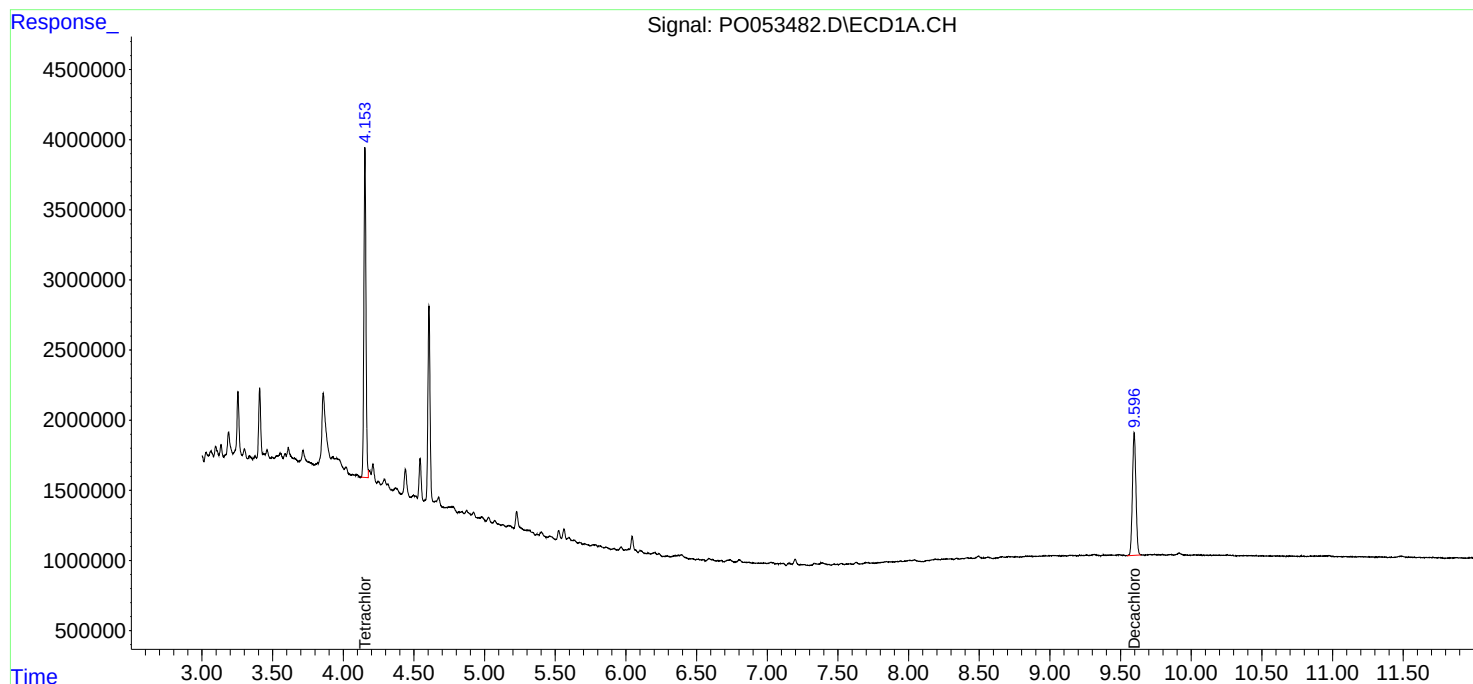

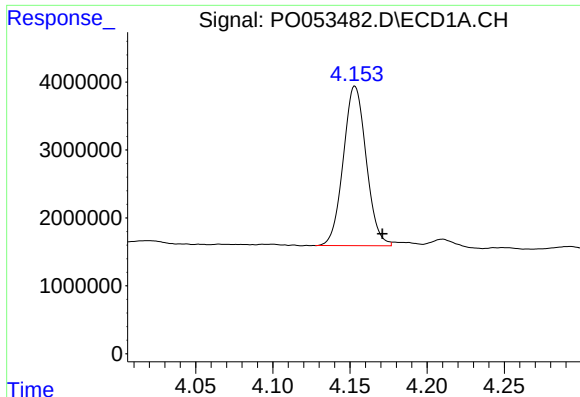


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: -0.018 min
Response: 24268548
Conc: 18.16 ng/ml m

Instrument :
ECD_O
ClientSampleId :
011519-BLST-E-D-B


Manual Integrations
APPROVED

Sohil
1/18/2019 9:08:53 AM

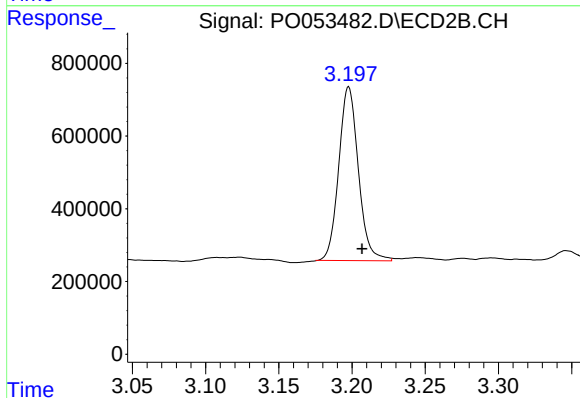


#1 Tetrachloro-m-xylene

R.T.: 3.197 min
Delta R.T.: -0.010 min
Response: 4466335
Conc: 17.86 ng/ml m

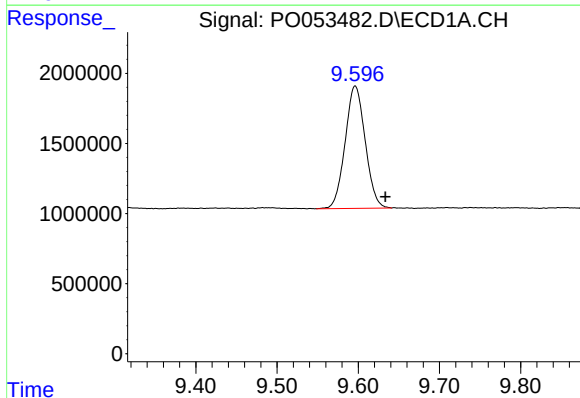

#2 Decachlorobiphenyl

R.T.: 9.596 min
Delta R.T.: -0.037 min
Response: 14997614
Conc: 18.99 ng/ml

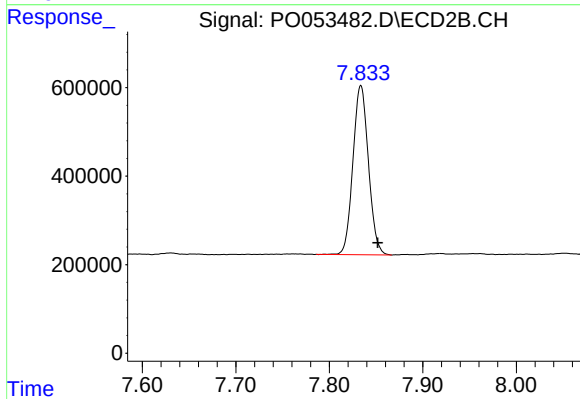

#2 Decachlorobiphenyl

R.T.: 7.834 min
Delta R.T.: -0.018 min
Response: 4407020
Conc: 19.24 ng/ml