

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011722\
 Data File : P0084275.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jan 2022 16:56
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 04:00:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 18 03:56:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	6.527	5.311	1494808	447168	19.885	20.042
2) SA Decachlor...	13.792	11.328	919501	368955	20.435	20.958
Target Compounds						
30) L6 AR-1254-5	10.405	9.058	30240	1637	9.126	1.121 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011722\
Data File : P0084275.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jan 2022 16:56
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 04:00:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 18 03:56:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

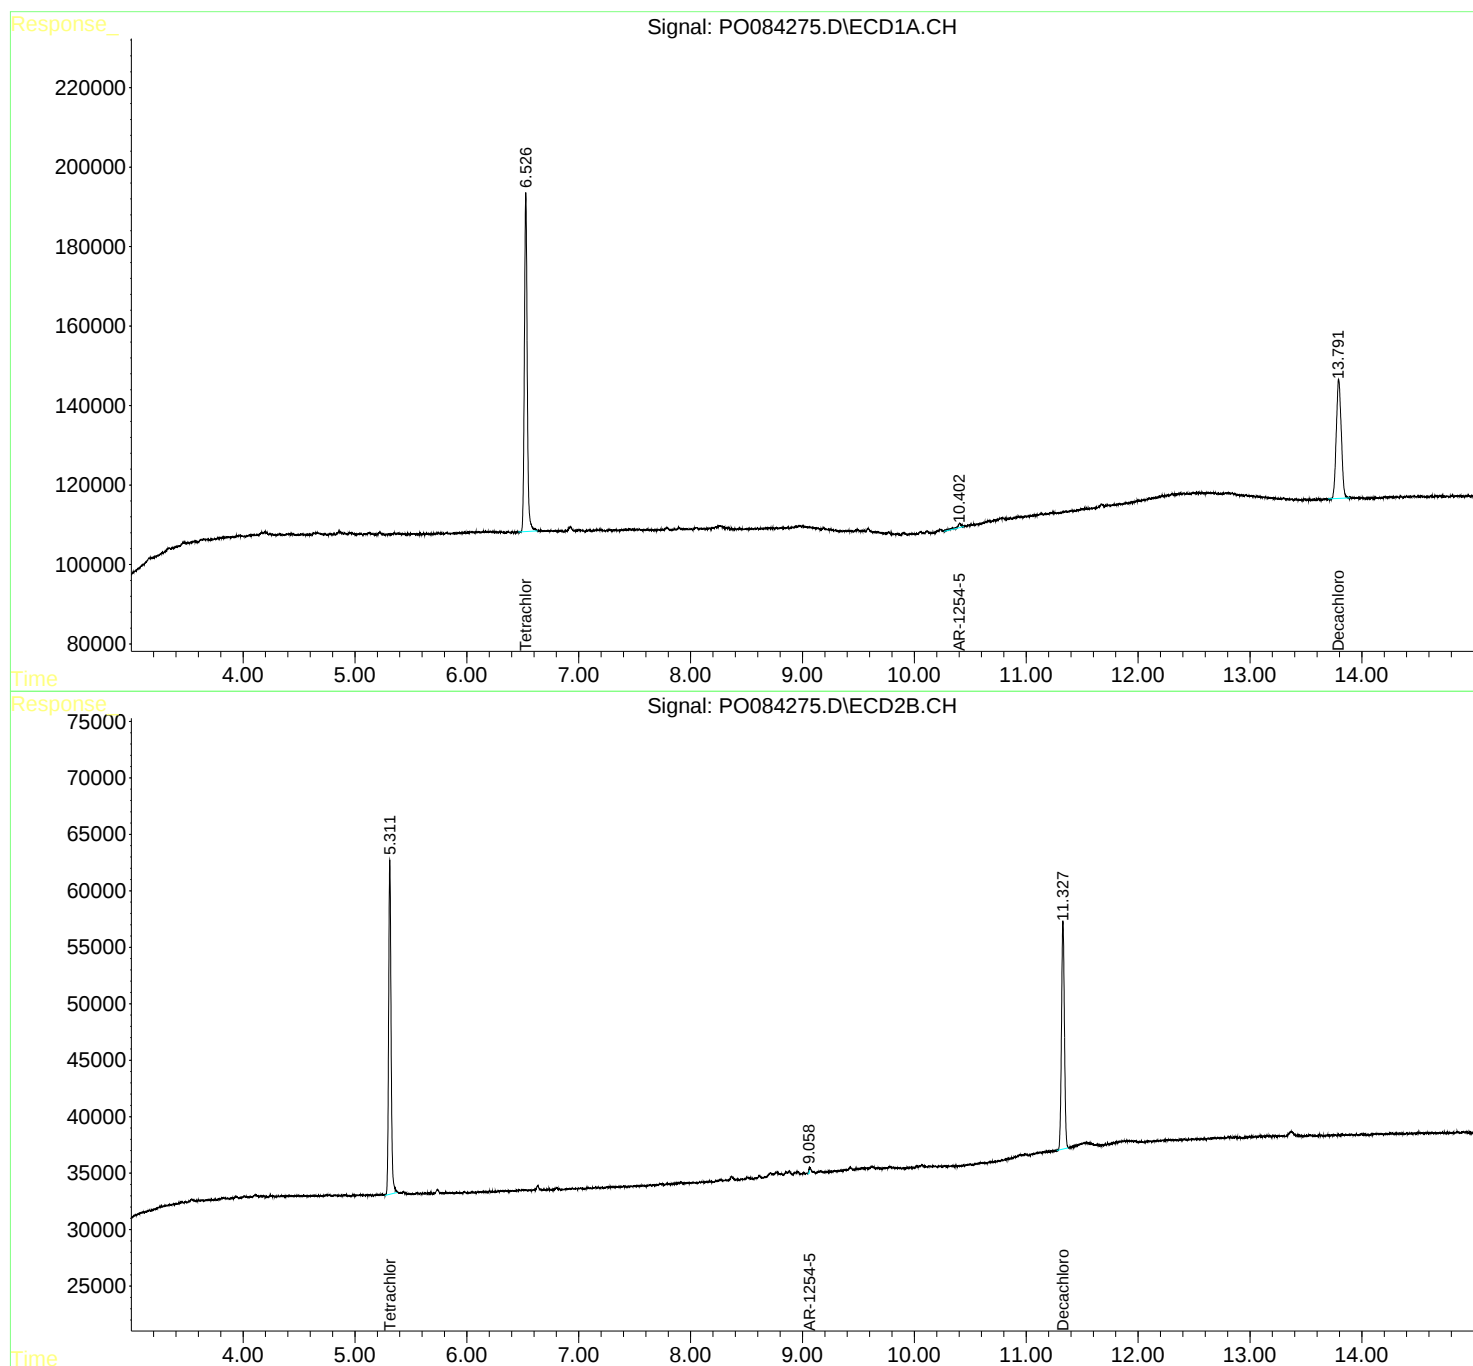


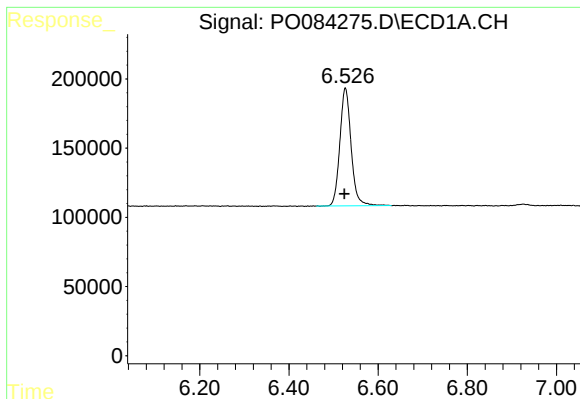

#1 Tetrachloro-m-xylene


R.T.: 6.527 min
Delta R.T.: 0.003 min
Response: 1494808
Conc: 19.88 ng/ml

Instrument :
ECD_O
ClientSampleId :

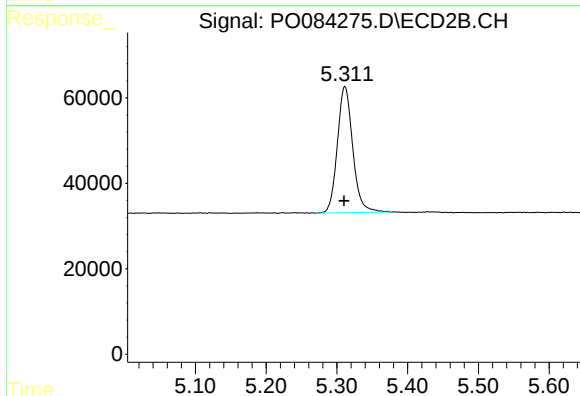


#1 Tetrachloro-m-xylene

R.T.: 5.311 min
Delta R.T.: 0.001 min
Response: 447168
Conc: 20.04 ng/ml

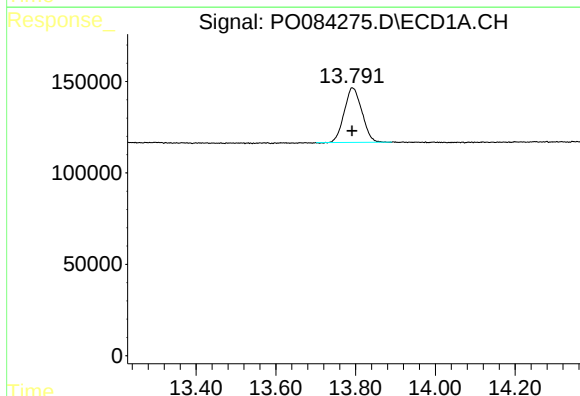


#2 Decachlorobiphenyl

R.T.: 13.792 min
Delta R.T.: 0.000 min
Response: 919501
Conc: 20.44 ng/ml

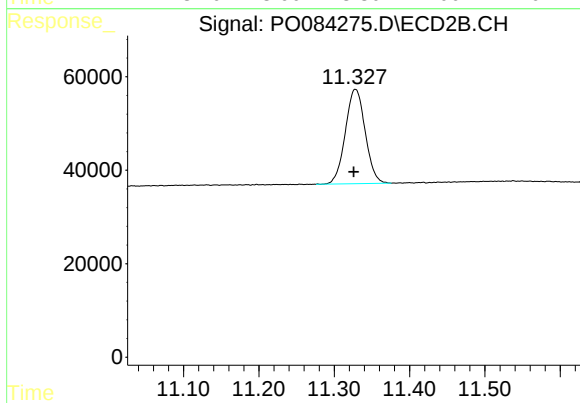

#2 Decachlorobiphenyl


R.T.: 11.328 min
Delta R.T.: 0.002 min
Response: 368955
Conc: 20.96 ng/ml

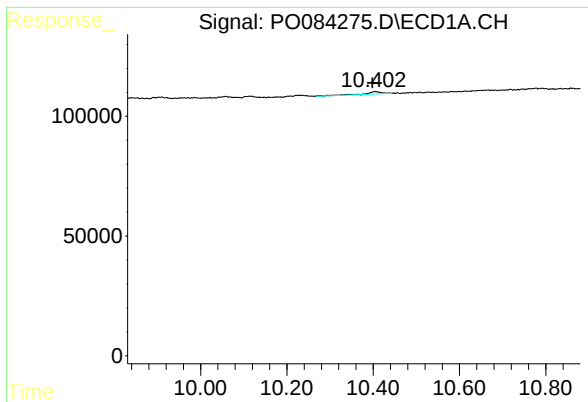

#30 AR-1254-5

R.T.: 10.405 min
Delta R.T.: 0.007 min
Response: 30240
Conc: 9.13 ng/ml

Instrument :
ECD_O
ClientSampleId :

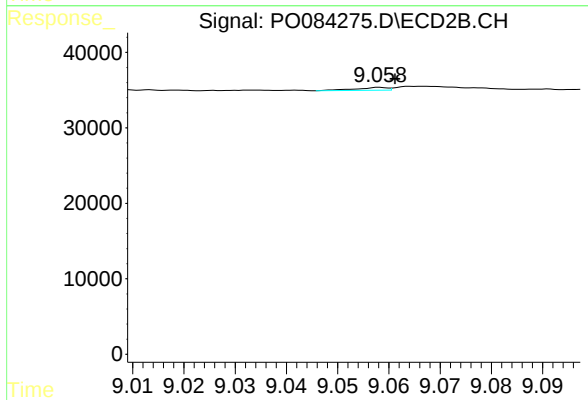

#30 AR-1254-5

R.T.: 9.058 min
Delta R.T.: -0.003 min
Response: 1637
Conc: 1.12 ng/ml