

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011821\
 Data File : P0074881.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jan 2021 17:36
 Operator : AJ/MA
 Sample : M1086-06DL 5X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S3-03-CDL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 01:02:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.931	4.003	385425	221263	3.653	3.933
2) SA Decachlor...	10.950	9.255	284056	230027	2.799	4.190 #
Target Compounds						
26) L6 AR-1254-1	7.167	6.113	1372478	964660	312.059	267.070
27) L6 AR-1254-2	7.397	6.271	2717565	1256257	399.010	403.094
28) L6 AR-1254-3	7.780	6.688	3845839	2580358	548.283	526.183
29) L6 AR-1254-4	8.077	6.926	4201618	2123342	692.802	612.306
30) L6 AR-1254-5	8.507	7.352	8191438	6537147	1410.144	1444.373



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011821\
Data File : PO074881.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jan 2021 17:36
Operator : AJ/MA
Sample : M1086-06DL 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S3-03-CDL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 01:02:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

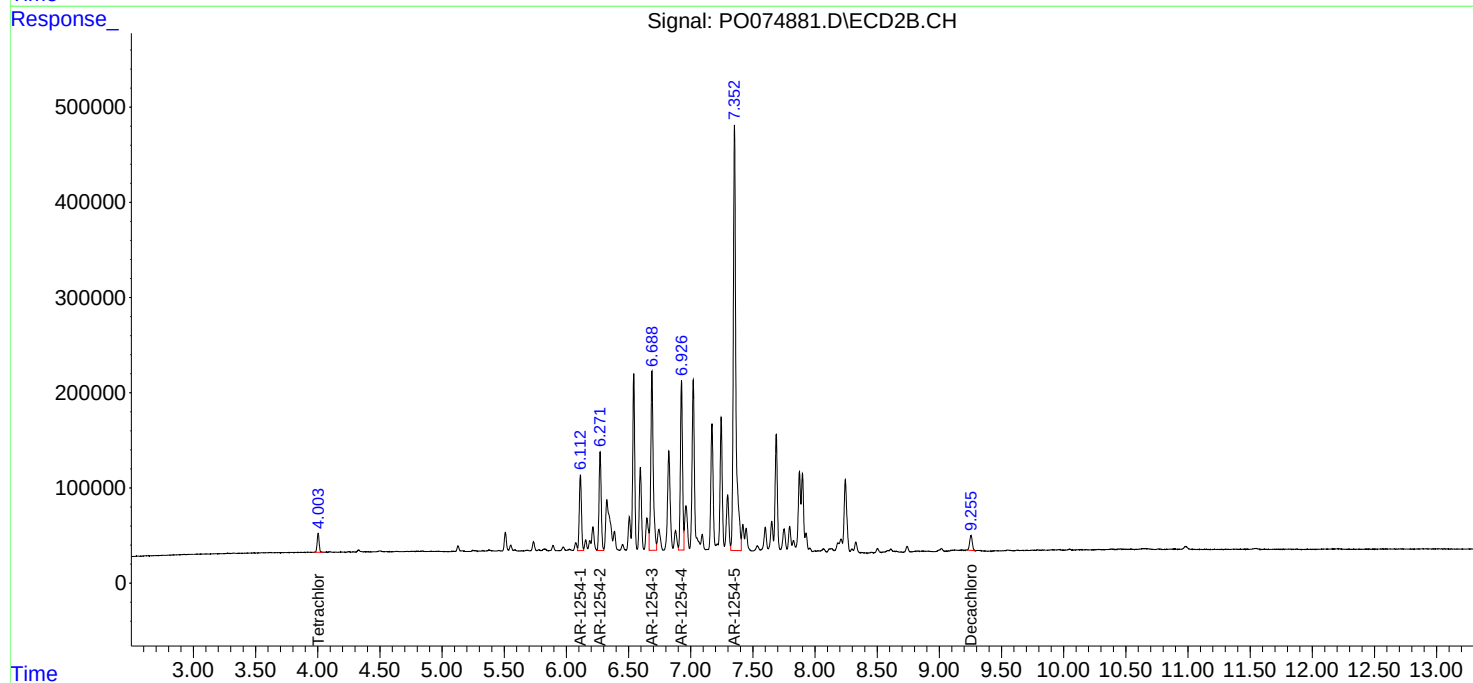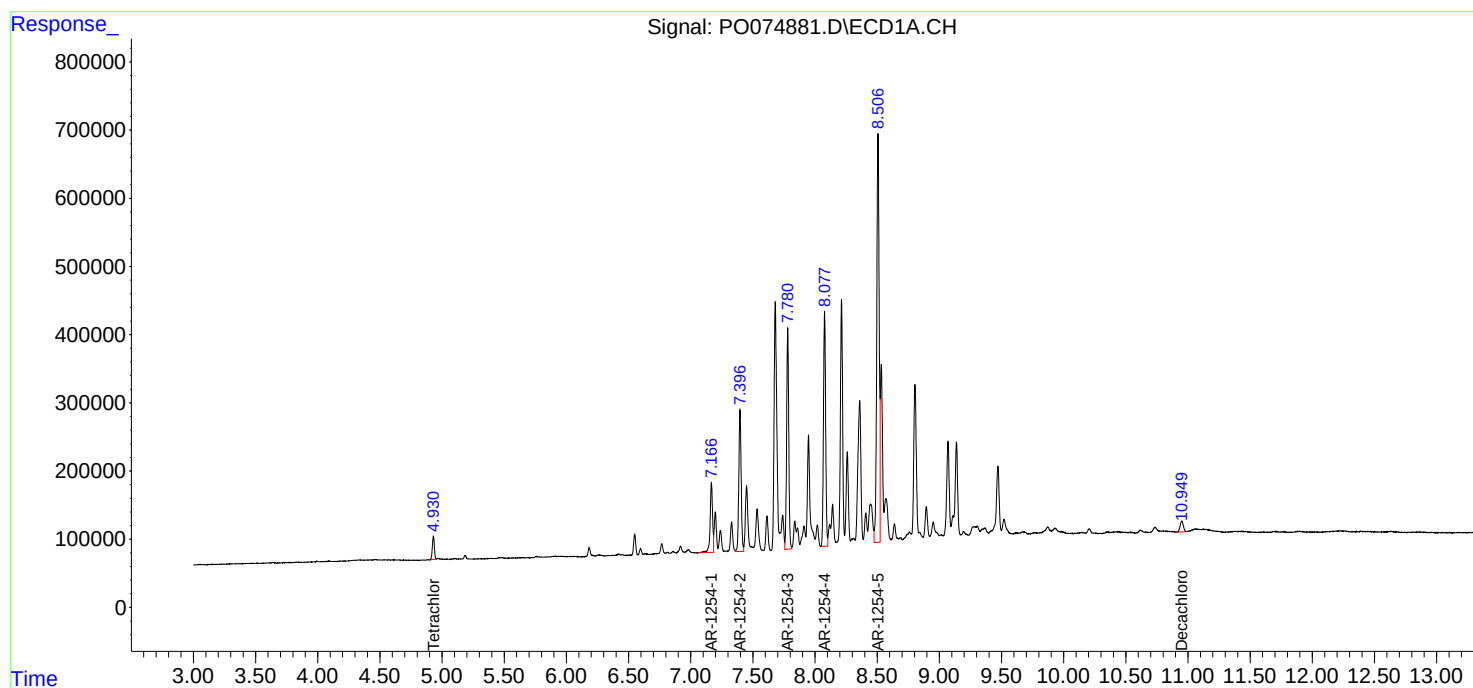


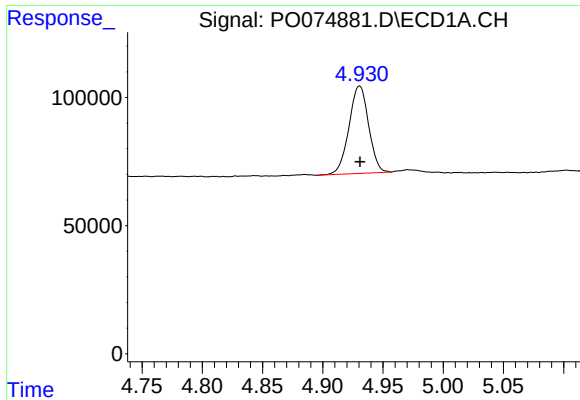

#1 Tetrachloro-m-xylene


R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 385425
Conc: 3.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-03-CDL

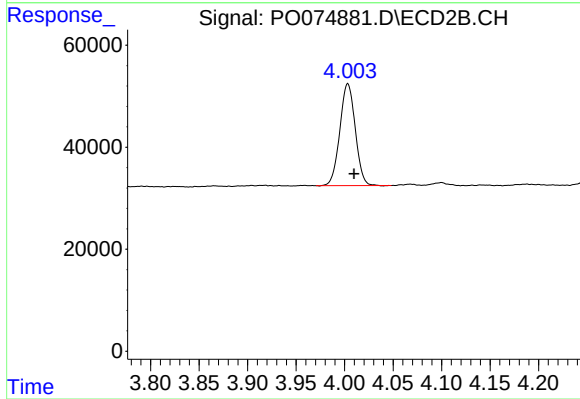


#1 Tetrachloro-m-xylene

R.T.: 4.003 min
Delta R.T.: -0.006 min
Response: 221263
Conc: 3.93 ng/ml

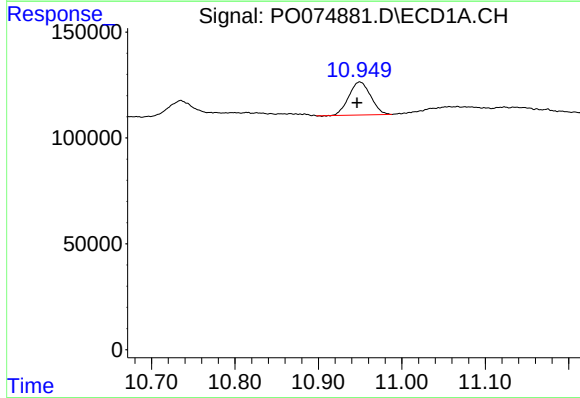


#2 Decachlorobiphenyl

R.T.: 10.950 min
Delta R.T.: 0.003 min
Response: 284056
Conc: 2.80 ng/ml

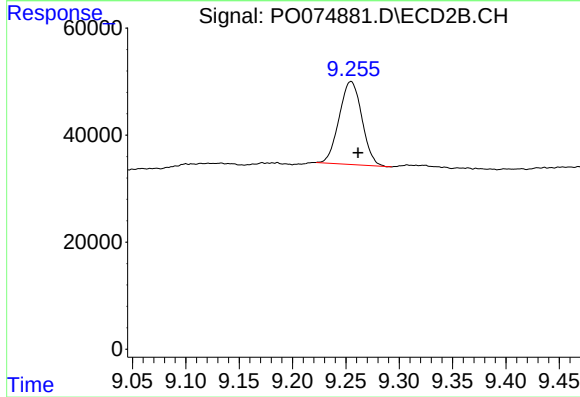

#2 Decachlorobiphenyl


R.T.: 9.255 min
Delta R.T.: -0.007 min
Response: 230027
Conc: 4.19 ng/ml

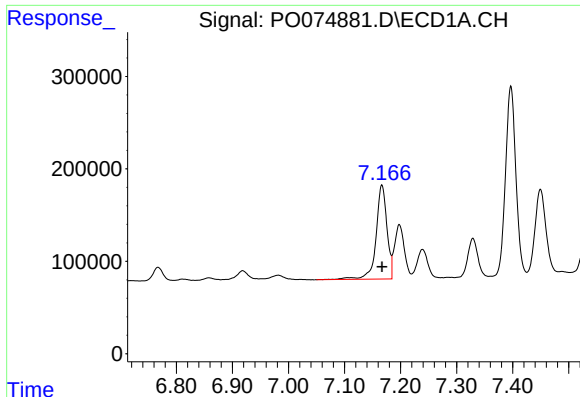

#26 AR-1254-1


R.T.: 7.167 min
Delta R.T.: 0.000 min
Response: 1372478
Conc: 312.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-03-CDL

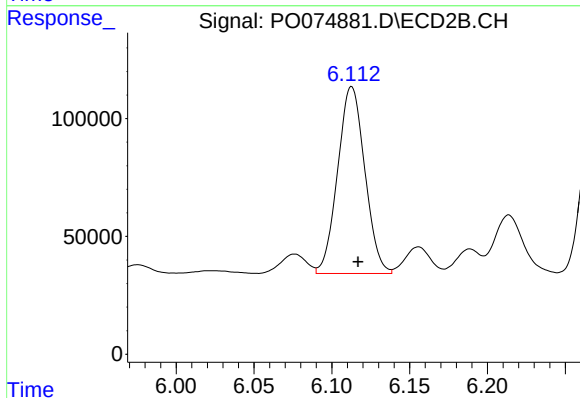


#26 AR-1254-1

R.T.: 6.113 min
Delta R.T.: -0.004 min
Response: 964660
Conc: 267.07 ng/ml

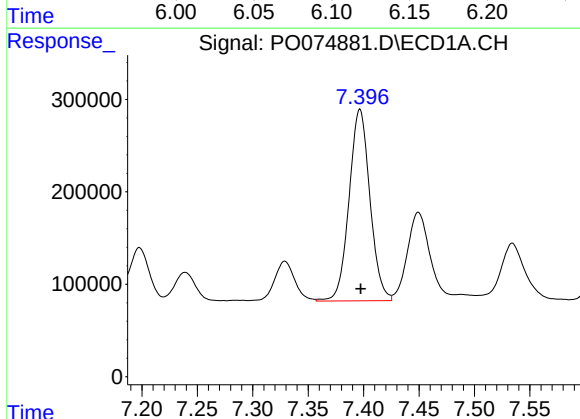


#27 AR-1254-2

R.T.: 7.397 min
Delta R.T.: 0.000 min
Response: 2717565
Conc: 399.01 ng/ml

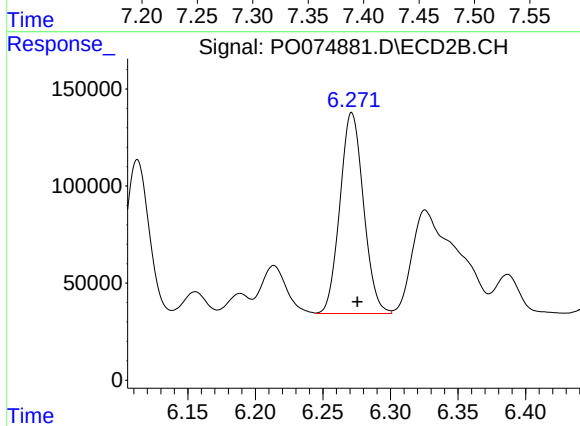

#27 AR-1254-2


R.T.: 6.271 min
Delta R.T.: -0.004 min
Response: 1256257
Conc: 403.09 ng/ml

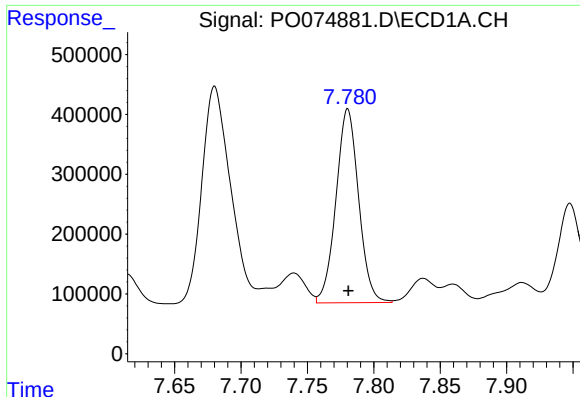

#28 AR-1254-3


R.T.: 7.780 min
Delta R.T.: 0.000 min
Response: 3845839
Conc: 548.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-03-CDL

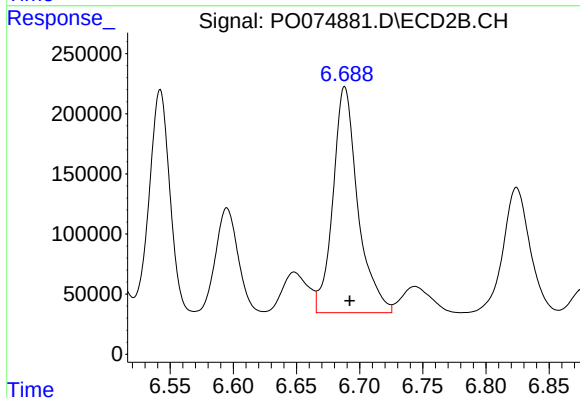


#28 AR-1254-3

R.T.: 6.688 min
Delta R.T.: -0.004 min
Response: 2580358
Conc: 526.18 ng/ml

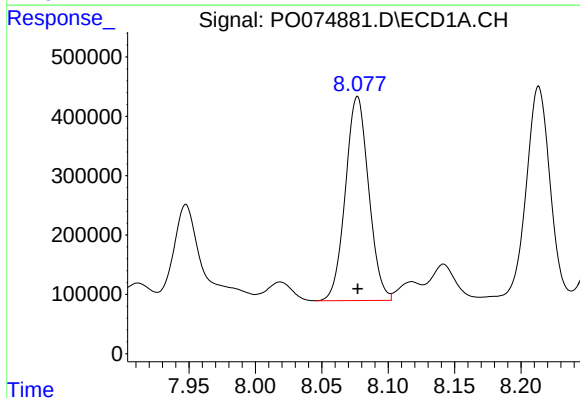


#29 AR-1254-4

R.T.: 8.077 min
Delta R.T.: 0.000 min
Response: 4201618
Conc: 692.80 ng/ml

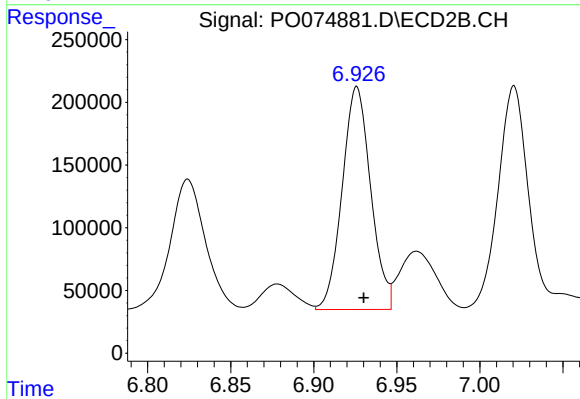

#29 AR-1254-4


R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 2123342
Conc: 612.31 ng/ml

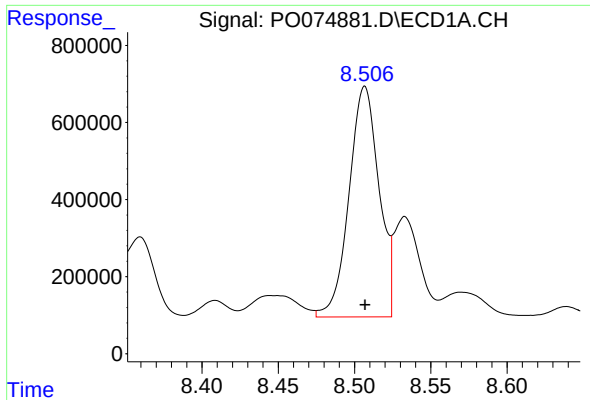

#30 AR-1254-5

R.T.: 8.507 min
Delta R.T.: 0.000 min
Response: 8191438
Conc: 1410.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-03-CDL

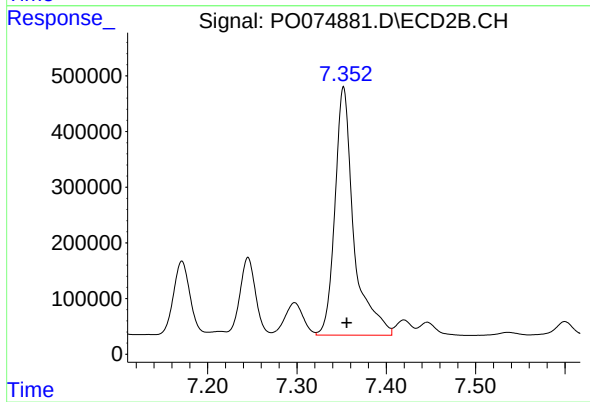

#30 AR-1254-5

R.T.: 7.352 min
Delta R.T.: -0.004 min
Response: 6537147
Conc: 1444.37 ng/ml