

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011821\
 Data File : P0074886.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jan 2021 19:01
 Operator : AJ/MA
 Sample : M1084-07DL 2X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S1-01-CDL

Manual Integrations
 APPROVED

Ankita
 1/19/2021 10:05:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 01:05:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.928	4.001	984097	618248	9.326m	10.991
2) SA Decachlor...	10.944	9.255	560221	317737	5.520	5.787
Target Compounds						
26) L6 AR-1254-1	7.165	6.111	1131436	838292	257.253	232.085
27) L6 AR-1254-2	7.395	6.270	2168777	1014424	318.433	325.497
28) L6 AR-1254-3	7.779	6.686	2813047	1899981	401.043	387.441
29) L6 AR-1254-4	8.075	6.924	3012060	1553325	496.657	447.931
30) L6 AR-1254-5	8.505	7.350	4554719	6901651	784.088	1524.910 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011821\
Data File : PO074886.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jan 2021 19:01
Operator : AJ/MA
Sample : M1084-07DL 2X
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S1-01-CDL


Manual Integrations
APPROVED

Ankita
1/19/2021 10:05:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 01:05:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

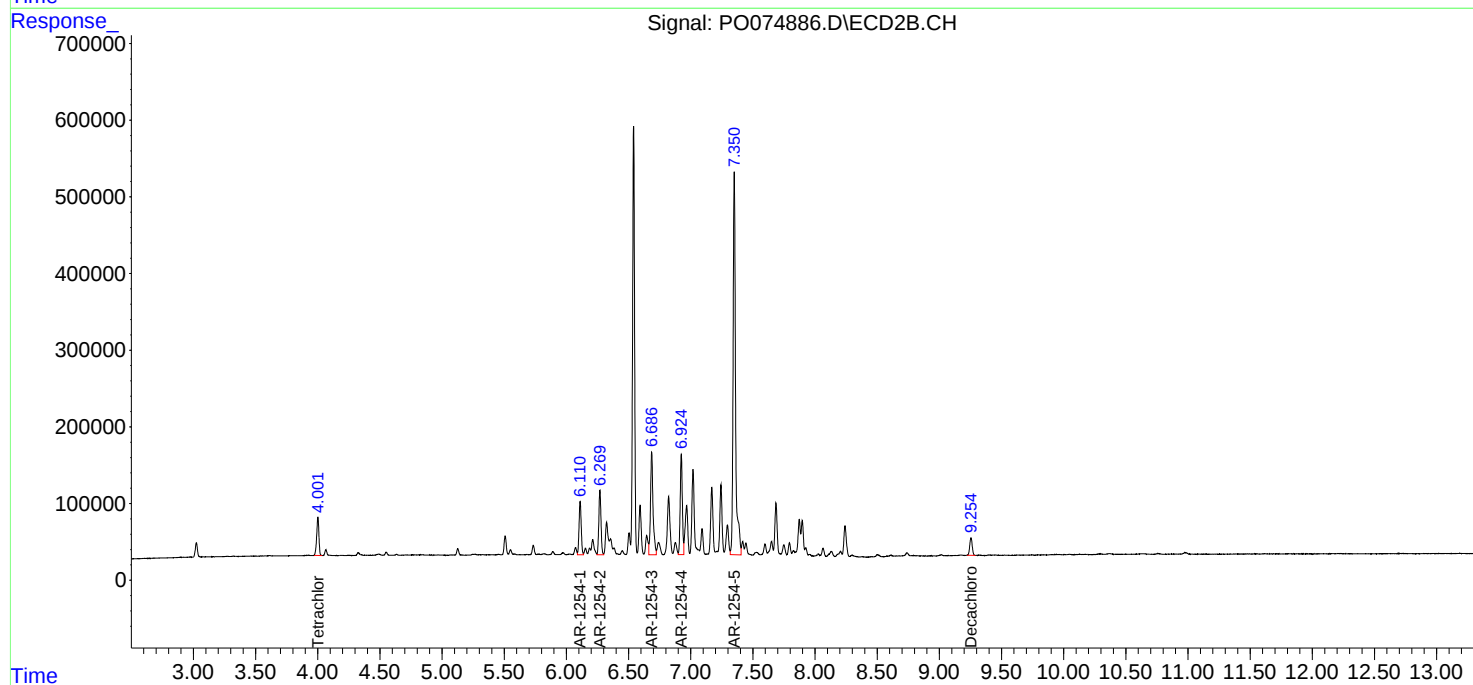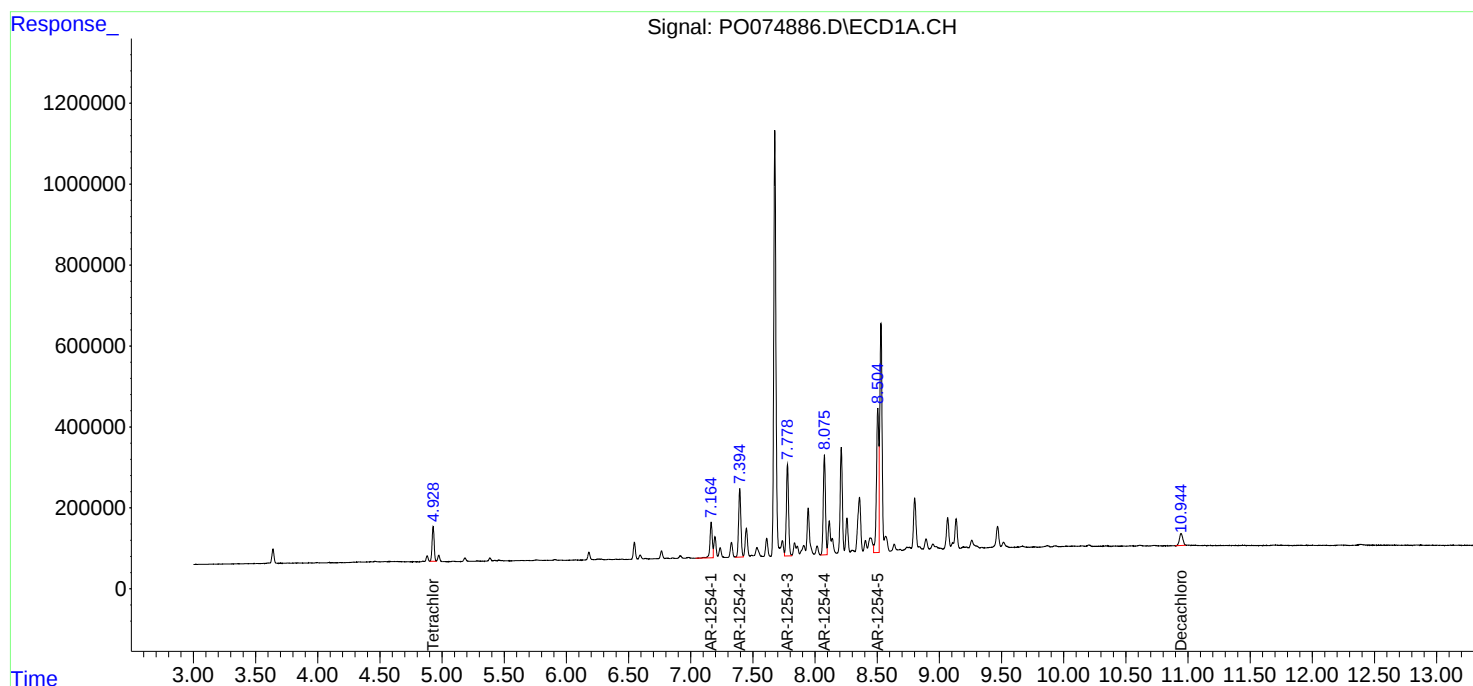

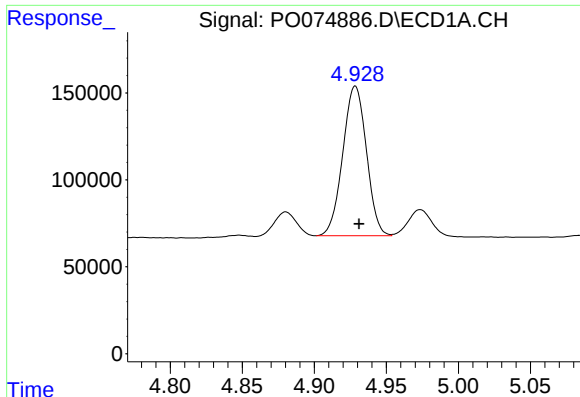


#1 Tetrachloro-m-xylene

R.T.: 4.928 min
Delta R.T.: -0.003 min
Response: 984097
Conc: 9.33 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S1-01-CDL


Manual Integrations
APPROVED

Ankita
1/19/2021 10:05:48 AM

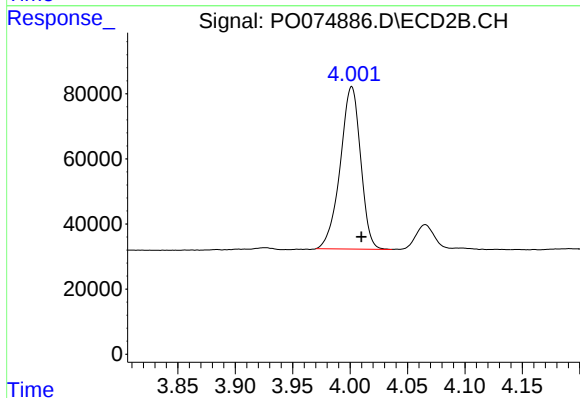


#1 Tetrachloro-m-xylene

R.T.: 4.001 min
Delta R.T.: -0.008 min
Response: 618248
Conc: 10.99 ng/ml

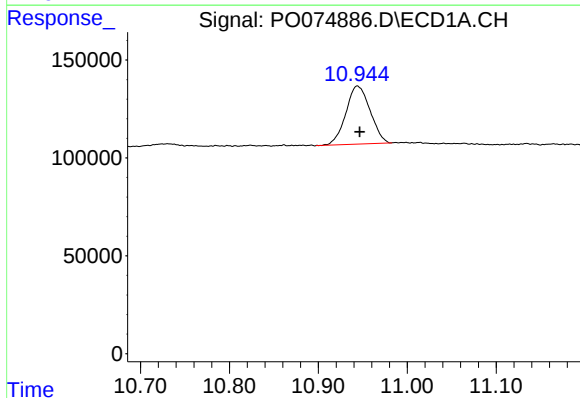


#2 Decachlorobiphenyl

R.T.: 10.944 min
Delta R.T.: -0.002 min
Response: 560221
Conc: 5.52 ng/ml

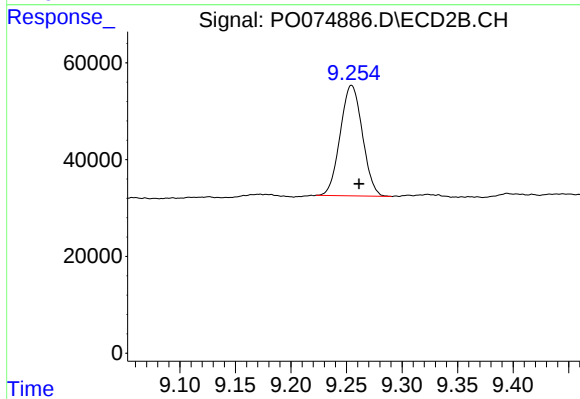

#2 Decachlorobiphenyl

R.T.: 9.255 min
Delta R.T.: -0.007 min
Response: 317737
Conc: 5.79 ng/ml

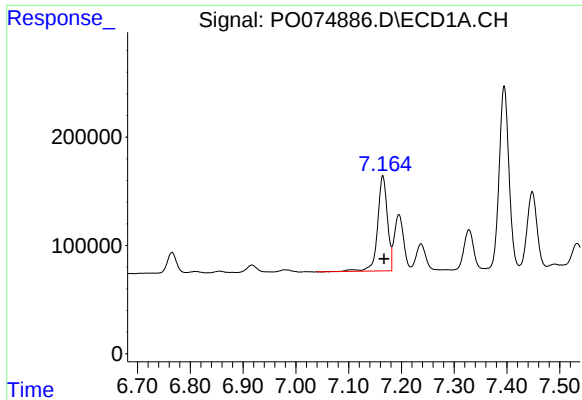


#26 AR-1254-1

R.T.: 7.165 min
Delta R.T.: -0.002 min
Response: 1131436
Conc: 257.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-01-CDL


Manual Integrations
APPROVED

Ankita
1/19/2021 10:05:48 AM

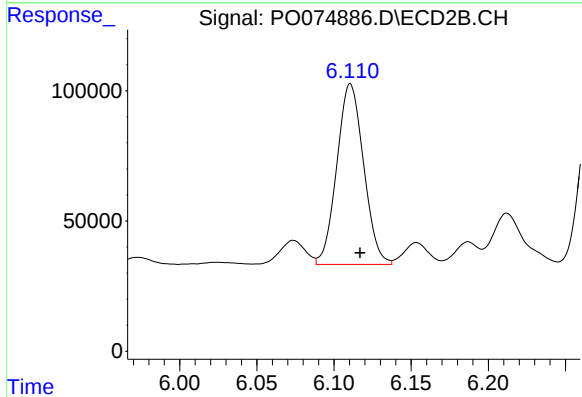


#26 AR-1254-1

R.T.: 6.111 min
Delta R.T.: -0.006 min
Response: 838292
Conc: 232.08 ng/ml

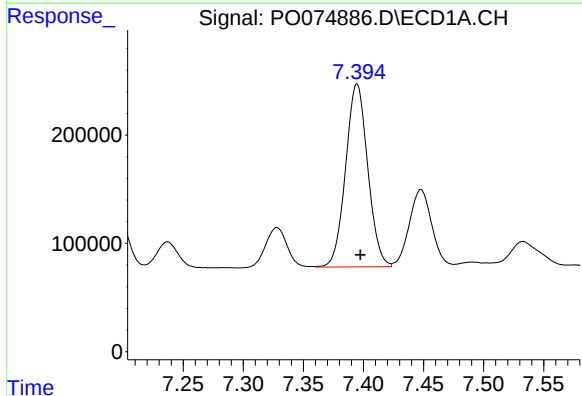


#27 AR-1254-2

R.T.: 7.395 min
Delta R.T.: -0.003 min
Response: 2168777
Conc: 318.43 ng/ml

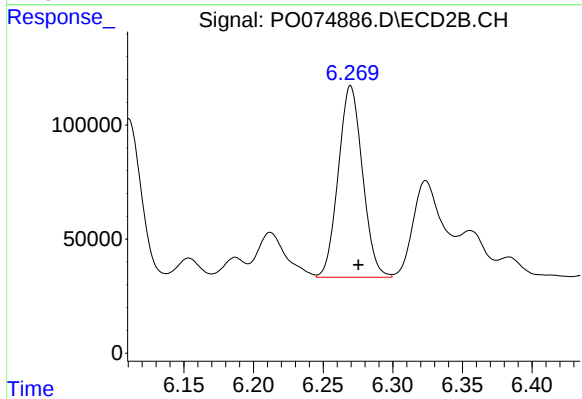

#27 AR-1254-2

R.T.: 6.270 min
Delta R.T.: -0.006 min
Response: 1014424
Conc: 325.50 ng/ml

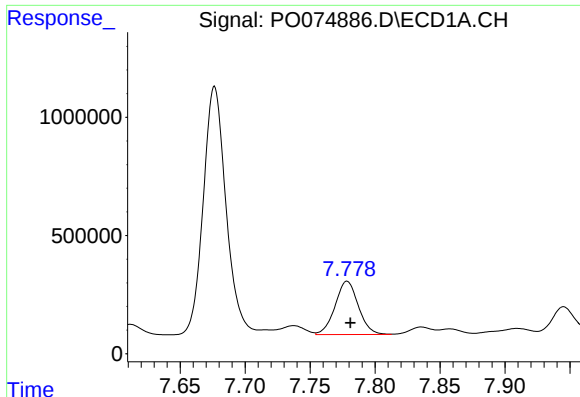


#28 AR-1254-3

R.T.: 7.779 min
Delta R.T.: -0.002 min
Response: 2813047
Conc: 401.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-01-CDL


Manual Integrations
APPROVED

Ankita
1/19/2021 10:05:48 AM

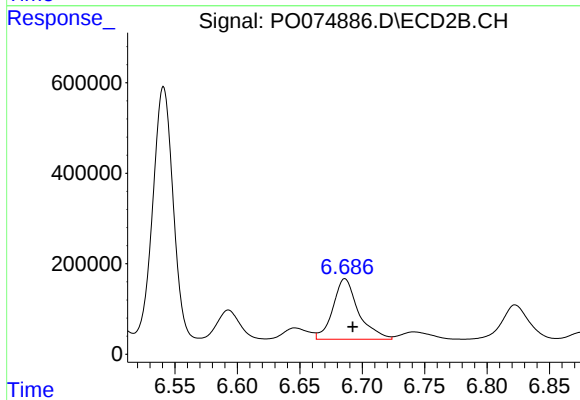


#28 AR-1254-3

R.T.: 6.686 min
Delta R.T.: -0.006 min
Response: 1899981
Conc: 387.44 ng/ml

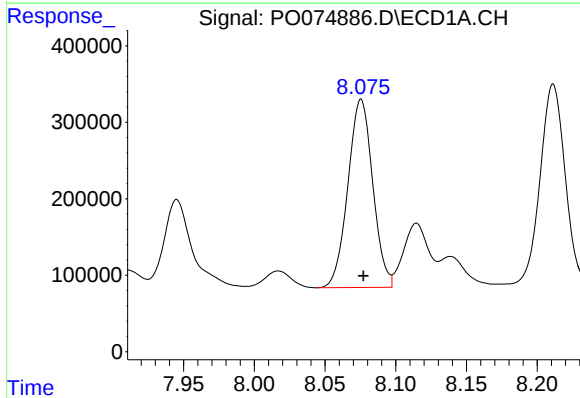


#29 AR-1254-4

R.T.: 8.075 min
Delta R.T.: -0.002 min
Response: 3012060
Conc: 496.66 ng/ml

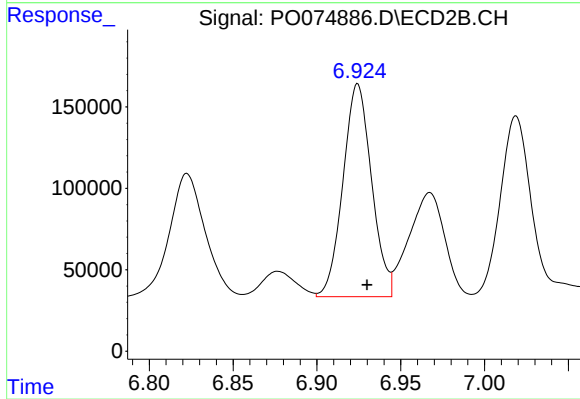

#29 AR-1254-4

R.T.: 6.924 min
Delta R.T.: -0.006 min
Response: 1553325
Conc: 447.93 ng/ml

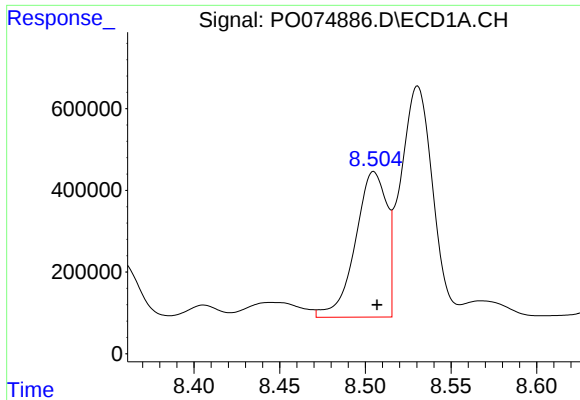


#30 AR-1254-5

R.T.: 8.505 min
Delta R.T.: -0.002 min
Response: 4554719
Conc: 784.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-01-CDL

Manual Integrations
APPROVED

Ankita
1/19/2021 10:05:48 AM

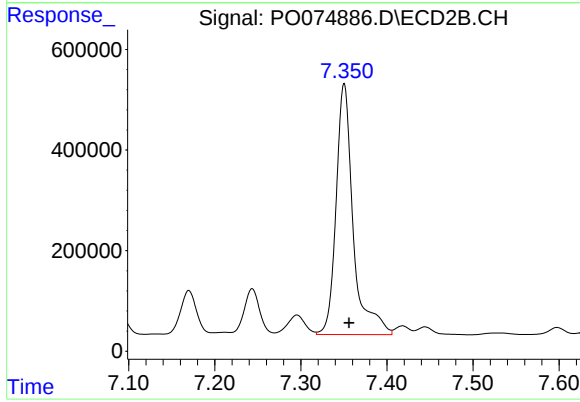

#30 AR-1254-5

R.T.: 7.350 min
Delta R.T.: -0.005 min
Response: 6901651
Conc: 1524.91 ng/ml