

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011821\
 Data File : P0074887.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jan 2021 19:18
 Operator : AJ/MA
 Sample : M1084-08DL 5X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S1-02-CDL

Manual Integrations
 APPROVED

Ankita
 1/19/2021 10:05:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 01:05:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.928	4.002	471598	267333	4.469	4.752
2) SA Decachlor...	10.946	9.254	347713	203080	3.426	3.699
Target Compounds						
26) L6 AR-1254-1	7.164	6.111	1398253	1033096	317.919m	286.017
27) L6 AR-1254-2	7.394	6.269	2553135	1176374	374.867	377.462
28) L6 AR-1254-3	7.778	6.686	3015941	2032575	429.969	414.479
29) L6 AR-1254-4	8.075	6.924	2665438	1363311	439.503	393.136
30) L6 AR-1254-5	8.504	7.350	4096943	4281281	705.283	945.943 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011821\
Data File : PO074887.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jan 2021 19:18
Operator : AJ/MA
Sample : M1084-08DL 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S1-02-CDL


Manual Integrations
APPROVED

Ankita
1/19/2021 10:05:50 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 01:05:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

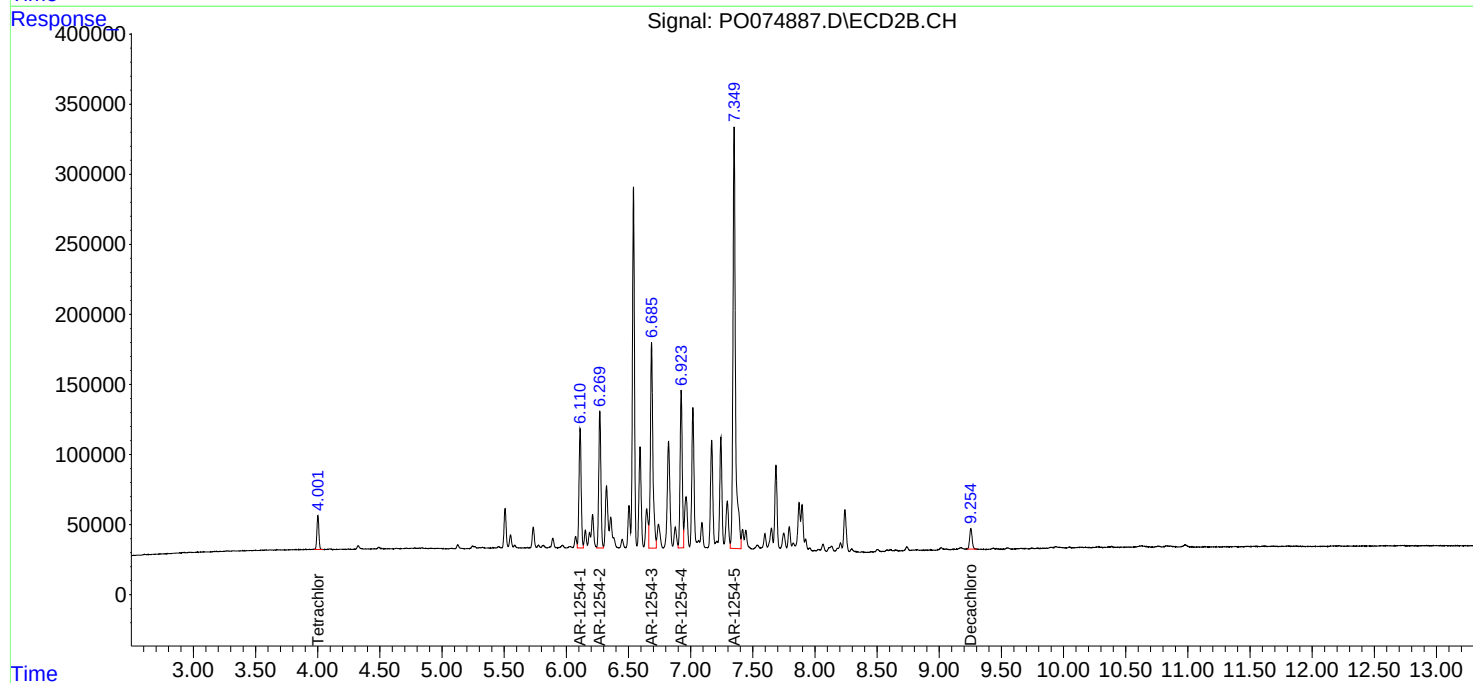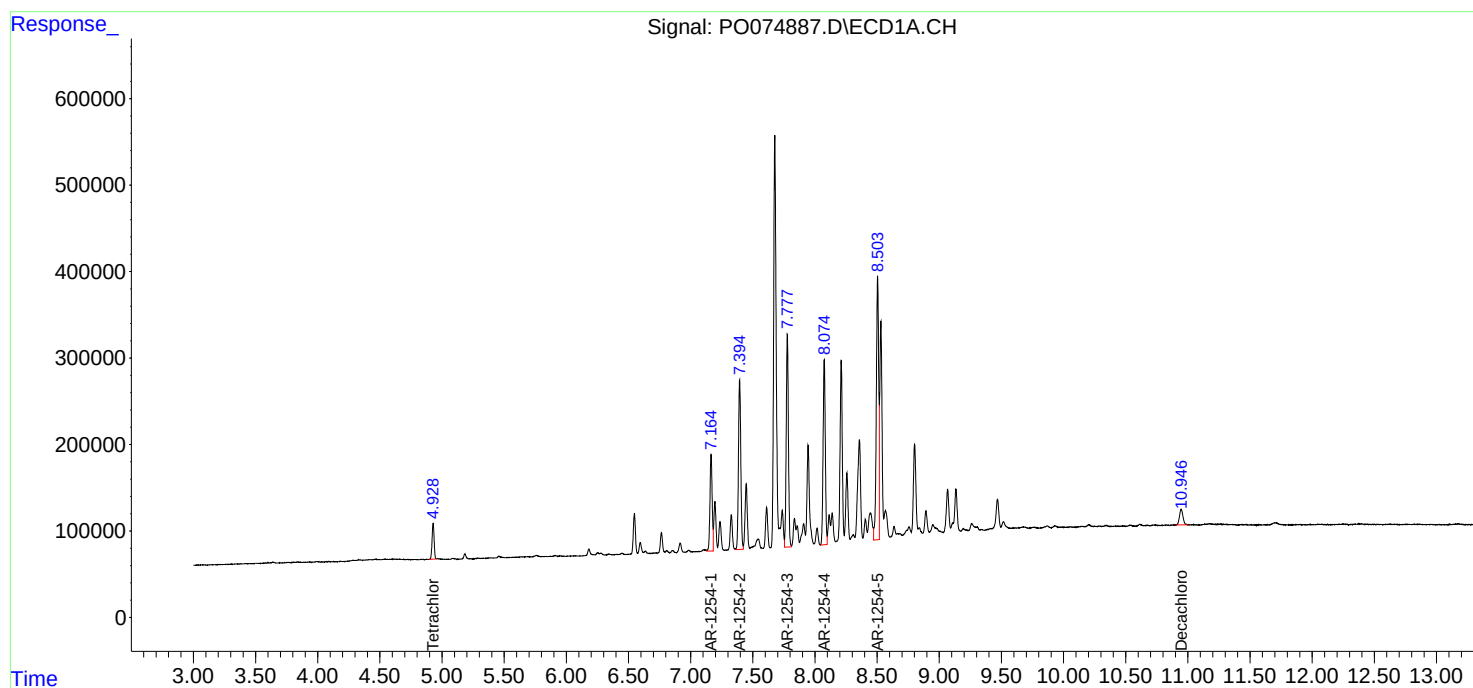

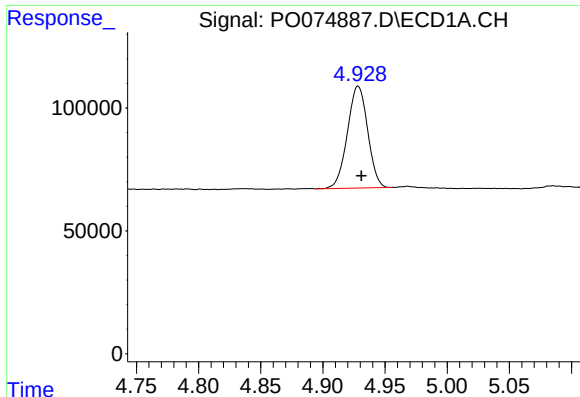


#1 Tetrachloro-m-xylene

R.T.: 4.928 min
Delta R.T.: -0.003 min
Response: 471598
Conc: 4.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-02-CDL


Manual Integrations
APPROVED

Ankita
1/19/2021 10:05:50 AM

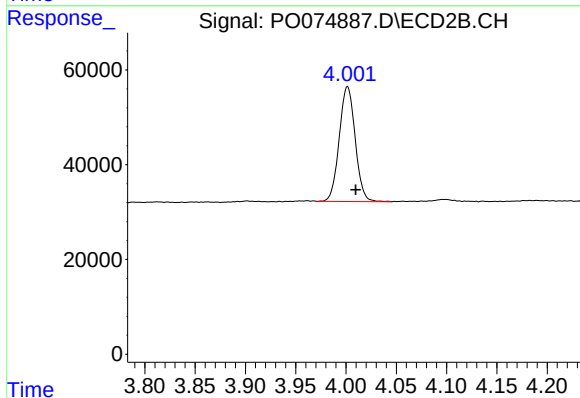


#1 Tetrachloro-m-xylene

R.T.: 4.002 min
Delta R.T.: -0.008 min
Response: 267333
Conc: 4.75 ng/ml

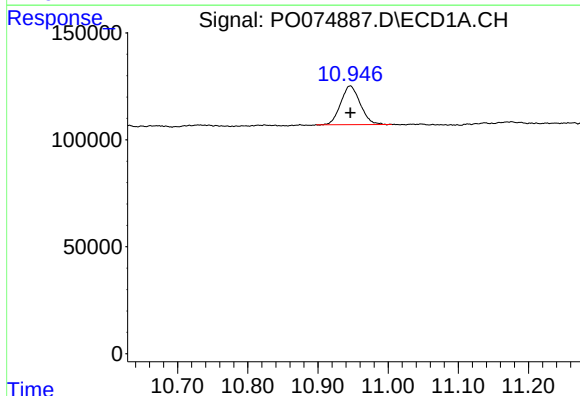


#2 Decachlorobiphenyl

R.T.: 10.946 min
Delta R.T.: 0.000 min
Response: 347713
Conc: 3.43 ng/ml

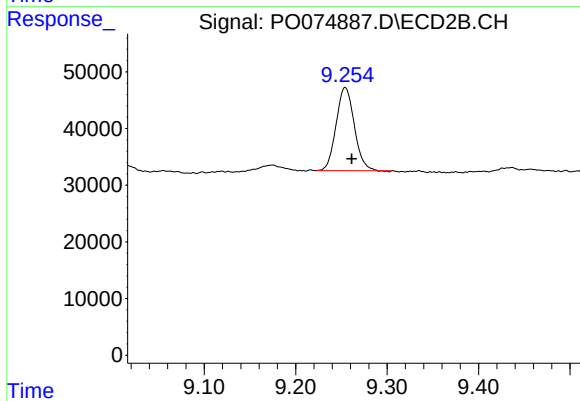

#2 Decachlorobiphenyl

R.T.: 9.254 min
Delta R.T.: -0.007 min
Response: 203080
Conc: 3.70 ng/ml

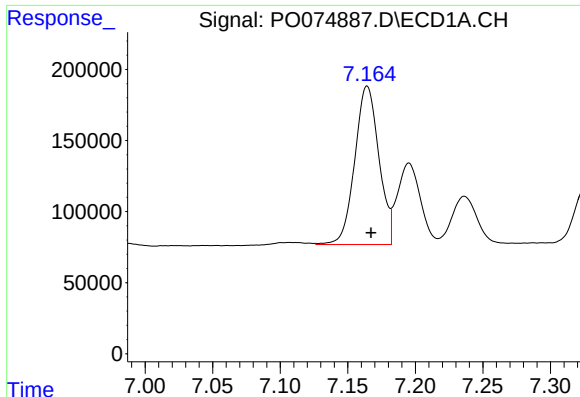


#26 AR-1254-1

R.T.: 7.164 min
Delta R.T.: -0.003 min
Response: 1398253
Conc: 317.92 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S1-02-CDL


Manual Integrations
APPROVED

Ankita
1/19/2021 10:05:50 AM

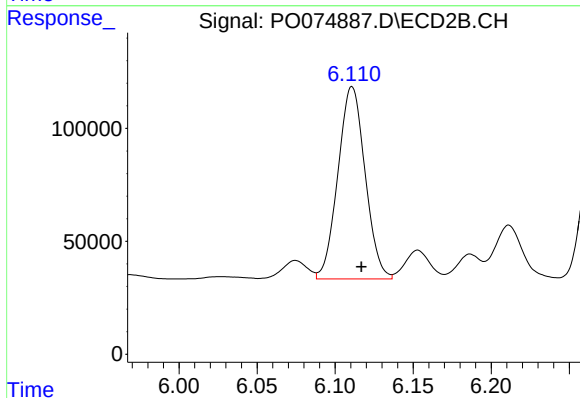


#26 AR-1254-1

R.T.: 6.111 min
Delta R.T.: -0.006 min
Response: 1033096
Conc: 286.02 ng/ml

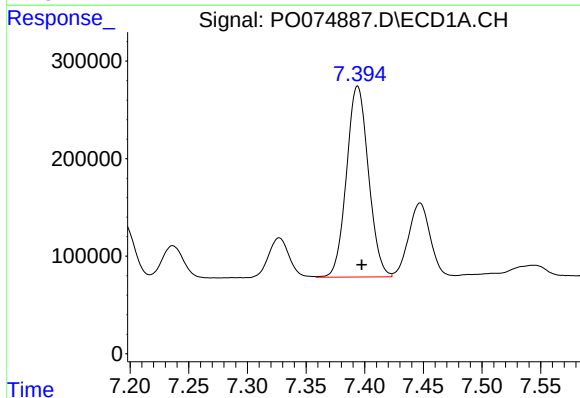


#27 AR-1254-2

R.T.: 7.394 min
Delta R.T.: -0.003 min
Response: 2553135
Conc: 374.87 ng/ml

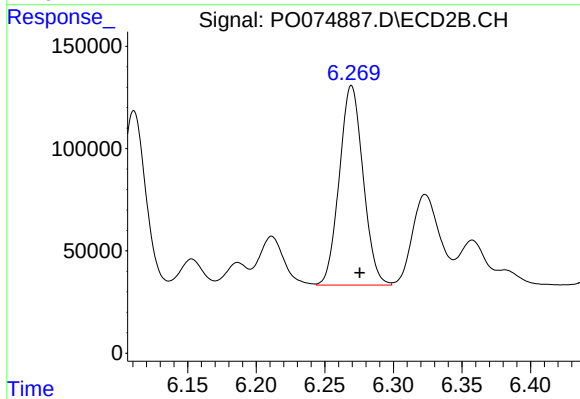

#27 AR-1254-2

R.T.: 6.269 min
Delta R.T.: -0.006 min
Response: 1176374
Conc: 377.46 ng/ml

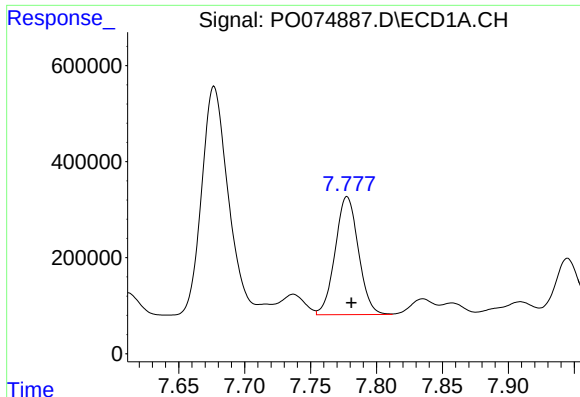


#28 AR-1254-3

R.T.: 7.778 min
Delta R.T.: -0.003 min
Response: 3015941
Conc: 429.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-02-CDL


Manual Integrations
APPROVED

Ankita
1/19/2021 10:05:50 AM

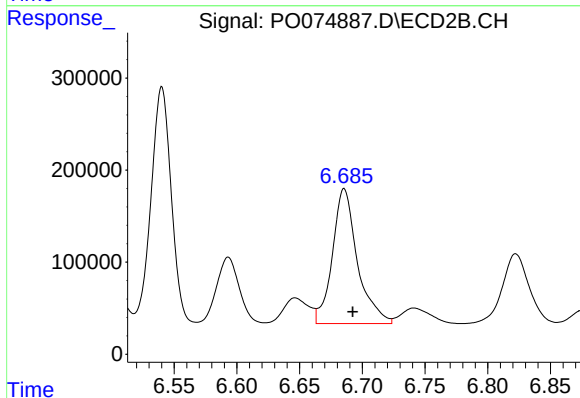


#28 AR-1254-3

R.T.: 6.686 min
Delta R.T.: -0.007 min
Response: 2032575
Conc: 414.48 ng/ml

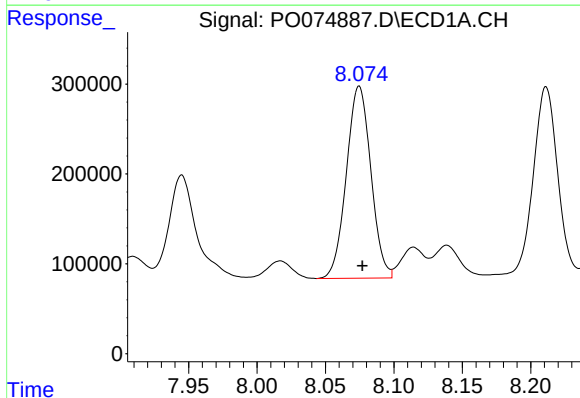


#29 AR-1254-4

R.T.: 8.075 min
Delta R.T.: -0.002 min
Response: 2665438
Conc: 439.50 ng/ml

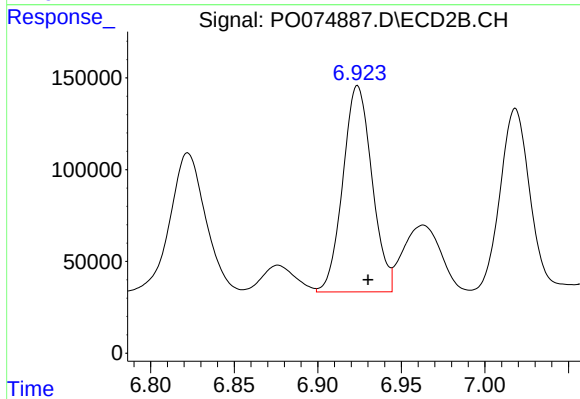

#29 AR-1254-4

R.T.: 6.924 min
Delta R.T.: -0.006 min
Response: 1363311
Conc: 393.14 ng/ml

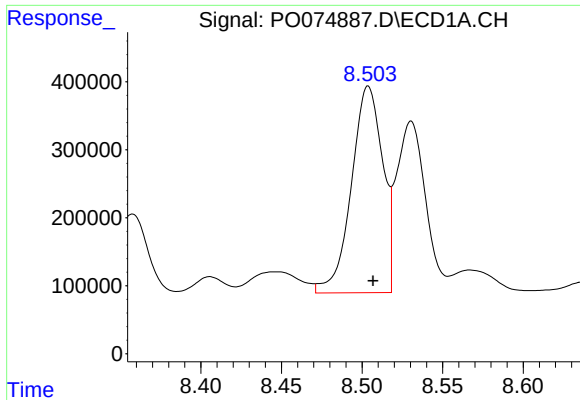


#30 AR-1254-5

R.T.: 8.504 min
Delta R.T.: -0.003 min
Response: 4096943
Conc: 705.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-02-CDL

Manual Integrations
APPROVED

Ankita
1/19/2021 10:05:50 AM

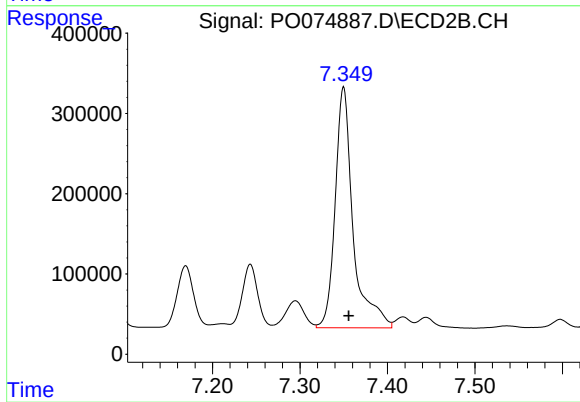

#30 AR-1254-5

R.T.: 7.350 min
Delta R.T.: -0.006 min
Response: 4281281
Conc: 945.94 ng/ml