

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011821\
 Data File : P0074893.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jan 2021 21:01
 Operator : AJ/MA
 Sample : M1088-09DL 2X
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S5-01-CDL

Manual Integrations
 APPROVED

Ankita
 1/19/2021 10:05:52 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 01:07:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.928	4.002	1117005	666089	10.586m	11.841
2) SA Decachlor...	10.946	9.255	880808	491131	8.679	8.945
Target Compounds						
26) L6 AR-1254-1	7.164	6.111	1476324	1058729	335.670	293.114
27) L6 AR-1254-2	7.394	6.270	3142644	1522083	461.423	488.389
28) L6 AR-1254-3	7.778	6.687	4006762	2631039	571.225	536.517
29) L6 AR-1254-4	8.074	6.925	3530771	1778548	582.187	512.878
30) L6 AR-1254-5	8.505	7.350	5368934	8188034	924.254	1809.134 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011821\
Data File : PO074893.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jan 2021 21:01
Operator : AJ/MA
Sample : M1088-09DL 2X
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S5-01-CDL


Manual Integrations
APPROVED

Ankita
1/19/2021 10:05:52 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 01:07:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

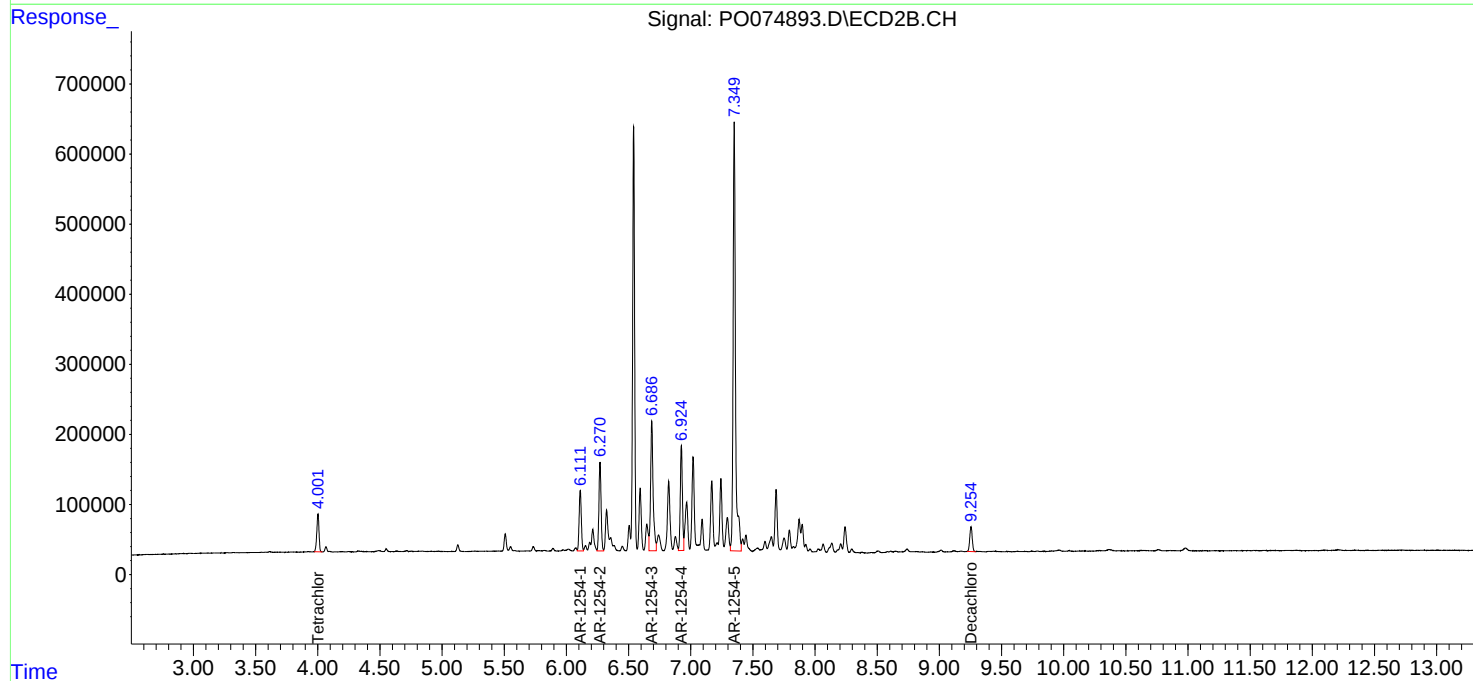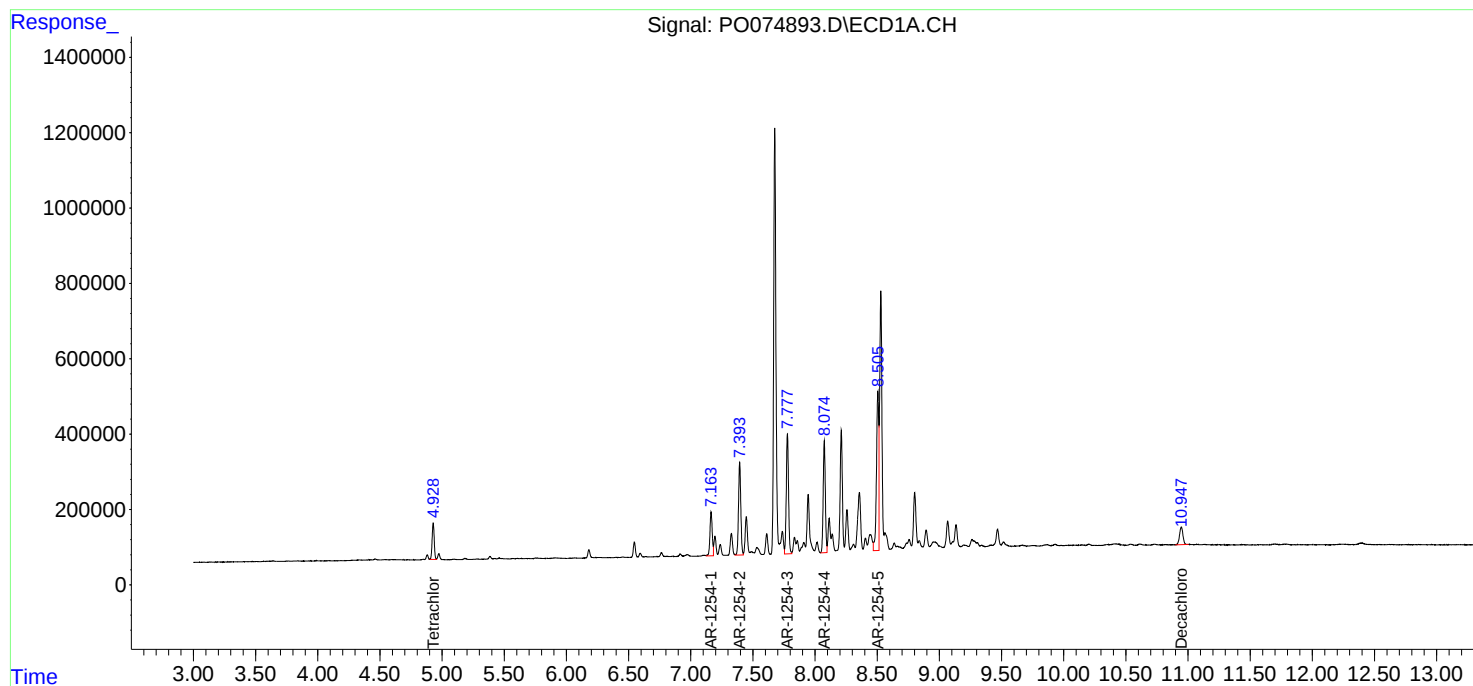

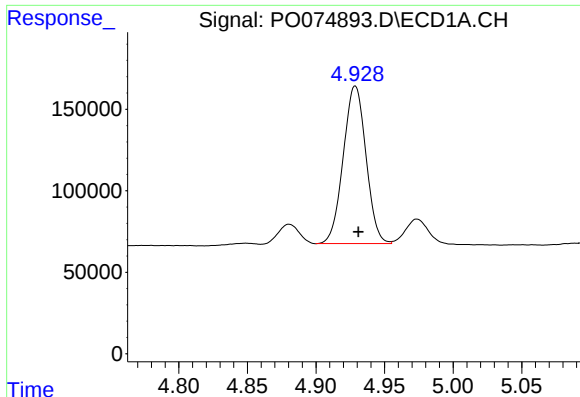


#1 Tetrachloro-m-xylene

R.T.: 4.928 min
Delta R.T.: -0.003 min
Response: 1117005
Conc: 10.59 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S5-01-CDL


Manual Integrations
APPROVED

Ankita
1/19/2021 10:05:52 AM

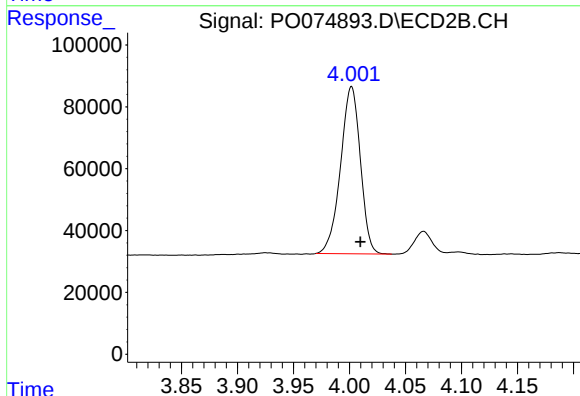


#1 Tetrachloro-m-xylene

R.T.: 4.002 min
Delta R.T.: -0.008 min
Response: 666089
Conc: 11.84 ng/ml

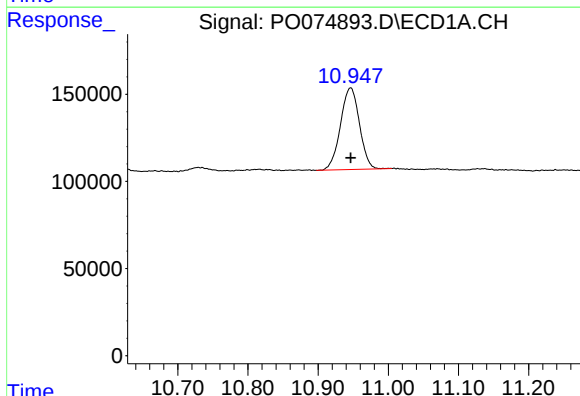


#2 Decachlorobiphenyl

R.T.: 10.946 min
Delta R.T.: 0.000 min
Response: 880808
Conc: 8.68 ng/ml

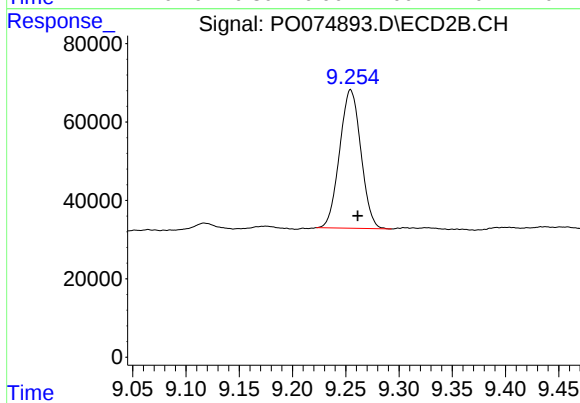

#2 Decachlorobiphenyl

R.T.: 9.255 min
Delta R.T.: -0.007 min
Response: 491131
Conc: 8.95 ng/ml

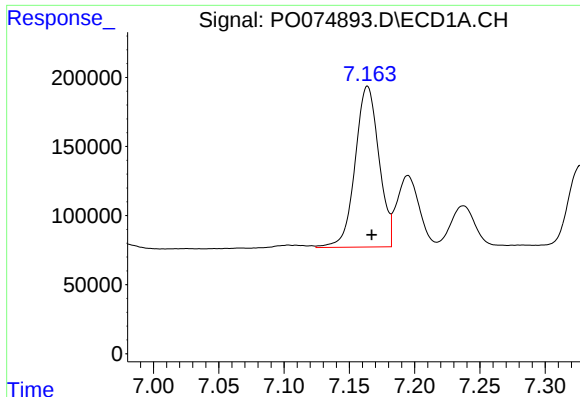


#26 AR-1254-1

R.T.: 7.164 min
Delta R.T.: -0.003 min
Response: 1476324
Conc: 335.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-01-CDL


Manual Integrations
APPROVED

Ankita
1/19/2021 10:05:52 AM

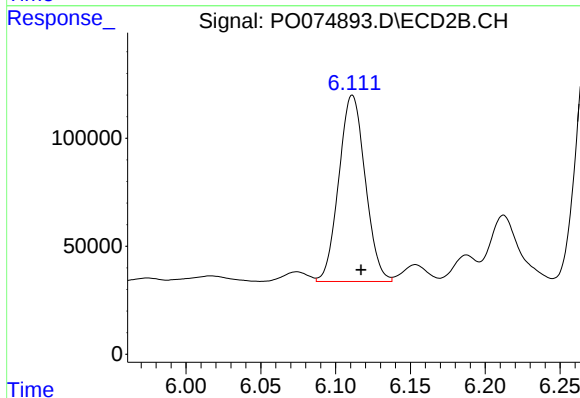


#26 AR-1254-1

R.T.: 6.111 min
Delta R.T.: -0.006 min
Response: 1058729
Conc: 293.11 ng/ml

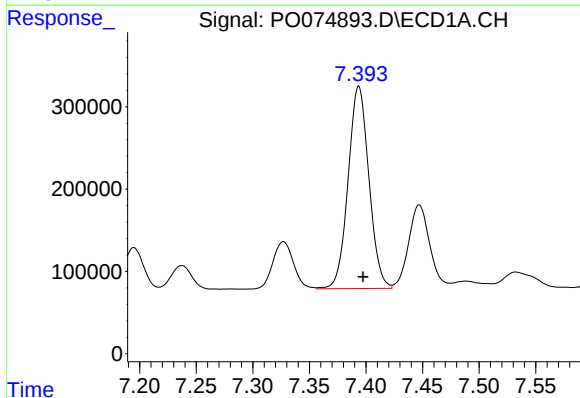


#27 AR-1254-2

R.T.: 7.394 min
Delta R.T.: -0.004 min
Response: 3142644
Conc: 461.42 ng/ml

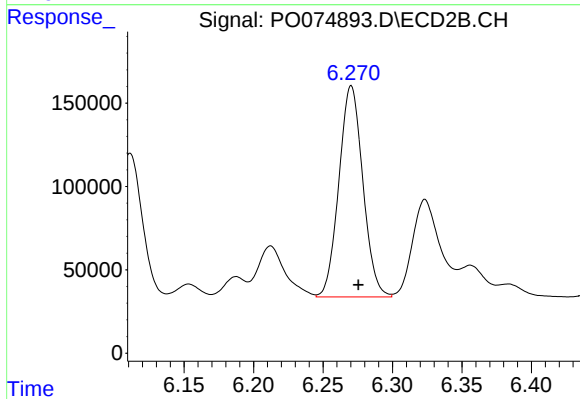

#27 AR-1254-2

R.T.: 6.270 min
Delta R.T.: -0.005 min
Response: 1522083
Conc: 488.39 ng/ml

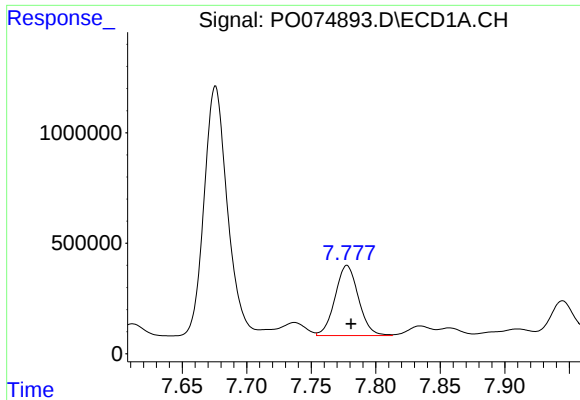


#28 AR-1254-3

R.T.: 7.778 min
Delta R.T.: -0.003 min
Response: 4006762
Conc: 571.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-01-CDL


Manual Integrations
APPROVED

Ankita
1/19/2021 10:05:52 AM

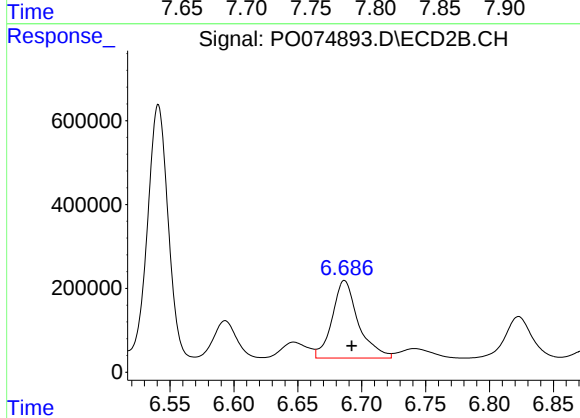


#28 AR-1254-3

R.T.: 6.687 min
Delta R.T.: -0.006 min
Response: 2631039
Conc: 536.52 ng/ml

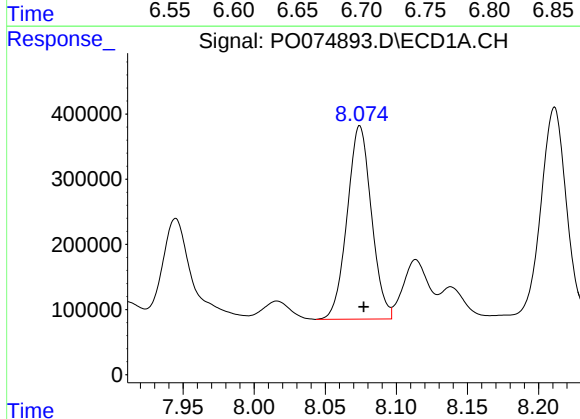


#29 AR-1254-4

R.T.: 8.074 min
Delta R.T.: -0.003 min
Response: 3530771
Conc: 582.19 ng/ml

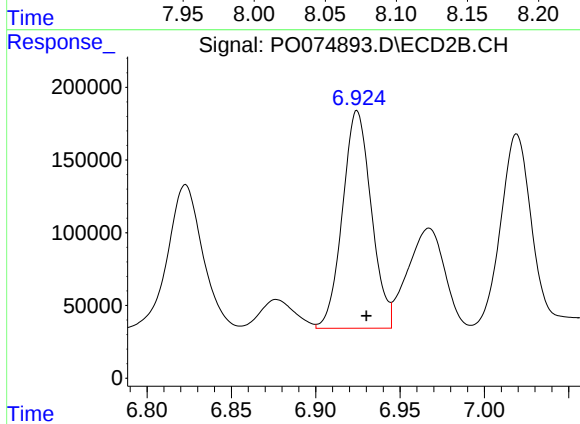

#29 AR-1254-4

R.T.: 6.925 min
Delta R.T.: -0.005 min
Response: 1778548
Conc: 512.88 ng/ml

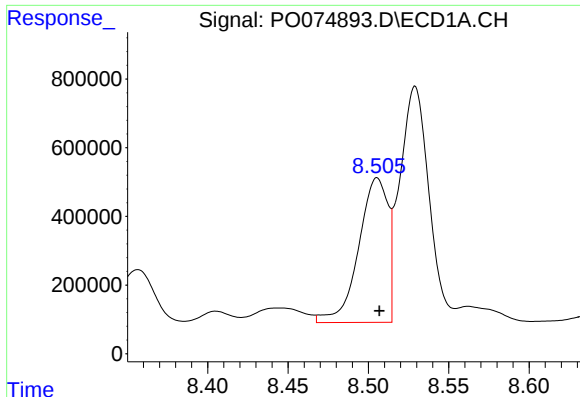


#30 AR-1254-5

R.T.: 8.505 min
Delta R.T.: -0.001 min
Response: 5368934
Conc: 924.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-01-CDL

Manual Integrations
APPROVED

Ankita
1/19/2021 10:05:52 AM

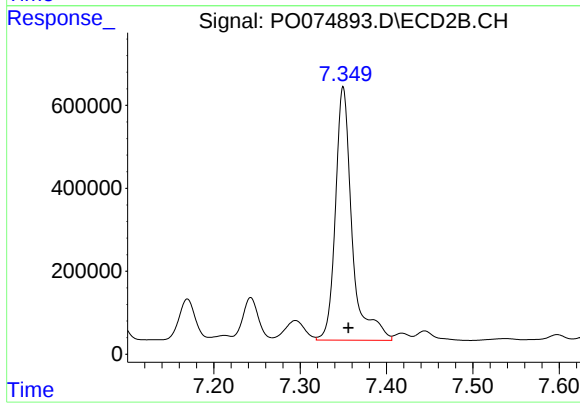

#30 AR-1254-5

R.T.: 7.350 min
Delta R.T.: -0.006 min
Response: 8188034
Conc: 1809.13 ng/ml