

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011822\
 Data File : P0084315.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jan 2022 14:21
 Operator : AJ\MA
 Sample : PB142098BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 04:02:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 18 03:56:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	6.519	5.303	1674541	474298	22.275	21.258
2)	SA Decachlor...	13.770	11.311	1141216	430770	25.363	24.469
Target Compounds							
8)	L2 AR-1221-1	6.791	0.000	83539	0	99.546	N.D. #
9)	L2 AR-1221-2	0.000	5.729	0	6556	N.D.	34.400 #
15)	L3 AR-1232-5	8.266f	0.000	6160	0	10.603	N.D. #
22)	L5 AR-1248-2	8.266f	0.000	6160	0	2.727	N.D. #
28)	L6 AR-1254-3	0.000	8.356	0	3136	N.D.	1.809 #
29)	L6 AR-1254-4	0.000	8.604	0	5221	N.D.	4.945 #
30)	L6 AR-1254-5	0.000	9.057	0	6803	N.D.	4.659 #
32)	L7 AR-1260-2	0.000	8.697	0	3753	N.D.	3.132 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011822\
Data File : P0084315.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jan 2022 14:21
Operator : AJ\MA
Sample : PB142098BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 04:02:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 18 03:56:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

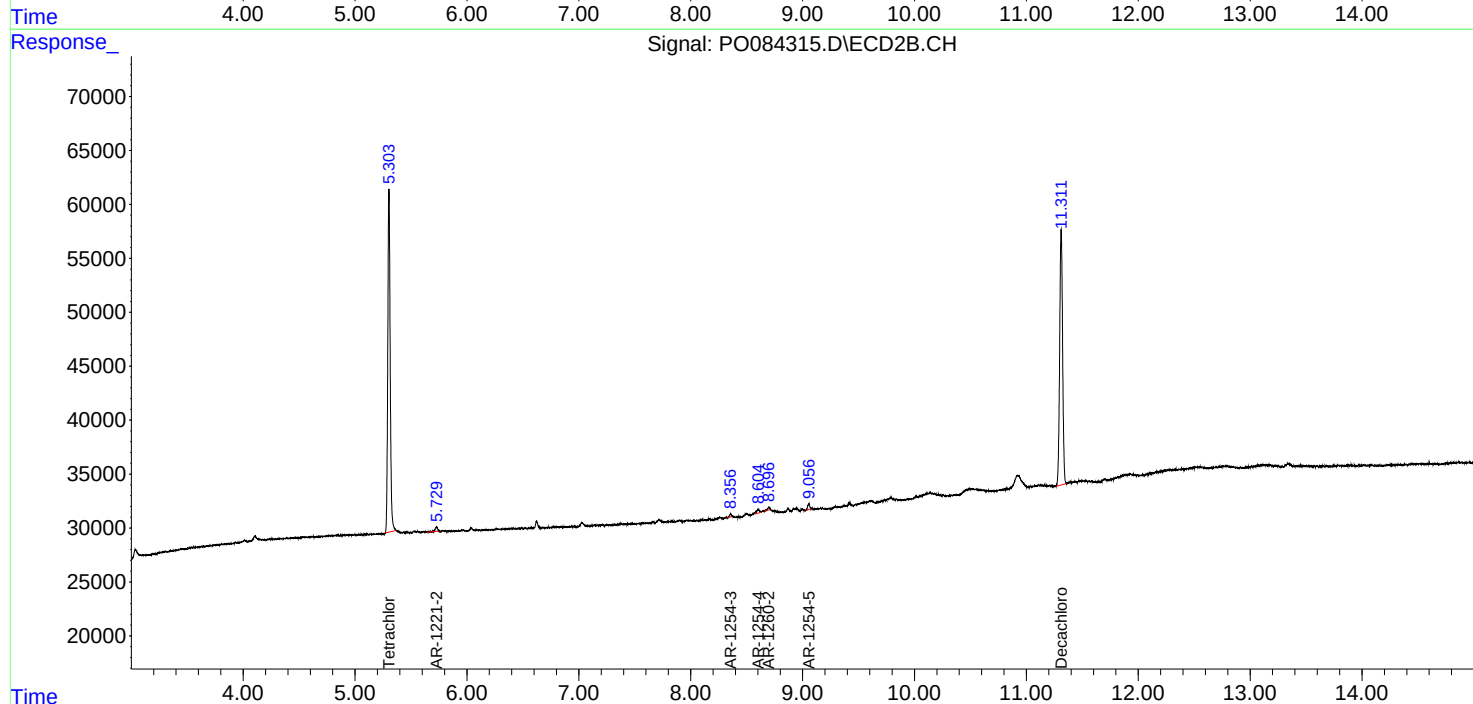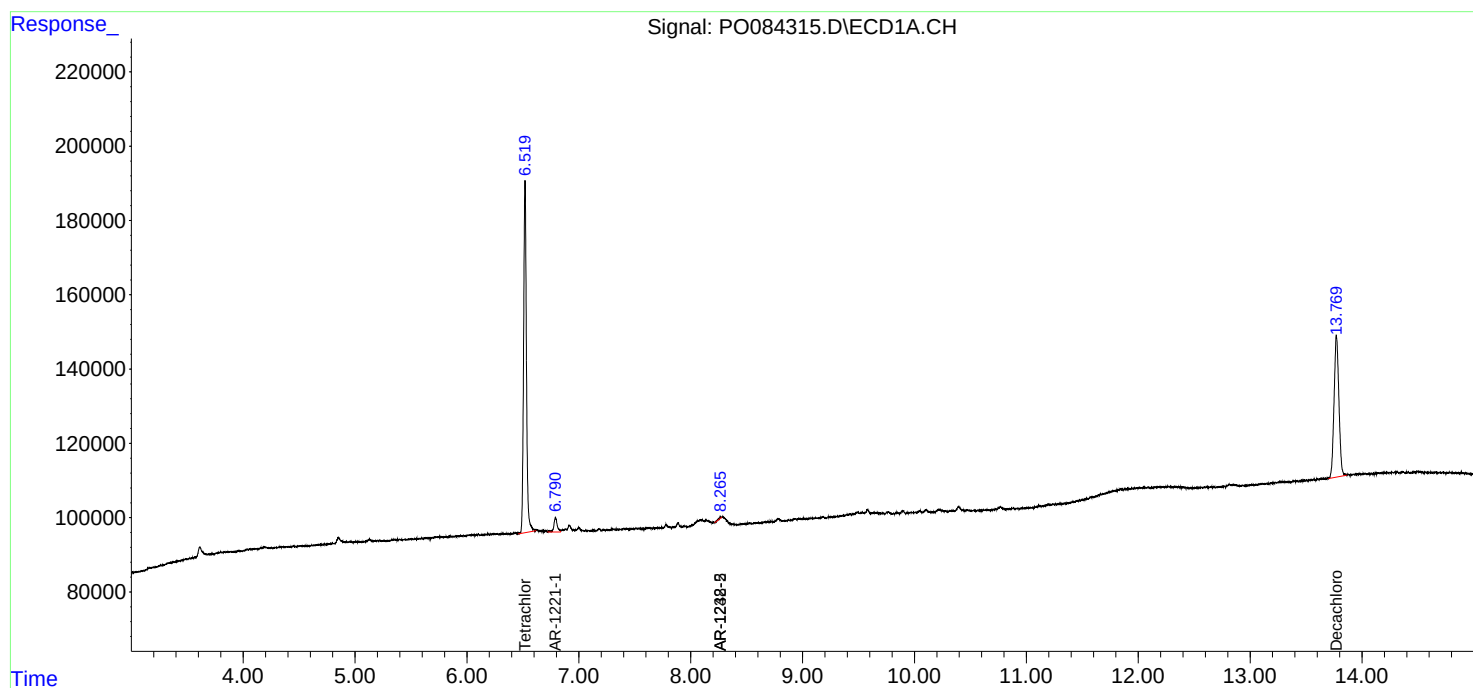


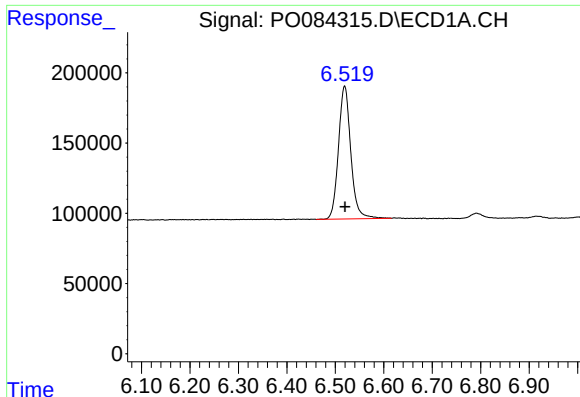

#1 Tetrachloro-m-xylene


R.T.: 6.519 min
Delta R.T.: 0.000 min
Response: 1674541
Conc: 22.28 ng/ml

Instrument :
ECD_O
ClientSampleId :

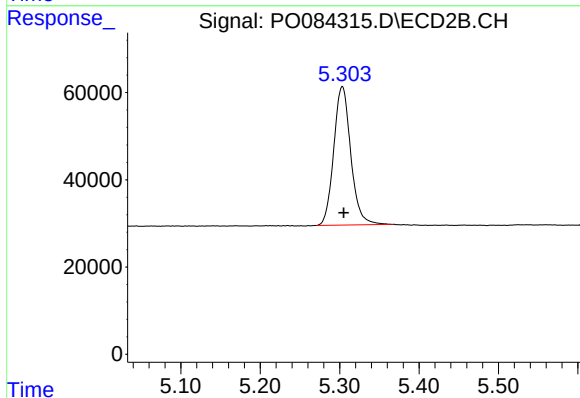


#1 Tetrachloro-m-xylene

R.T.: 5.303 min
Delta R.T.: -0.002 min
Response: 474298
Conc: 21.26 ng/ml

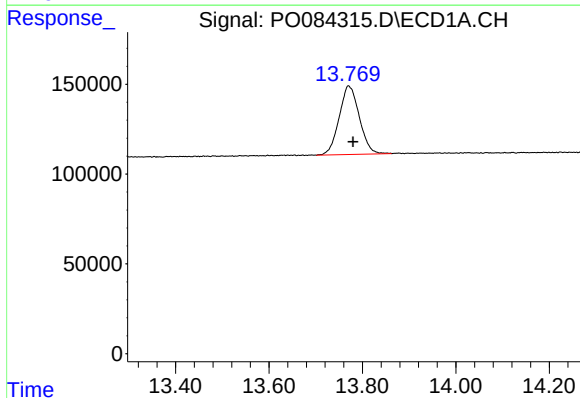


#2 Decachlorobiphenyl

R.T.: 13.770 min
Delta R.T.: -0.010 min
Response: 1141216
Conc: 25.36 ng/ml

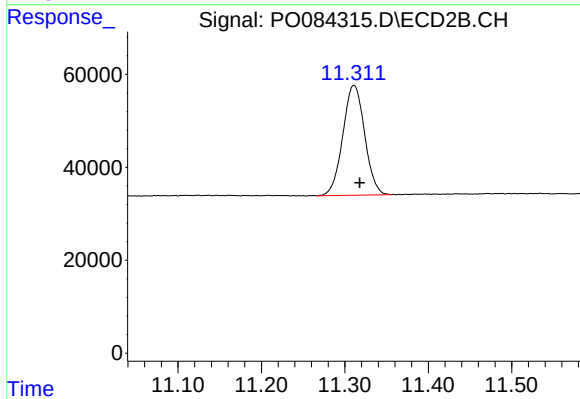

#2 Decachlorobiphenyl


R.T.: 11.311 min
Delta R.T.: -0.007 min
Response: 430770
Conc: 24.47 ng/ml

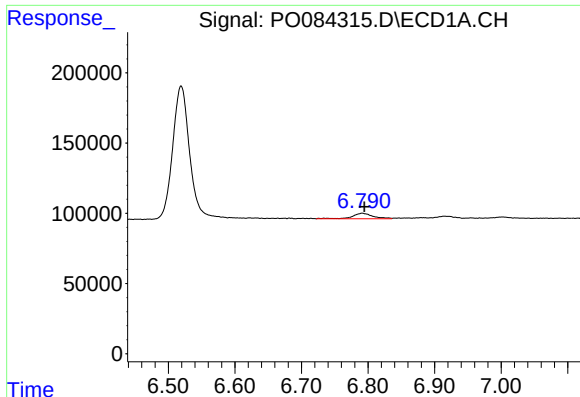

#8 AR-1221-1


R.T.: 6.791 min
Delta R.T.: -0.003 min
Response: 83539
Conc: 99.55 ng/ml

Instrument :
ECD_O
ClientSampleId :

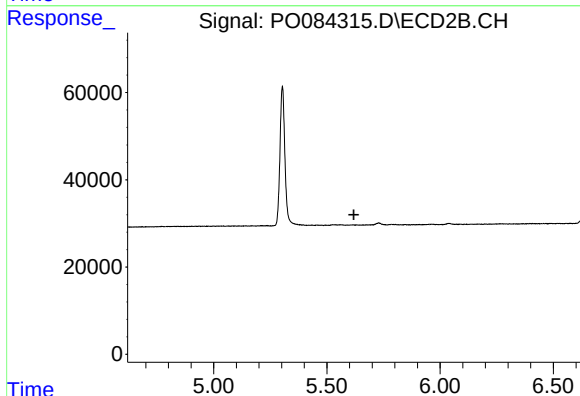


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 5.619 min
Response: 0
Conc: N.D.

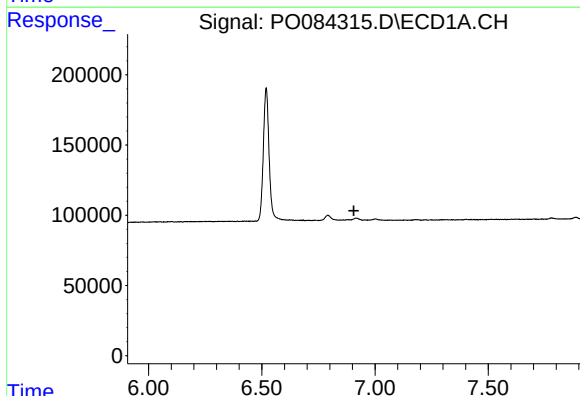


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 6.907 min
Response: 0
Conc: N.D.

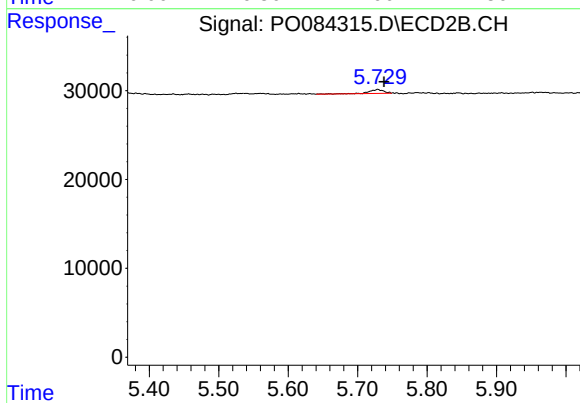

#9 AR-1221-2


R.T.: 5.729 min
Delta R.T.: -0.009 min
Response: 6556
Conc: 34.40 ng/ml

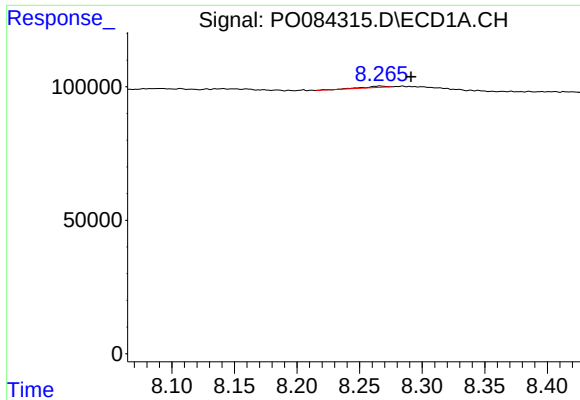

#15 AR-1232-5


R.T.: 8.266 min
Delta R.T.: -0.025 min
Response: 6160
Conc: 10.60 ng/ml

Instrument :
ECD_O
ClientSampleId :

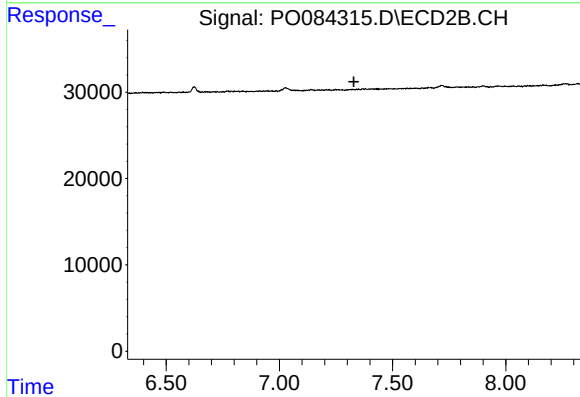


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 7.329 min
Response: 0
Conc: N.D.

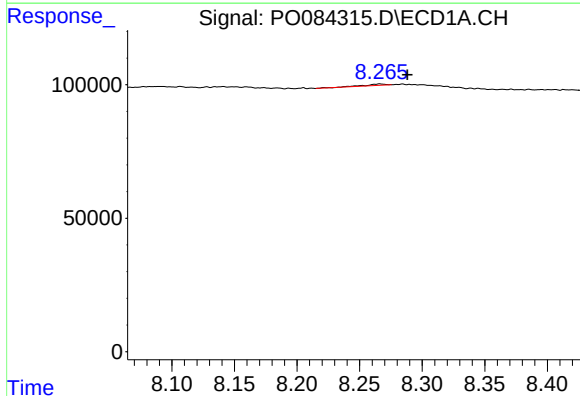


#22 AR-1248-2

R.T.: 8.266 min
Delta R.T.: -0.022 min
Response: 6160
Conc: 2.73 ng/ml

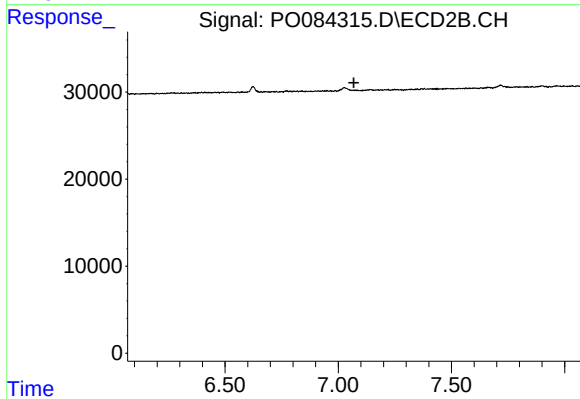

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 7.069 min
Response: 0
Conc: N.D.

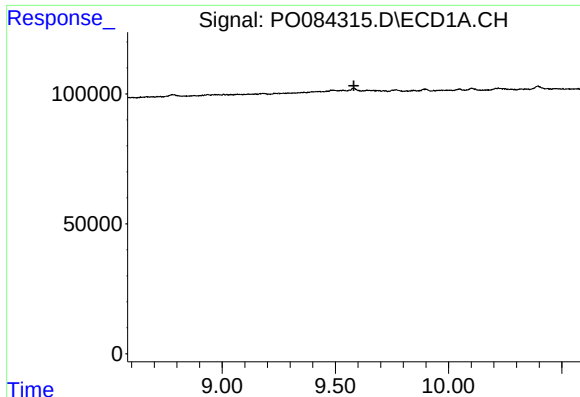

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 9.581 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

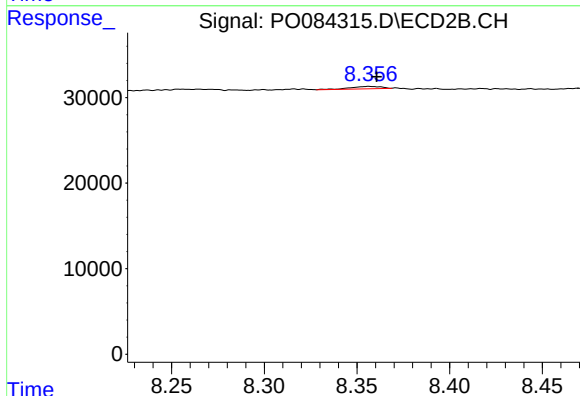


#28 AR-1254-3

R.T.: 8.356 min
Delta R.T.: -0.004 min
Response: 3136
Conc: 1.81 ng/ml

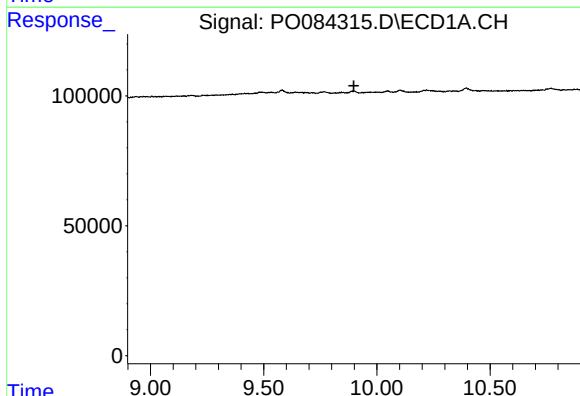


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T.: 9.898 min
Response: 0
Conc: N.D.

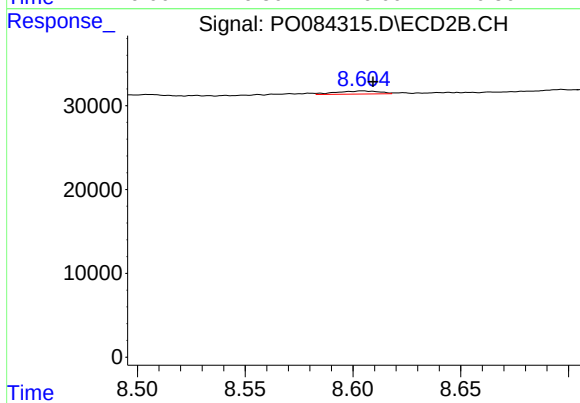

#29 AR-1254-4


R.T.: 8.604 min
Delta R.T.: -0.005 min
Response: 5221
Conc: 4.95 ng/ml

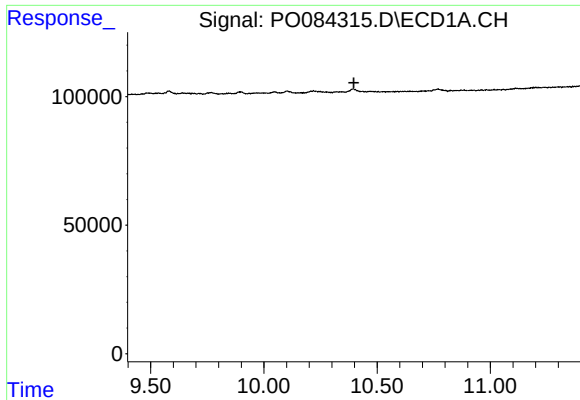

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 10.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

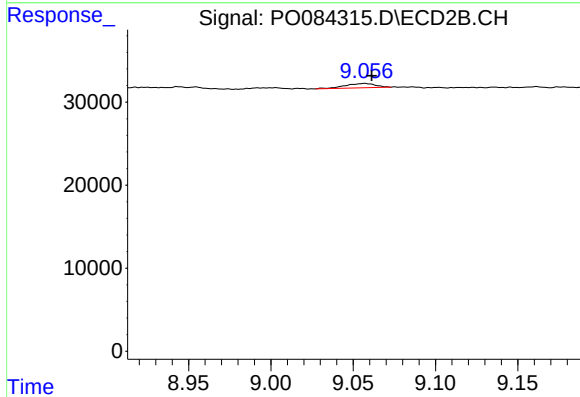


#30 AR-1254-5

R.T.: 9.057 min
Delta R.T.: -0.004 min
Response: 6803
Conc: 4.66 ng/ml

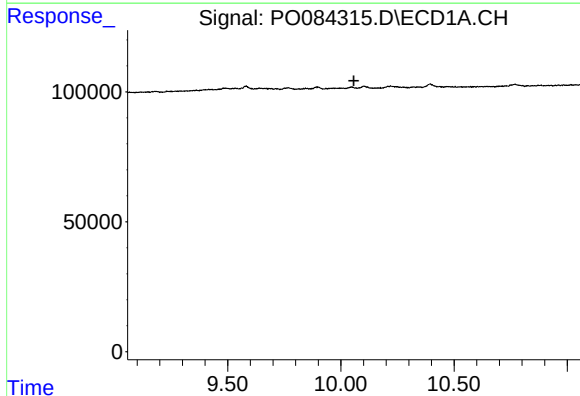

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 10.057 min
Response: 0
Conc: N.D.

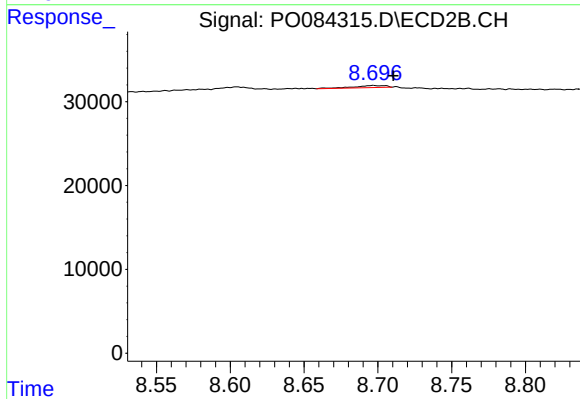

#32 AR-1260-2

R.T.: 8.697 min
Delta R.T.: -0.014 min
Response: 3753
Conc: 3.13 ng/ml