

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011822\
 Data File : P0084321.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jan 2022 16:13
 Operator : AJ\MA
 Sample : N1154-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 04:05:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 18 03:56:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	6.523	5.310	1623720	478517	21.599	21.447
2) SA Decachlor...	13.771	11.313	726044	279758	16.136	15.891
Target Compounds						
8) L2 AR-1221-1	6.792	0.000	89657	0	106.837	N.D. #
30) L6 AR-1254-5	0.000	9.085f	0	8236	N.D.	5.640 #
36) L8 AR-1262-1	0.000	9.085	0	8236	N.D.	5.920 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011822\
Data File : PO084321.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jan 2022 16:13
Operator : AJ\MA
Sample : N1154-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 04:05:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 18 03:56:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

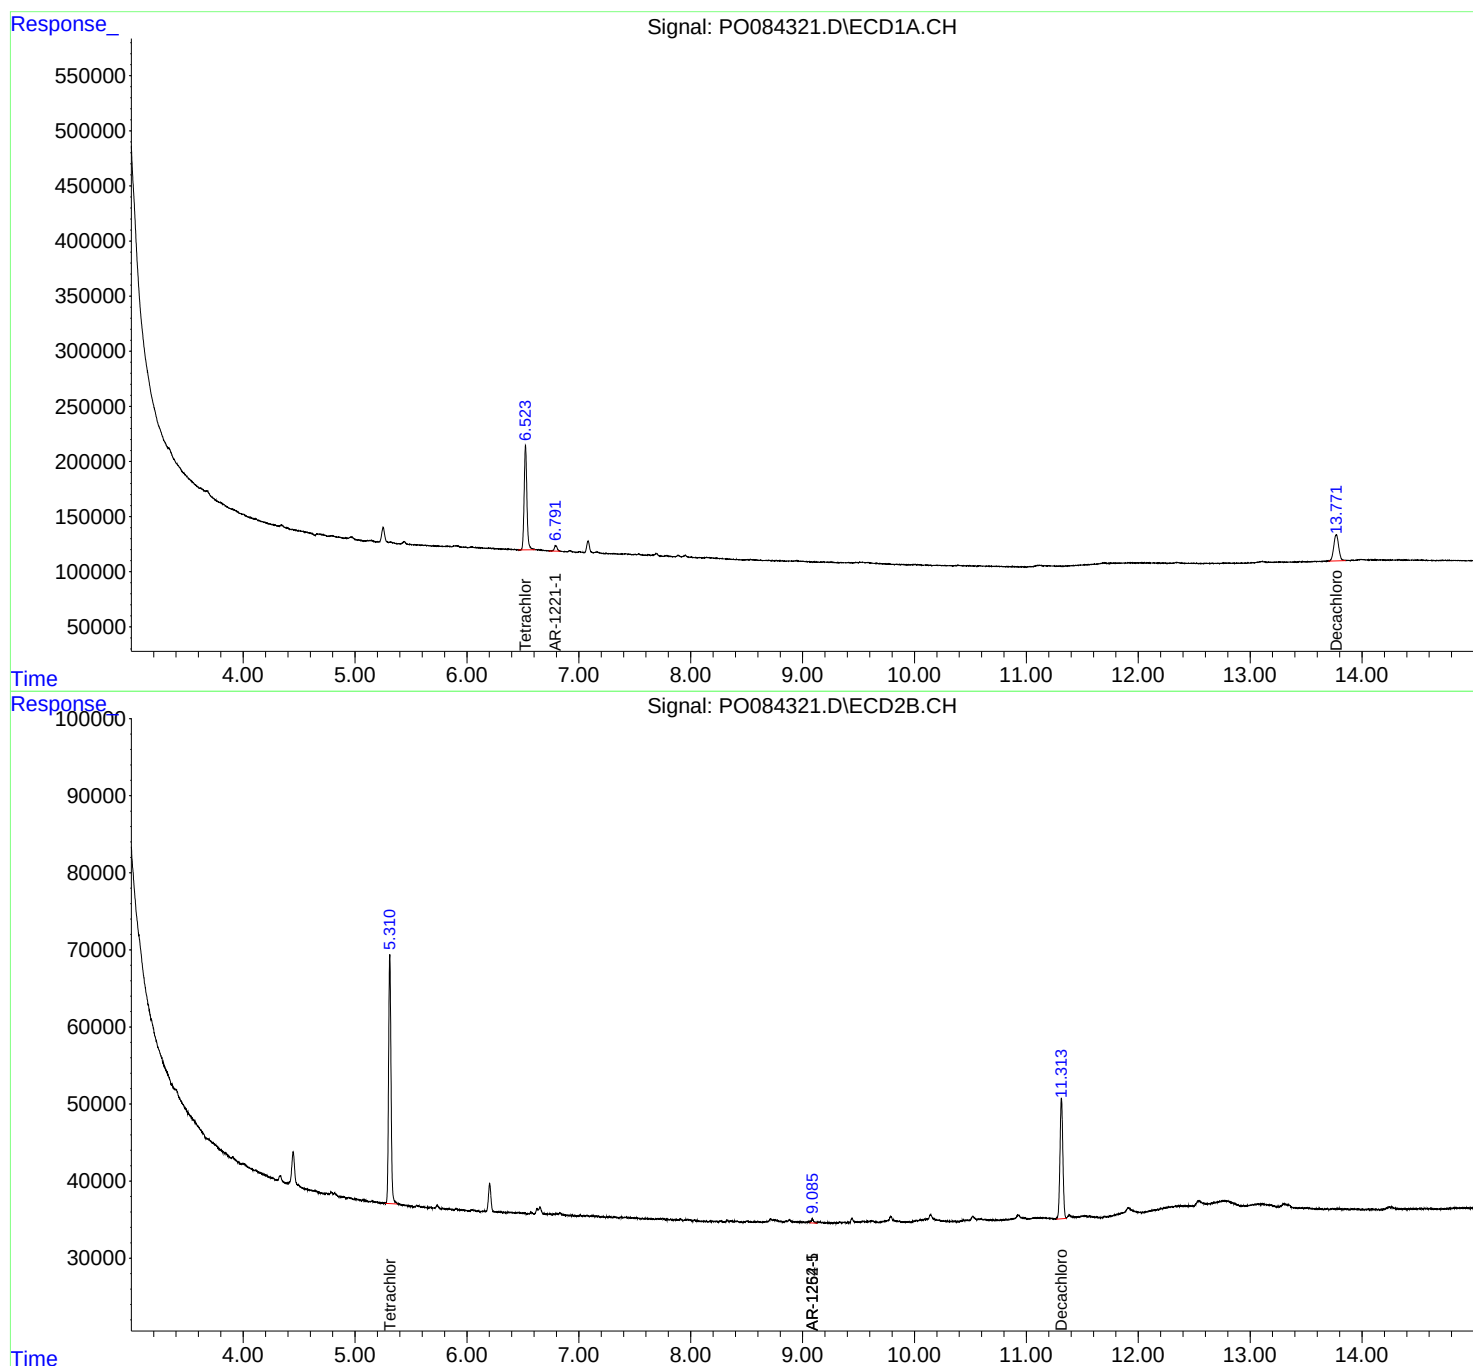


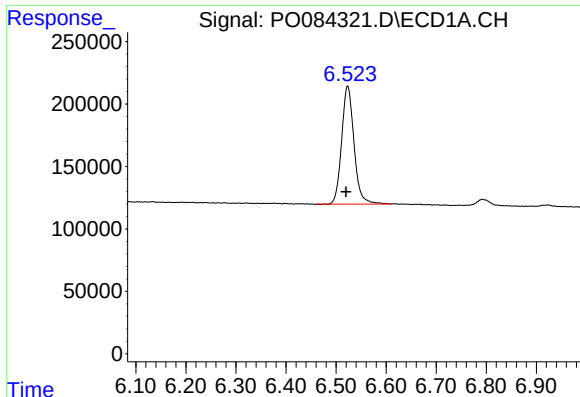

#1 Tetrachloro-m-xylene


R.T.: 6.523 min
Delta R.T.: 0.003 min
Response: 1623720
Conc: 21.60 ng/ml

Instrument :
ECD_O
ClientSampleId :

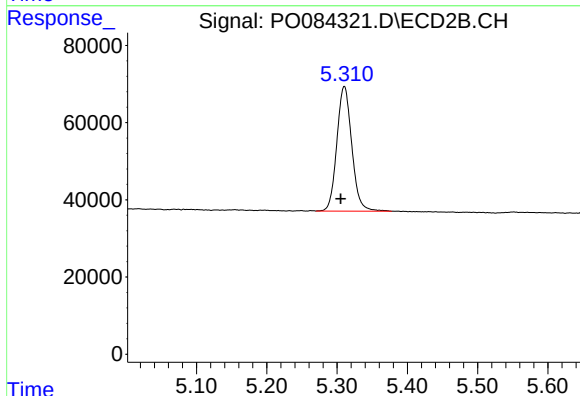


#1 Tetrachloro-m-xylene

R.T.: 5.310 min
Delta R.T.: 0.005 min
Response: 478517
Conc: 21.45 ng/ml

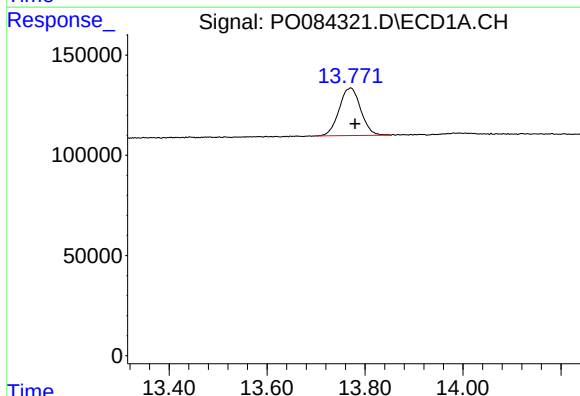


#2 Decachlorobiphenyl

R.T.: 13.771 min
Delta R.T.: -0.009 min
Response: 726044
Conc: 16.14 ng/ml

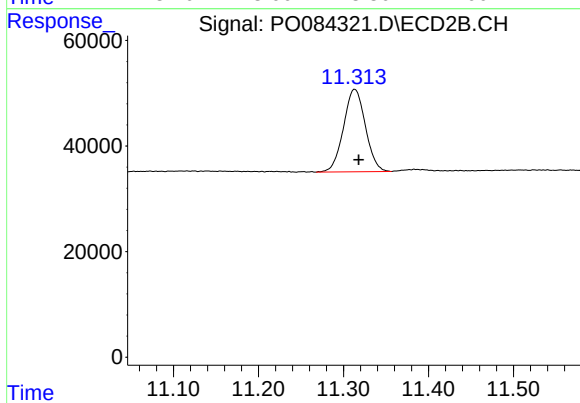

#2 Decachlorobiphenyl


R.T.: 11.313 min
Delta R.T.: -0.005 min
Response: 279758
Conc: 15.89 ng/ml

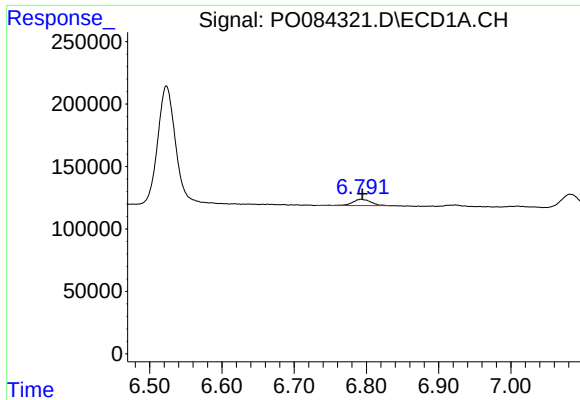

#8 AR-1221-1


R.T.: 6.792 min
Delta R.T.: -0.002 min
Response: 89657
Conc: 106.84 ng/ml

Instrument :
ECD_O
ClientSampleId :

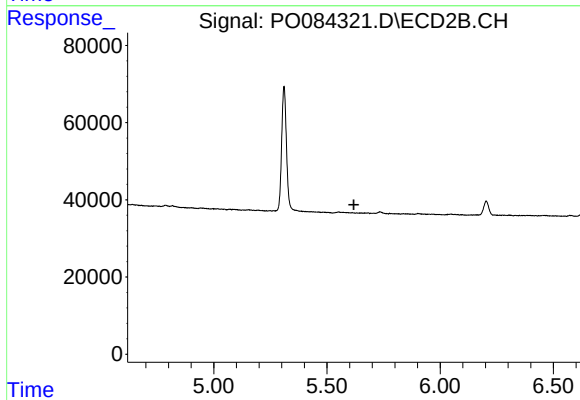


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 5.619 min
Response: 0
Conc: N.D.

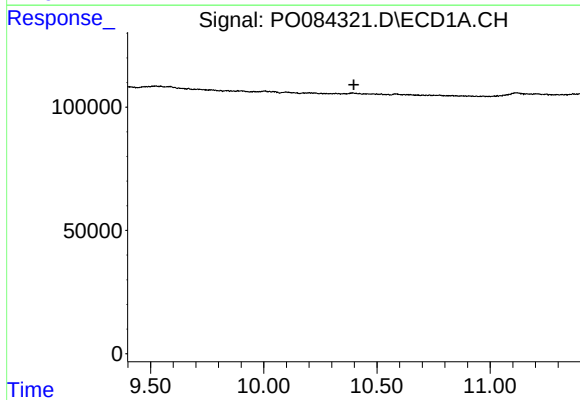


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 10.398 min
Response: 0
Conc: N.D.

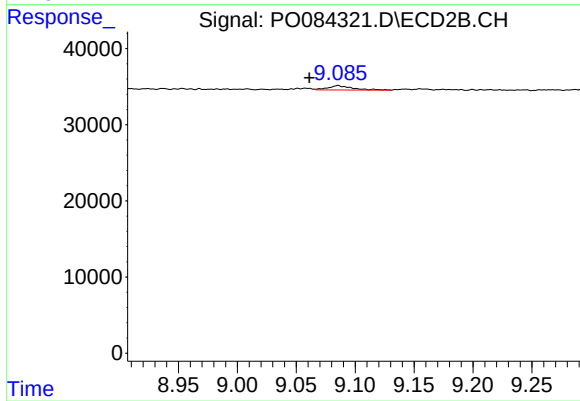

#30 AR-1254-5


R.T.: 9.085 min
Delta R.T.: 0.024 min
Response: 8236
Conc: 5.64 ng/ml

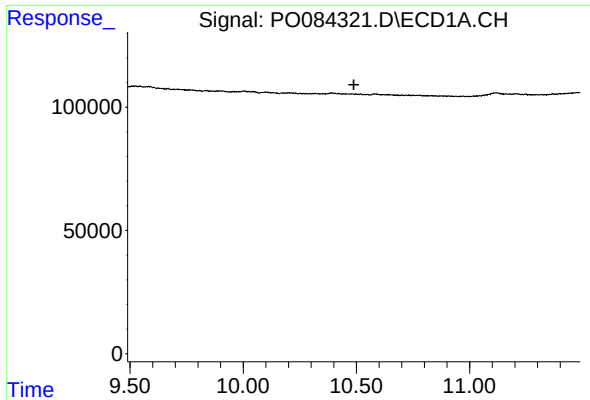

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 10.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

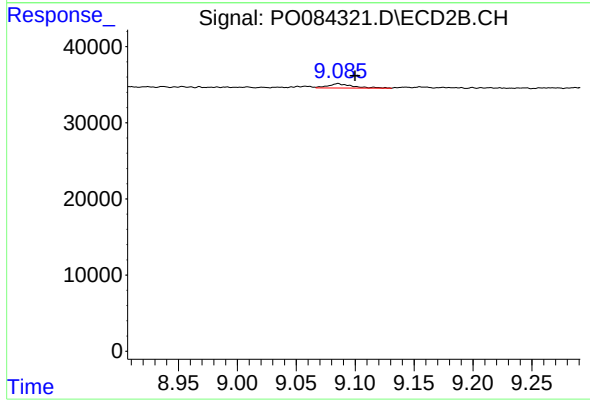

#36 AR-1262-1

R.T.: 9.085 min
Delta R.T.: -0.014 min
Response: 8236
Conc: 5.92 ng/ml