

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011822\
 Data File : P0084314.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jan 2022 11:35
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 04:02:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 18 03:56:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	6.521	5.307	1544574	437472	20.547	19.608
2)	SA Decachlor...	13.770	11.311	1050843	400661	23.354	22.759

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011822\
Data File : P0084314.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jan 2022 11:35
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 04:02:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 18 03:56:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

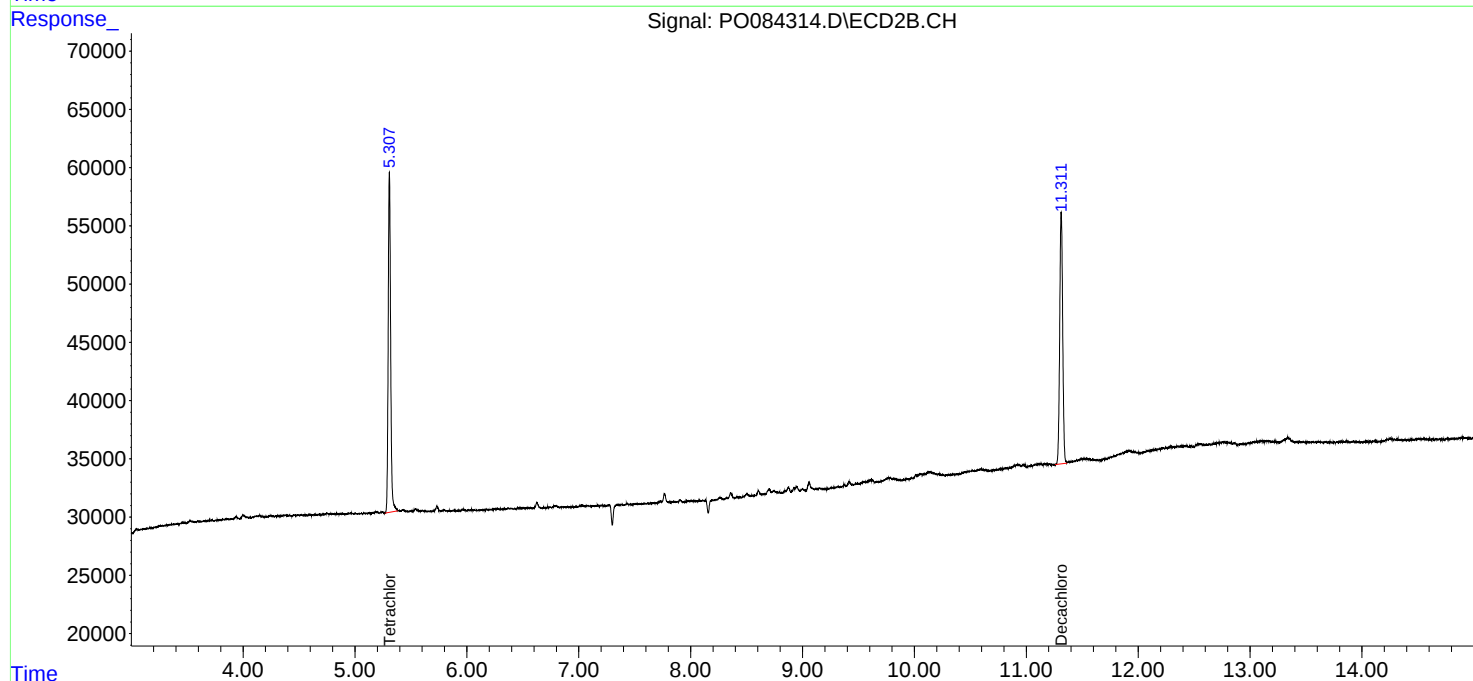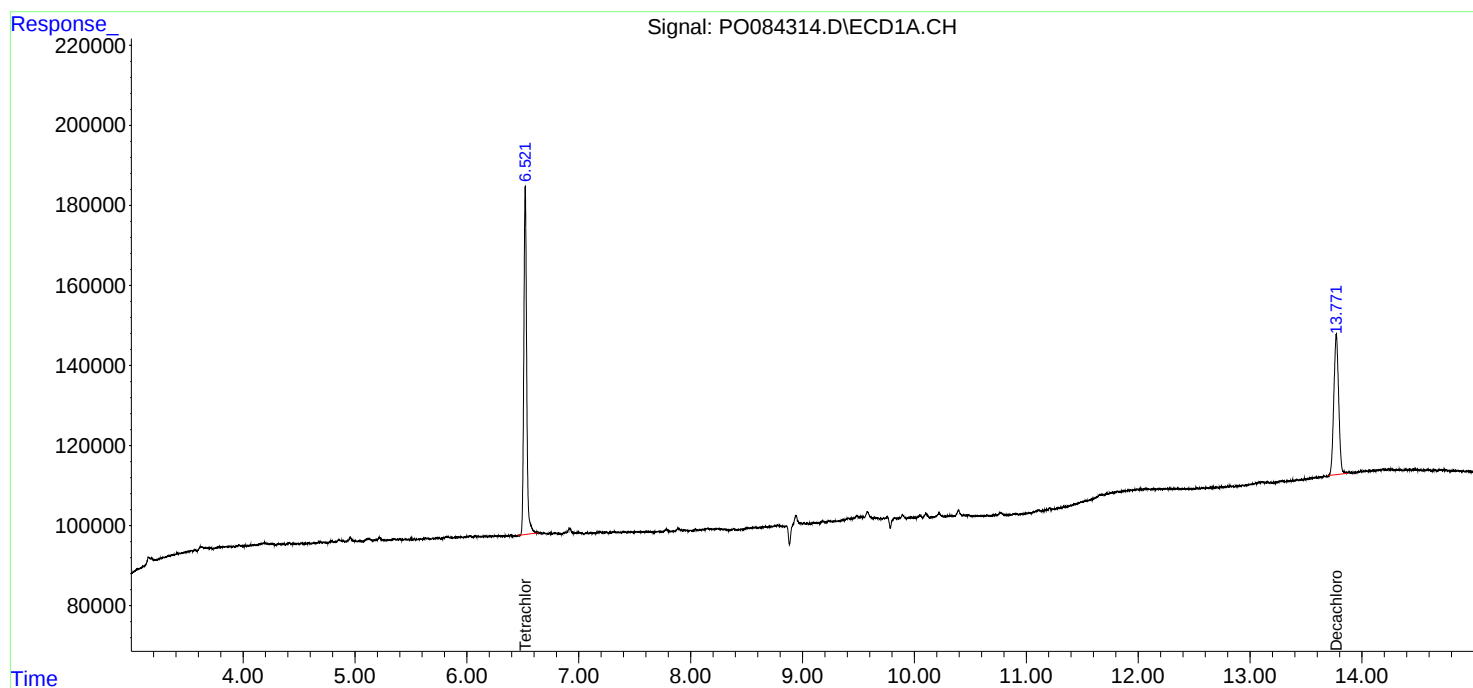


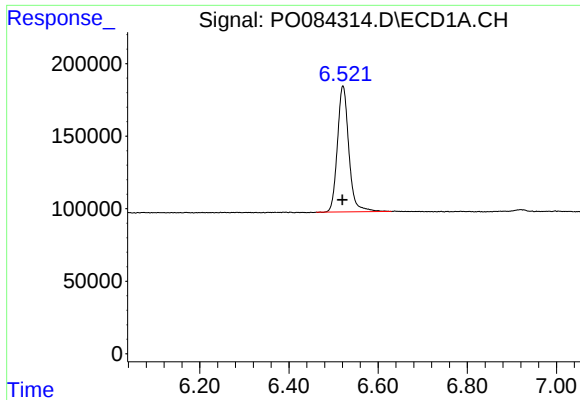

#1 Tetrachloro-m-xylene


R.T.: 6.521 min
Delta R.T.: 0.001 min
Response: 1544574
Conc: 20.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

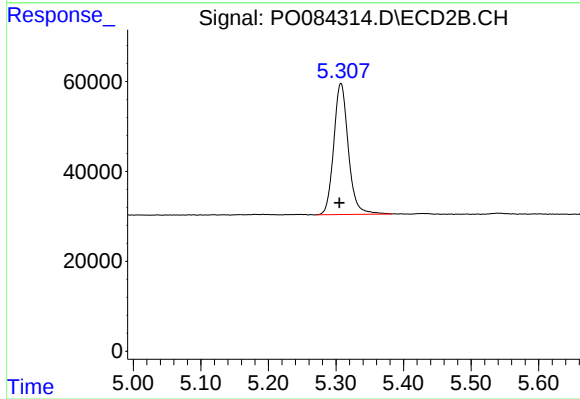


#1 Tetrachloro-m-xylene

R.T.: 5.307 min
Delta R.T.: 0.002 min
Response: 437472
Conc: 19.61 ng/ml

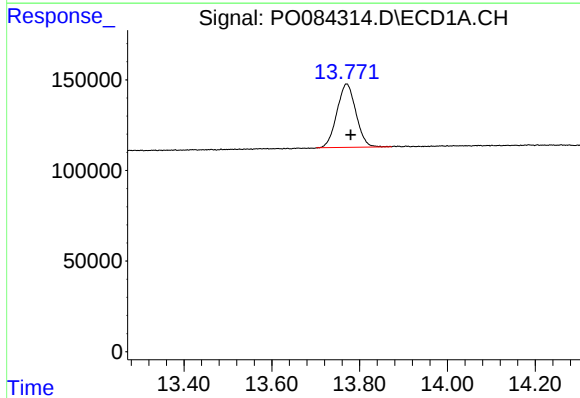

#2 Decachlorobiphenyl

R.T.: 13.770 min
Delta R.T.: -0.010 min
Response: 1050843
Conc: 23.35 ng/ml

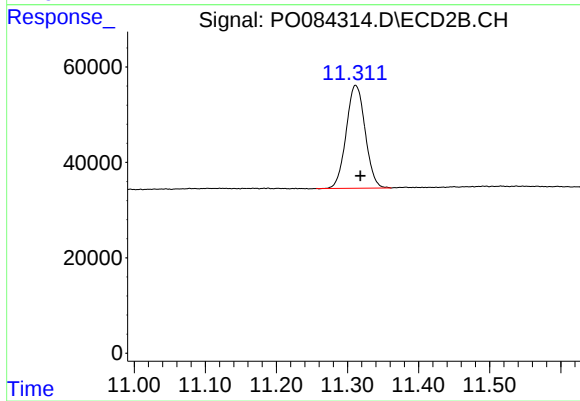

#2 Decachlorobiphenyl

R.T.: 11.311 min
Delta R.T.: -0.007 min
Response: 400661
Conc: 22.76 ng/ml