

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0011822\  
 Data File : P0084315.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 18 Jan 2022 14:21  
 Operator : AJ\MA  
 Sample : PB142098BL  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 PB142098BL

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jan 19 04:02:37 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0011722.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Jan 18 03:56:07 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2   | Resp#1  | Resp#2 | ng/ml  | ng/ml  |
|-----------------------------|--------|--------|---------|--------|--------|--------|
| -----                       |        |        |         |        |        |        |
| System Monitoring Compounds |        |        |         |        |        |        |
| 1) SA Tetrachlo...          | 6.519  | 5.303  | 1674541 | 474298 | 22.275 | 21.258 |
| 2) SA Decachlor...          | 13.770 | 11.311 | 1141216 | 430770 | 25.363 | 24.469 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0011822\  
Data File : P0084315.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 18 Jan 2022 14:21  
Operator : AJ\MA  
Sample : PB142098BL  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
PB142098BL

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jan 19 04:02:37 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0011722.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Tue Jan 18 03:56:07 2022  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

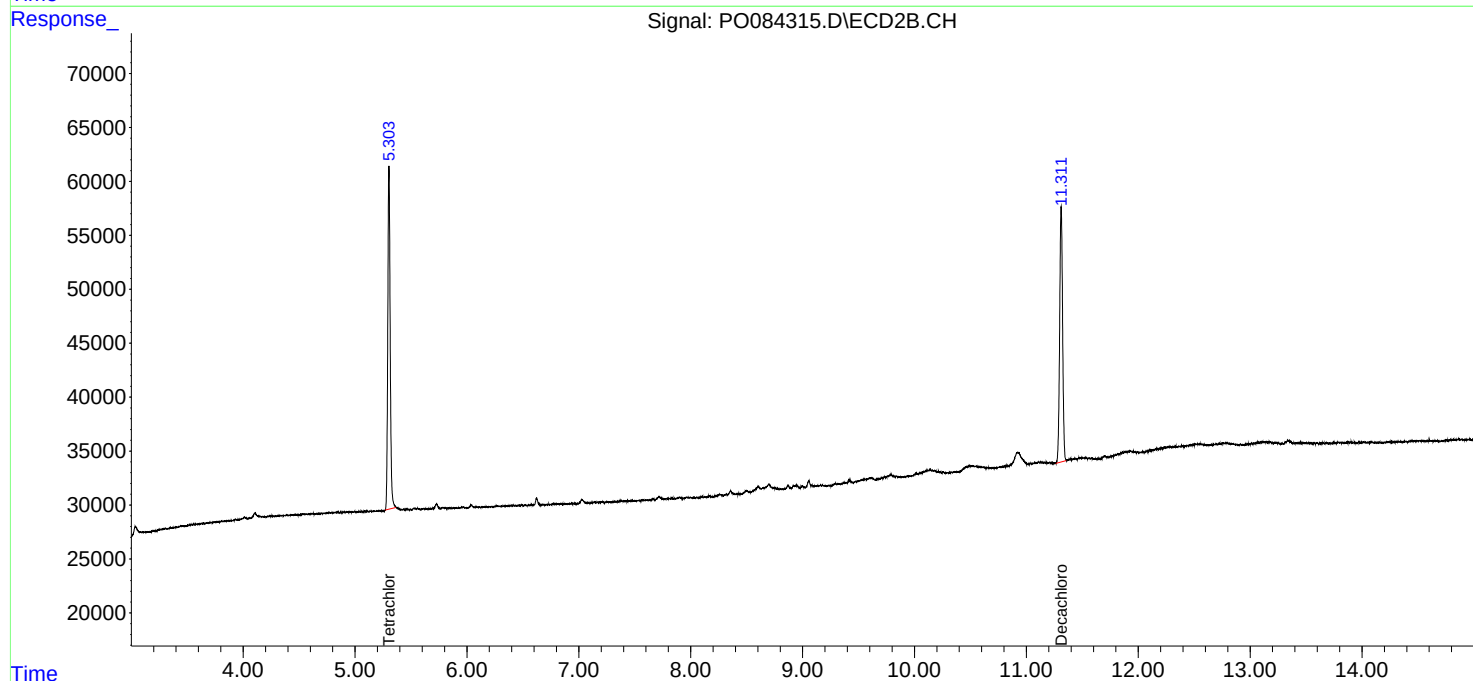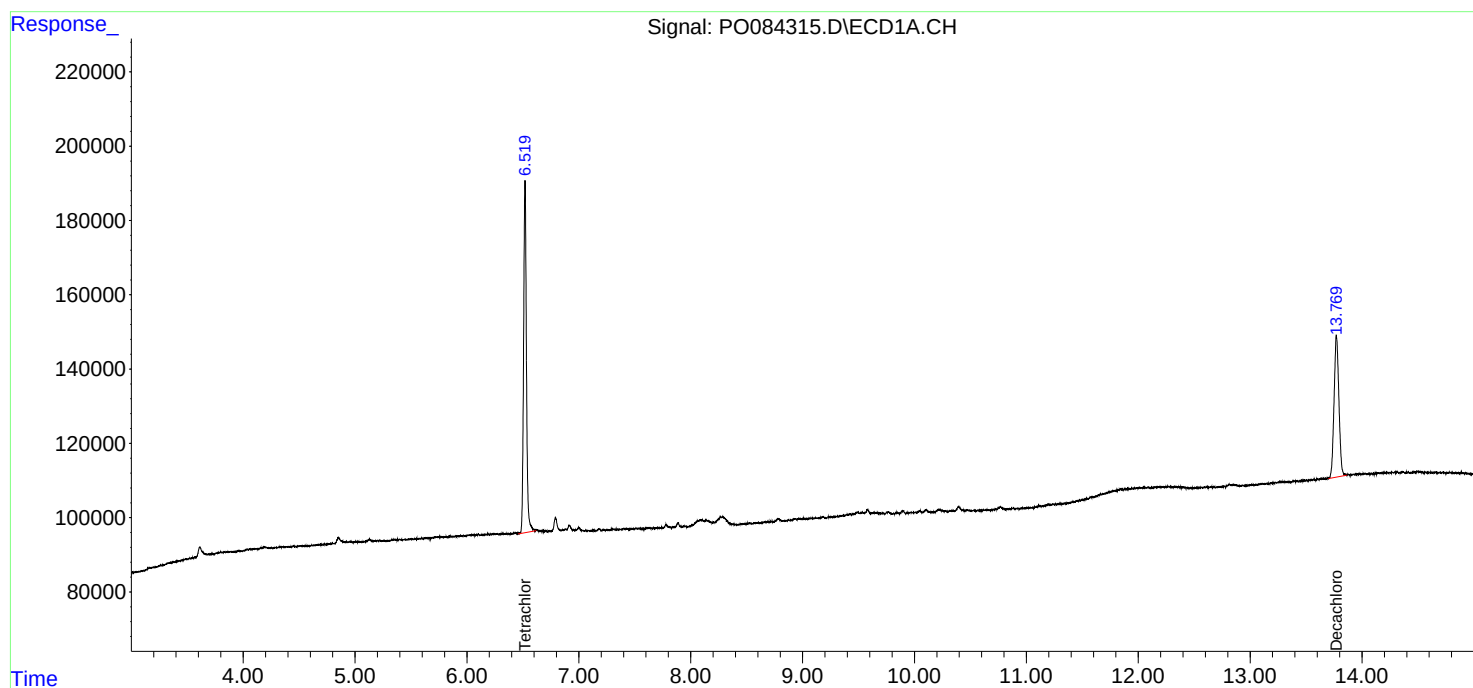


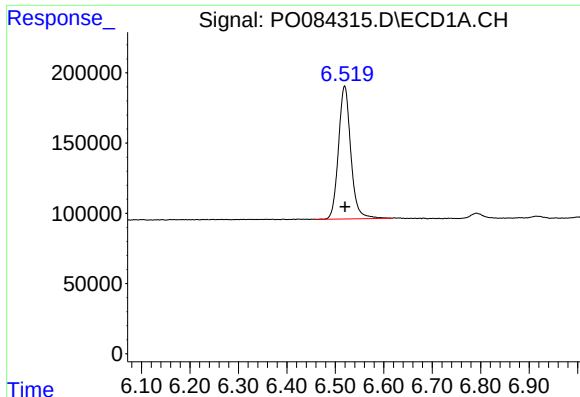

#1 Tetrachloro-m-xylene


R.T.: 6.519 min  
Delta R.T.: 0.000 min  
Response: 1674541  
Conc: 22.28 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
PB142098BL

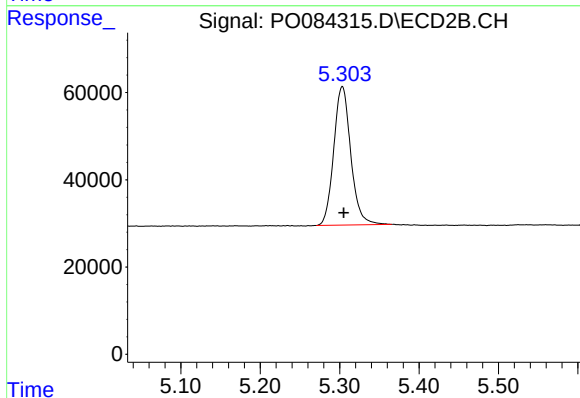


#1 Tetrachloro-m-xylene

R.T.: 5.303 min  
Delta R.T.: -0.002 min  
Response: 474298  
Conc: 21.26 ng/ml

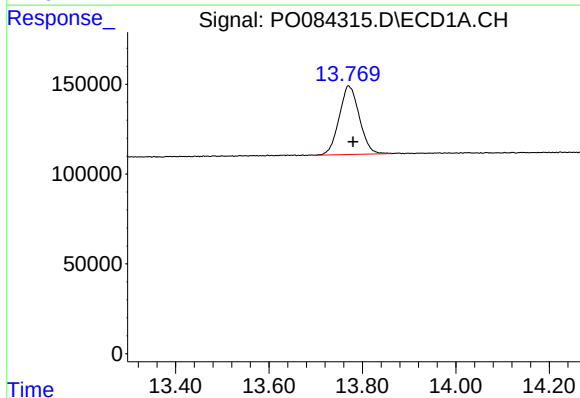

#2 Decachlorobiphenyl

R.T.: 13.770 min  
Delta R.T.: -0.010 min  
Response: 1141216  
Conc: 25.36 ng/ml

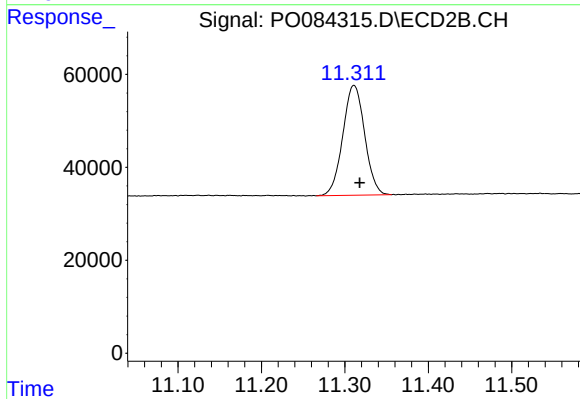

#2 Decachlorobiphenyl

R.T.: 11.311 min  
Delta R.T.: -0.007 min  
Response: 430770  
Conc: 24.47 ng/ml