

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011822\
 Data File : P0084331.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jan 2022 19:22
 Operator : AJ\MA
 Sample : N1154-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20220011-KEANSBURG-1-SITE-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 14:25:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 18 03:56:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	6.520	5.307	1700175	497590	22.616	22.302
2) SA Decachlor...	13.762	11.309	924985	350947	20.557	19.935

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011822\
Data File : P0084331.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jan 2022 19:22
Operator : AJ\MA
Sample : N1154-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20220011-KEANSBURG-1-SITE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 14:25:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 18 03:56:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

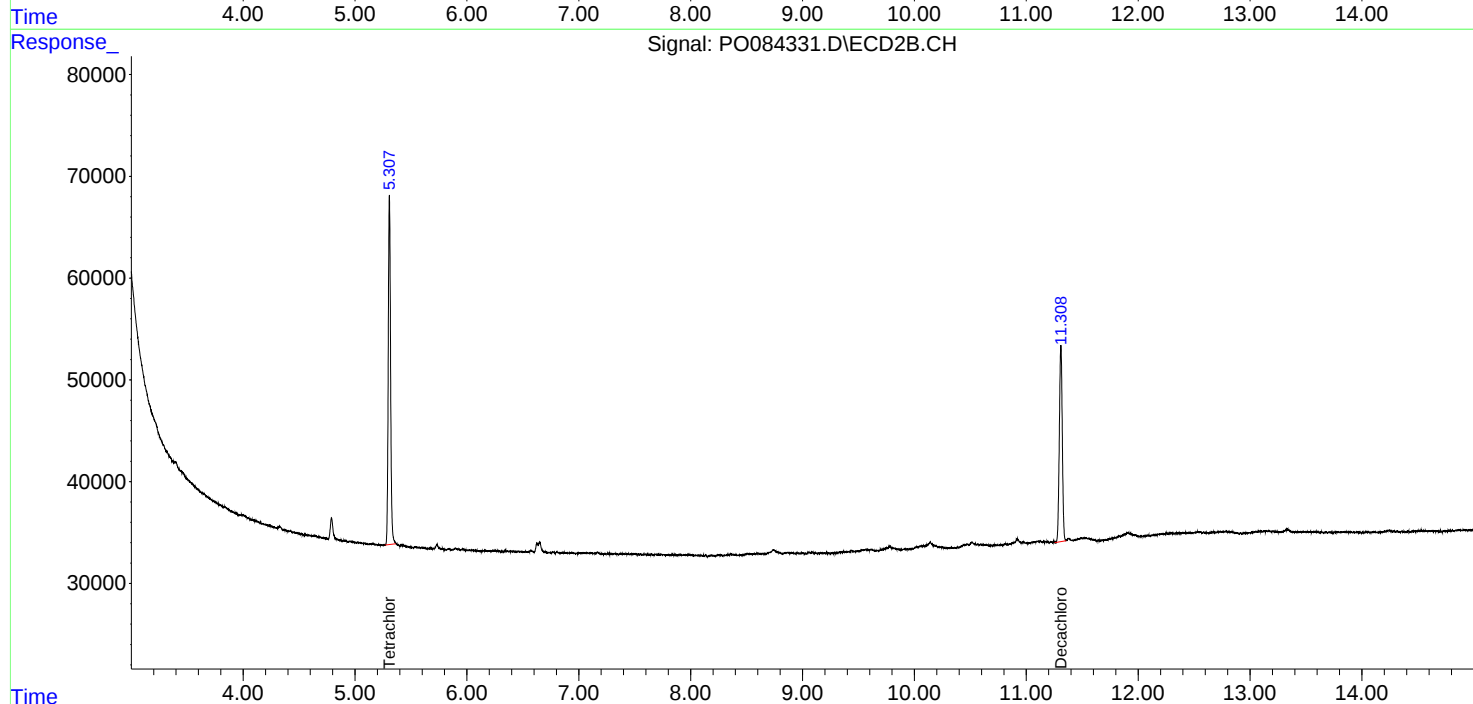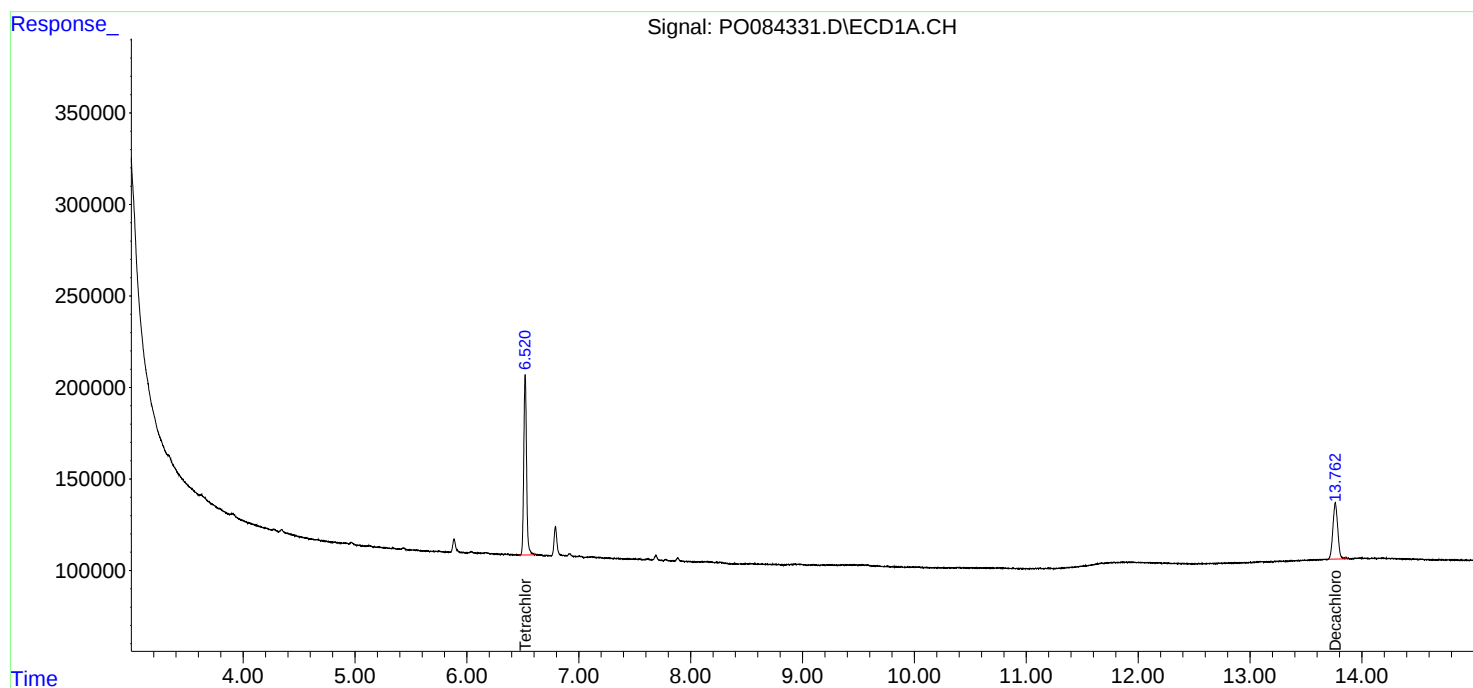


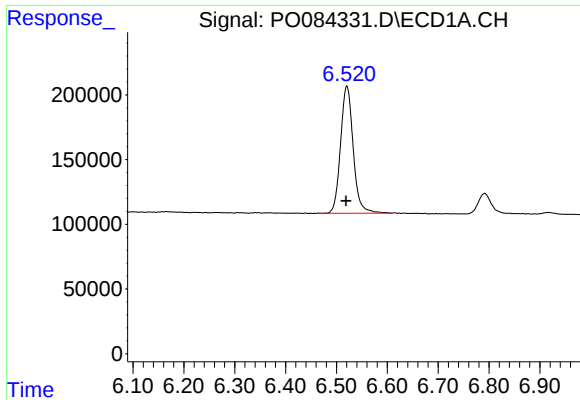

#1 Tetrachloro-m-xylene


R.T.: 6.520 min
Delta R.T.: 0.001 min
Response: 1700175
Conc: 22.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
20220011-KEANSBURG-1-SITE-WATER

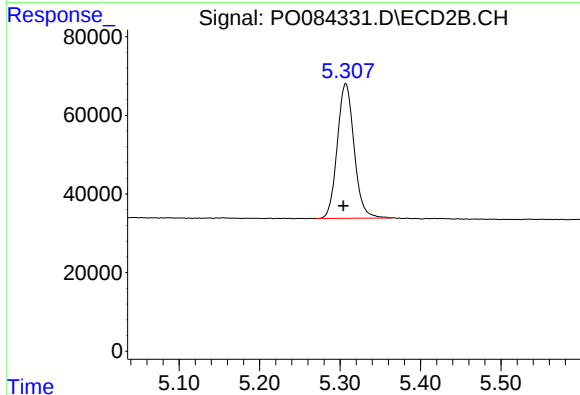


#1 Tetrachloro-m-xylene

R.T.: 5.307 min
Delta R.T.: 0.003 min
Response: 497590
Conc: 22.30 ng/ml

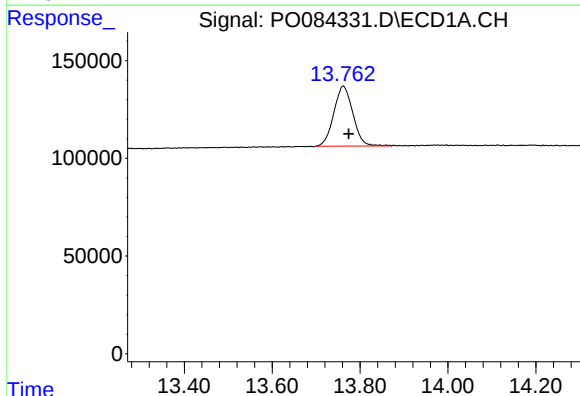

#2 Decachlorobiphenyl

R.T.: 13.762 min
Delta R.T.: -0.012 min
Response: 924985
Conc: 20.56 ng/ml

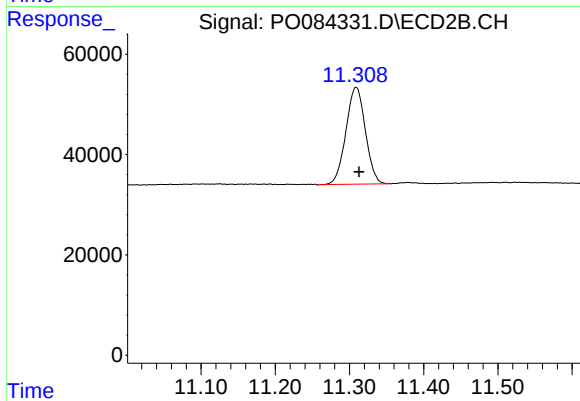

#2 Decachlorobiphenyl

R.T.: 11.309 min
Delta R.T.: -0.004 min
Response: 350947
Conc: 19.93 ng/ml