

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011822\
 Data File : P0084339.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jan 2022 22:10
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/19/2022
 Supervised By :Ankita Jodhani 01/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 14:26:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 18 03:56:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	6.517	5.303	1568737	440407	20.868	19.739
2) SA Decachlor...	13.755f	11.305	1052755	411237	23.397	23.359

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0011822\
Data File : P0084339.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jan 2022 22:10
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_0
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/19/2022
Supervised By :Ankita Jodhani 01/19/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 14:26:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0011722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 18 03:56:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

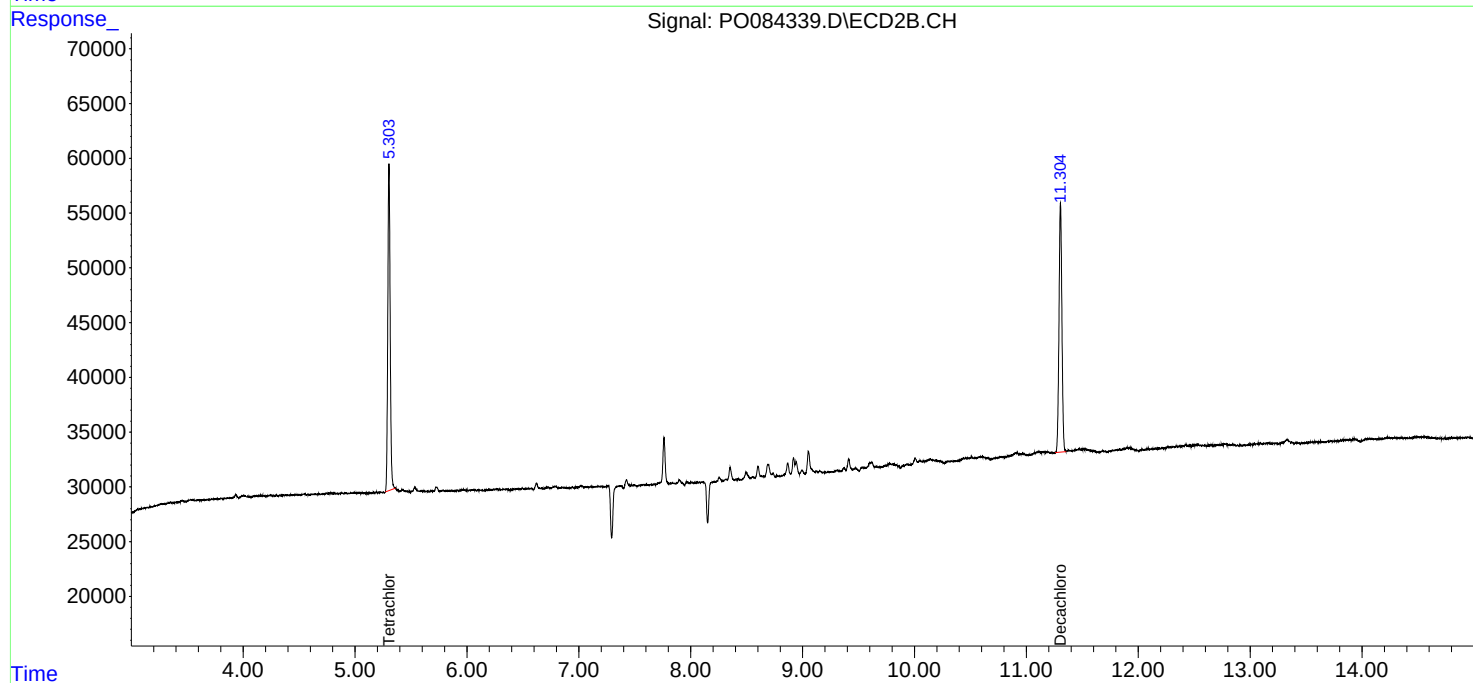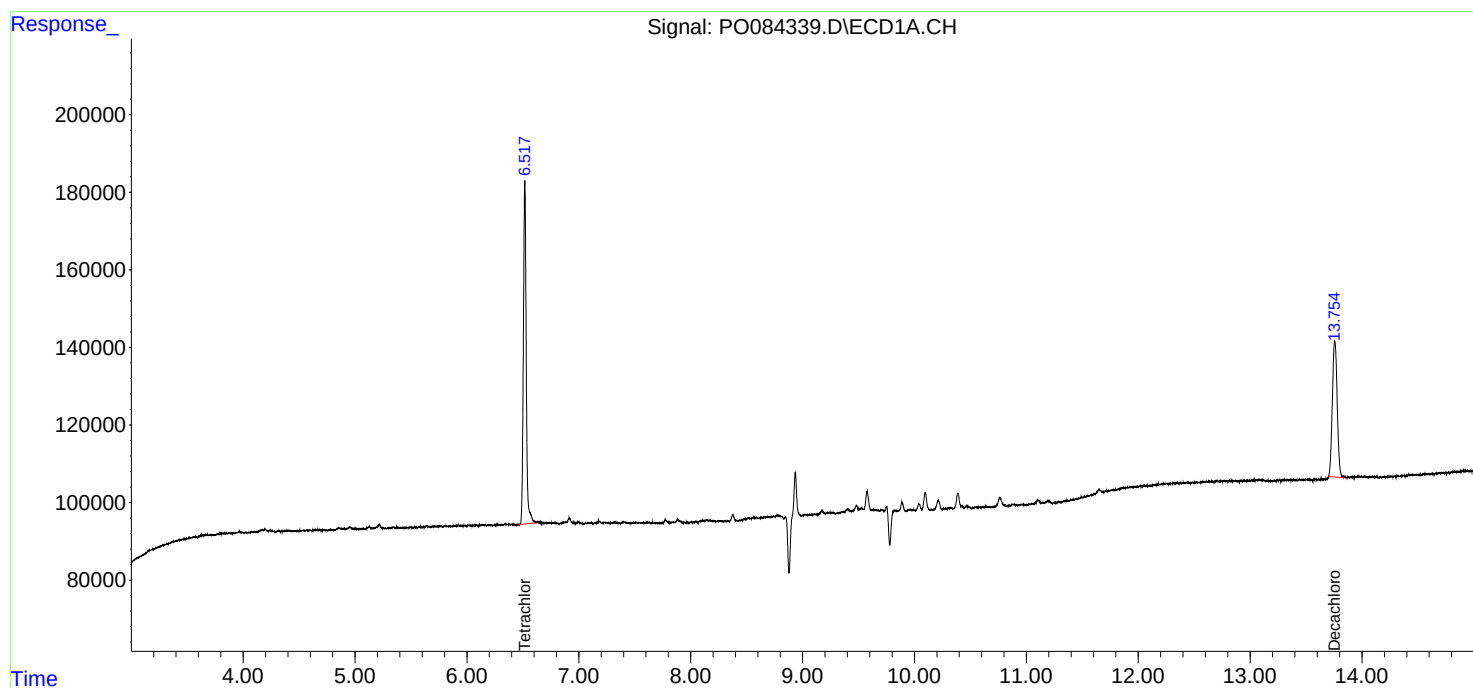

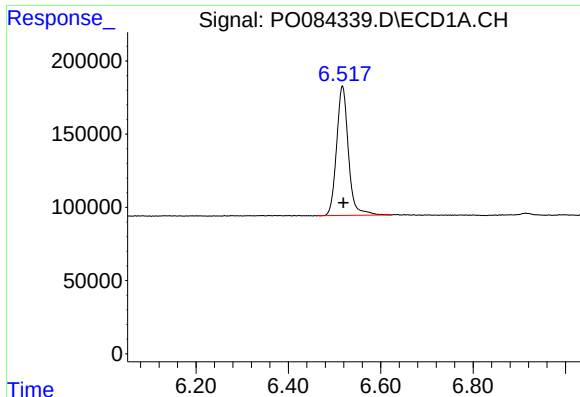


#1 Tetrachloro-m-xylene

R.T.: 6.517 min
Delta R.T.: -0.002 min
Response: 1568737
Conc: 20.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/19/2022
Supervised By :Ankita Jodhani 01/19/2022

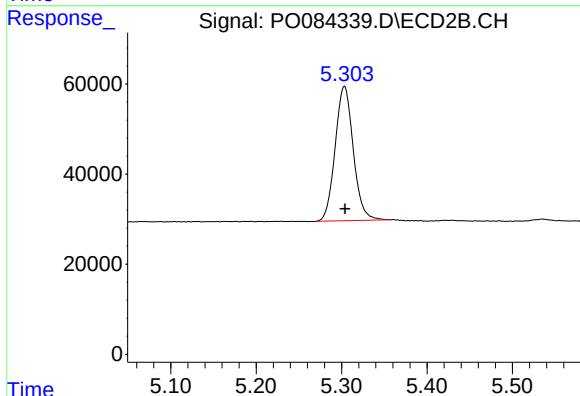


#1 Tetrachloro-m-xylene

R.T.: 5.303 min
Delta R.T.: 0.000 min
Response: 440407
Conc: 19.74 ng/ml

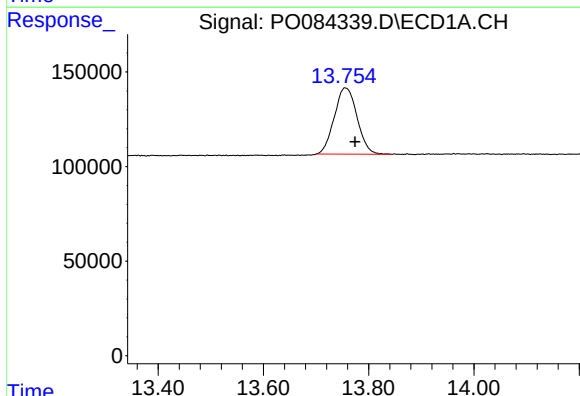

#2 Decachlorobiphenyl

R.T.: 13.755 min
Delta R.T.: -0.019 min
Response: 1052755
Conc: 23.40 ng/ml

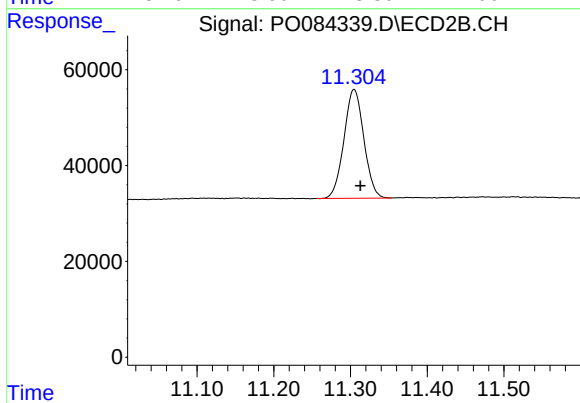

#2 Decachlorobiphenyl

R.T.: 11.305 min
Delta R.T.: -0.008 min
Response: 411237
Conc: 23.36 ng/ml