

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011823\
 Data File : P0092123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2023 14:09
 Operator : YP/AJ
 Sample : 01173-02 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FDH135Y-END-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/19/2023
 Supervised By :Ankita Jodhani 01/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 16:32:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 11 04:41:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.448	3.648	4098023	2014715	1.469	1.451
2) SA Decachlor...	10.366	8.697	4219826	2417941	2.156	2.727m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011823\
Data File : PO092123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2023 14:09
Operator : YP/AJ
Sample : 01173-02 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FDH135Y-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/19/2023
Supervised By :Ankita Jodhani 01/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 16:32:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 11 04:41:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

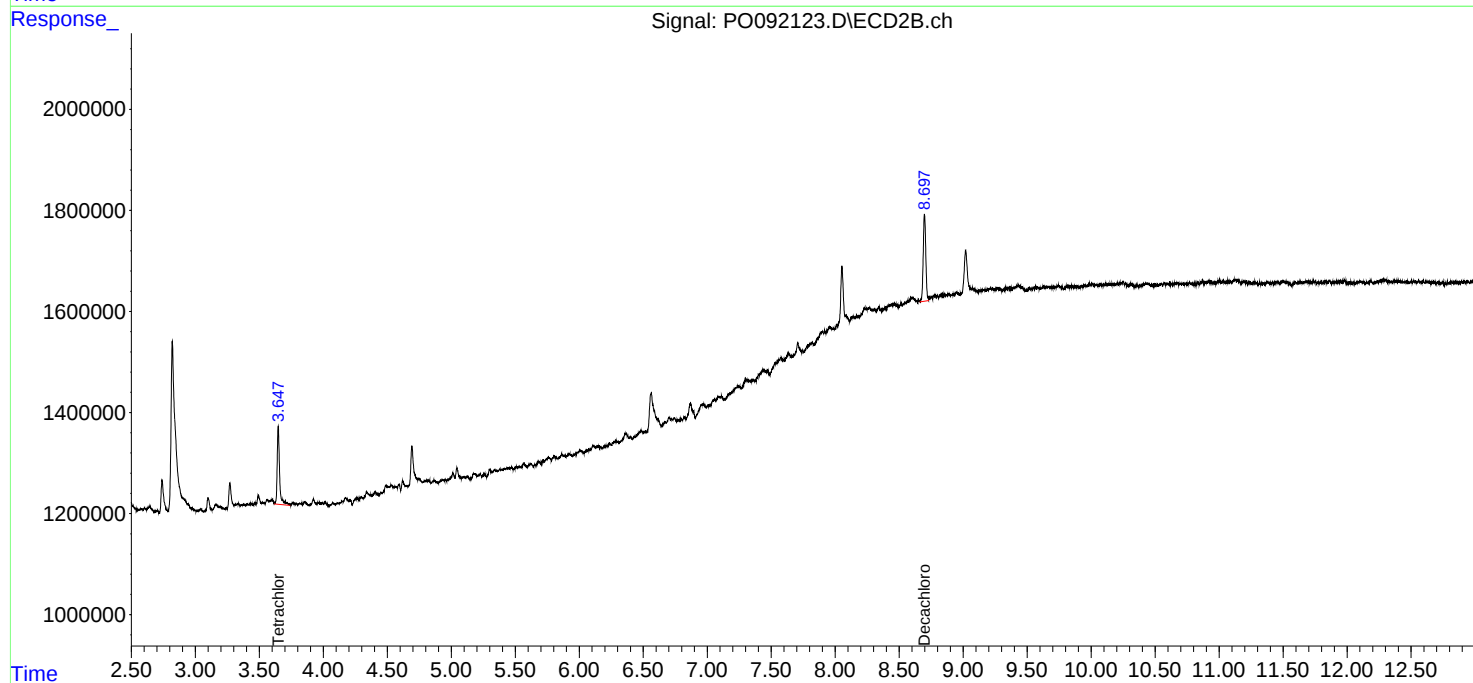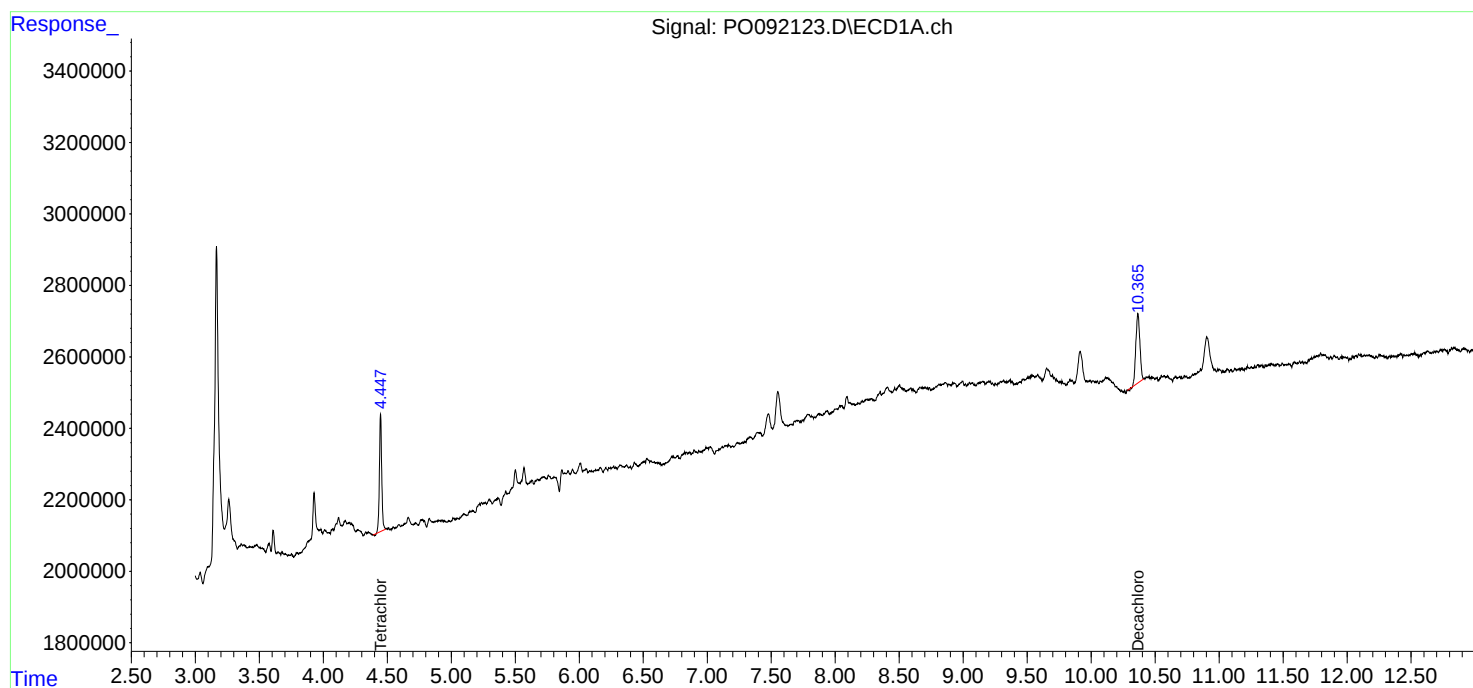

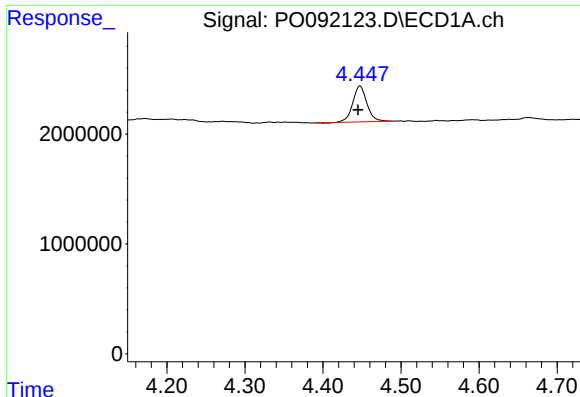


#1 Tetrachloro-m-xylene

R.T.: 4.448 min
Delta R.T.: 0.003 min
Response: 4098023
Conc: 1.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
FDH135Y-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/19/2023
Supervised By :Ankita Jodhani 01/19/2023

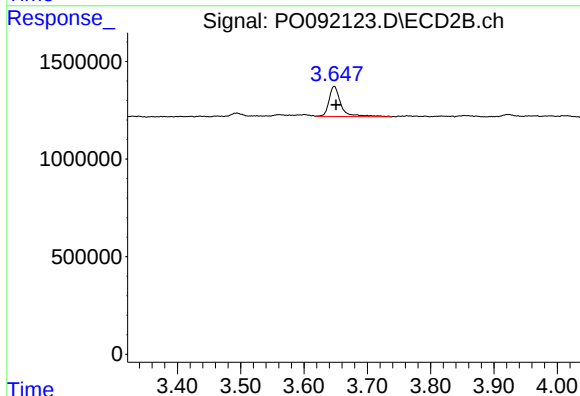


#1 Tetrachloro-m-xylene

R.T.: 3.648 min
Delta R.T.: -0.003 min
Response: 2014715
Conc: 1.45 ng/ml

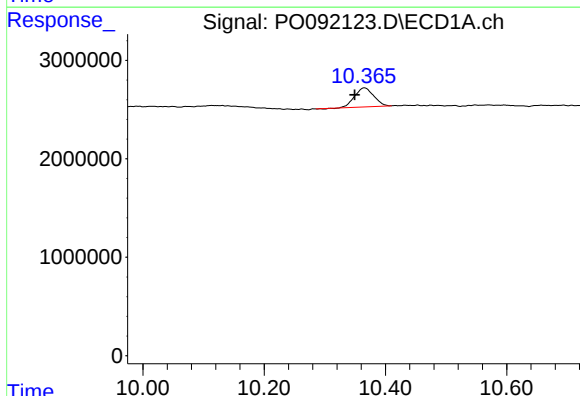

#2 Decachlorobiphenyl

R.T.: 10.366 min
Delta R.T.: 0.016 min
Response: 4219826
Conc: 2.16 ng/ml

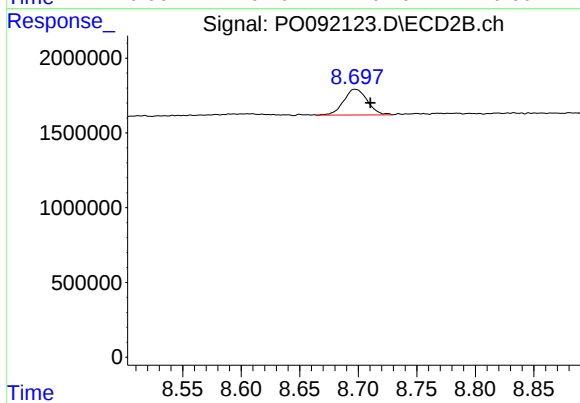

#2 Decachlorobiphenyl

R.T.: 8.697 min
Delta R.T.: -0.014 min
Response: 2417941
Conc: 2.73 ng/ml m