

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011823\
 Data File : P0092157.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jan 2023 01:18
 Operator : YP/AJ
 Sample : 01174-10 10X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IRV-2023-5B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/19/2023
 Supervised By :Ankita Jodhani 01/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 03:38:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 11 04:41:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.447	3.646	4139763	1709792	1.484	1.232
2) SA Decachlor...	10.366	8.693	5361818	2223094	2.739	2.507m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011823\
Data File : PO092157.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jan 2023 01:18
Operator : YP/AJ
Sample : 01174-10 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
IRV-2023-5B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/19/2023
Supervised By :Ankita Jodhani 01/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 03:38:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 11 04:41:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

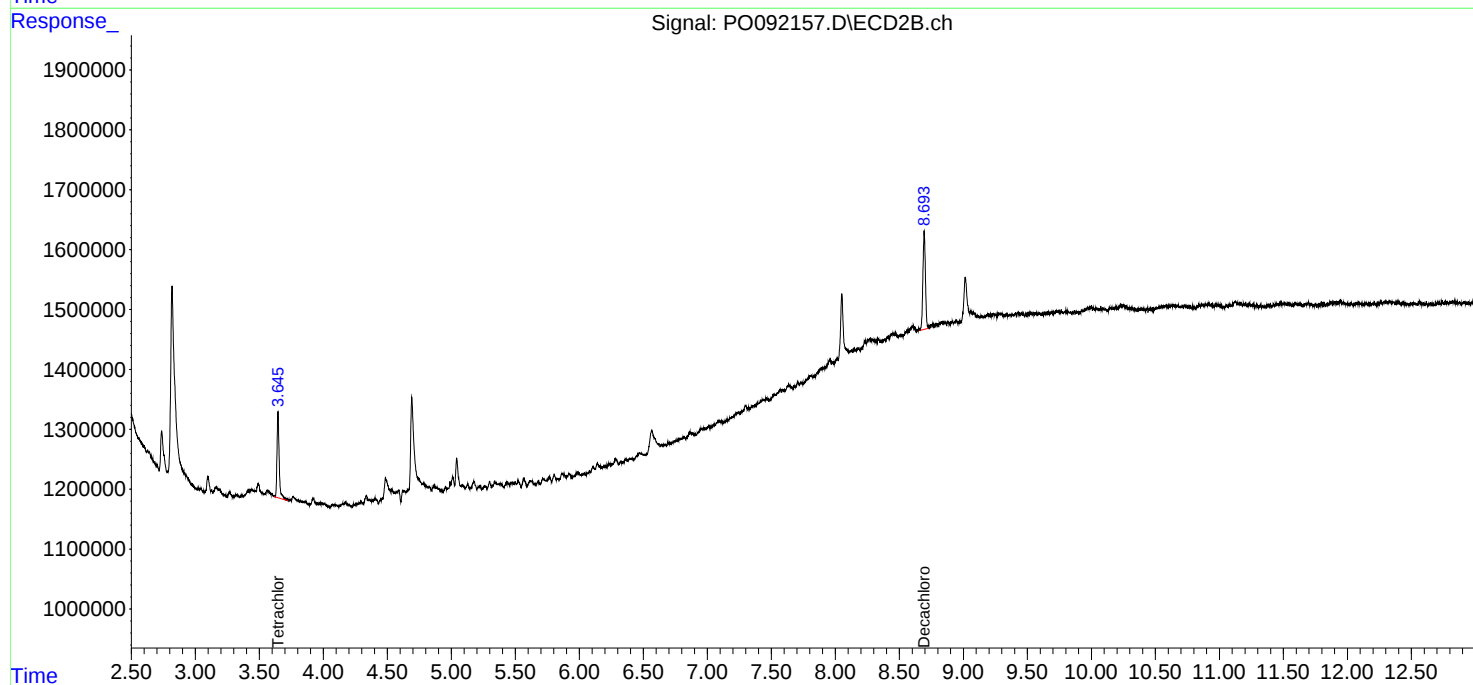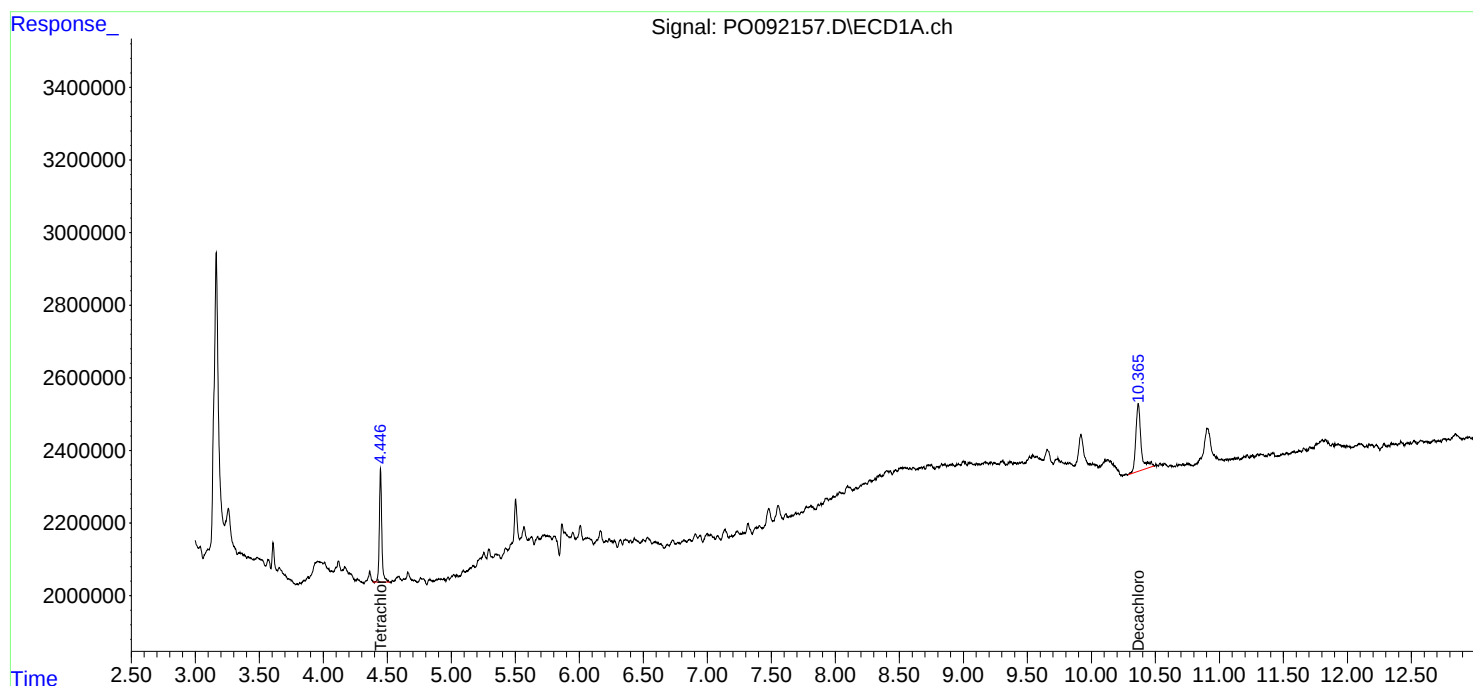

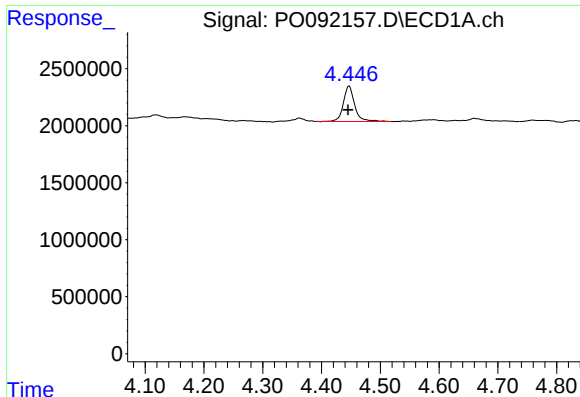

#1 Tetrachloro-m-xylene

R.T.: 4.447 min
Delta R.T.: 0.002 min
Response: 4139763
Conc: 1.48 ng/ml

Instrument :

ECD_O


ClientSampleId :

IRV-2023-5B

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 01/19/2023
Supervised By :Ankita Jodhani 01/19/2023

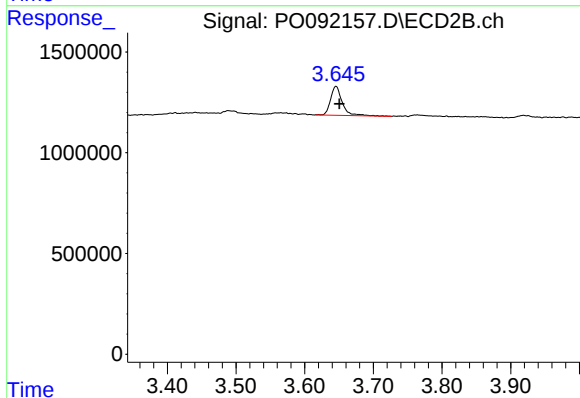


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: -0.005 min
Response: 1709792
Conc: 1.23 ng/ml

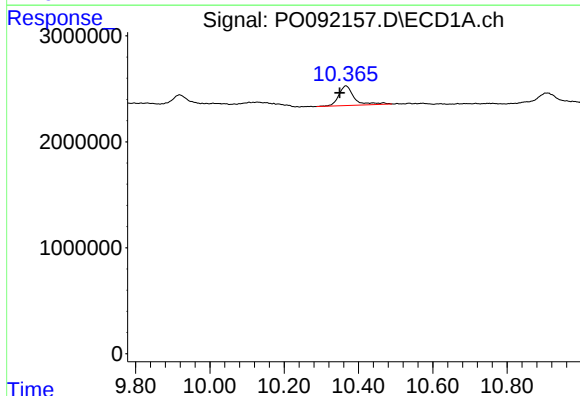

#2 Decachlorobiphenyl

R.T.: 10.366 min
Delta R.T.: 0.017 min
Response: 5361818
Conc: 2.74 ng/ml

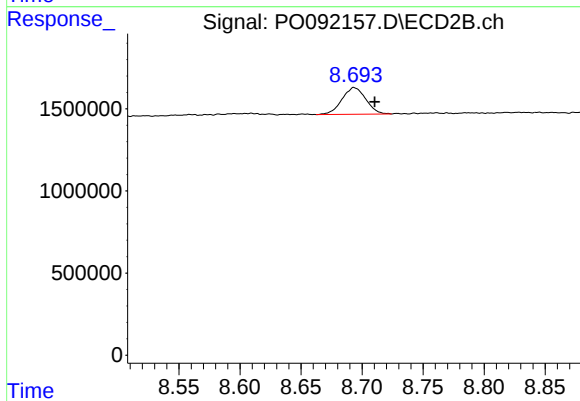

#2 Decachlorobiphenyl

R.T.: 8.693 min
Delta R.T.: -0.018 min
Response: 2223094
Conc: 2.51 ng/ml m