

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011921\
 Data File : P0074927.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jan 2021 9:53
 Operator : AJ/MA
 Sample : M1082-03RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 03:38:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.928	4.000	2450248	1241010	23.221	22.062
2)	SA Decachlor...	10.942	9.252	2320821	1189105	22.867	21.658
Target Compounds							
8)	L2 AR-1221-1	5.183	0.000	84779	0	69.022	N.D. #
30)	L6 AR-1254-5	8.507	0.000	42081	0	7.244	N.D. #
35)	L7 AR-1260-5	0.000	7.892	0	30606	N.D.	3.850 #
37)	L8 AR-1262-2	0.000	7.892	0	30606	N.D.	3.329 #
39)	L8 AR-1262-4	9.517f	0.000	65636	0	8.813	N.D. #
42)	L9 AR-1268-2	9.517f	0.000	65636	0	4.114	N.D. #
45)	L9 AR-1268-5	0.000	9.014	0	5764	N.D.	0.243 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011921\
Data File : PO074927.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jan 2021 9:53
Operator : AJ/MA
Sample : M1082-03RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 03:38:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

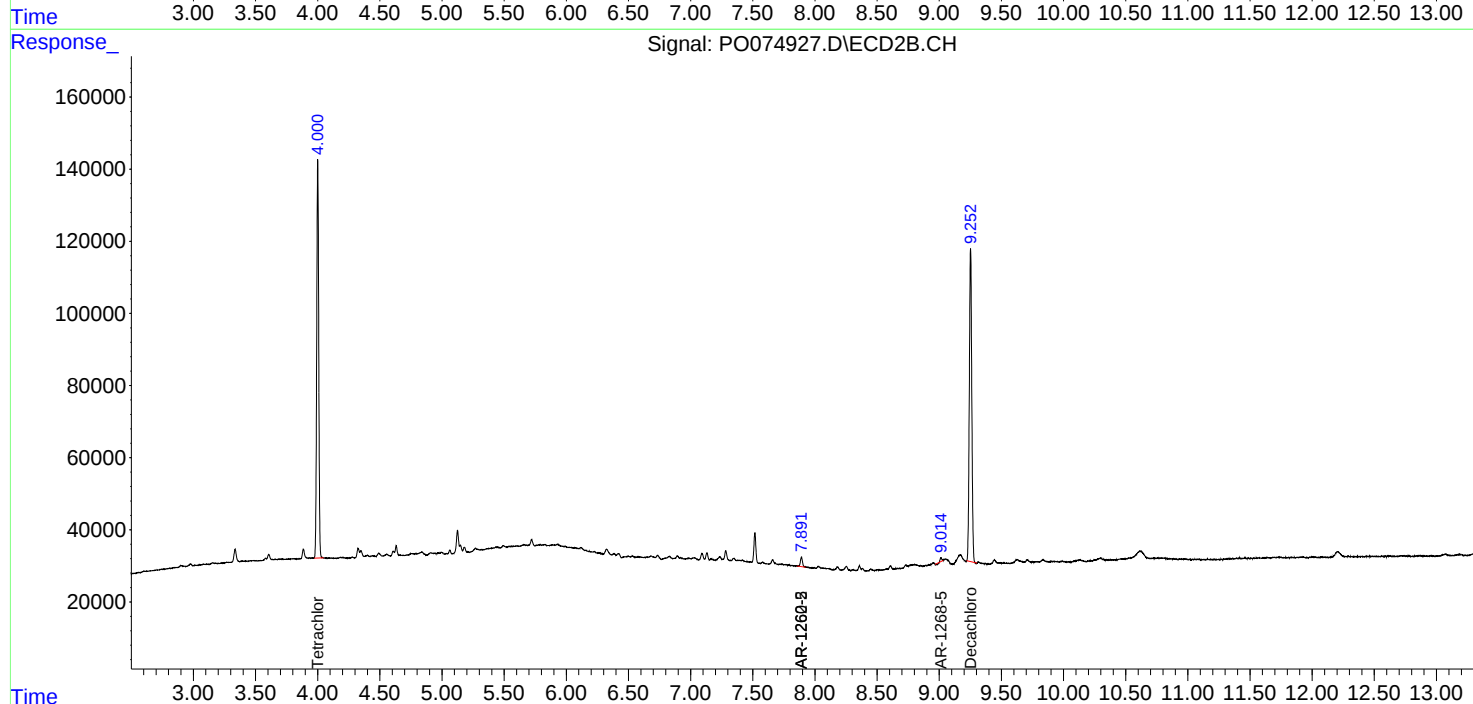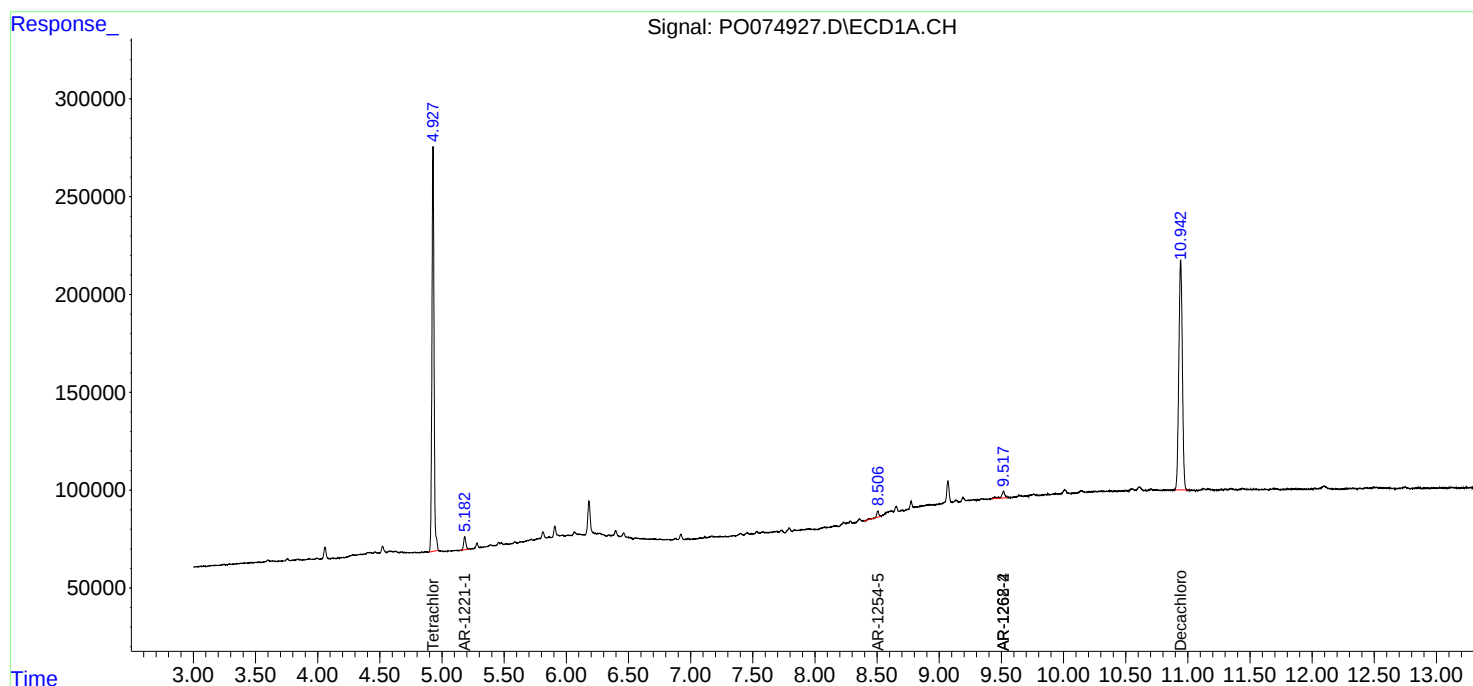


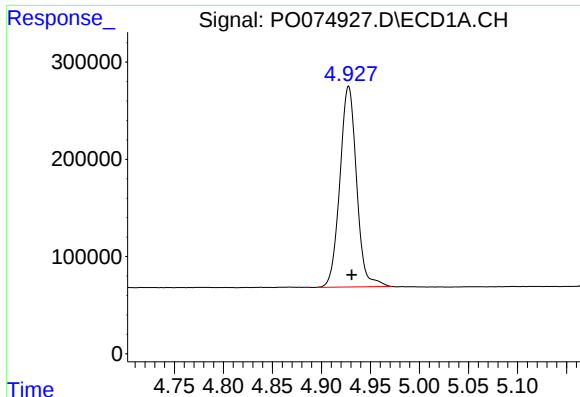

#1 Tetrachloro-m-xylene


R.T.: 4.928 min
Delta R.T.: -0.003 min
Response: 2450248
Conc: 23.22 ng/ml

Instrument :
ECD_O
ClientSampleId :

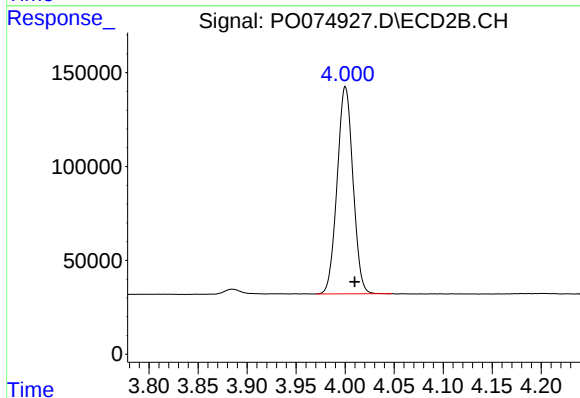


#1 Tetrachloro-m-xylene

R.T.: 4.000 min
Delta R.T.: -0.009 min
Response: 1241010
Conc: 22.06 ng/ml

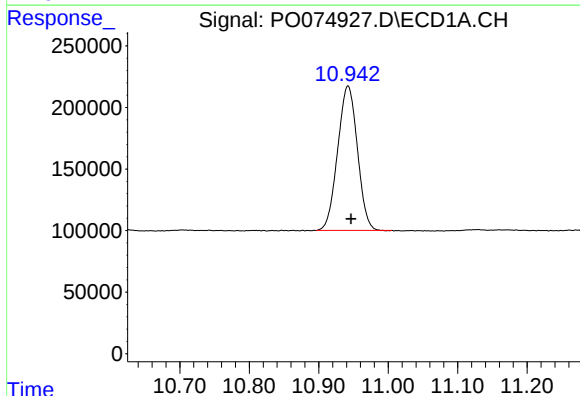


#2 Decachlorobiphenyl

R.T.: 10.942 min
Delta R.T.: -0.004 min
Response: 2320821
Conc: 22.87 ng/ml

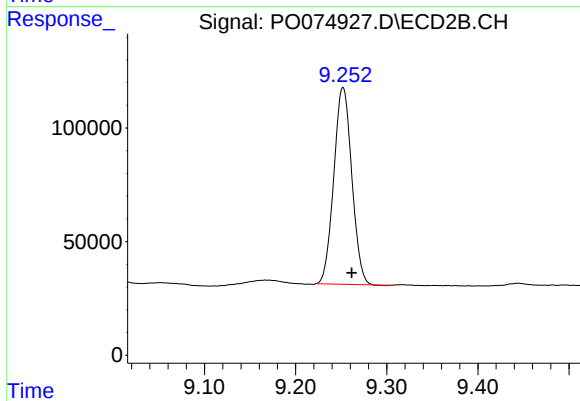

#2 Decachlorobiphenyl


R.T.: 9.252 min
Delta R.T.: -0.009 min
Response: 1189105
Conc: 21.66 ng/ml

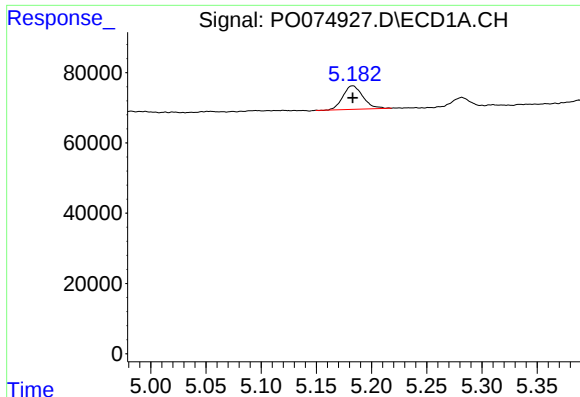

#8 AR-1221-1


R.T.: 5.183 min
Delta R.T.: 0.000 min
Response: 84779
Conc: 69.02 ng/ml

Instrument :
ECD_O
ClientSampleId :

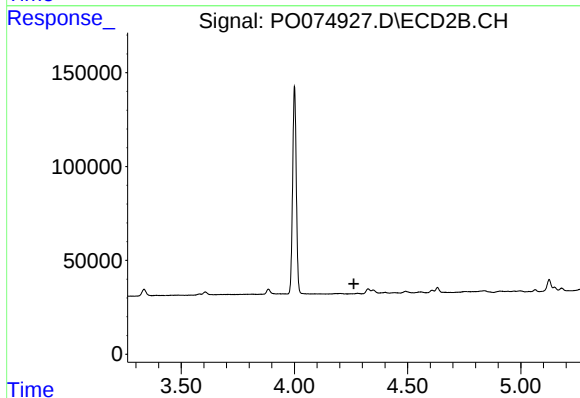


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.263 min
Response: 0
Conc: N.D.

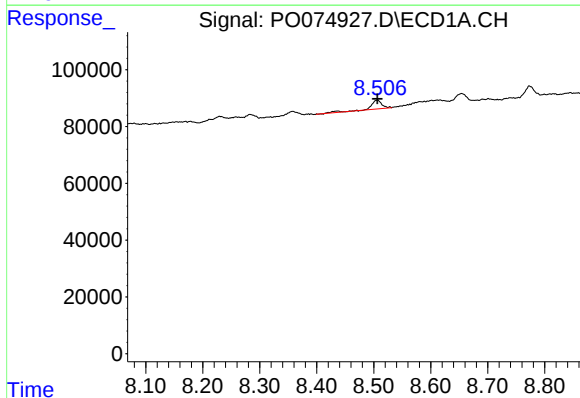


#30 AR-1254-5

R.T.: 8.507 min
Delta R.T.: 0.000 min
Response: 42081
Conc: 7.24 ng/ml

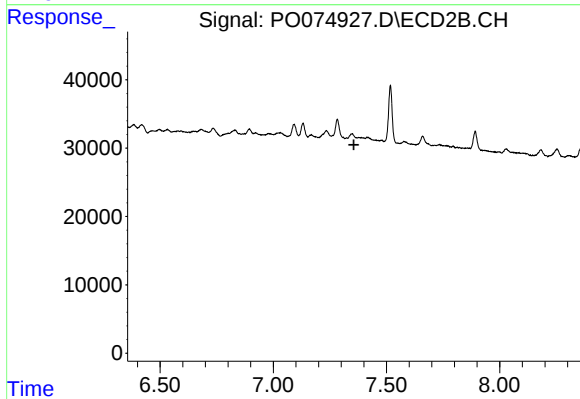

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.356 min
Response: 0
Conc: N.D.

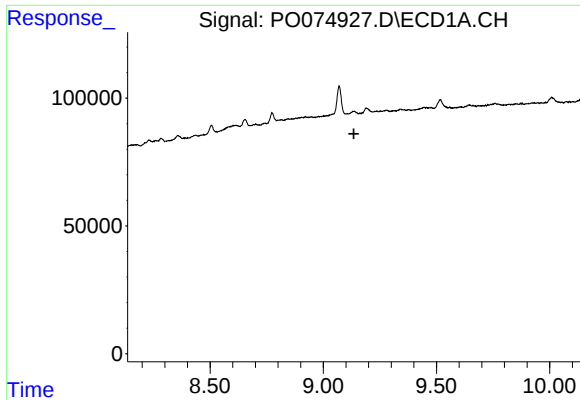

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 9.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

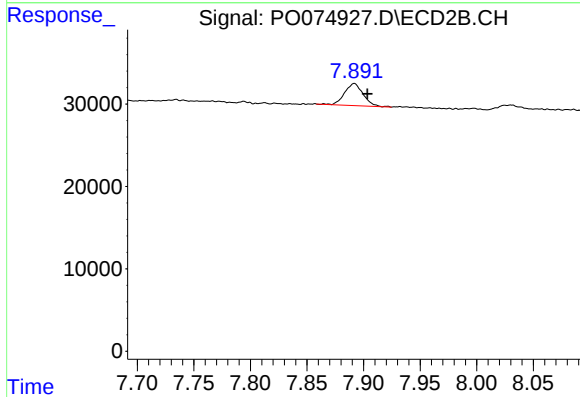


#35 AR-1260-5

R.T.: 7.892 min
Delta R.T.: -0.012 min
Response: 30606
Conc: 3.85 ng/ml

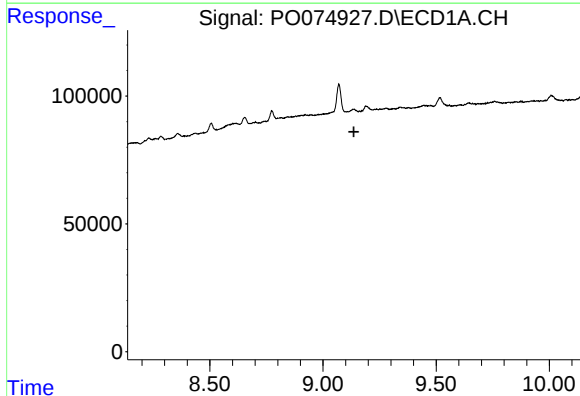


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 9.136 min
Response: 0
Conc: N.D.

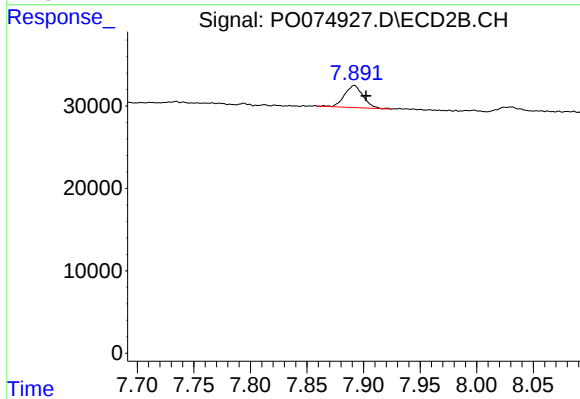

#37 AR-1262-2


R.T.: 7.892 min
Delta R.T.: -0.010 min
Response: 30606
Conc: 3.33 ng/ml

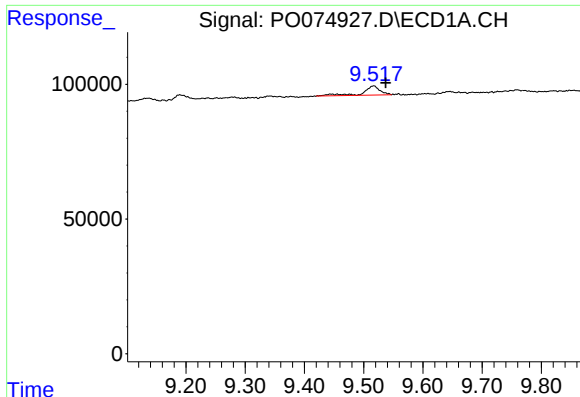

#39 AR-1262-4


R.T.: 9.517 min
Delta R.T.: -0.020 min
Response: 65636
Conc: 8.81 ng/ml

Instrument :
ECD_O
ClientSampleId :

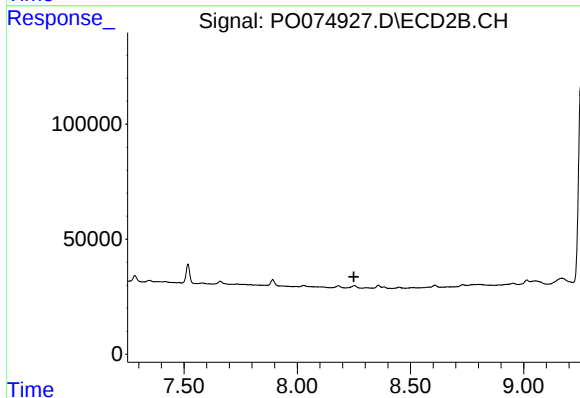


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.250 min
Response: 0
Conc: N.D.

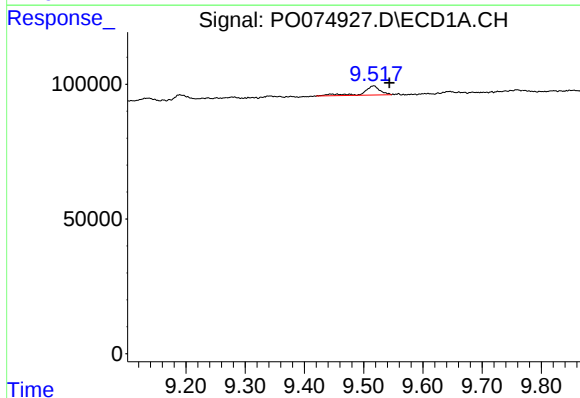


#42 AR-1268-2

R.T.: 9.517 min
Delta R.T.: -0.026 min
Response: 65636
Conc: 4.11 ng/ml

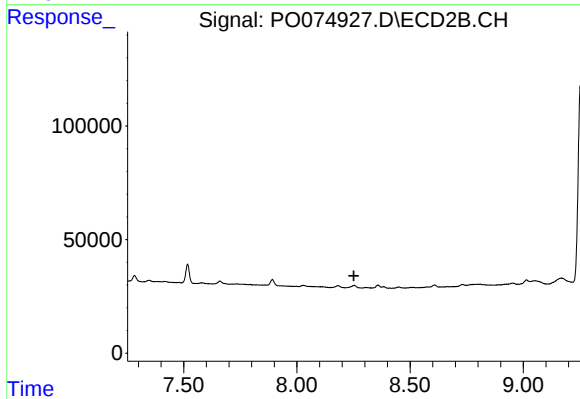

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.252 min
Response: 0
Conc: N.D.

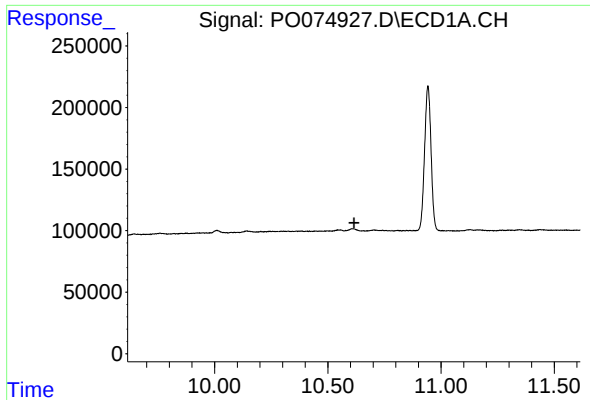

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.616 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

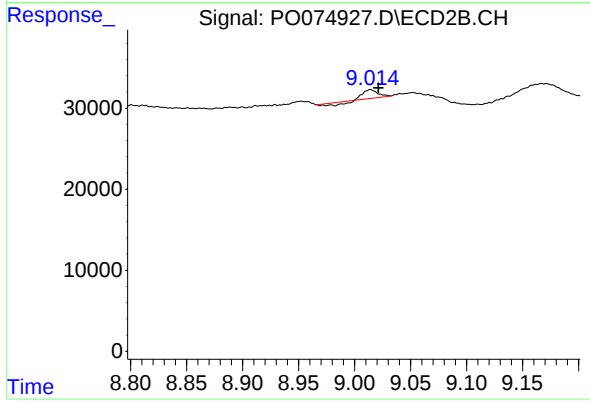

#45 AR-1268-5

R.T.: 9.014 min
Delta R.T.: -0.007 min
Response: 5764
Conc: 0.24 ng/ml