

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011921\
 Data File : P0074949.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jan 2021 16:44
 Operator : AJ/MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 03:48:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.927	4.001	2135481	1103890	20.238	19.624
2)	SA Decachlor...	10.942	9.252	2040505	1036799	20.105	18.884
Target Compounds							
20)	L4 AR-1242-5	0.000	6.132	0	36231	N.D.	20.693 #
24)	L5 AR-1248-4	7.169f	0.000	109425	0	24.538	N.D. #
25)	L5 AR-1248-5	0.000	6.132f	0	36231	N.D.	15.411 #
26)	L6 AR-1254-1	7.169	6.132	109425	36231	24.880	10.031 #
29)	L6 AR-1254-4	8.075	0.000	16751	0	2.762	N.D. #
30)	L6 AR-1254-5	8.503	0.000	27004	0	4.649	N.D. #
32)	L7 AR-1260-2	8.209	0.000	22972	0	3.377	N.D. #
45)	L9 AR-1268-5	0.000	9.012	0	28696	N.D.	1.212 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011921\
Data File : P0074949.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jan 2021 16:44
Operator : AJ/MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 03:48:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

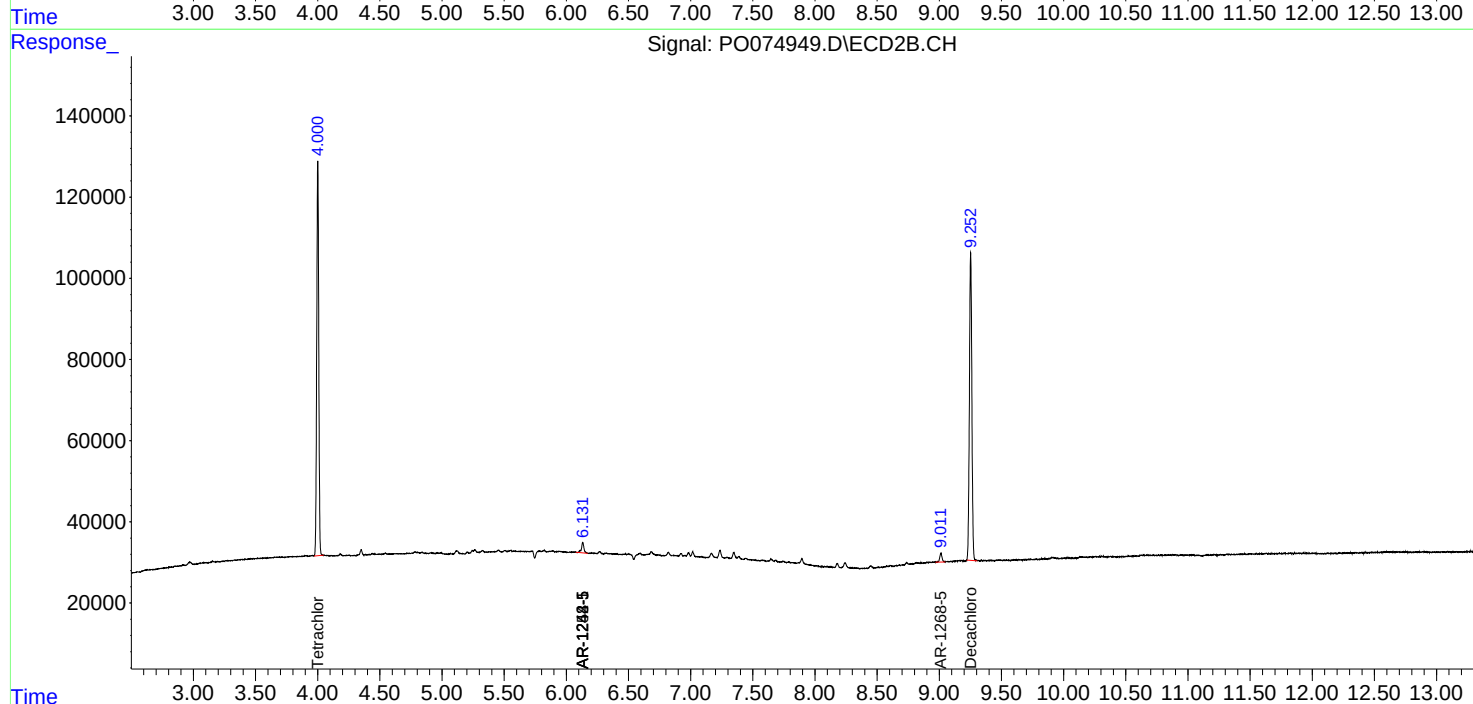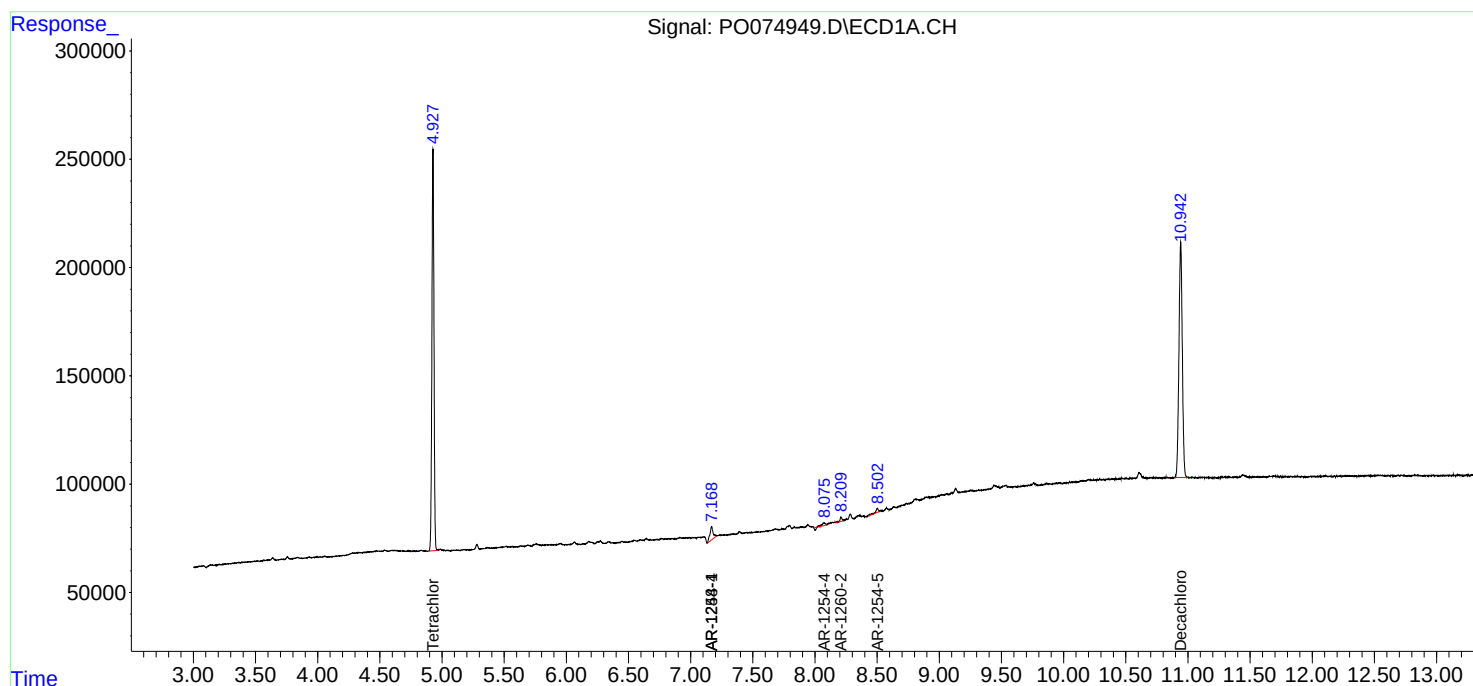


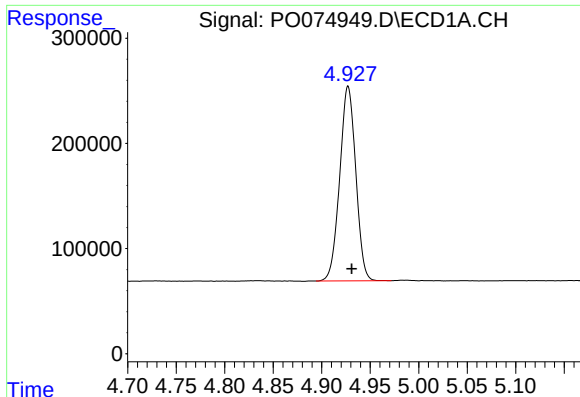

#1 Tetrachloro-m-xylene


R.T.: 4.927 min
Delta R.T.: -0.004 min
Response: 2135481
Conc: 20.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

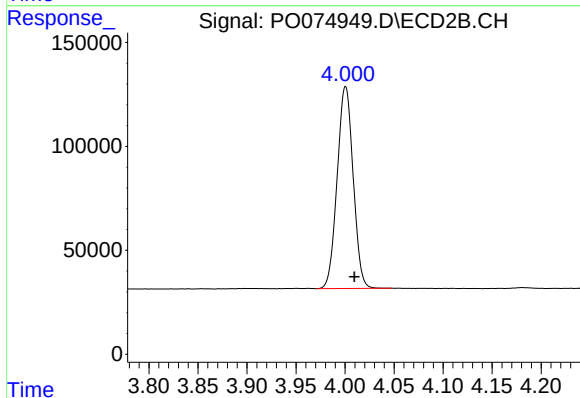


#1 Tetrachloro-m-xylene

R.T.: 4.001 min
Delta R.T.: -0.009 min
Response: 1103890
Conc: 19.62 ng/ml

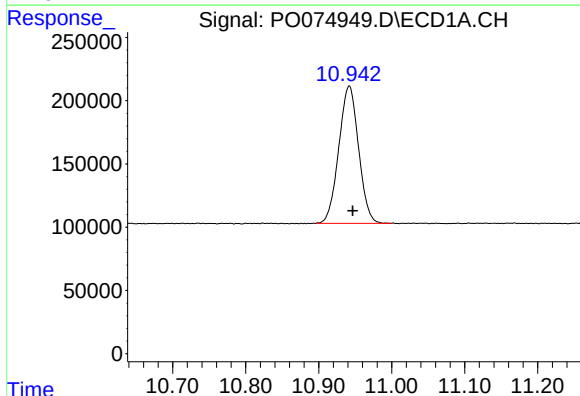


#2 Decachlorobiphenyl

R.T.: 10.942 min
Delta R.T.: -0.004 min
Response: 2040505
Conc: 20.11 ng/ml

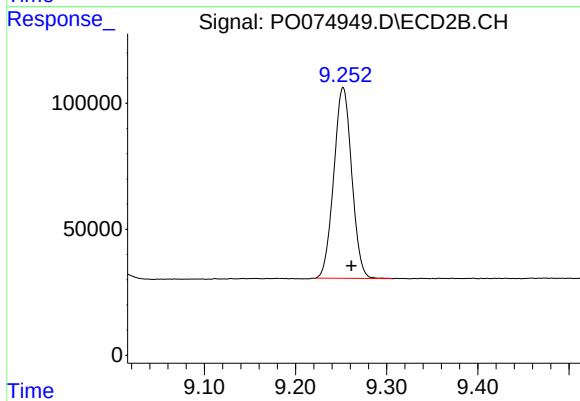

#2 Decachlorobiphenyl


R.T.: 9.252 min
Delta R.T.: -0.009 min
Response: 1036799
Conc: 18.88 ng/ml

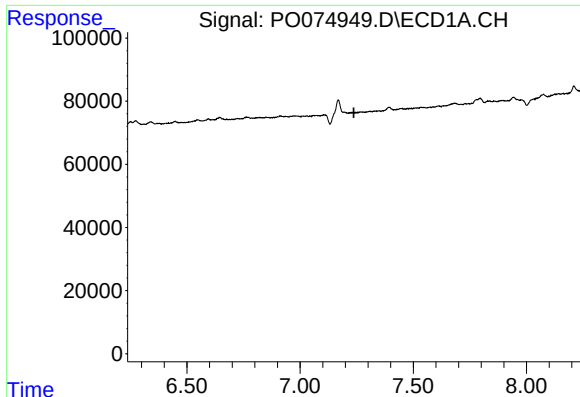

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.238 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

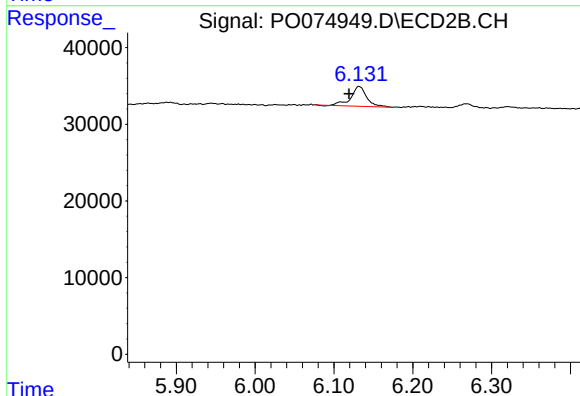


#20 AR-1242-5

R.T.: 6.132 min
Delta R.T.: 0.013 min
Response: 36231
Conc: 20.69 ng/ml

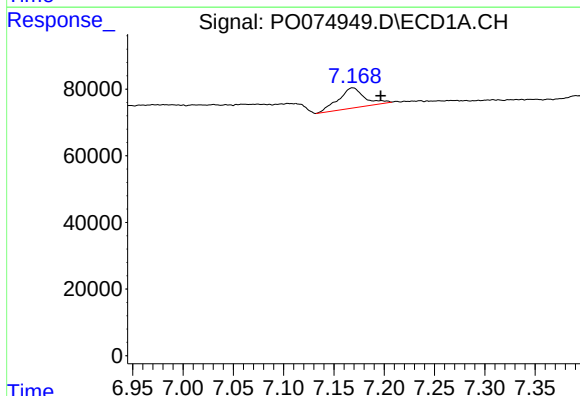


#24 AR-1248-4

R.T.: 7.169 min
Delta R.T.: -0.028 min
Response: 109425
Conc: 24.54 ng/ml

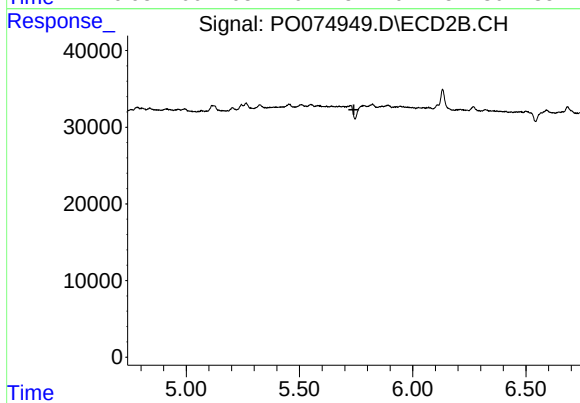

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.740 min
Response: 0
Conc: N.D.

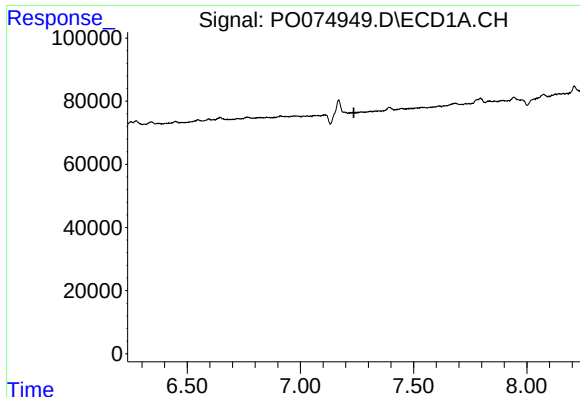

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.236 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

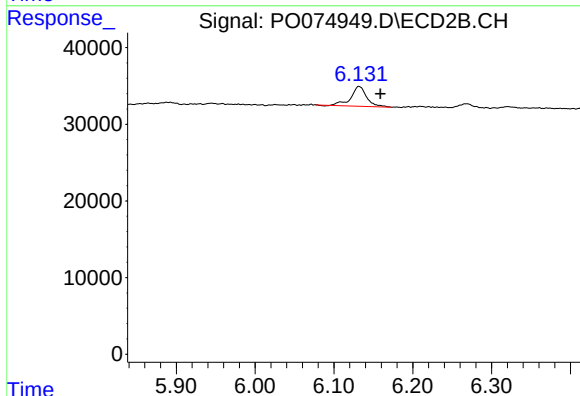


#25 AR-1248-5

R.T.: 6.132 min
Delta R.T.: -0.027 min
Response: 36231
Conc: 15.41 ng/ml

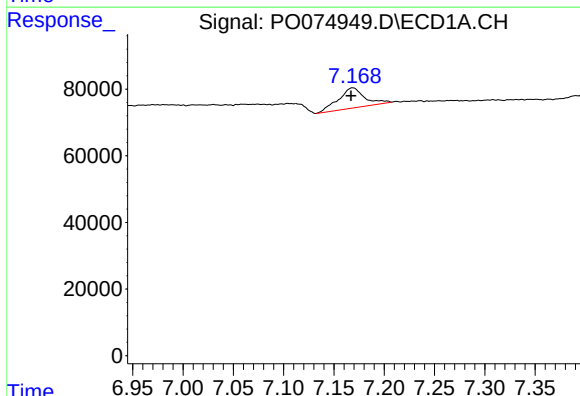


#26 AR-1254-1

R.T.: 7.169 min
Delta R.T.: 0.001 min
Response: 109425
Conc: 24.88 ng/ml

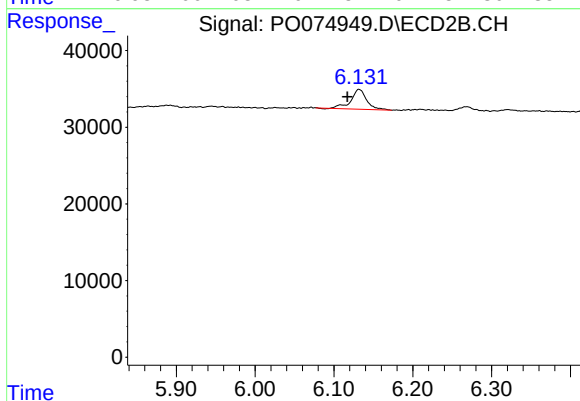

#26 AR-1254-1


R.T.: 6.132 min
Delta R.T.: 0.015 min
Response: 36231
Conc: 10.03 ng/ml

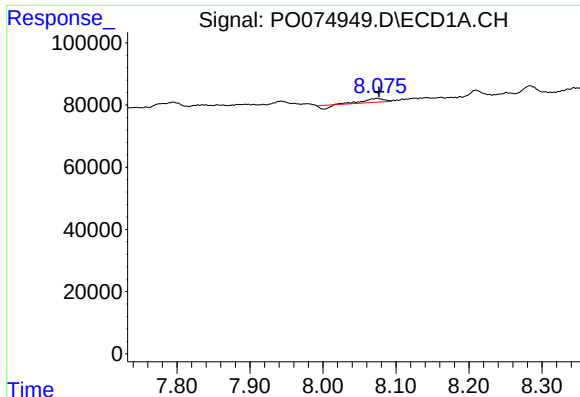

#29 AR-1254-4


R.T.: 8.075 min
Delta R.T.: -0.002 min
Response: 16751
Conc: 2.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

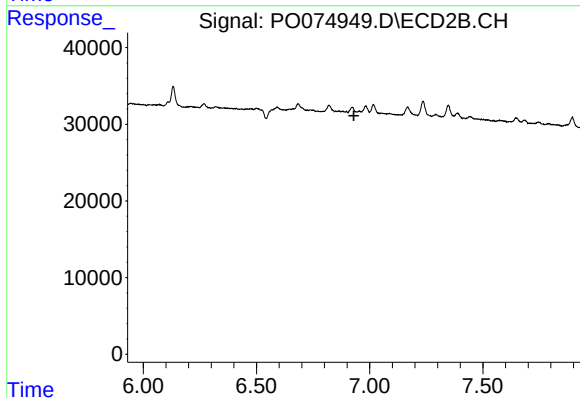


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.930 min
Response: 0
Conc: N.D.

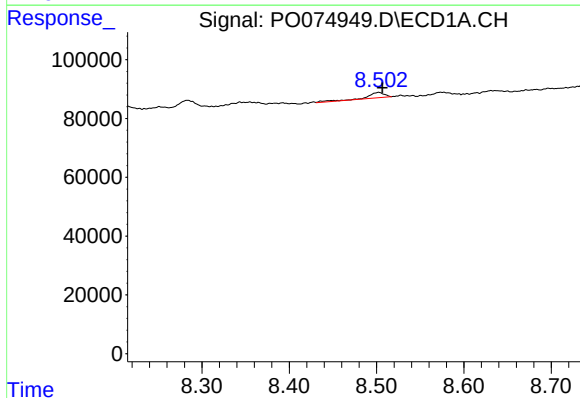


#30 AR-1254-5

R.T.: 8.503 min
Delta R.T.: -0.004 min
Response: 27004
Conc: 4.65 ng/ml

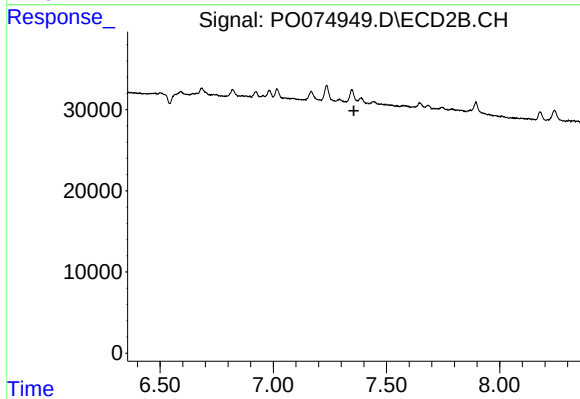

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.356 min
Response: 0
Conc: N.D.

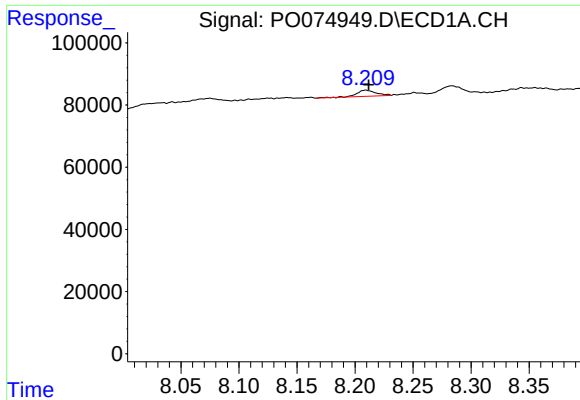

#32 AR-1260-2


R.T.: 8.209 min
Delta R.T.: -0.002 min
Response: 22972
Conc: 3.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

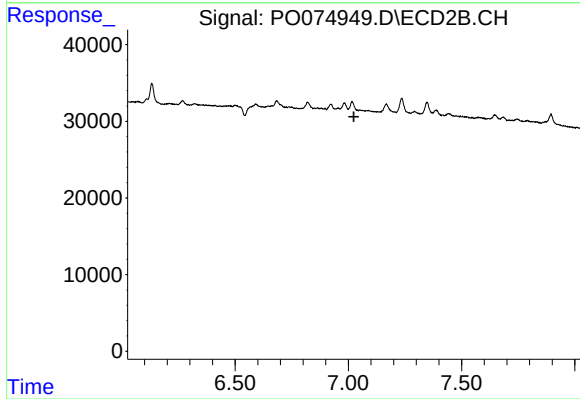


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.025 min
Response: 0
Conc: N.D.

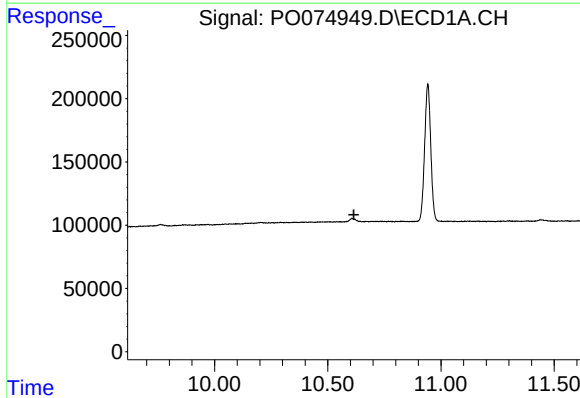

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.616 min
Response: 0
Conc: N.D.

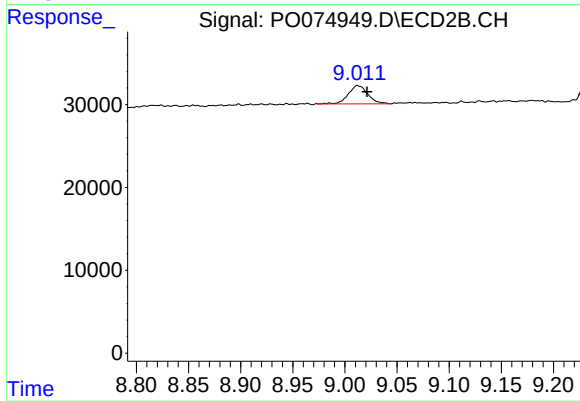

#45 AR-1268-5

R.T.: 9.012 min
Delta R.T.: -0.009 min
Response: 28696
Conc: 1.21 ng/ml