

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011921\
 Data File : P0074938.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jan 2021 13:01
 Operator : AJ/MA
 Sample : M1107-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S19-02-C

Manual Integrations
 APPROVED

Ankita
 1/20/2021 9:59:58 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 03:43:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.929	4.002	2328193	1207508	22.064	21.466
2) SA Decachlor...	10.946	9.254	2194321	1123653	21.621	20.466
Target Compounds						
41) L9 AR-1268-1	9.444	8.182	699444	423777	37.437	37.855
42) L9 AR-1268-2	9.540	8.246	459647	304066	28.809	31.782
43) L9 AR-1268-3	9.766	8.450	489015	292358	34.433	35.186m
44) L9 AR-1268-4	10.202	8.738	128601	86254	21.951	24.863
45) L9 AR-1268-5	10.613	9.015	1357578	716799	32.487	30.272

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO011921\
Data File : PO074938.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jan 2021 13:01
Operator : AJ/MA
Sample : M1107-08
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S19-02-C


Manual Integrations
APPROVED

Ankita
1/20/2021 9:59:58 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 03:43:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

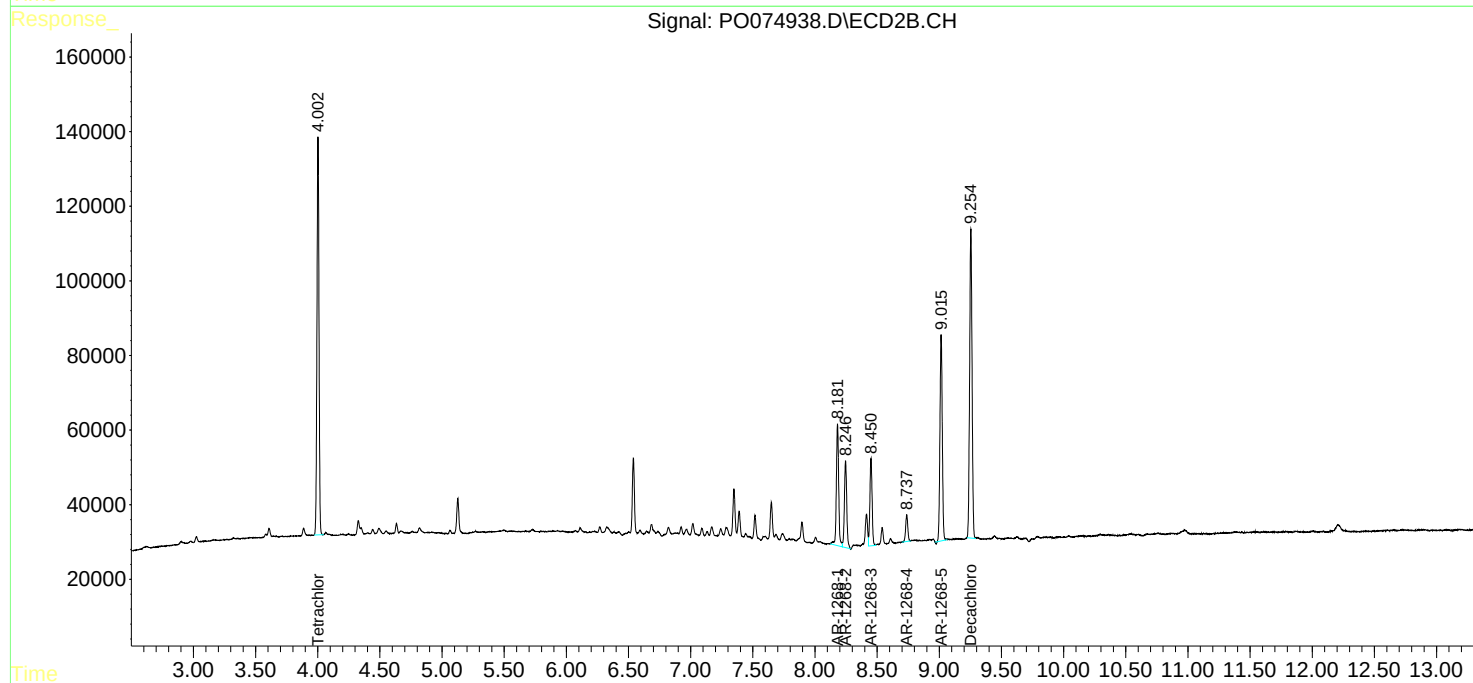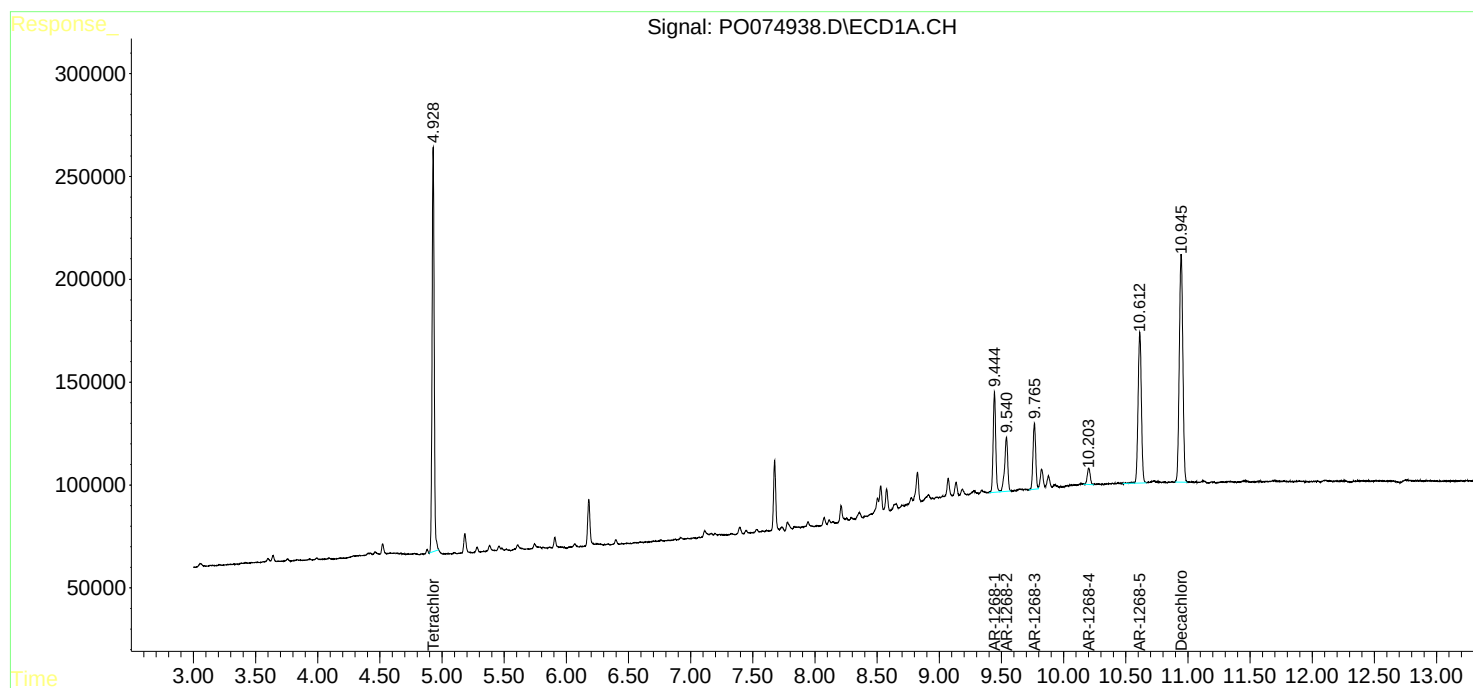

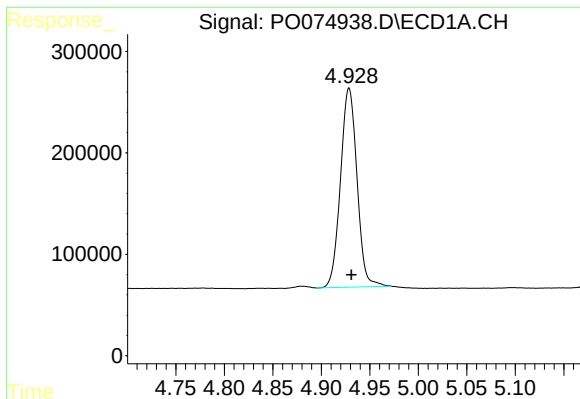


#1 Tetrachloro-m-xylene

R.T.: 4.929 min
Delta R.T.: -0.002 min
Response: 2328193
Conc: 22.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
S19-02-C


Manual Integrations
APPROVED

Ankita
1/20/2021 9:59:58 AM

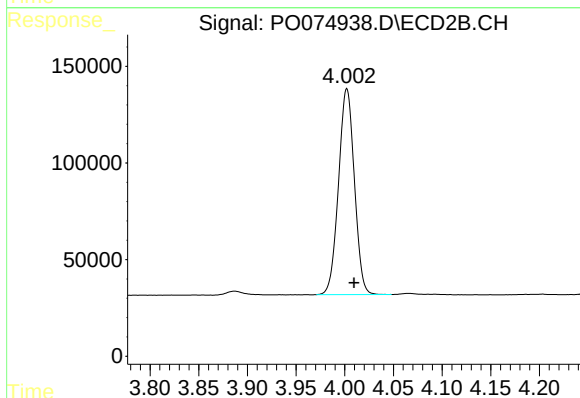


#1 Tetrachloro-m-xylene

R.T.: 4.002 min
Delta R.T.: -0.008 min
Response: 1207508
Conc: 21.47 ng/ml

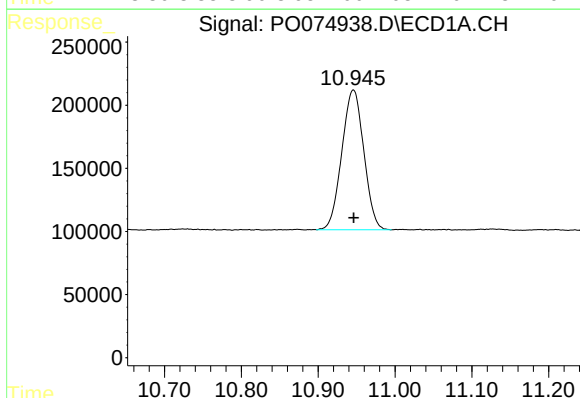


#2 Decachlorobiphenyl

R.T.: 10.946 min
Delta R.T.: 0.000 min
Response: 2194321
Conc: 21.62 ng/ml

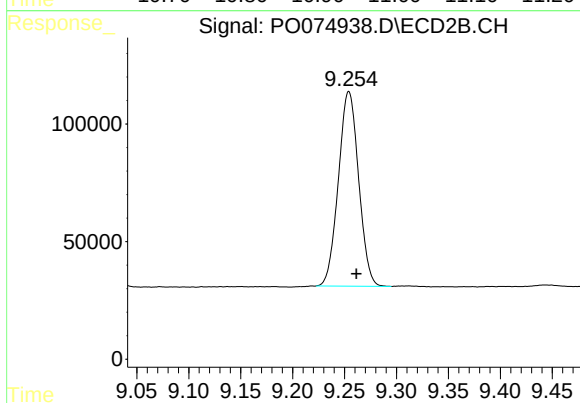

#2 Decachlorobiphenyl

R.T.: 9.254 min
Delta R.T.: -0.007 min
Response: 1123653
Conc: 20.47 ng/ml

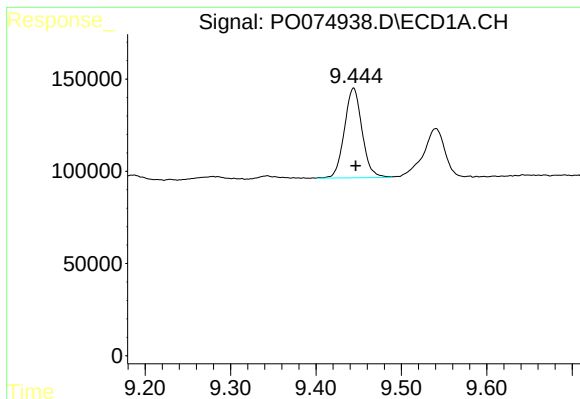


#41 AR-1268-1

R.T.: 9.444 min
Delta R.T.: -0.002 min
Response: 699444
Conc: 37.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
S19-02-C


Manual Integrations
APPROVED

Ankita
1/20/2021 9:59:58 AM

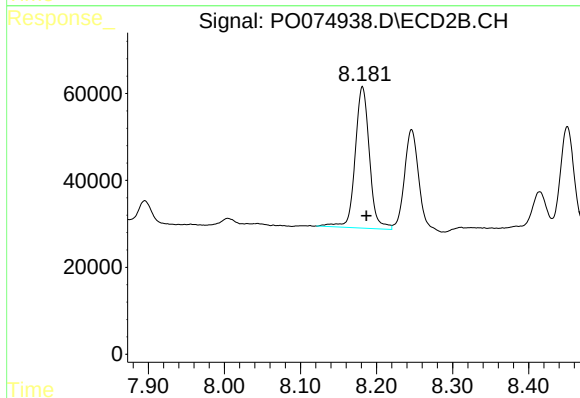


#41 AR-1268-1

R.T.: 8.182 min
Delta R.T.: -0.005 min
Response: 423777
Conc: 37.85 ng/ml

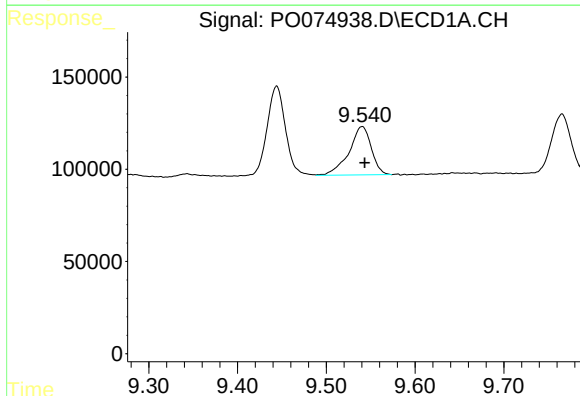


#42 AR-1268-2

R.T.: 9.540 min
Delta R.T.: -0.003 min
Response: 459647
Conc: 28.81 ng/ml

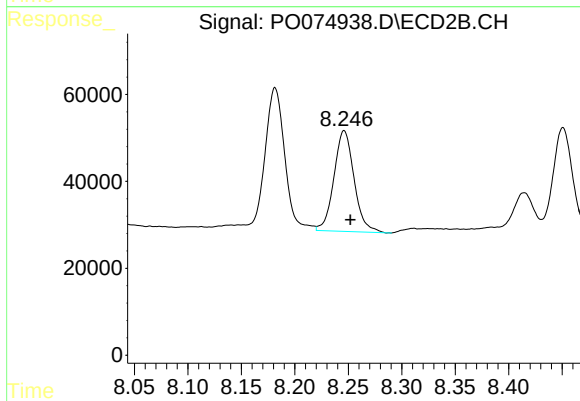

#42 AR-1268-2

R.T.: 8.246 min
Delta R.T.: -0.006 min
Response: 304066
Conc: 31.78 ng/ml

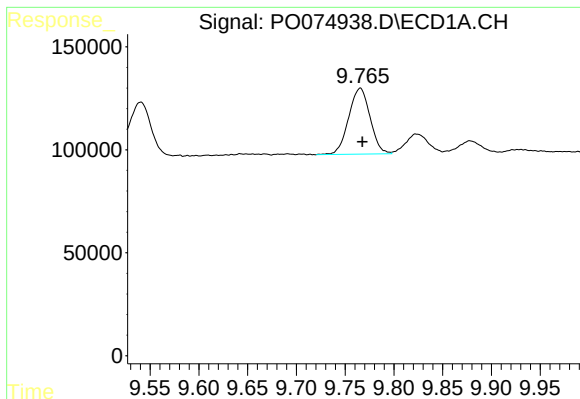


#43 AR-1268-3

R.T.: 9.766 min
Delta R.T.: -0.002 min
Response: 489015
Conc: 34.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
S19-02-C


Manual Integrations
APPROVED

Ankita
1/20/2021 9:59:58 AM

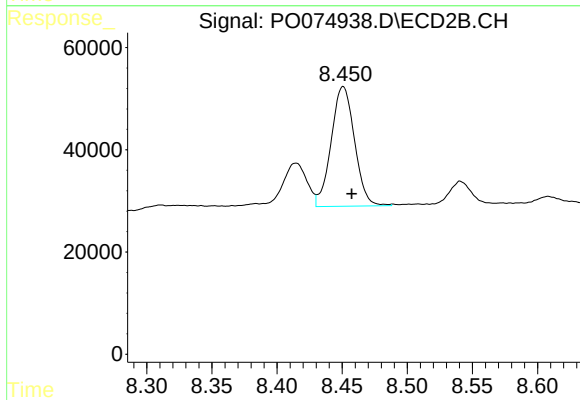


#43 AR-1268-3

R.T.: 8.450 min
Delta R.T.: -0.007 min
Response: 292358
Conc: 35.19 ng/ml m

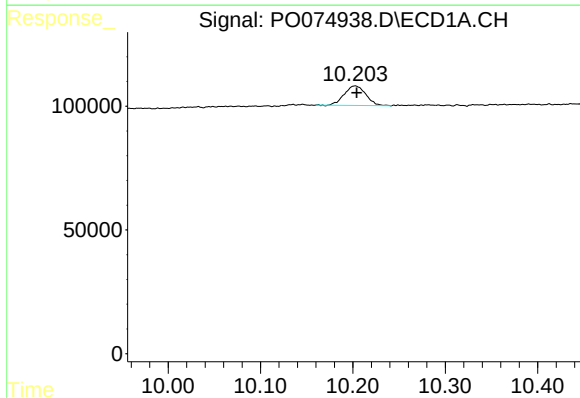


#44 AR-1268-4

R.T.: 10.202 min
Delta R.T.: -0.002 min
Response: 128601
Conc: 21.95 ng/ml

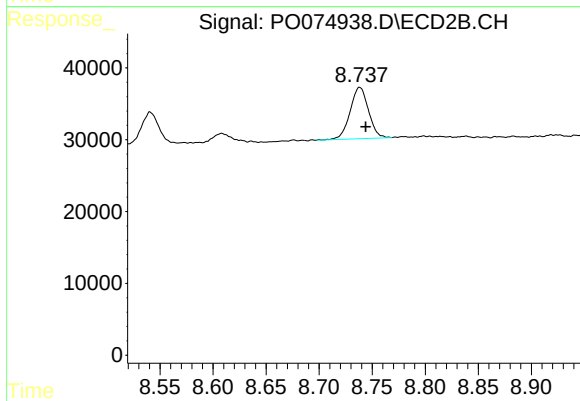

#44 AR-1268-4

R.T.: 8.738 min
Delta R.T.: -0.006 min
Response: 86254
Conc: 24.86 ng/ml

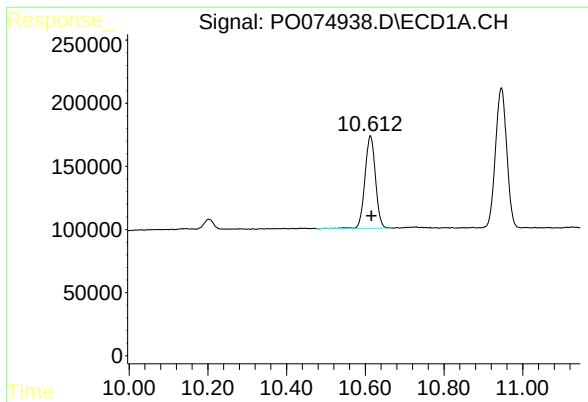


#45 AR-1268-5

R.T.: 10.613 min
Delta R.T.: -0.003 min
Response: 1357578
Conc: 32.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
S19-02-C

Manual Integrations
APPROVED

Ankita
1/20/2021 9:59:58 AM

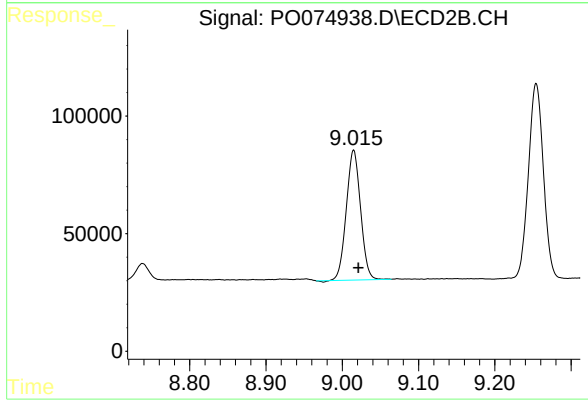

#45 AR-1268-5

R.T.: 9.015 min
Delta R.T.: -0.006 min
Response: 716799
Conc: 30.27 ng/ml