

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011921\
 Data File : P0074953.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jan 2021 17:53
 Operator : AJ/MA
 Sample : M1110-10
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S17-03-C

Manual Integrations
 APPROVED

Ankita
 1/20/2021 10:00:25 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 03:50:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.927	4.000	1457990	876144	13.817	15.575
2)	SA Decachlor...	10.942	9.251	917974	462283	9.045	8.420
Target Compounds							
26)	L6 AR-1254-1	7.176	6.113	199610	163691	45.385m	45.319
27)	L6 AR-1254-2	7.402	6.267	508372	65720	74.642	21.087 #
28)	L6 AR-1254-3	7.779	6.684	271137	104545	38.655	21.319 #
29)	L6 AR-1254-4	8.073	6.923	149555	56114	24.660	16.182 #
30)	L6 AR-1254-5	8.503	7.347	126446	345084	21.768m	76.246 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011921\
Data File : PO074953.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jan 2021 17:53
Operator : AJ/MA
Sample : M1110-10
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S17-03-C


Manual Integrations
APPROVED

Ankita
1/20/2021 10:00:25 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 03:50:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

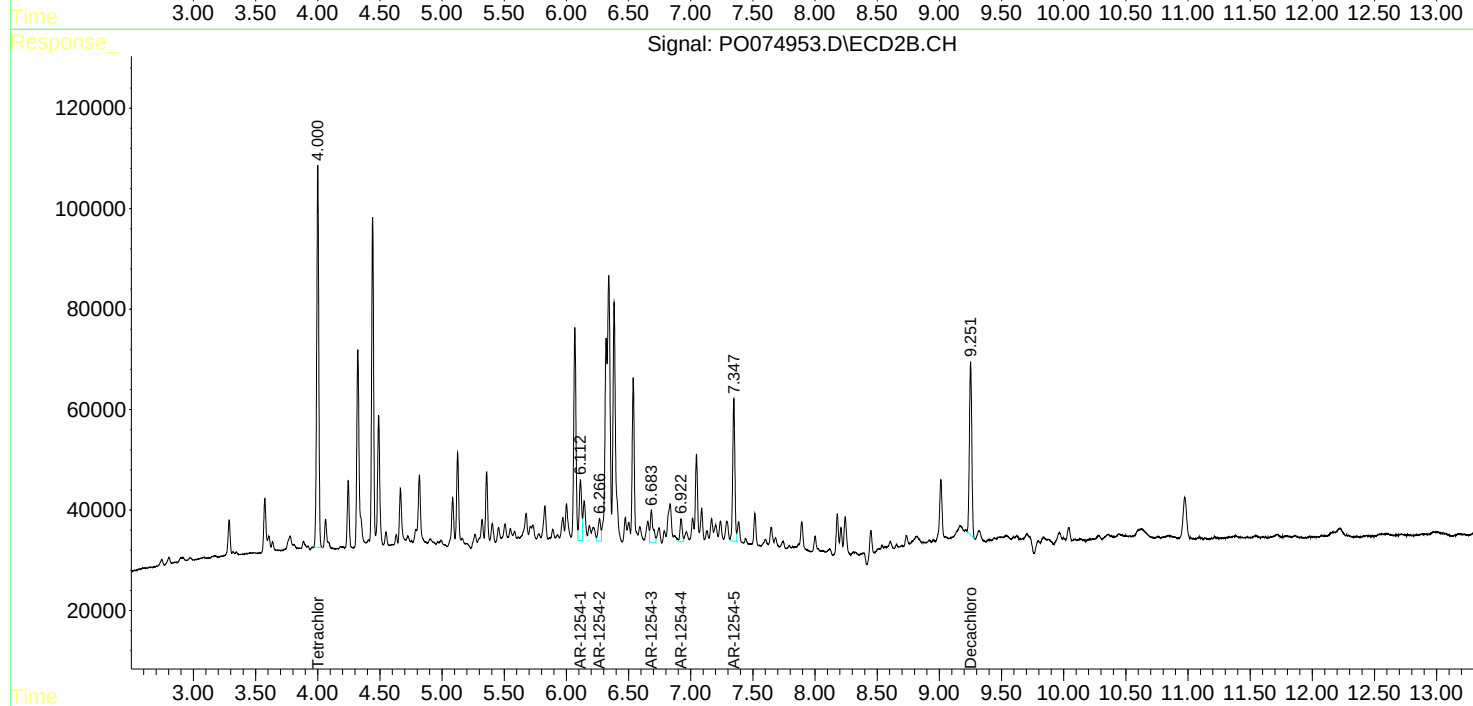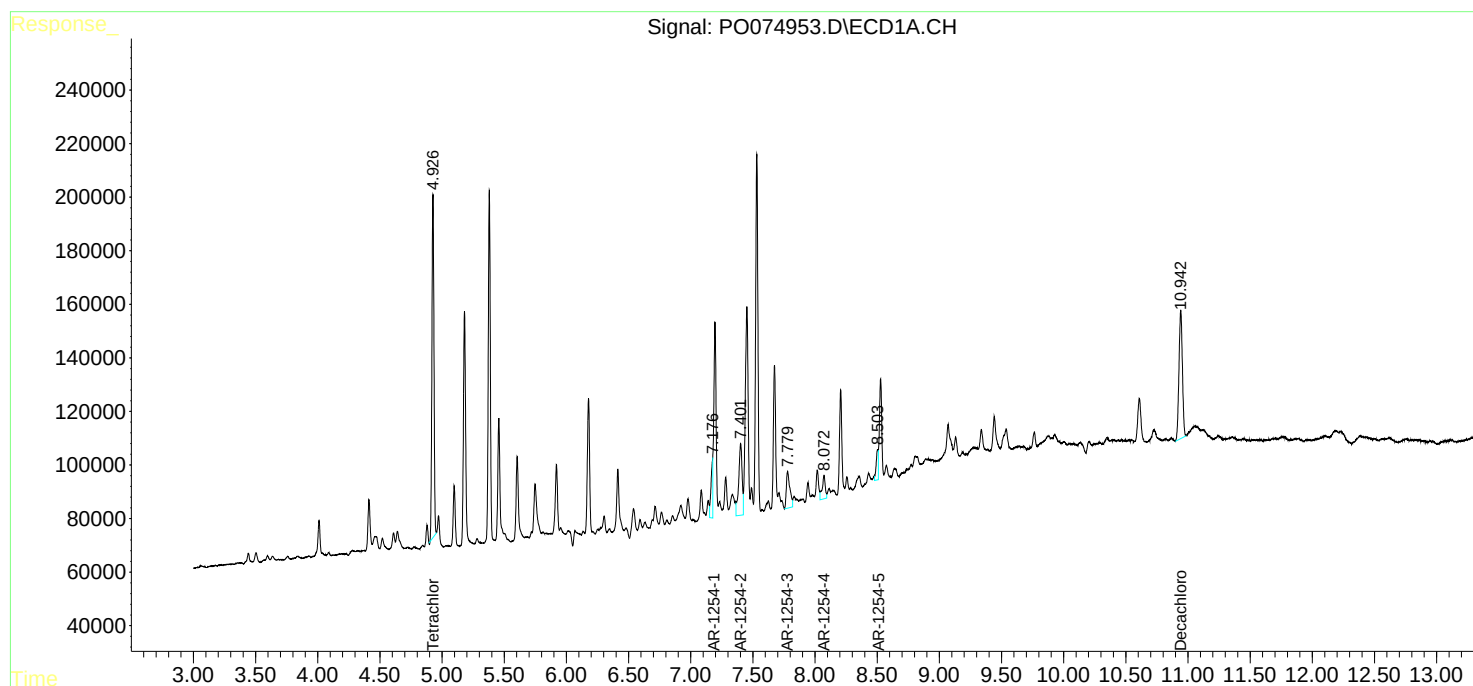

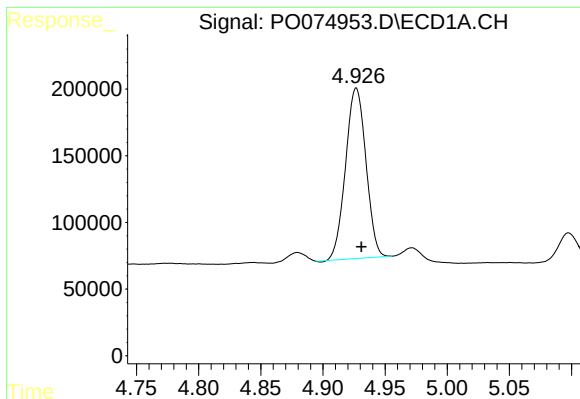


#1 Tetrachloro-m-xylene

R.T.: 4.927 min
Delta R.T.: -0.004 min
Response: 1457990
Conc: 13.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
S17-03-C


Manual Integrations
APPROVED

Ankita
1/20/2021 10:00:25 AM

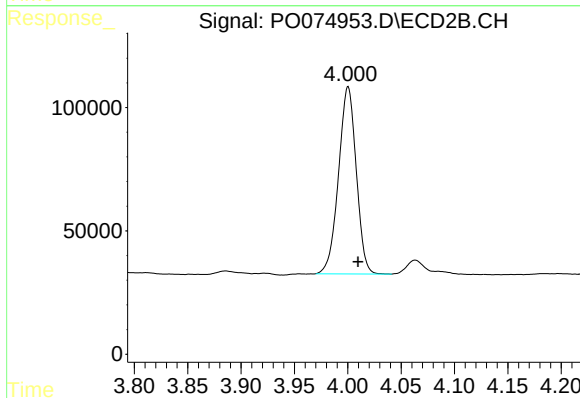


#1 Tetrachloro-m-xylene

R.T.: 4.000 min
Delta R.T.: -0.009 min
Response: 876144
Conc: 15.58 ng/ml

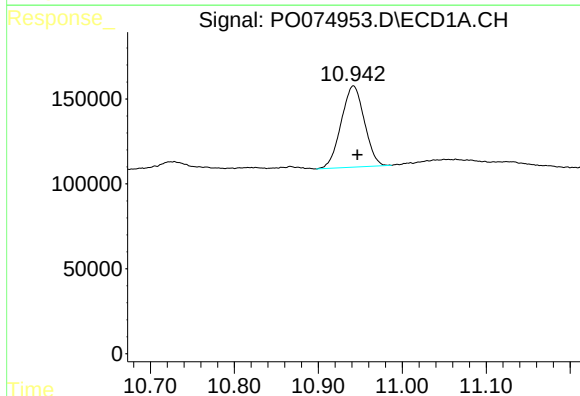


#2 Decachlorobiphenyl

R.T.: 10.942 min
Delta R.T.: -0.005 min
Response: 917974
Conc: 9.04 ng/ml

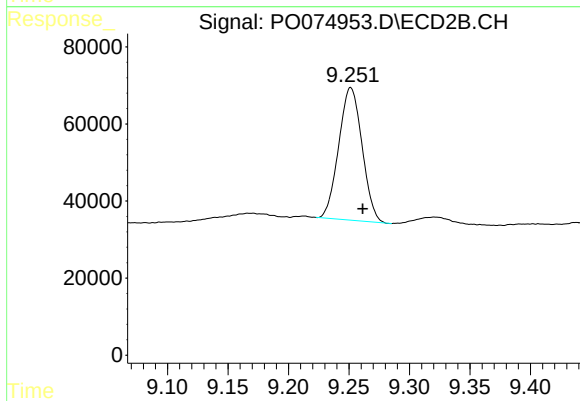

#2 Decachlorobiphenyl

R.T.: 9.251 min
Delta R.T.: -0.010 min
Response: 462283
Conc: 8.42 ng/ml

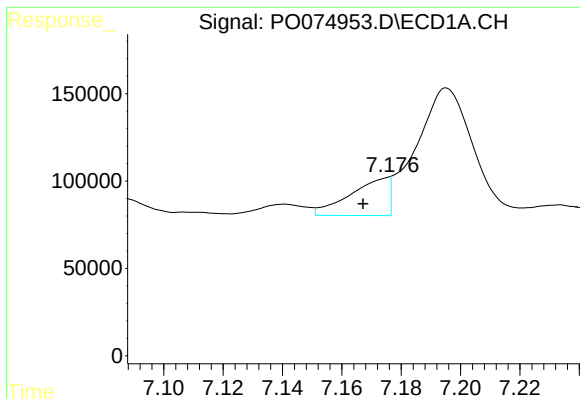


#26 AR-1254-1

R.T.: 7.176 min
Delta R.T.: 0.009 min
Response: 199610
Conc: 45.39 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S17-03-C


Manual Integrations
APPROVED

Ankita
1/20/2021 10:00:25 AM

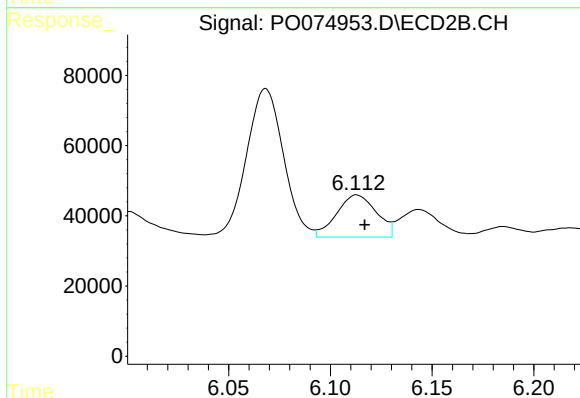


#26 AR-1254-1

R.T.: 6.113 min
Delta R.T.: -0.004 min
Response: 163691
Conc: 45.32 ng/ml

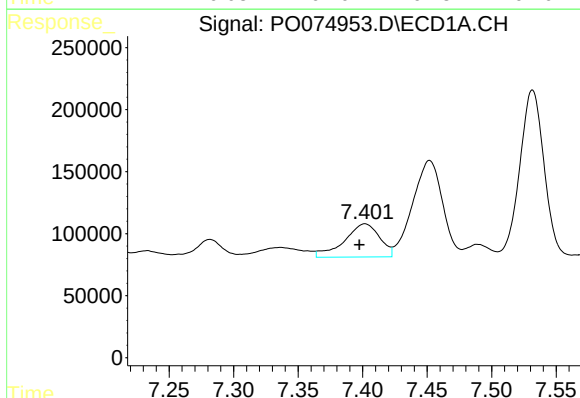


#27 AR-1254-2

R.T.: 7.402 min
Delta R.T.: 0.004 min
Response: 508372
Conc: 74.64 ng/ml

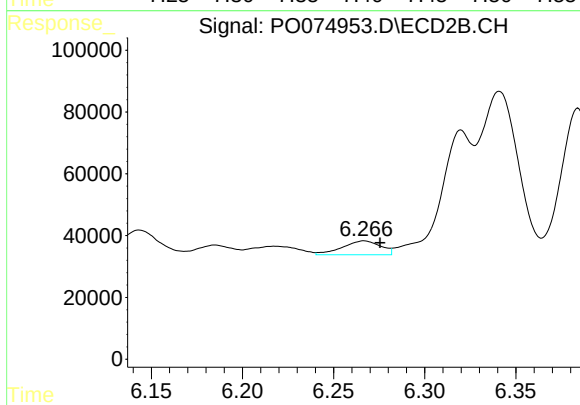

#27 AR-1254-2

R.T.: 6.267 min
Delta R.T.: -0.009 min
Response: 65720
Conc: 21.09 ng/ml

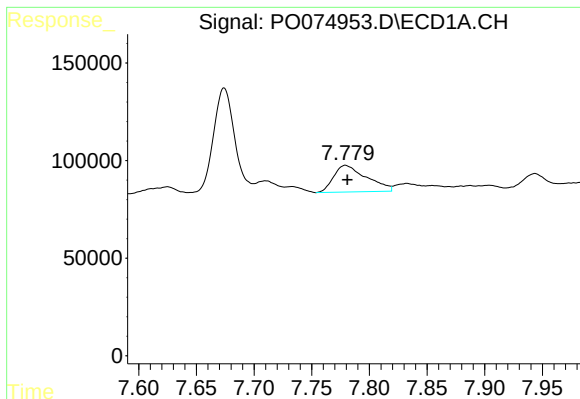


#28 AR-1254-3

R.T.: 7.779 min
Delta R.T.: -0.002 min
Response: 271137
Conc: 38.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
S17-03-C


Manual Integrations
APPROVED

Ankita
1/20/2021 10:00:25 AM

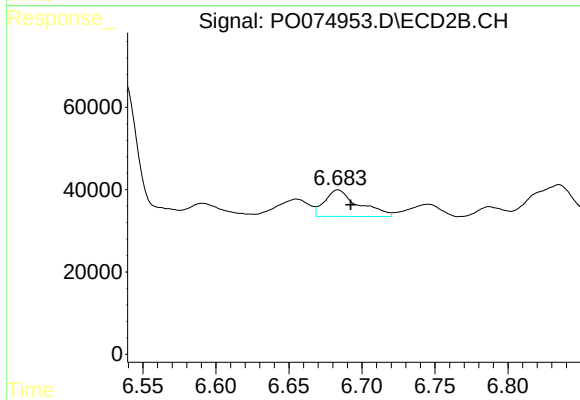


#28 AR-1254-3

R.T.: 6.684 min
Delta R.T.: -0.009 min
Response: 104545
Conc: 21.32 ng/ml

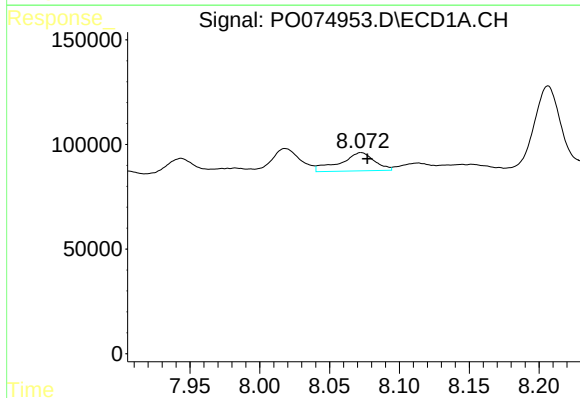


#29 AR-1254-4

R.T.: 8.073 min
Delta R.T.: -0.004 min
Response: 149555
Conc: 24.66 ng/ml

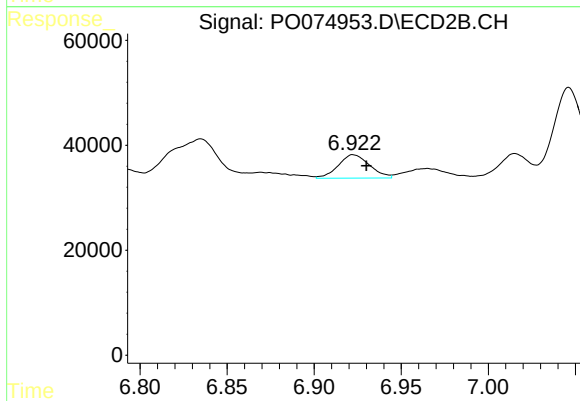

#29 AR-1254-4

R.T.: 6.923 min
Delta R.T.: -0.007 min
Response: 56114
Conc: 16.18 ng/ml

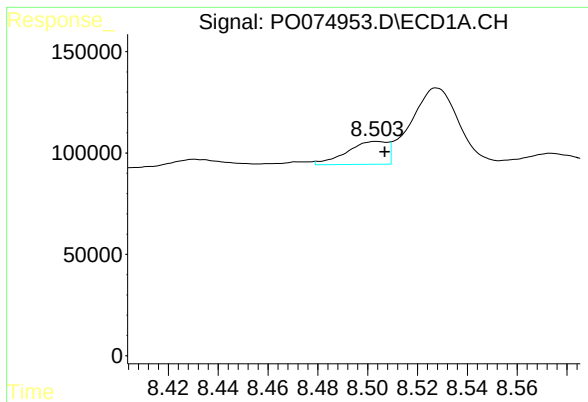


#30 AR-1254-5

R.T.: 8.503 min
Delta R.T.: -0.004 min
Response: 126446
Conc: 21.77 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S17-03-C

Manual Integrations
APPROVED

Ankita
1/20/2021 10:00:25 AM

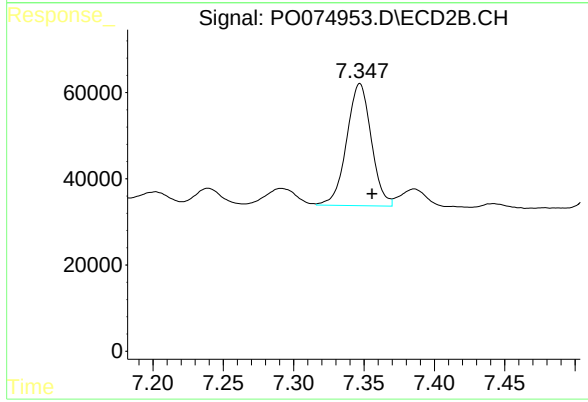

#30 AR-1254-5

R.T.: 7.347 min
Delta R.T.: -0.009 min
Response: 345084
Conc: 76.25 ng/ml