

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011921\
 Data File : P0074961.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jan 2021 20:10
 Operator : AJ/MA
 Sample : M1108-05DL 5X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S12-01-CDL

Manual Integrations
 APPROVED

Ankita
 1/20/2021 10:00:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 03:54:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.929	4.002	363368	214713	3.444	3.817
2)	SA Decachlor...	10.944	9.253	1797485	857771	17.711	15.623
Target Compounds							
26)	L6 AR-1254-1	7.164	6.111	170715	148138	38.815m	41.013
27)	L6 AR-1254-2	7.394	6.270	415834	191369	61.055	61.404
28)	L6 AR-1254-3	7.777	6.685	426930	315487	60.865	64.334
29)	L6 AR-1254-4	8.074	6.923	406328	227011	66.999	65.463
30)	L6 AR-1254-5	8.503	7.349	614156	338368	105.726	74.762 #
41)	L9 AR-1268-1	9.444	8.181	5859398	2686969	313.614	240.021
42)	L9 AR-1268-2	9.540	8.246	3882928	1899093	243.369	198.500
43)	L9 AR-1268-3	9.765	8.451	4482838	2082969	315.649	250.693
44)	L9 AR-1268-4	10.201	8.738	946887	471479	161.625	135.906
45)	L9 AR-1268-5	10.612	9.015	12687681	5767065	303.619	243.554

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO011921\
Data File : PO074961.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jan 2021 20:10
Operator : AJ/MA
Sample : M1108-05DL 5X
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S12-01-CDL


Manual Integrations
APPROVED

Ankita
1/20/2021 10:00:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 03:54:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

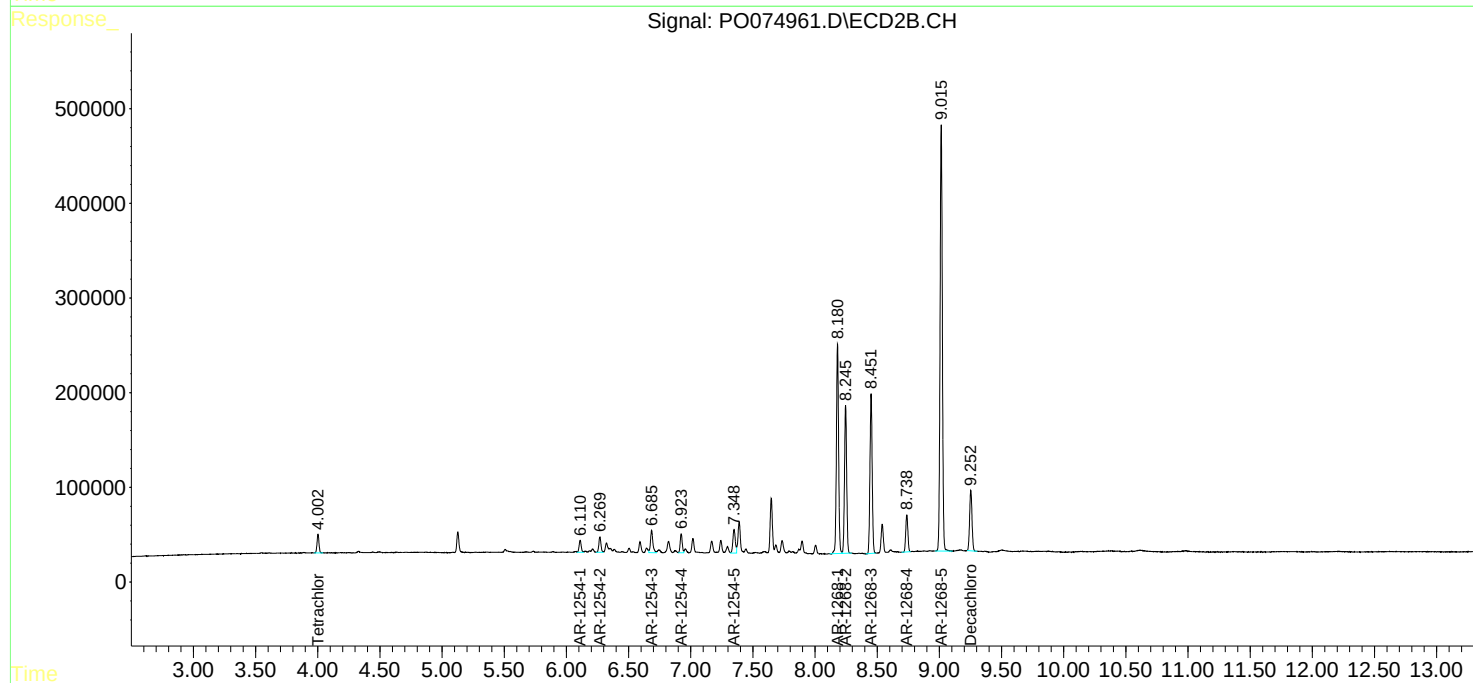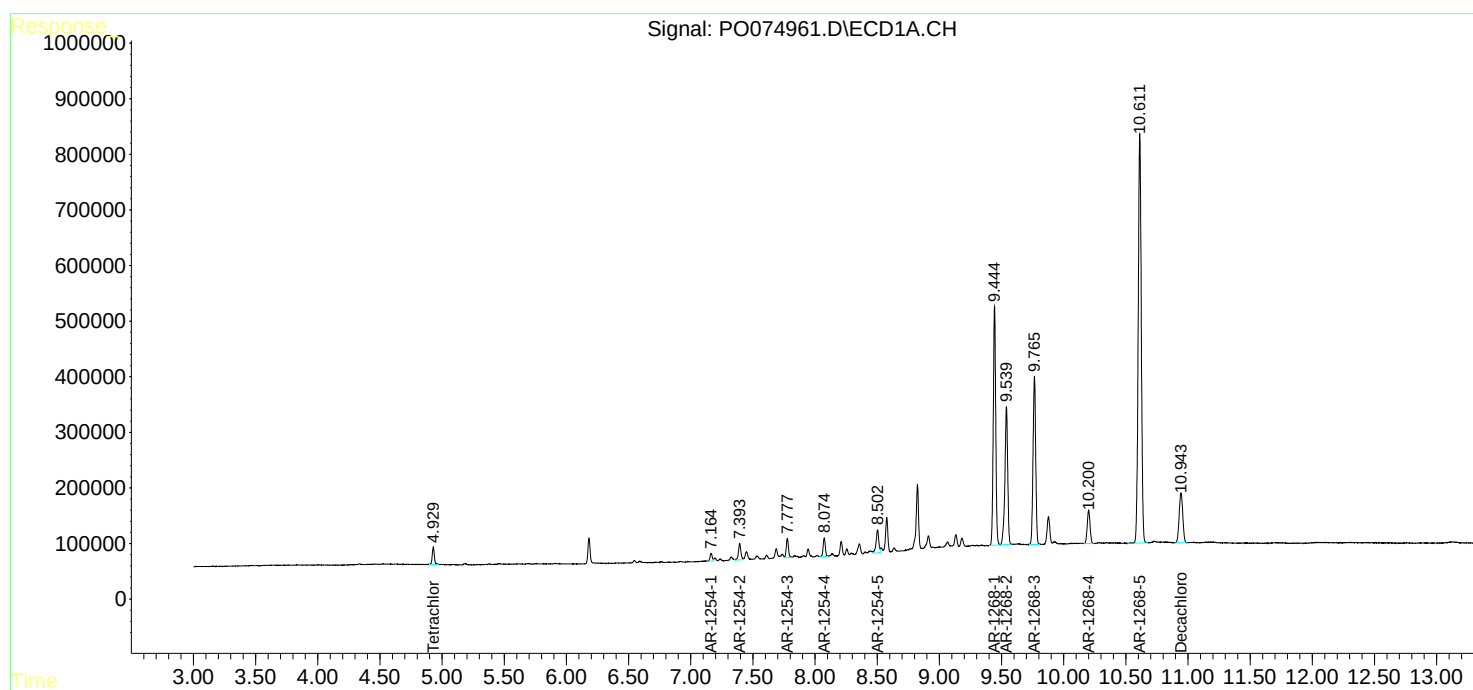

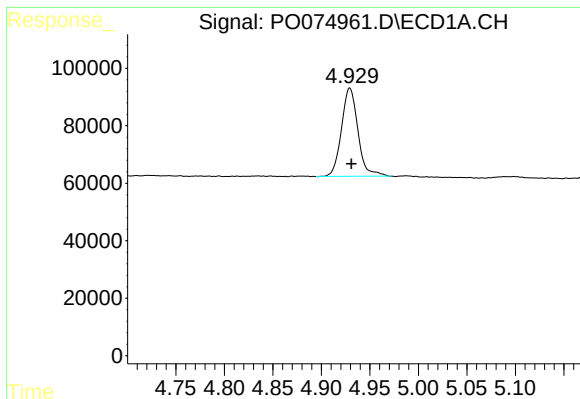


#1 Tetrachloro-m-xylene

R.T.: 4.929 min
Delta R.T.: -0.002 min
Response: 363368
Conc: 3.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
S12-01-CDL


Manual Integrations
APPROVED

Ankita
1/20/2021 10:00:48 AM

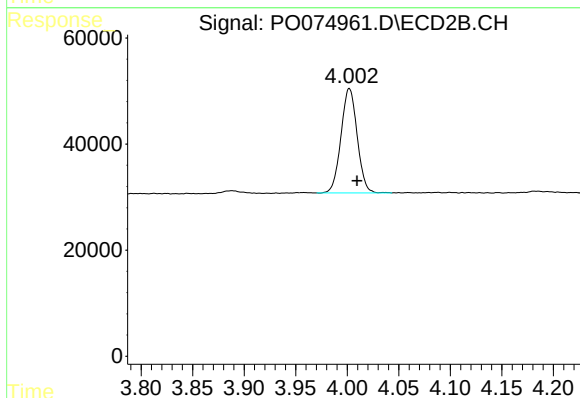


#1 Tetrachloro-m-xylene

R.T.: 4.002 min
Delta R.T.: -0.008 min
Response: 214713
Conc: 3.82 ng/ml

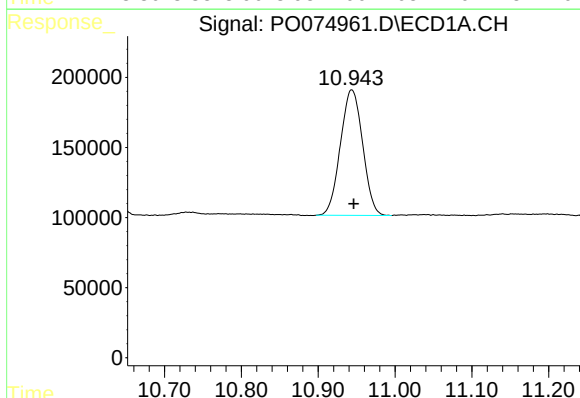


#2 Decachlorobiphenyl

R.T.: 10.944 min
Delta R.T.: -0.003 min
Response: 1797485
Conc: 17.71 ng/ml

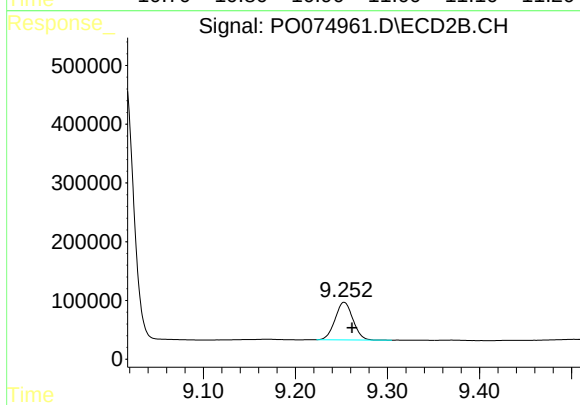

#2 Decachlorobiphenyl

R.T.: 9.253 min
Delta R.T.: -0.008 min
Response: 857771
Conc: 15.62 ng/ml

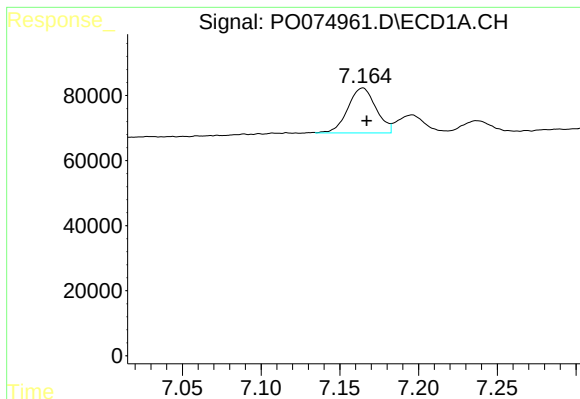


#26 AR-1254-1

R.T.: 7.164 min
Delta R.T.: -0.003 min
Response: 170715
Conc: 38.82 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S12-01-CDL


Manual Integrations
APPROVED

Ankita
1/20/2021 10:00:48 AM

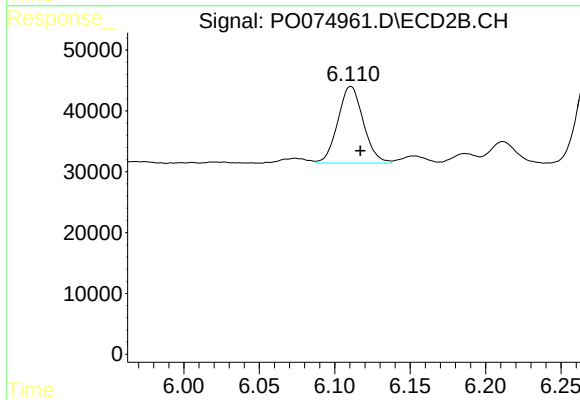


#26 AR-1254-1

R.T.: 6.111 min
Delta R.T.: -0.006 min
Response: 148138
Conc: 41.01 ng/ml

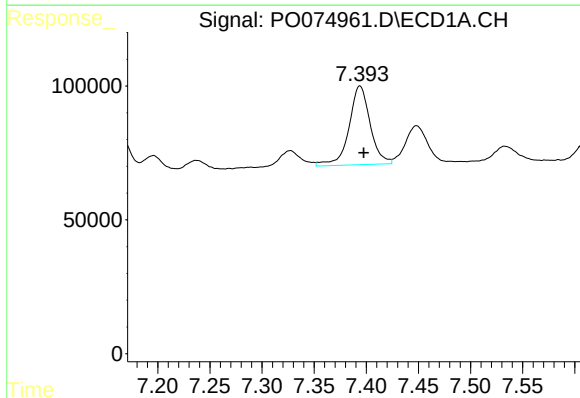


#27 AR-1254-2

R.T.: 7.394 min
Delta R.T.: -0.004 min
Response: 415834
Conc: 61.06 ng/ml

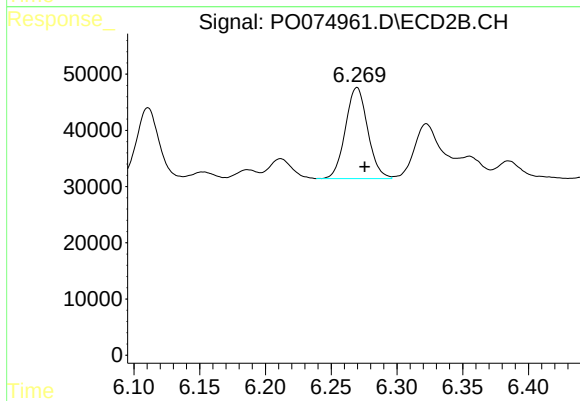

#27 AR-1254-2

R.T.: 6.270 min
Delta R.T.: -0.006 min
Response: 191369
Conc: 61.40 ng/ml

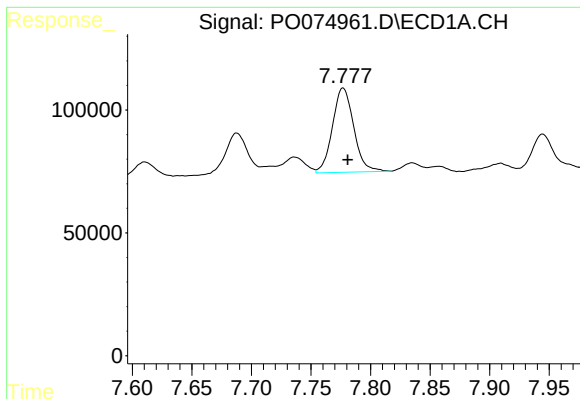


#28 AR-1254-3

R.T.: 7.777 min
Delta R.T.: -0.004 min
Response: 426930
Conc: 60.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
S12-01-CDL


Manual Integrations
APPROVED

Ankita
1/20/2021 10:00:48 AM

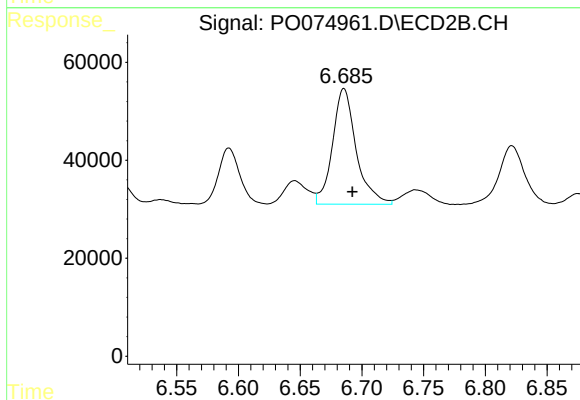


#28 AR-1254-3

R.T.: 6.685 min
Delta R.T.: -0.007 min
Response: 315487
Conc: 64.33 ng/ml

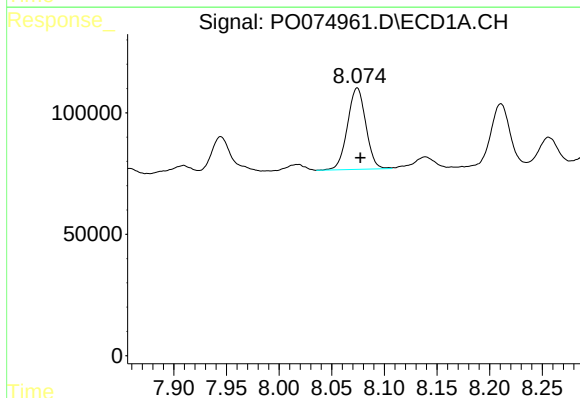


#29 AR-1254-4

R.T.: 8.074 min
Delta R.T.: -0.003 min
Response: 406328
Conc: 67.00 ng/ml

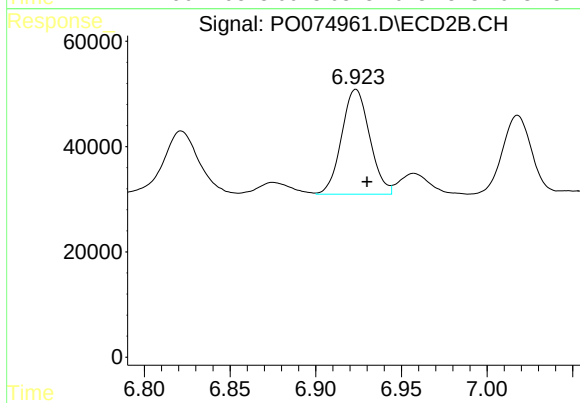

#29 AR-1254-4

R.T.: 6.923 min
Delta R.T.: -0.007 min
Response: 227011
Conc: 65.46 ng/ml

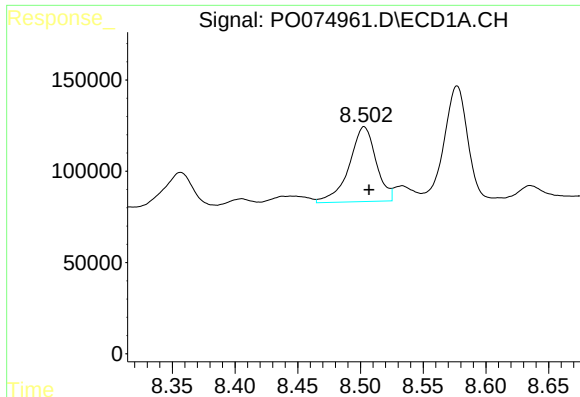


#30 AR-1254-5

R.T.: 8.503 min
Delta R.T.: -0.004 min
Response: 614156
Conc: 105.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
S12-01-CDL


Manual Integrations
APPROVED

Ankita
1/20/2021 10:00:48 AM

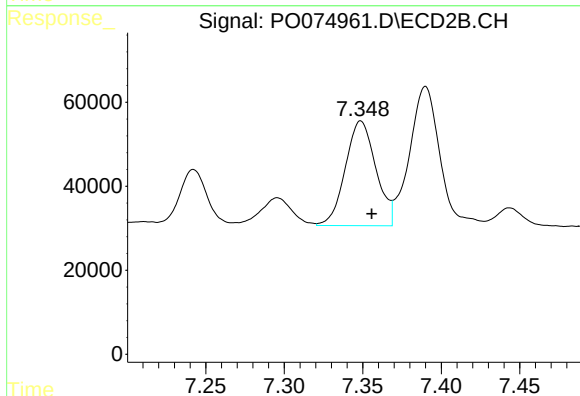


#30 AR-1254-5

R.T.: 7.349 min
Delta R.T.: -0.007 min
Response: 338368
Conc: 74.76 ng/ml

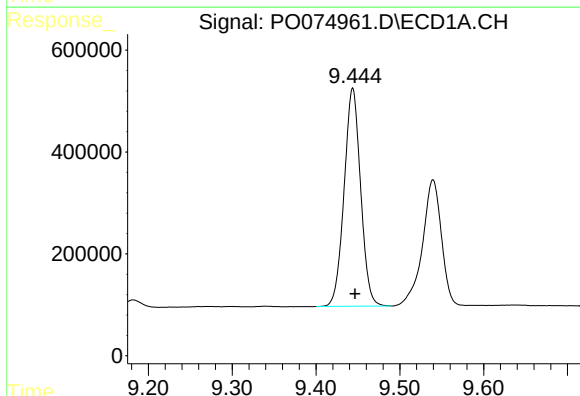


#41 AR-1268-1

R.T.: 9.444 min
Delta R.T.: -0.003 min
Response: 5859398
Conc: 313.61 ng/ml

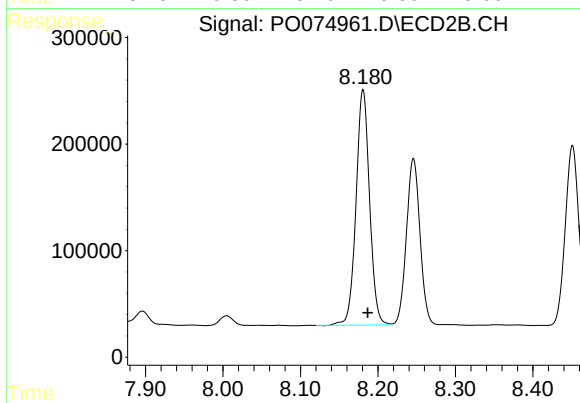

#41 AR-1268-1

R.T.: 8.181 min
Delta R.T.: -0.006 min
Response: 2686969
Conc: 240.02 ng/ml

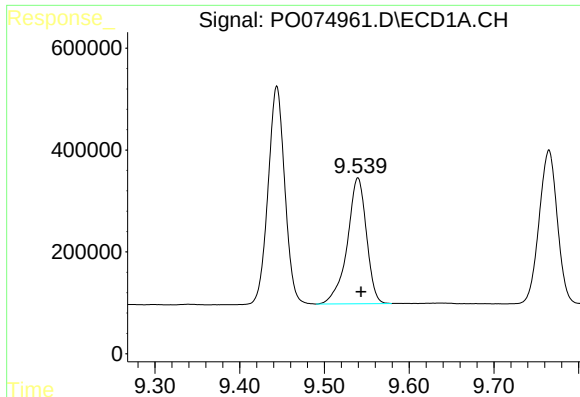


#42 AR-1268-2

R.T.: 9.540 min
Delta R.T.: -0.004 min
Response: 3882928
Conc: 243.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
S12-01-CDL


Manual Integrations
APPROVED

Ankita
1/20/2021 10:00:48 AM

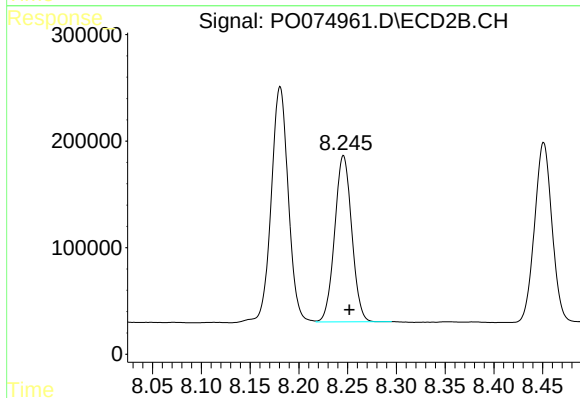


#42 AR-1268-2

R.T.: 8.246 min
Delta R.T.: -0.006 min
Response: 1899093
Conc: 198.50 ng/ml

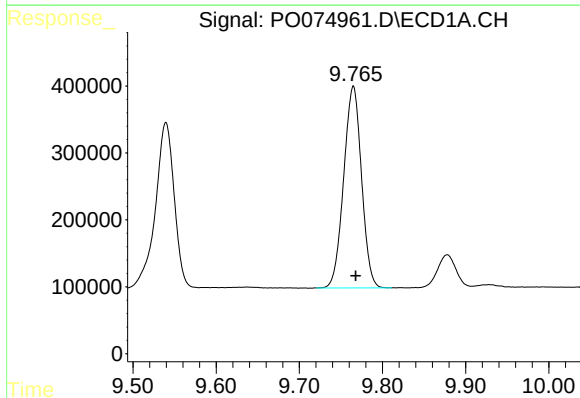


#43 AR-1268-3

R.T.: 9.765 min
Delta R.T.: -0.003 min
Response: 4482838
Conc: 315.65 ng/ml

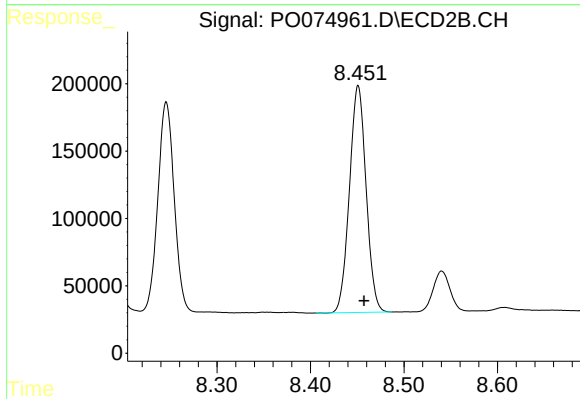

#43 AR-1268-3

R.T.: 8.451 min
Delta R.T.: -0.006 min
Response: 2082969
Conc: 250.69 ng/ml

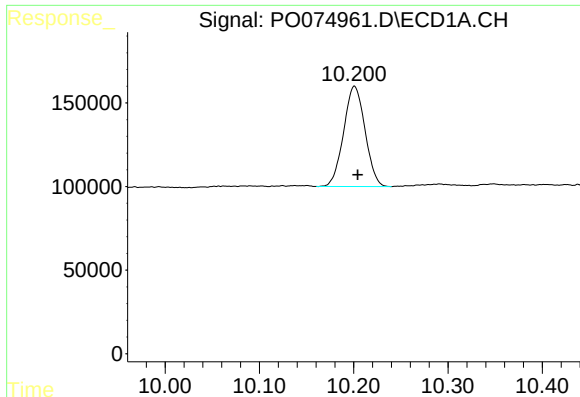


#44 AR-1268-4

R.T.: 10.201 min
Delta R.T.: -0.003 min
Response: 946887
Conc: 161.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
S12-01-CDL


Manual Integrations
APPROVED

Ankita
1/20/2021 10:00:48 AM

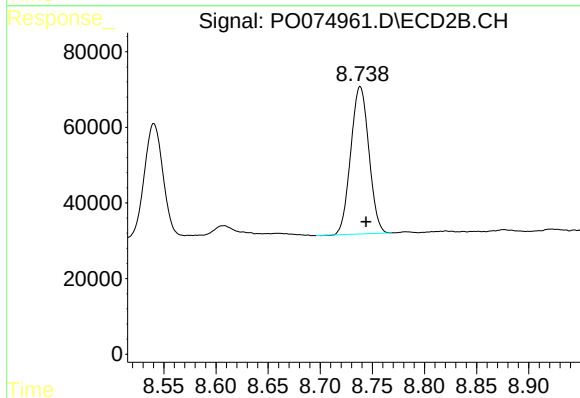


#44 AR-1268-4

R.T.: 8.738 min
Delta R.T.: -0.006 min
Response: 471479
Conc: 135.91 ng/ml

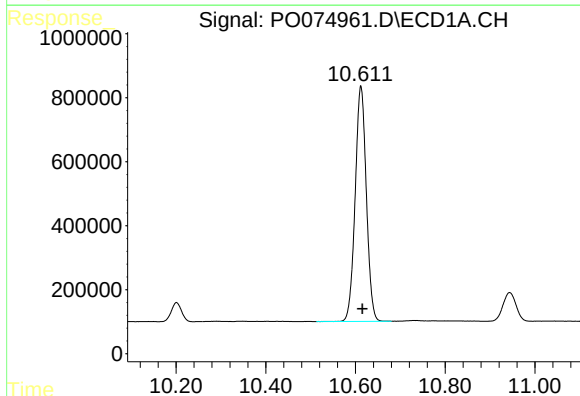

#45 AR-1268-5

R.T.: 10.612 min
Delta R.T.: -0.004 min
Response: 12687681
Conc: 303.62 ng/ml

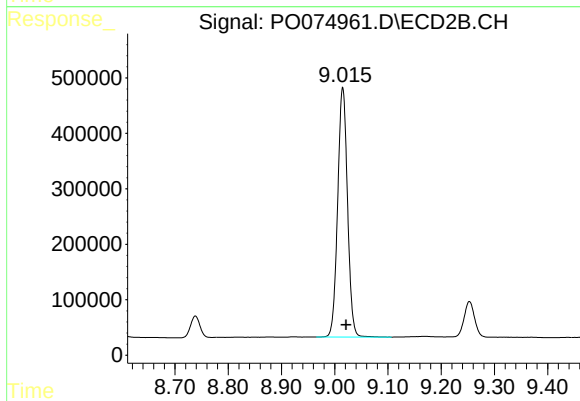

#45 AR-1268-5

R.T.: 9.015 min
Delta R.T.: -0.006 min
Response: 5767065
Conc: 243.55 ng/ml