

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011921\
 Data File : P0074966.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jan 2021 21:35
 Operator : AJ/MA
 Sample : M1110-10DL 5X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S17-03-CDL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 03:57:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.927	4.001	298590	181073	2.830	3.219
2) SA Decachlor...	10.941	9.251	159087	93616	1.567	1.705

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011921\
Data File : P0074966.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jan 2021 21:35
Operator : AJ/MA
Sample : M1110-10DL 5X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S17-03-CDL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 03:57:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

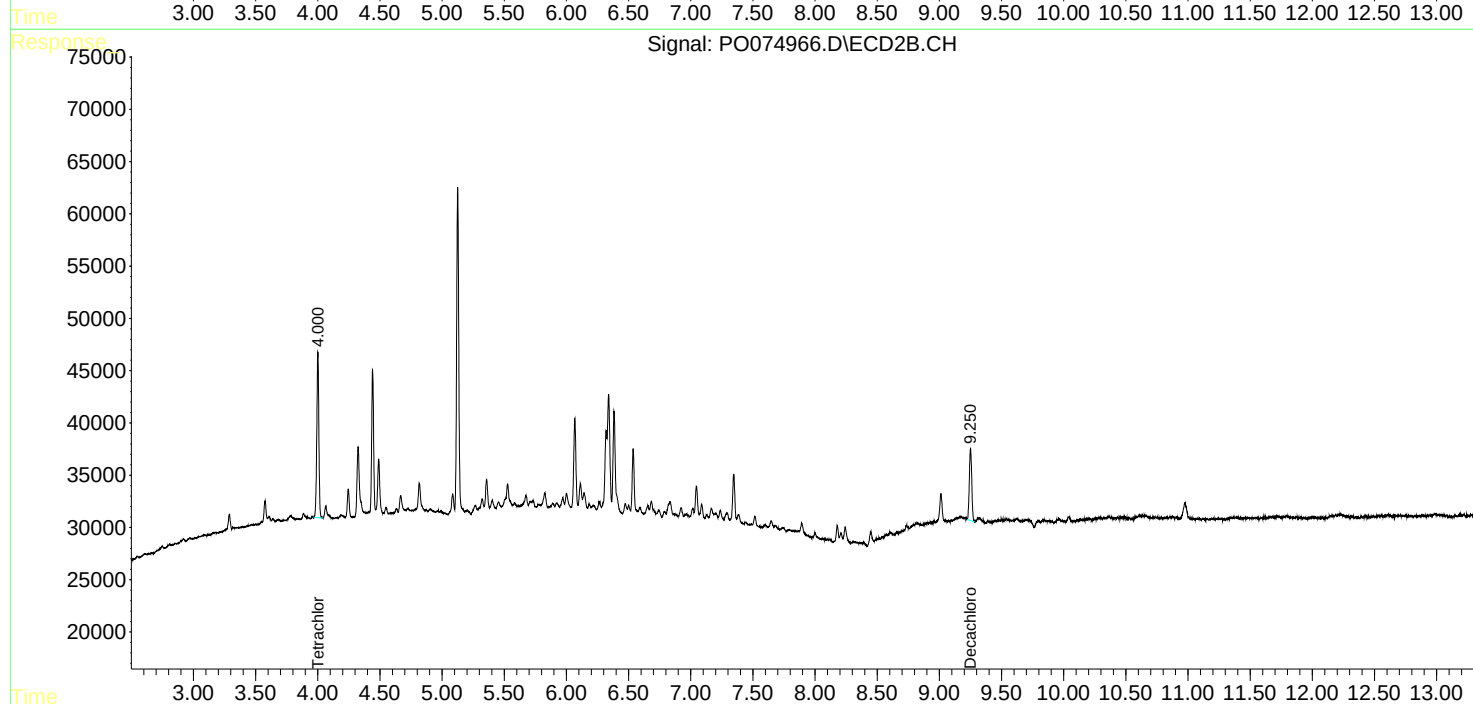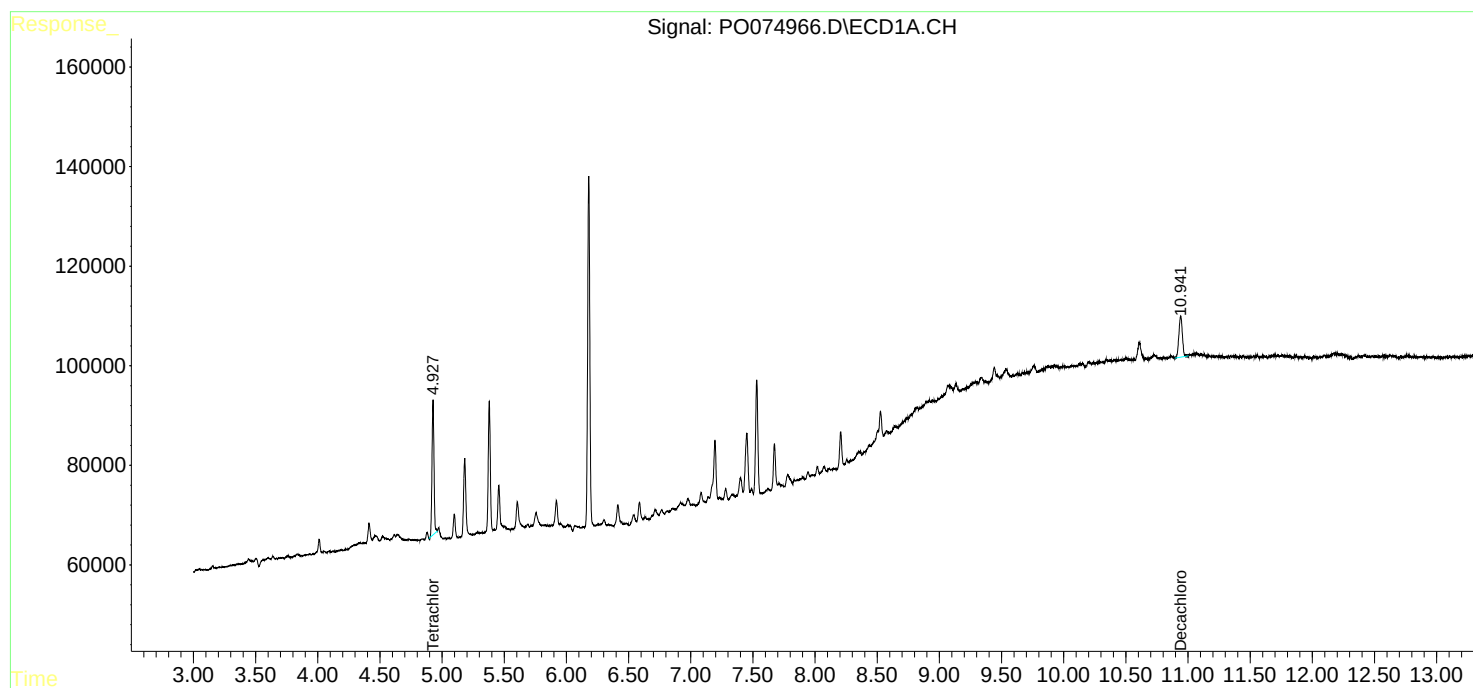


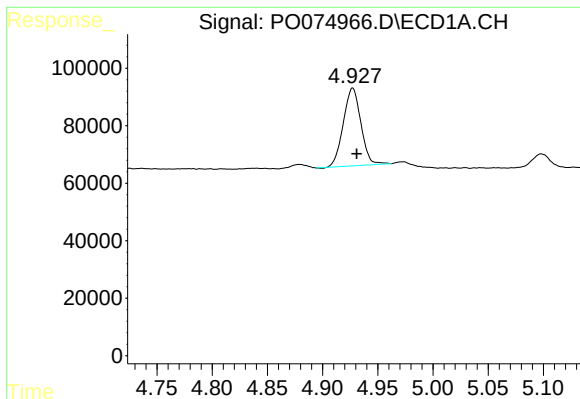

#1 Tetrachloro-m-xylene


R.T.: 4.927 min
Delta R.T.: -0.004 min
Response: 298590
Conc: 2.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
S17-03-CDL

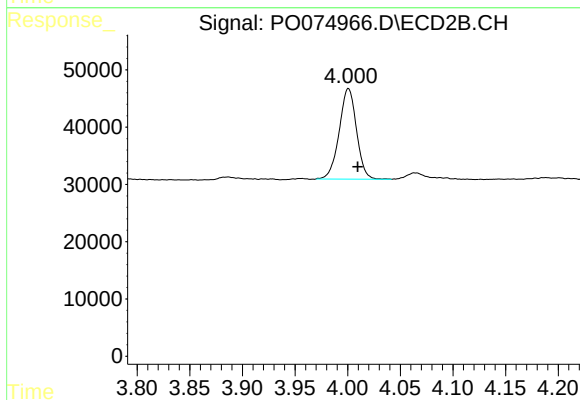


#1 Tetrachloro-m-xylene

R.T.: 4.001 min
Delta R.T.: -0.009 min
Response: 181073
Conc: 3.22 ng/ml

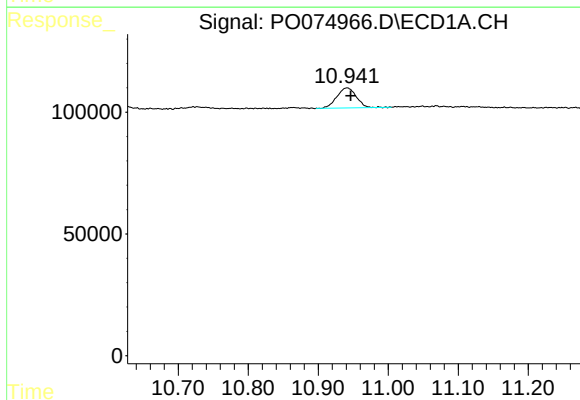

#2 Decachlorobiphenyl

R.T.: 10.941 min
Delta R.T.: -0.005 min
Response: 159087
Conc: 1.57 ng/ml

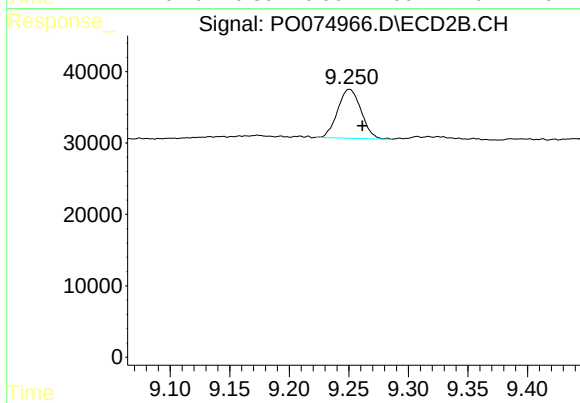

#2 Decachlorobiphenyl

R.T.: 9.251 min
Delta R.T.: -0.011 min
Response: 93616
Conc: 1.71 ng/ml