

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012020\
 Data File : P0065667.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jan 2020 16:40
 Operator : DD\AJ
 Sample : PB126195BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 17:34:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.163	3.433	473024	567446	25.904	25.796
2)	SA Decachlor...	9.662	8.336	591873	728417	17.468	17.565
Target Compounds							
9)	L2 AR-1221-2	0.000	3.725	0	35045	N.D.	177.735 #
12)	L3 AR-1232-2	5.110	0.000	144628	0	687.749	N.D. #
28)	L6 AR-1254-3	6.743	0.000	26390	0	17.027	N.D. #
29)	L6 AR-1254-4	0.000	6.127	0	23176	N.D.	15.373 #
32)	L7 AR-1260-2	0.000	6.127	0	23176	N.D.	9.539 #
43)	L9 AR-1268-3	0.000	7.549	0	8282	N.D.	1.950 #
45)	L9 AR-1268-5	0.000	8.103	0	23184	N.D.	1.612 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012020\
Data File : PO065667.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jan 2020 16:40
Operator : DD\AJ
Sample : PB126195BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 17:34:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

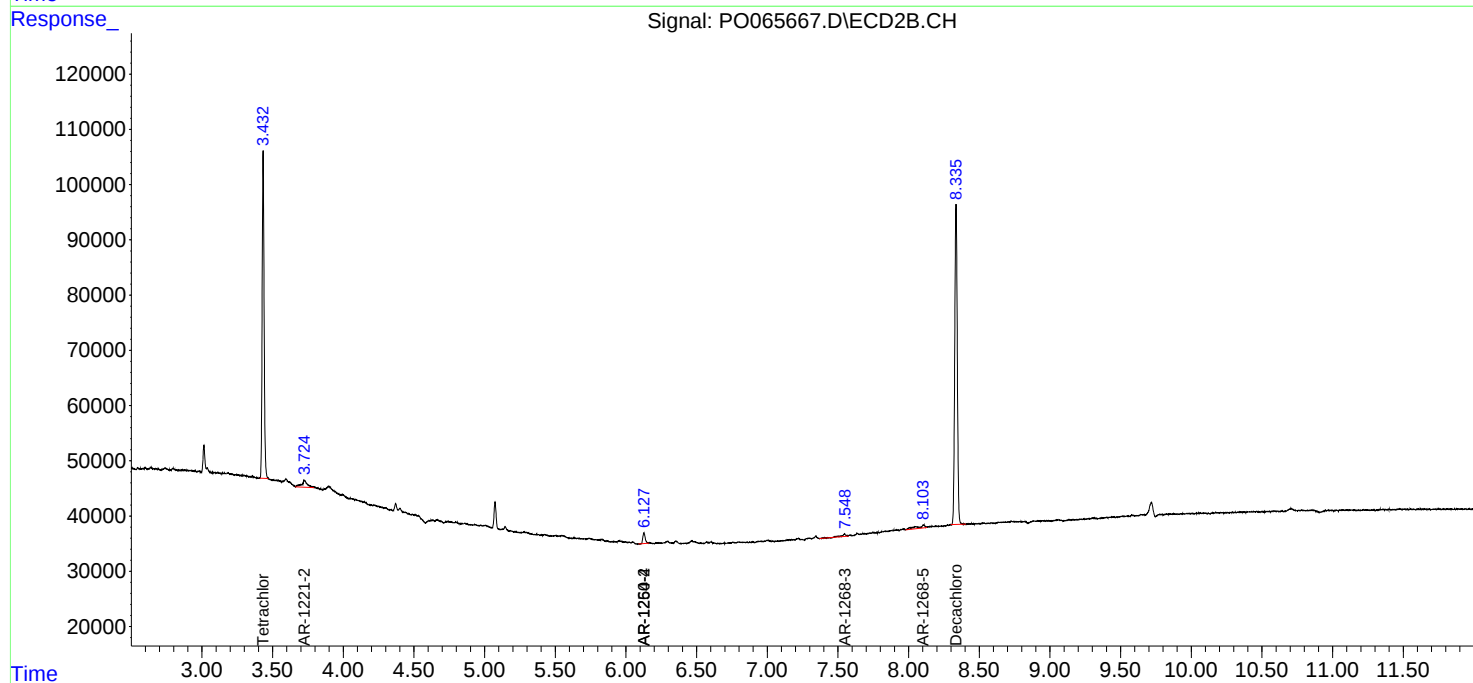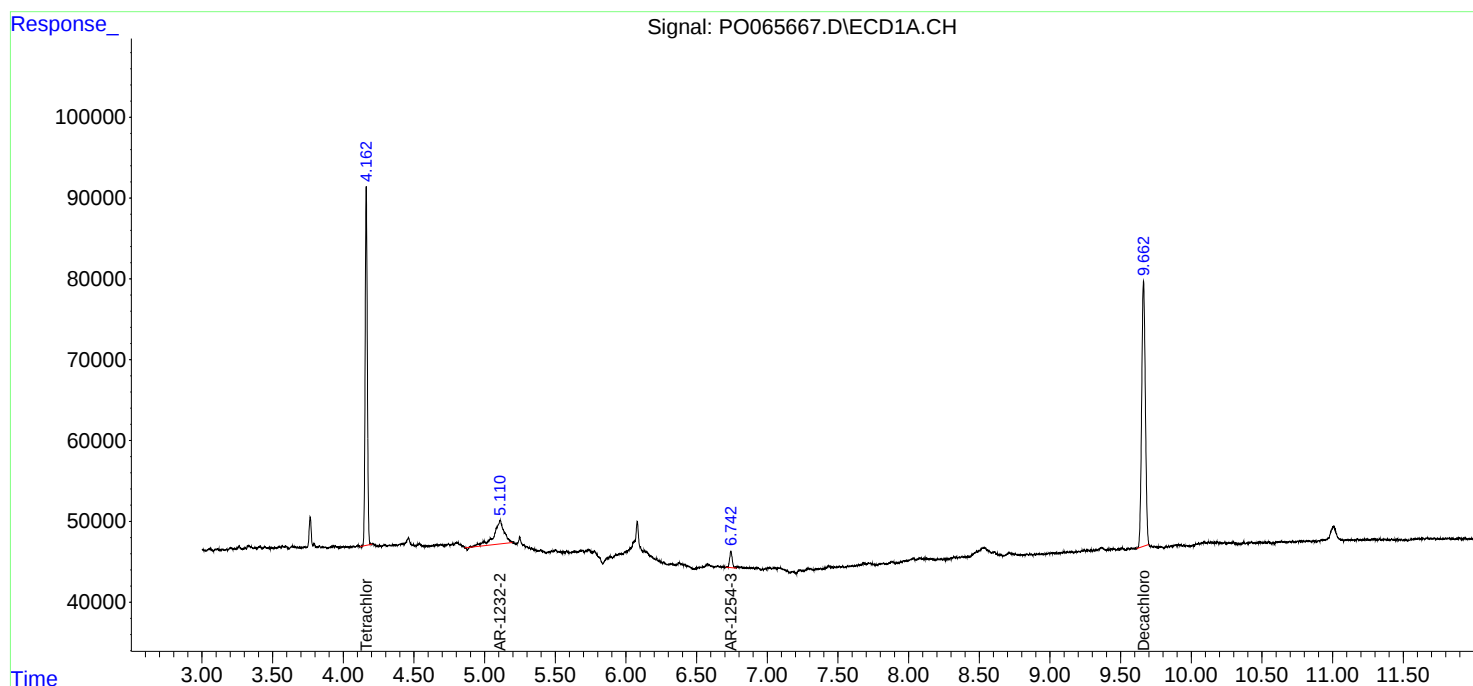


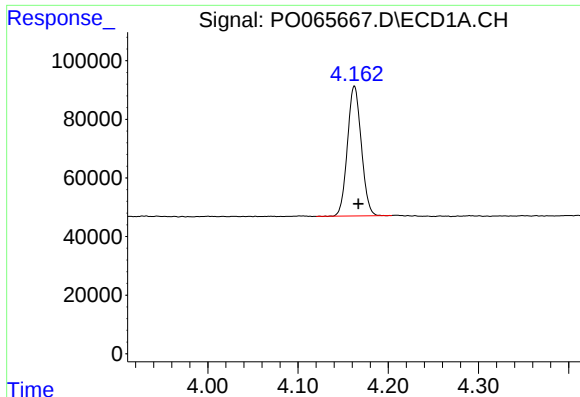

#1 Tetrachloro-m-xylene


R.T.: 4.163 min
Delta R.T.: -0.004 min
Response: 473024
Conc: 25.90 ng/ml

Instrument :
ECD_O
ClientSampleId :

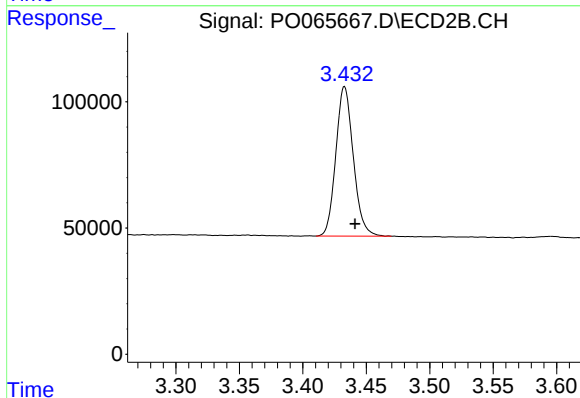


#1 Tetrachloro-m-xylene

R.T.: 3.433 min
Delta R.T.: -0.008 min
Response: 567446
Conc: 25.80 ng/ml

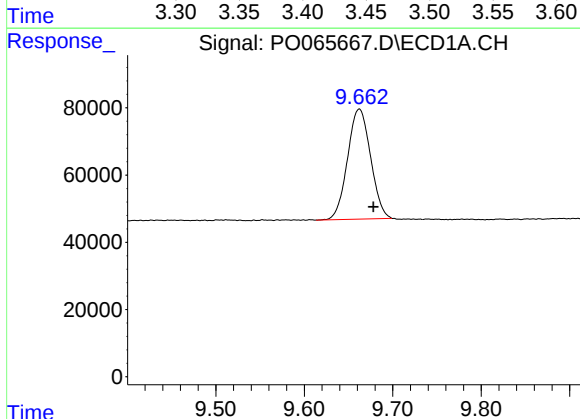


#2 Decachlorobiphenyl

R.T.: 9.662 min
Delta R.T.: -0.016 min
Response: 591873
Conc: 17.47 ng/ml

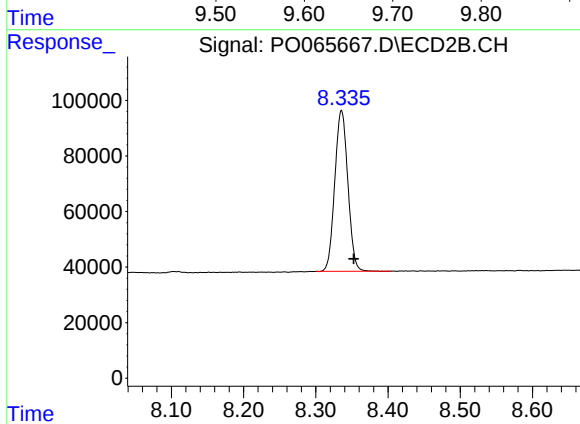

#2 Decachlorobiphenyl


R.T.: 8.336 min
Delta R.T.: -0.017 min
Response: 728417
Conc: 17.56 ng/ml

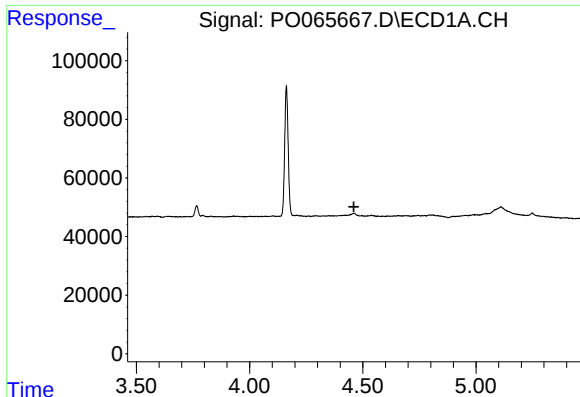

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.461 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

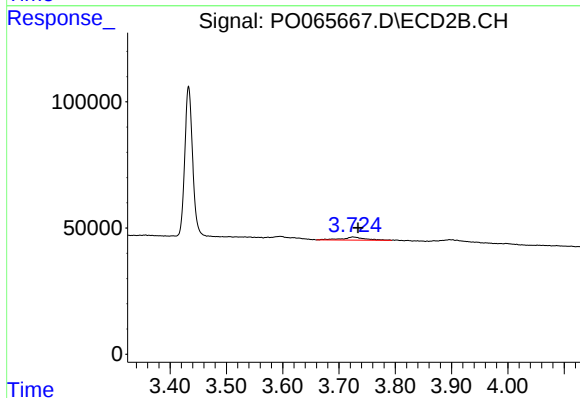


#9 AR-1221-2

R.T.: 3.725 min
Delta R.T.: -0.009 min
Response: 35045
Conc: 177.74 ng/ml

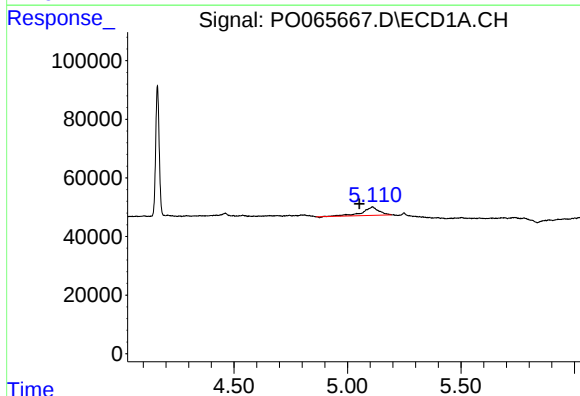


#12 AR-1232-2

R.T.: 5.110 min
Delta R.T.: 0.057 min
Response: 144628
Conc: 687.75 ng/ml

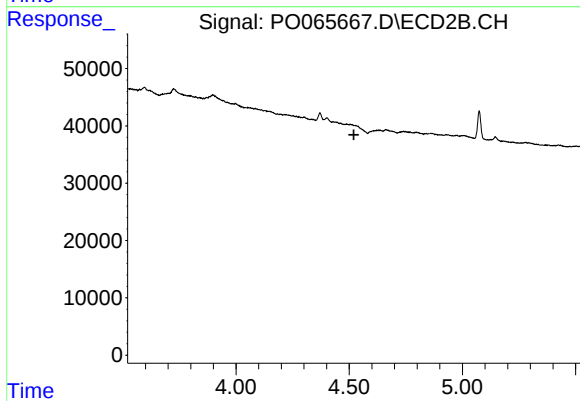

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 4.520 min
Response: 0
Conc: N.D.

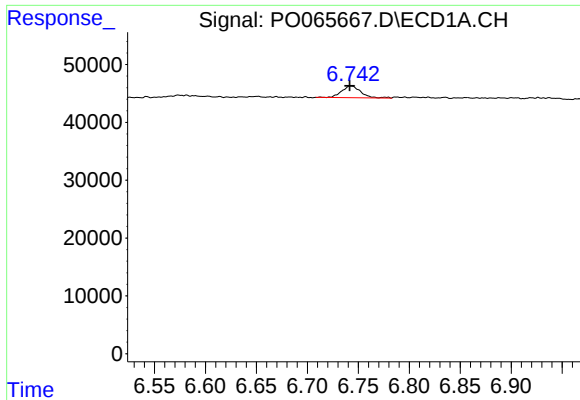

#28 AR-1254-3


R.T.: 6.743 min
Delta R.T.: 0.001 min
Response: 26390
Conc: 17.03 ng/ml

Instrument :
ECD_O
ClientSampleId :

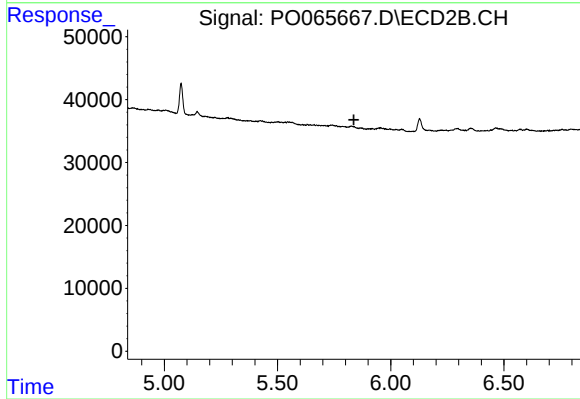


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 5.837 min
Response: 0
Conc: N.D.

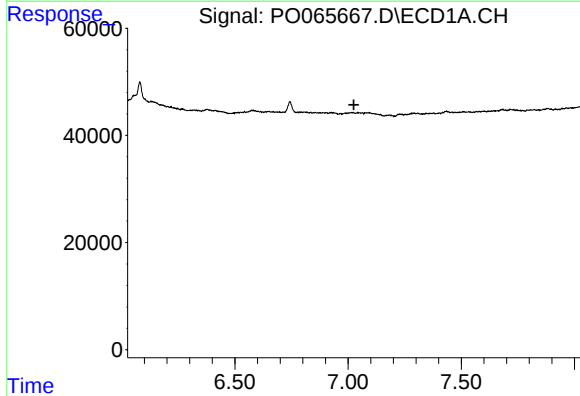


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.026 min
Response: 0
Conc: N.D.

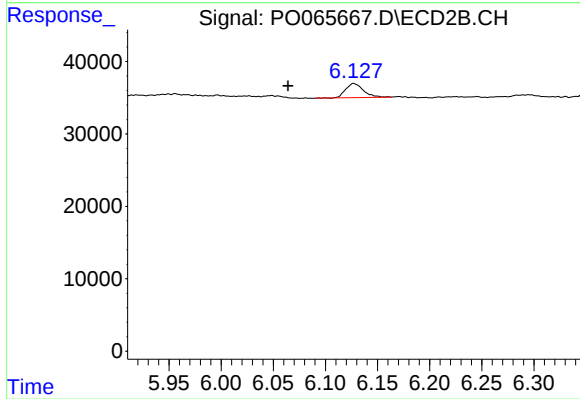

#29 AR-1254-4


R.T.: 6.127 min
Delta R.T.: 0.063 min
Response: 23176
Conc: 15.37 ng/ml

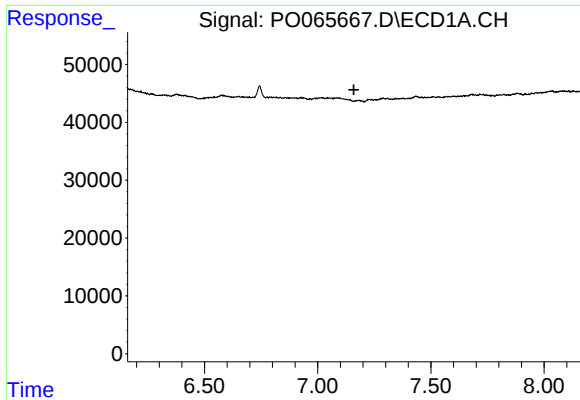

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.160 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

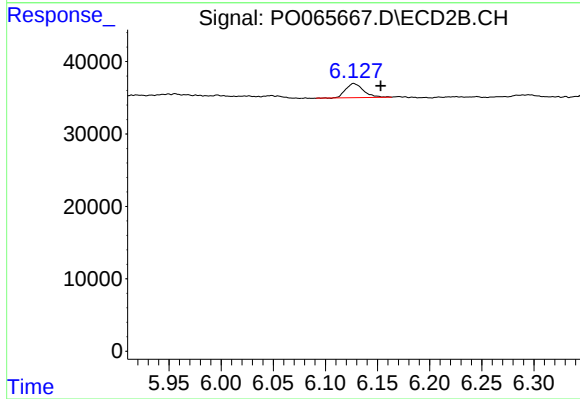


#32 AR-1260-2

R.T.: 6.127 min
Delta R.T.: -0.026 min
Response: 23176
Conc: 9.54 ng/ml

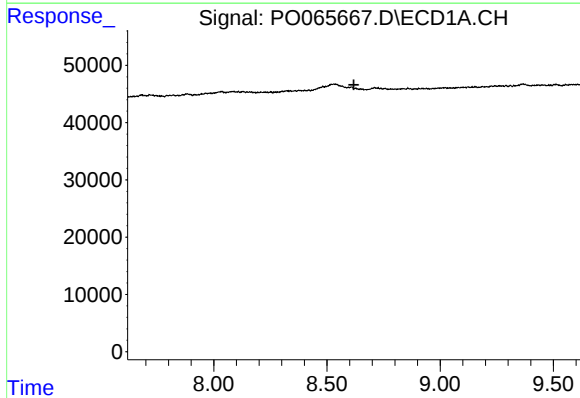


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 8.619 min
Response: 0
Conc: N.D.

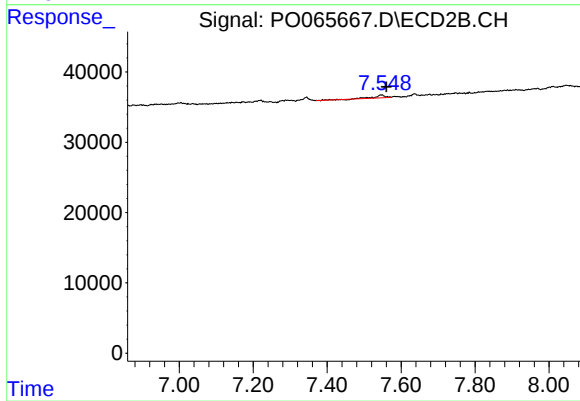

#43 AR-1268-3


R.T.: 7.549 min
Delta R.T.: -0.012 min
Response: 8282
Conc: 1.95 ng/ml

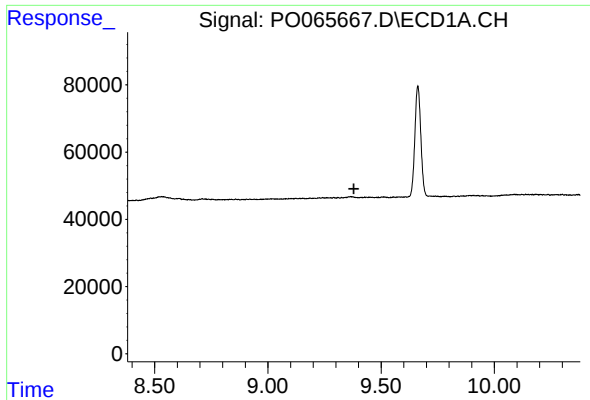

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.380 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

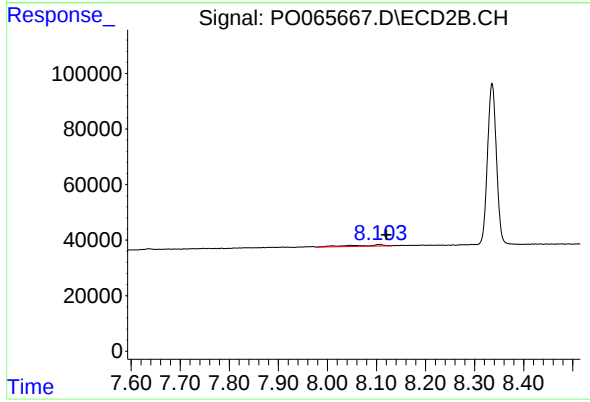

#45 AR-1268-5

R.T.: 8.103 min
Delta R.T.: -0.017 min
Response: 23184
Conc: 1.61 ng/ml