

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012020\
 Data File : P0065686.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jan 2020 22:15
 Operator : DD\AJ
 Sample : L1014-06
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-02-011720

Manual Integrations
 APPROVED

mohammad
 1/21/2020 3:00:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 03:07:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.155	3.431	757650	952302	41.492m	43.292
2) SA Decachlor...	9.654	8.332	688731	761955	20.327	18.374

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012020\
Data File : P0065686.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jan 2020 22:15
Operator : DD\AJ
Sample : L1014-06
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OR-02-011720


Manual Integrations
APPROVED

mohammad
1/21/2020 3:00:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 03:07:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

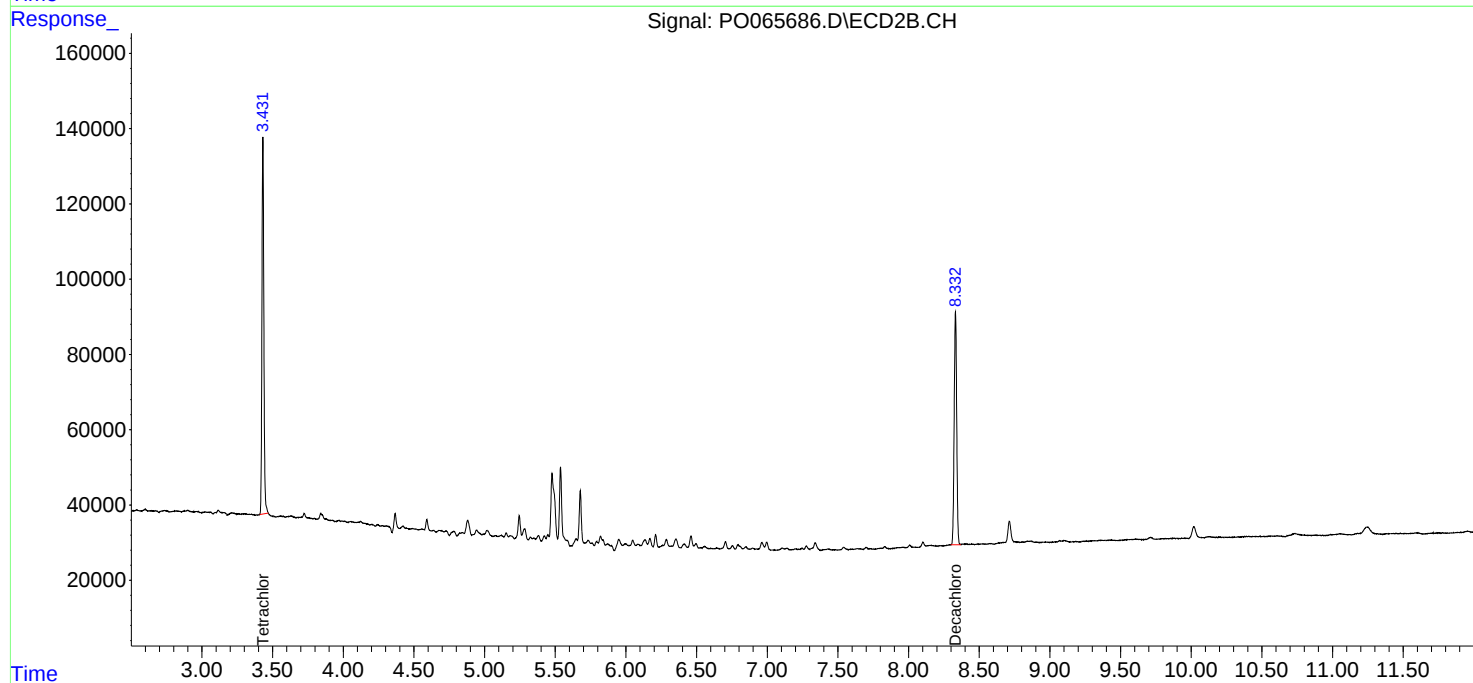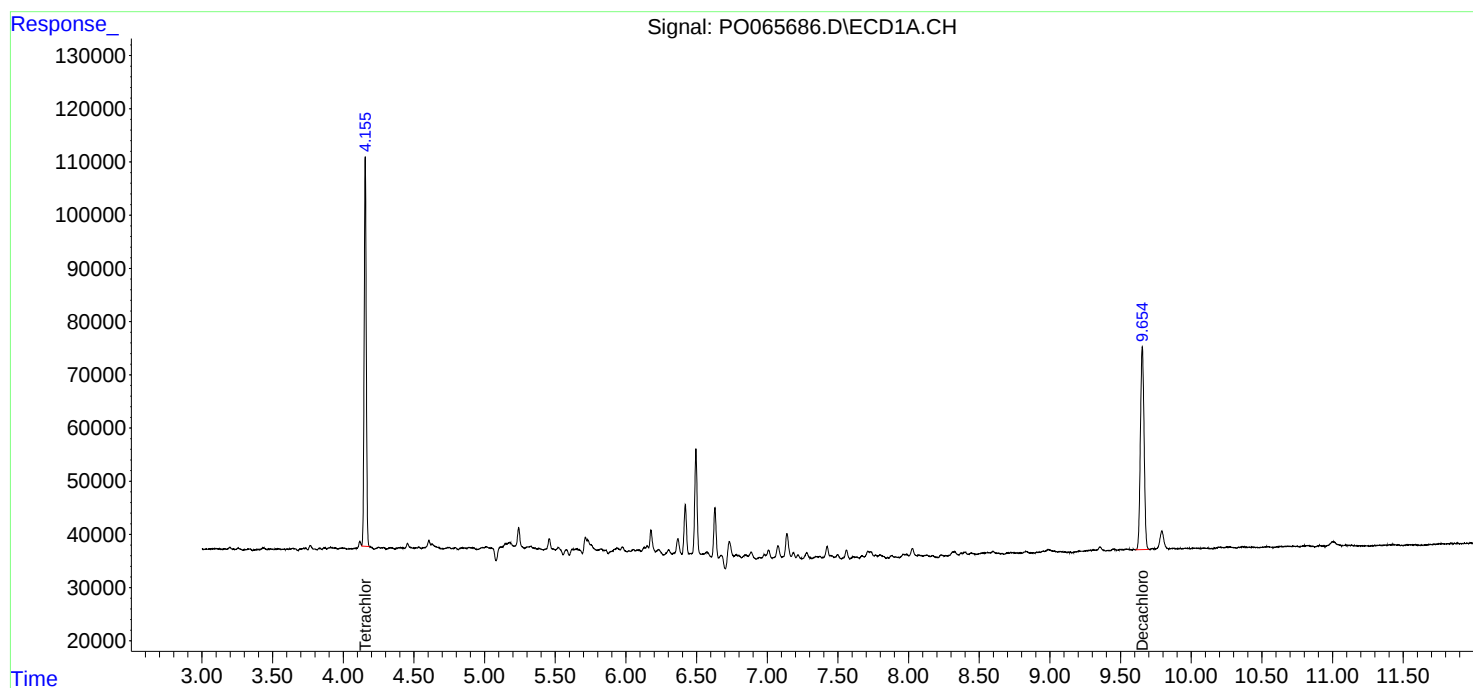

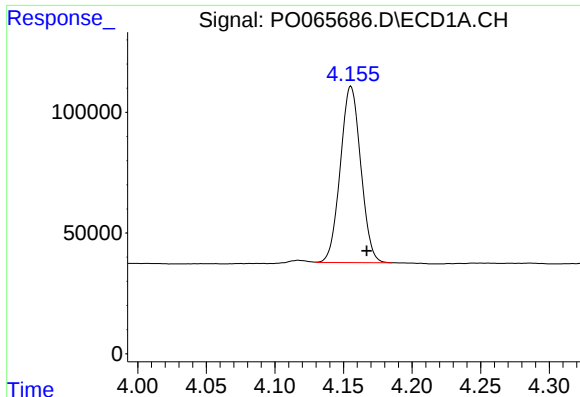


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: -0.012 min
Response: 757650
Conc: 41.49 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OR-02-011720


Manual Integrations
APPROVED

mohammad
1/21/2020 3:00:45 PM

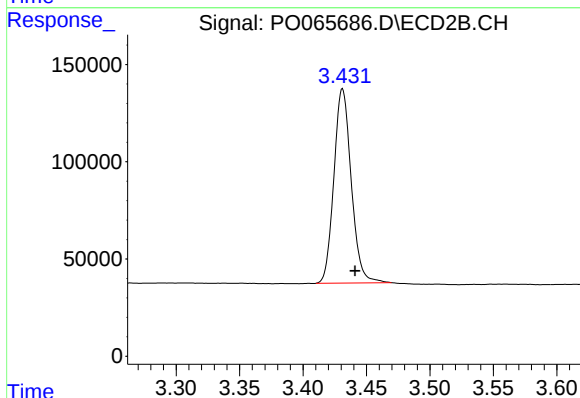


#1 Tetrachloro-m-xylene

R.T.: 3.431 min
Delta R.T.: -0.010 min
Response: 952302
Conc: 43.29 ng/ml

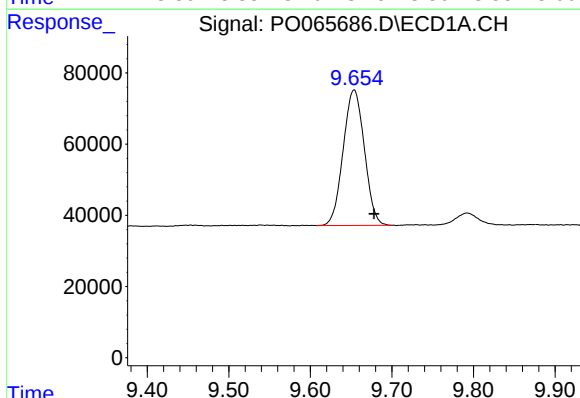

#2 Decachlorobiphenyl

R.T.: 9.654 min
Delta R.T.: -0.024 min
Response: 688731
Conc: 20.33 ng/ml

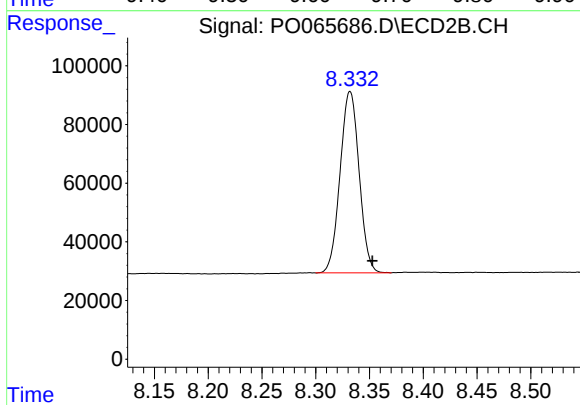

#2 Decachlorobiphenyl

R.T.: 8.332 min
Delta R.T.: -0.021 min
Response: 761955
Conc: 18.37 ng/ml