

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012021\
 Data File : P0074999.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jan 2021 16:28
 Operator : AJ/MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 05:27:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.931	4.002	2422631	1228338	22.959	21.836
2)	SA Decachlor...	10.944	9.253	2245704	1127447	22.127	20.535
Target Compounds							
20)	L4 AR-1242-5	7.234	6.134	28119	42892	11.174	24.498 #
24)	L5 AR-1248-4	7.172f	0.000	163756	0	36.721	N.D. #
25)	L5 AR-1248-5	7.234	6.134f	28119	42892	6.673	18.244 #
26)	L6 AR-1254-1	7.172	6.134f	163756	42892	37.233	11.875 #
28)	L6 AR-1254-3	7.798f	0.000	66849	0	9.530	N.D. #
30)	L6 AR-1254-5	8.515	0.000	20745	0	3.571	N.D. #
31)	L7 AR-1260-1	7.950	0.000	227500	0	45.603	N.D. #
32)	L7 AR-1260-2	8.212	0.000	50376	0	7.406	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012021\
Data File : PO074999.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jan 2021 16:28
Operator : AJ/MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 05:27:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

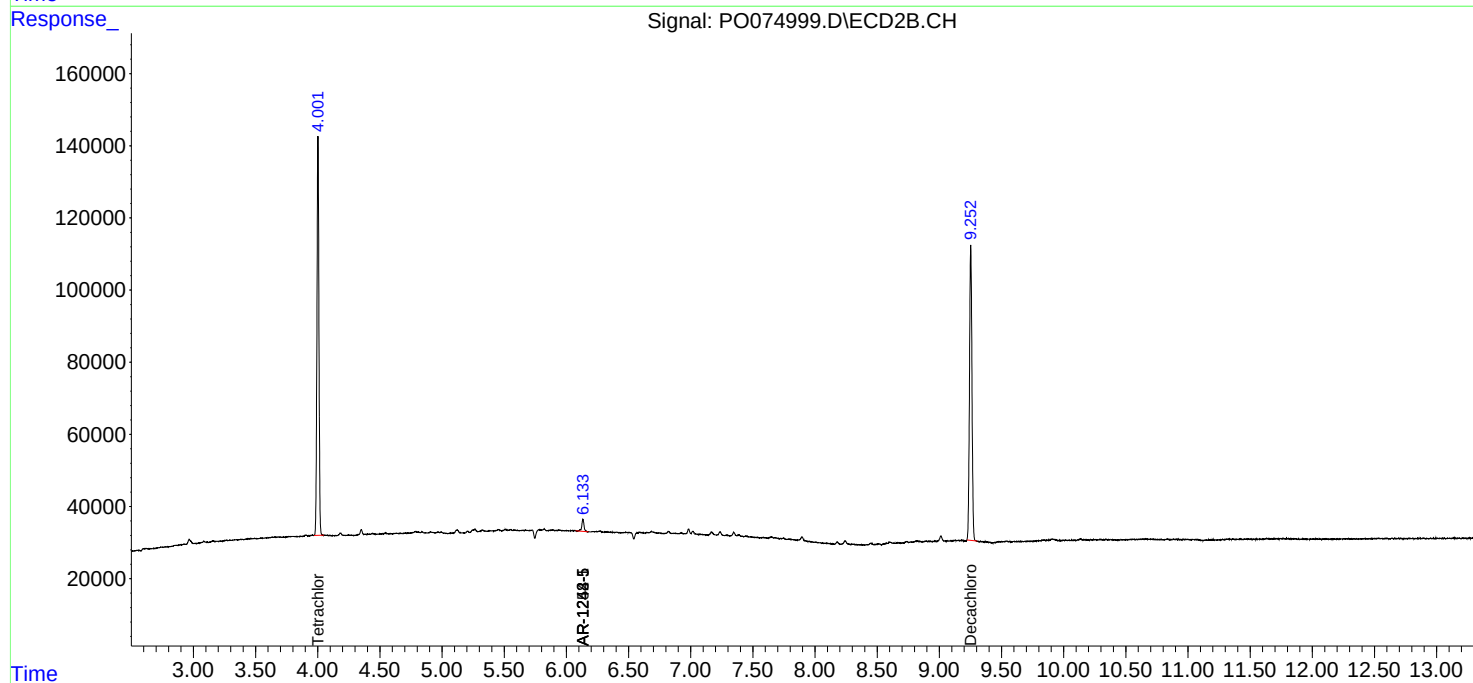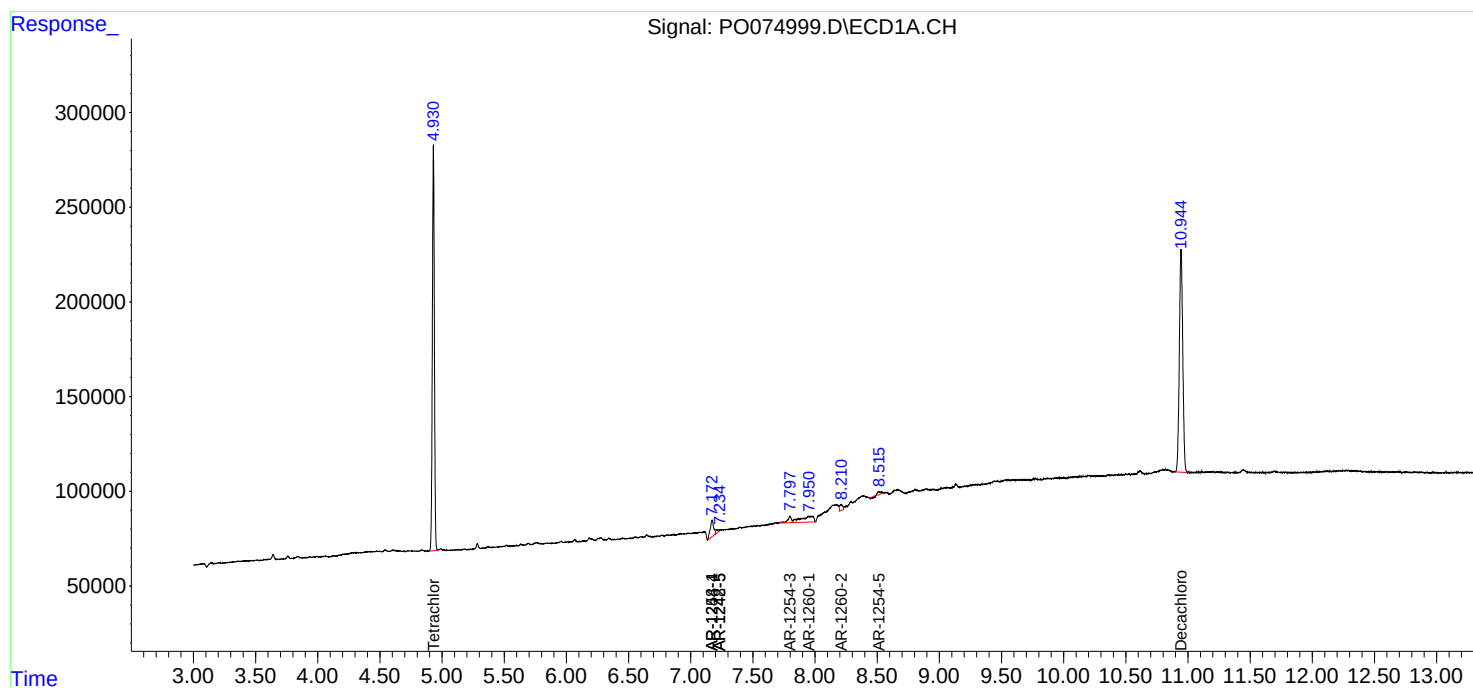


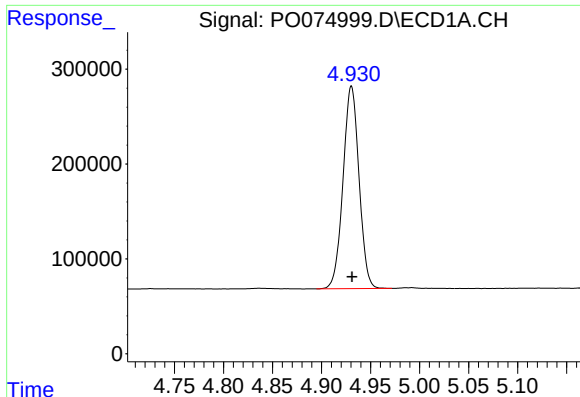

#1 Tetrachloro-m-xylene


R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 2422631
Conc: 22.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

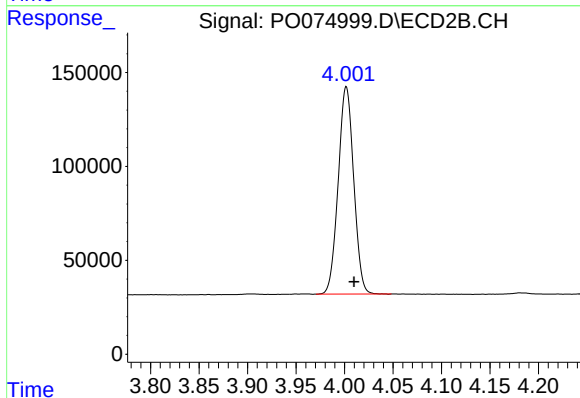


#1 Tetrachloro-m-xylene

R.T.: 4.002 min
Delta R.T.: -0.008 min
Response: 1228338
Conc: 21.84 ng/ml

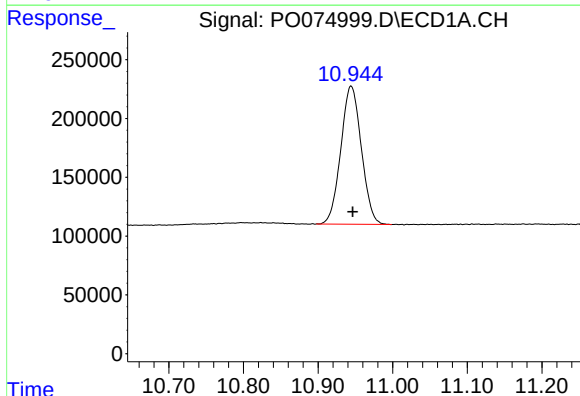


#2 Decachlorobiphenyl

R.T.: 10.944 min
Delta R.T.: -0.002 min
Response: 2245704
Conc: 22.13 ng/ml

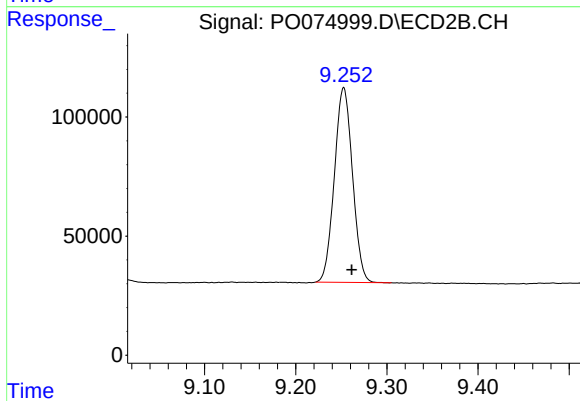

#2 Decachlorobiphenyl


R.T.: 9.253 min
Delta R.T.: -0.009 min
Response: 1127447
Conc: 20.53 ng/ml

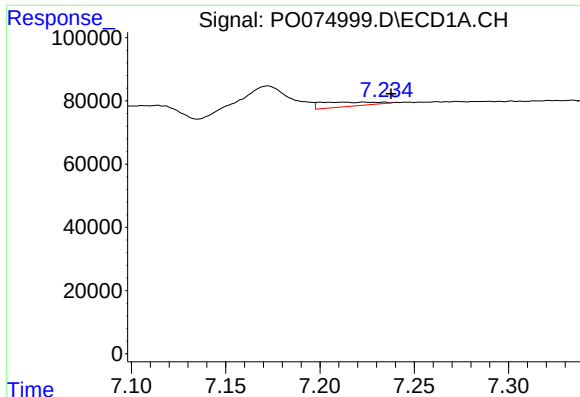

#20 AR-1242-5


R.T.: 7.234 min
Delta R.T.: -0.003 min
Response: 28119
Conc: 11.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

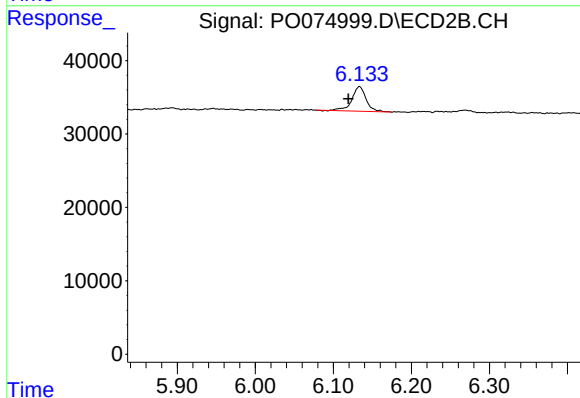


#20 AR-1242-5

R.T.: 6.134 min
Delta R.T.: 0.014 min
Response: 42892
Conc: 24.50 ng/ml

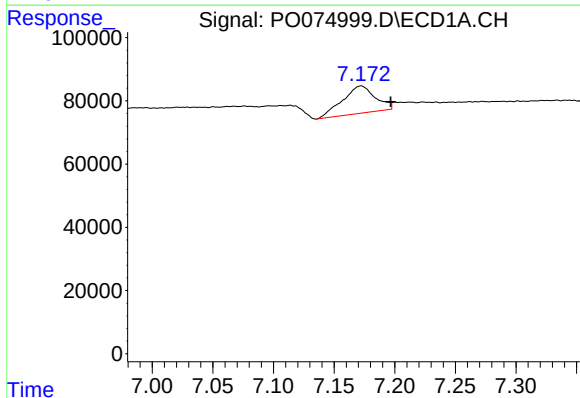


#24 AR-1248-4

R.T.: 7.172 min
Delta R.T.: -0.024 min
Response: 163756
Conc: 36.72 ng/ml

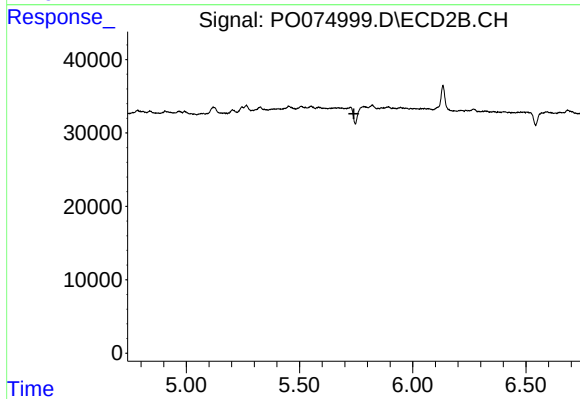

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.740 min
Response: 0
Conc: N.D.

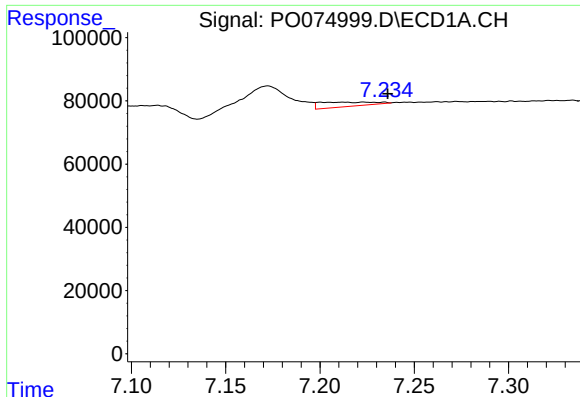

#25 AR-1248-5


R.T.: 7.234 min
Delta R.T.: -0.002 min
Response: 28119
Conc: 6.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

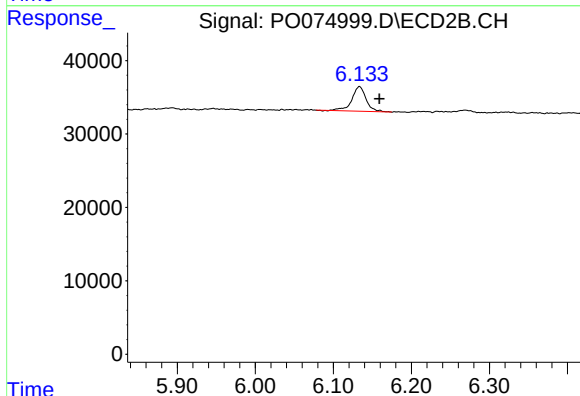


#25 AR-1248-5

R.T.: 6.134 min
Delta R.T.: -0.025 min
Response: 42892
Conc: 18.24 ng/ml

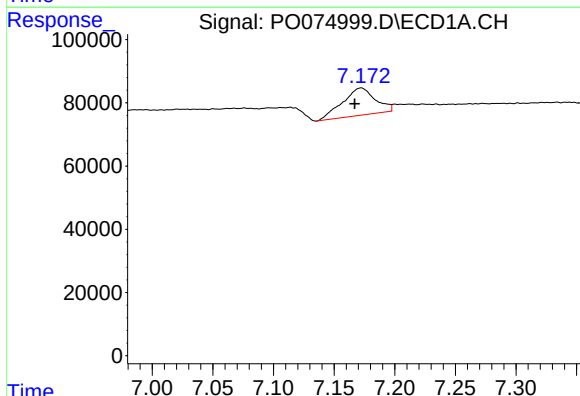


#26 AR-1254-1

R.T.: 7.172 min
Delta R.T.: 0.005 min
Response: 163756
Conc: 37.23 ng/ml

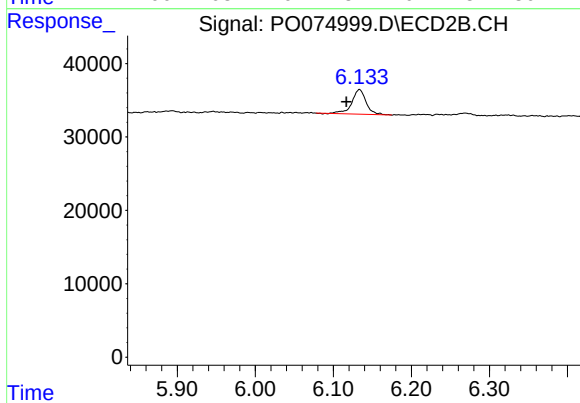

#26 AR-1254-1


R.T.: 6.134 min
Delta R.T.: 0.017 min
Response: 42892
Conc: 11.87 ng/ml

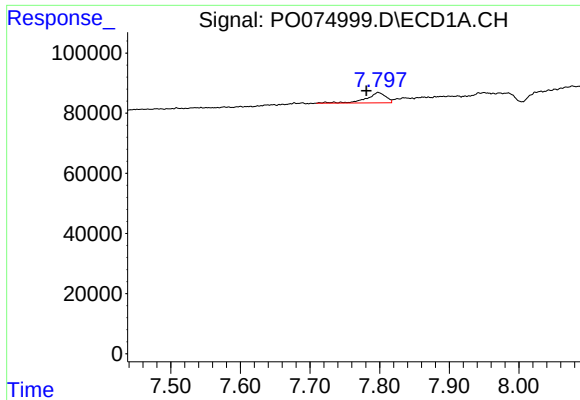

#28 AR-1254-3


R.T.: 7.798 min
Delta R.T.: 0.017 min
Response: 66849
Conc: 9.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

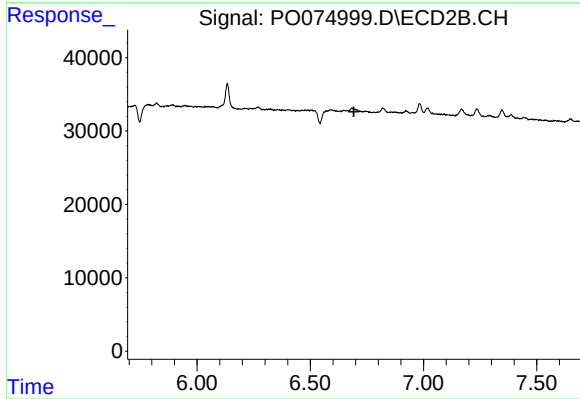


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.692 min
Response: 0
Conc: N.D.

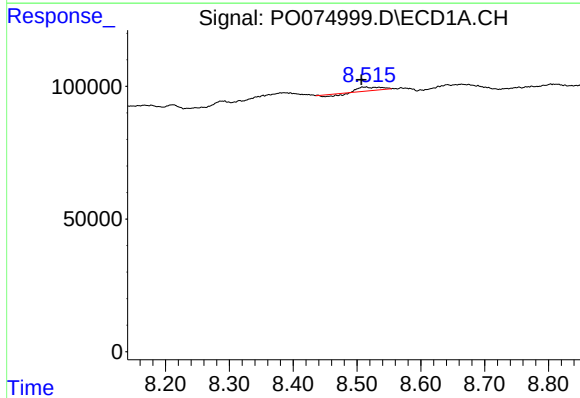


#30 AR-1254-5

R.T.: 8.515 min
Delta R.T.: 0.008 min
Response: 20745
Conc: 3.57 ng/ml

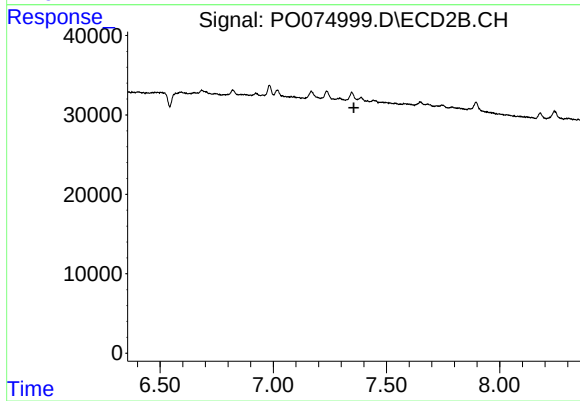

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.356 min
Response: 0
Conc: N.D.

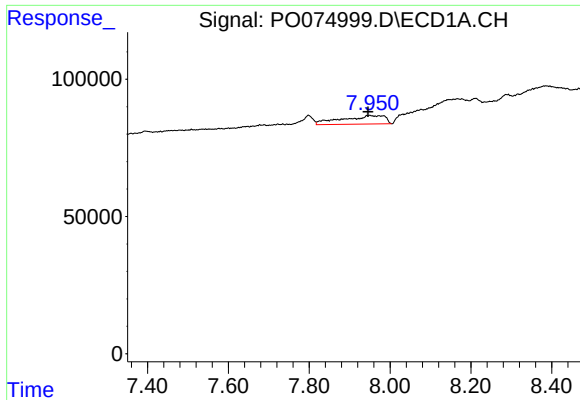

#31 AR-1260-1


R.T.: 7.950 min
Delta R.T.: 0.004 min
Response: 227500
Conc: 45.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

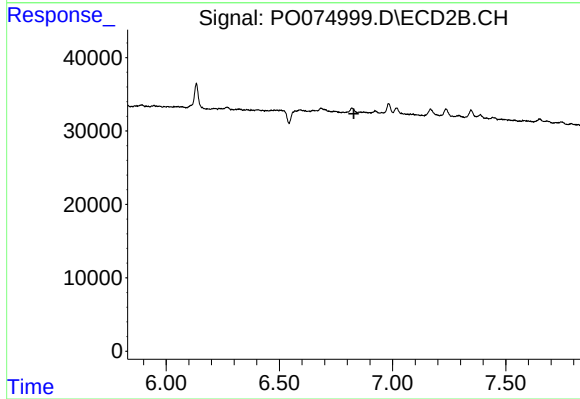


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.829 min
Response: 0
Conc: N.D.

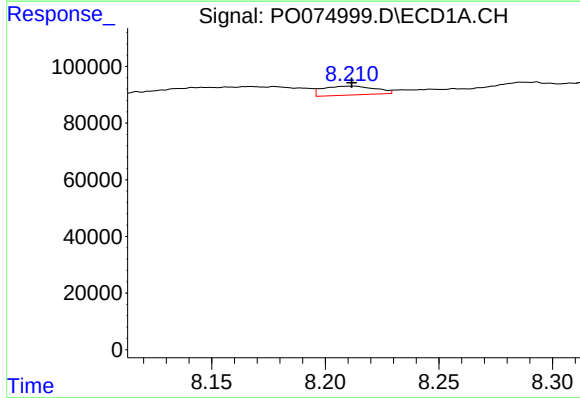

#32 AR-1260-2

R.T.: 8.212 min
Delta R.T.: 0.000 min
Response: 50376
Conc: 7.41 ng/ml

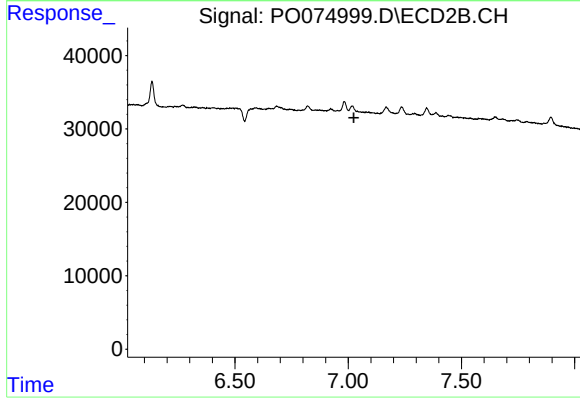

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.025 min
Response: 0
Conc: N.D.