

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012021\
 Data File : P0074981.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jan 2021 10:25
 Operator : AJ/MA
 Sample : M1106-08
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S6-03-C

Manual Integrations
 APPROVED

Ankita
 1/21/2021 10:38:43 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 13:05:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.938	4.003	2092175	1055065	19.828m	18.756
2) SA Decachlor...	10.956	9.256	1155454	615887	11.385	11.217m
Target Compounds						
41) L9 AR-1268-1	9.452	8.183	541791	325812	28.998	29.104
42) L9 AR-1268-2	9.548	8.247	404490	265900	25.352	27.793
43) L9 AR-1268-3	9.773	8.453	335540	191171	23.626	23.008
44) L9 AR-1268-4	10.212	8.740	54266	57759	9.263	16.649 #
45) L9 AR-1268-5	10.623	9.017	1018993	535252	24.385	22.605

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012021\
Data File : PO074981.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jan 2021 10:25
Operator : AJ/MA
Sample : M1106-08
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S6-03-C


Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:43 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 13:05:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

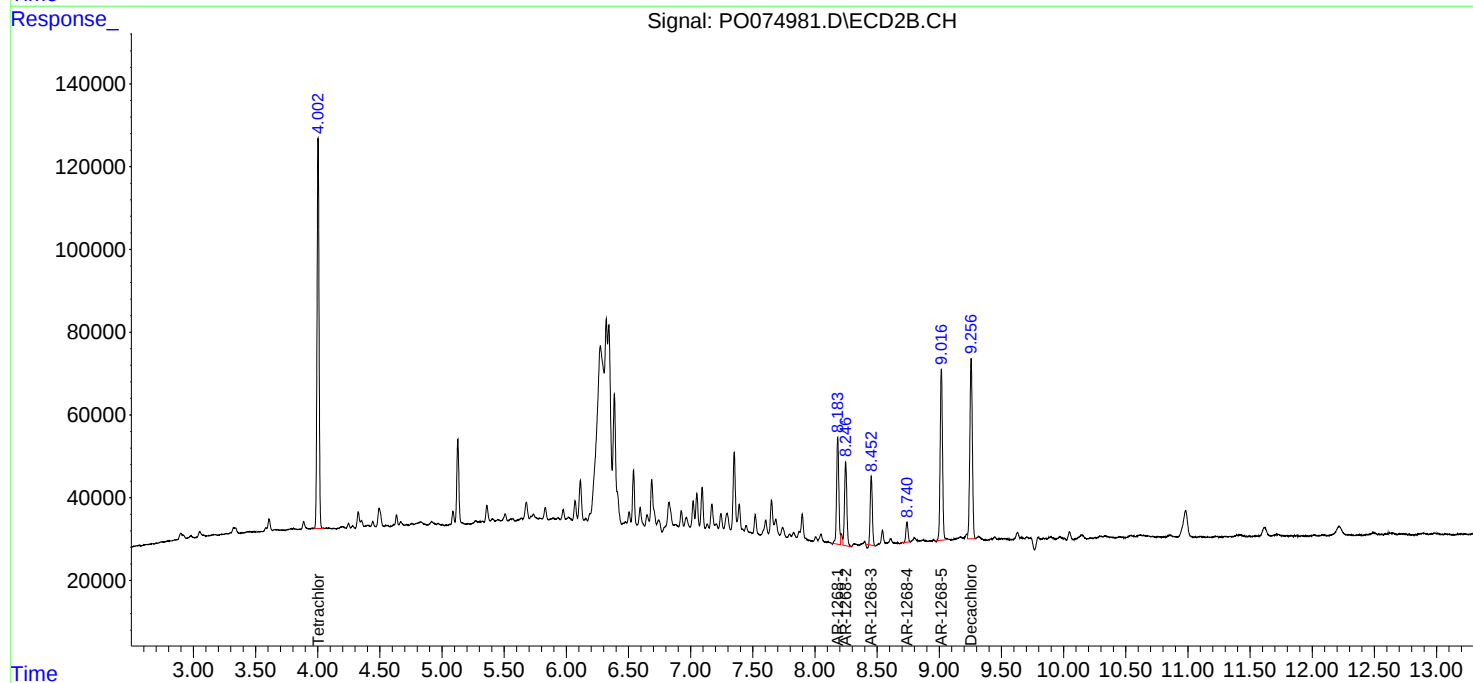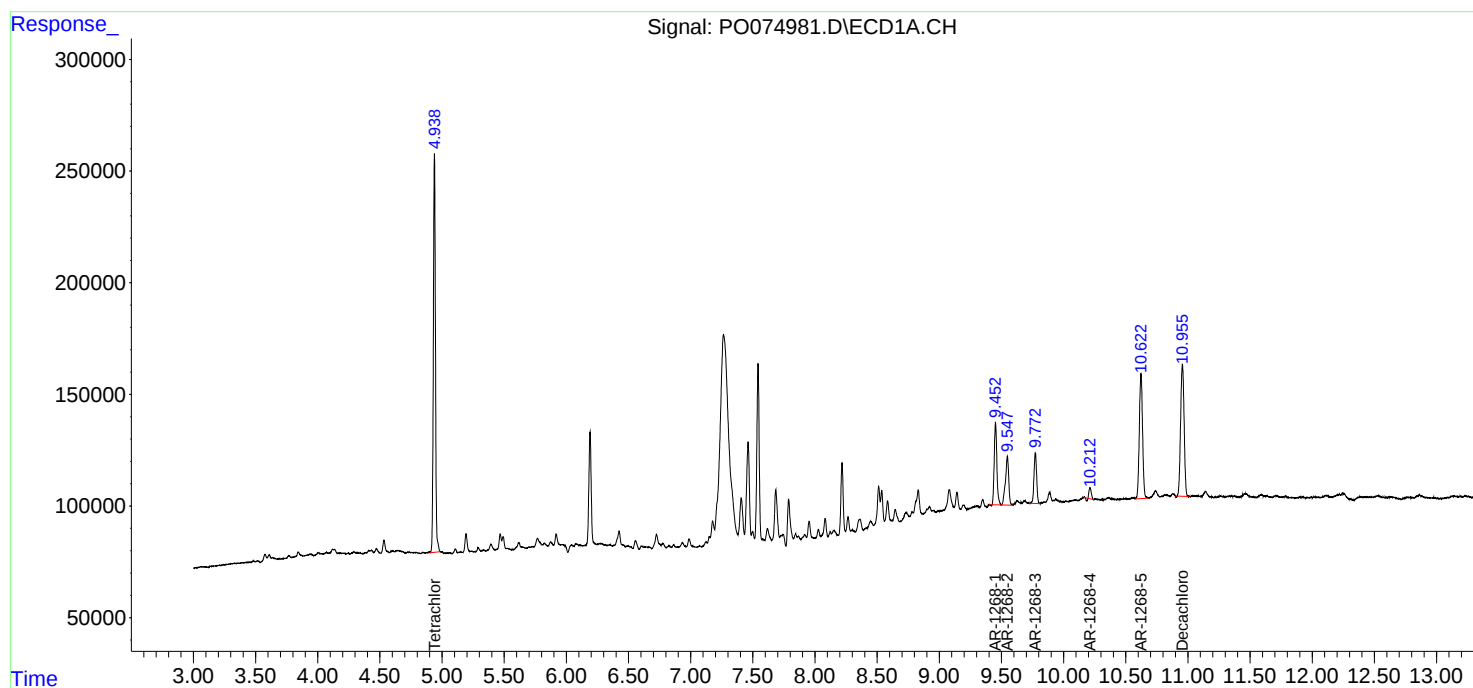

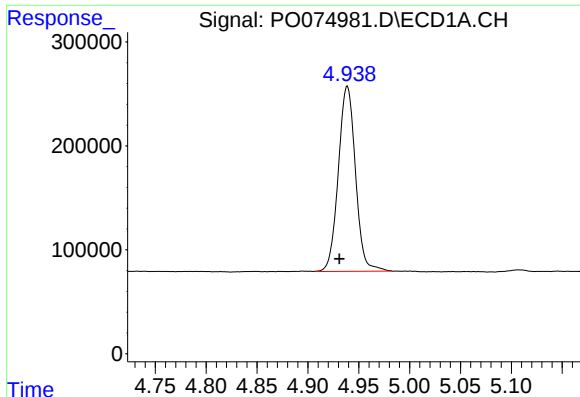


#1 Tetrachloro-m-xylene

R.T.: 4.938 min
Delta R.T.: 0.007 min
Response: 2092175
Conc: 19.83 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S6-03-C


Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:43 AM

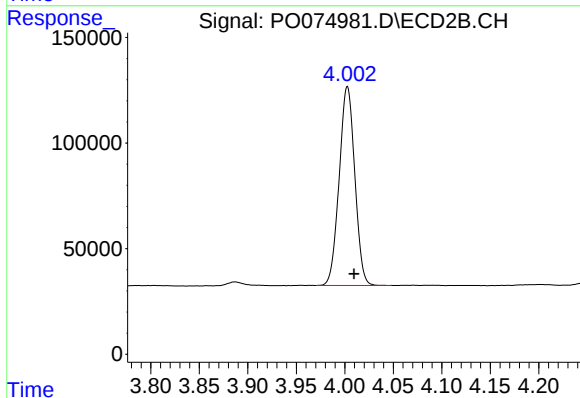


#1 Tetrachloro-m-xylene

R.T.: 4.003 min
Delta R.T.: -0.007 min
Response: 1055065
Conc: 18.76 ng/ml

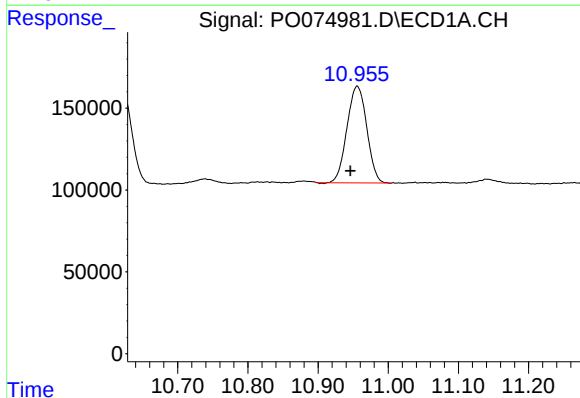


#2 Decachlorobiphenyl

R.T.: 10.956 min
Delta R.T.: 0.009 min
Response: 1155454
Conc: 11.38 ng/ml

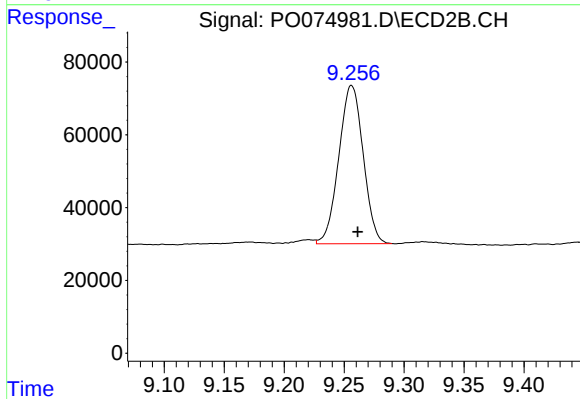

#2 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: -0.006 min
Response: 615887
Conc: 11.22 ng/ml m

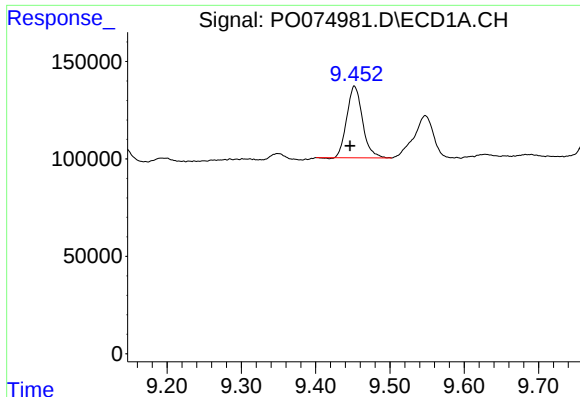


#41 AR-1268-1

R.T.: 9.452 min
Delta R.T.: 0.006 min
Response: 541791
Conc: 29.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
S6-03-C


Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:43 AM

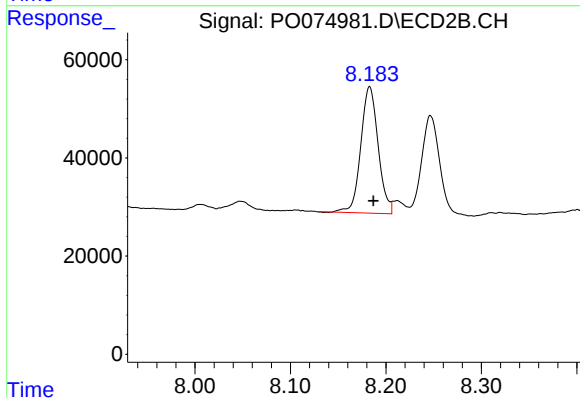


#41 AR-1268-1

R.T.: 8.183 min
Delta R.T.: -0.004 min
Response: 325812
Conc: 29.10 ng/ml

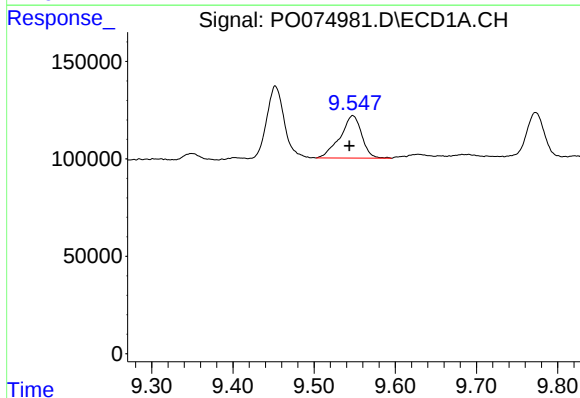


#42 AR-1268-2

R.T.: 9.548 min
Delta R.T.: 0.004 min
Response: 404490
Conc: 25.35 ng/ml

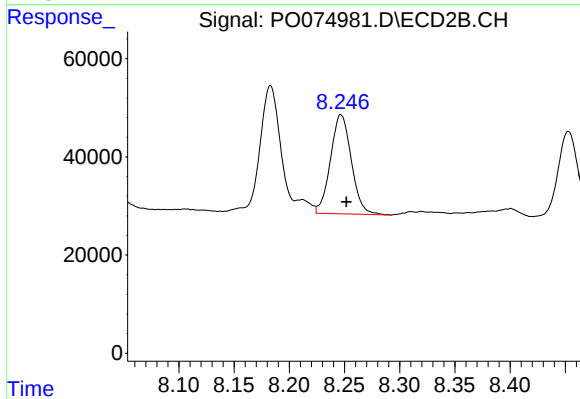

#42 AR-1268-2

R.T.: 8.247 min
Delta R.T.: -0.005 min
Response: 265900
Conc: 27.79 ng/ml

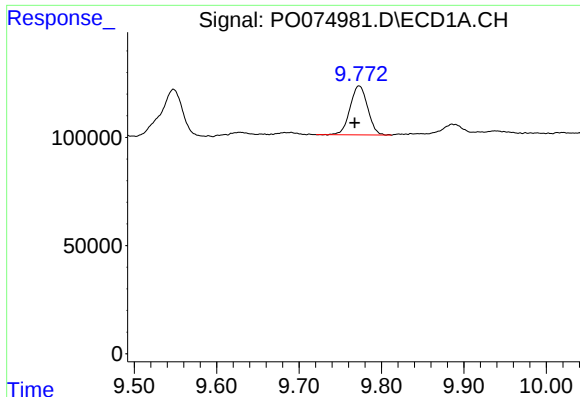


#43 AR-1268-3

R.T.: 9.773 min
Delta R.T.: 0.005 min
Response: 335540
Conc: 23.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
S6-03-C


Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:43 AM

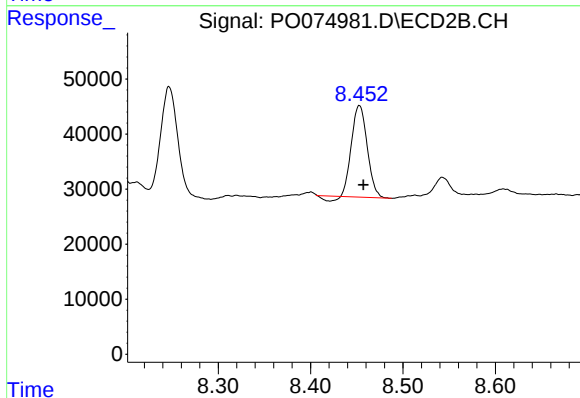


#43 AR-1268-3

R.T.: 8.453 min
Delta R.T.: -0.004 min
Response: 191171
Conc: 23.01 ng/ml

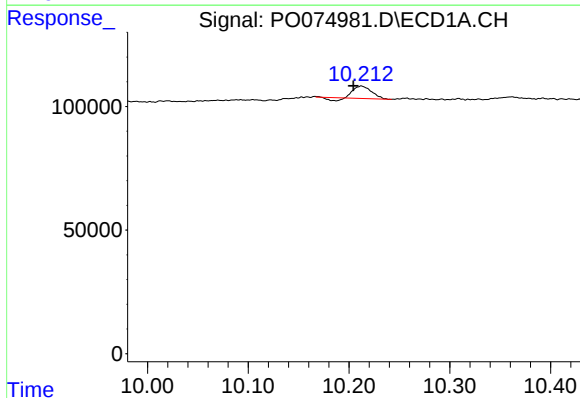


#44 AR-1268-4

R.T.: 10.212 min
Delta R.T.: 0.008 min
Response: 54266
Conc: 9.26 ng/ml

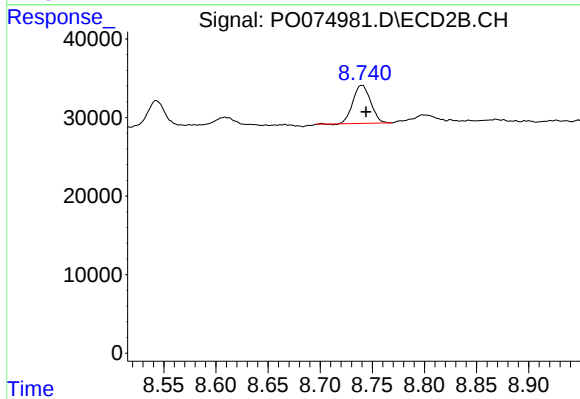

#44 AR-1268-4

R.T.: 8.740 min
Delta R.T.: -0.004 min
Response: 57759
Conc: 16.65 ng/ml

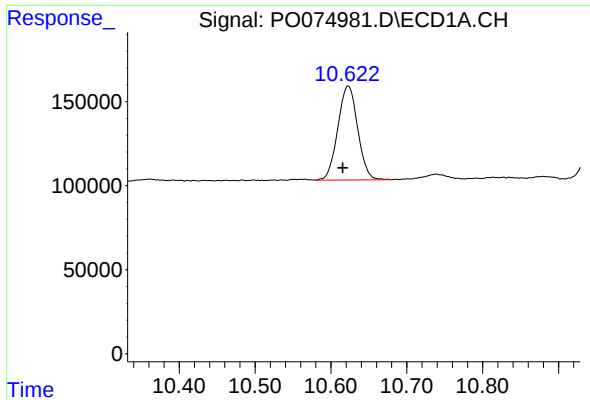


#45 AR-1268-5

R.T.: 10.623 min
Delta R.T.: 0.007 min
Response: 1018993
Conc: 24.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
S6-03-C

Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:43 AM

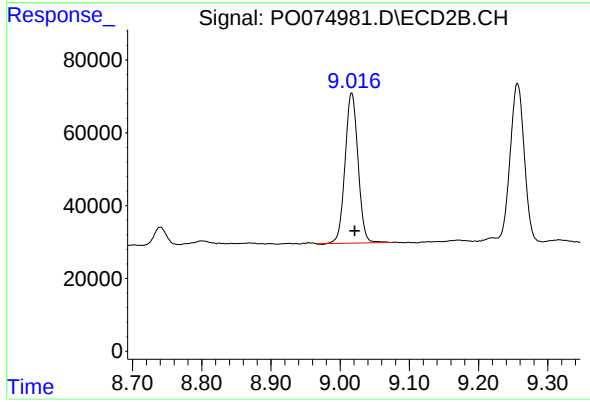

#45 AR-1268-5

R.T.: 9.017 min
Delta R.T.: -0.005 min
Response: 535252
Conc: 22.60 ng/ml