

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012021\
 Data File : P0074986.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jan 2021 12:42
 Operator : AJ/MA
 Sample : M1177-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PILE-1-(0.5-1.0)

Manual Integrations
 APPROVED

Ankita
 1/21/2021 10:38:45 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 13:07:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.928	4.002	2419870	1236557	22.933	21.982
2) SA Decachlor...	10.946	9.251	1334331	681788	13.147	12.418m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012021\
Data File : P0074986.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jan 2021 12:42
Operator : AJ/MA
Sample : M1177-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PILE-1-(0.5-1.0)


Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:45 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 13:07:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

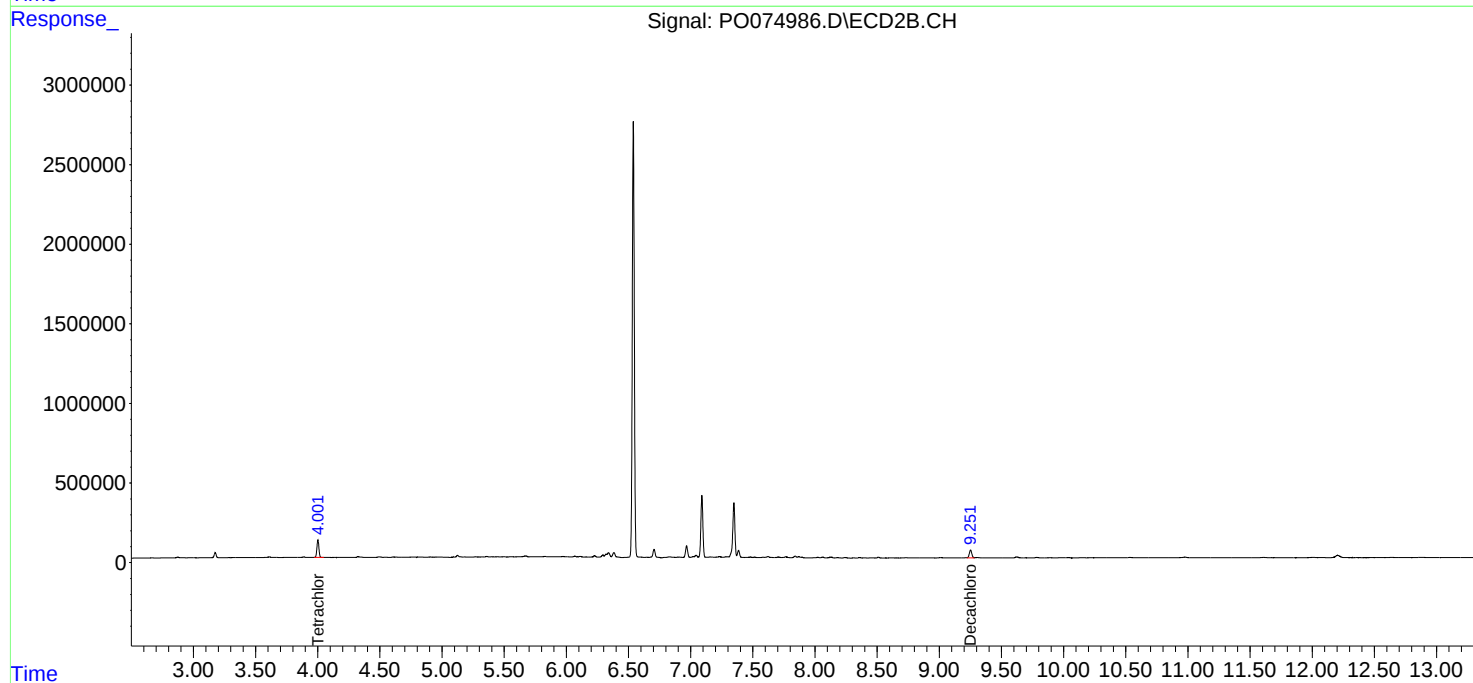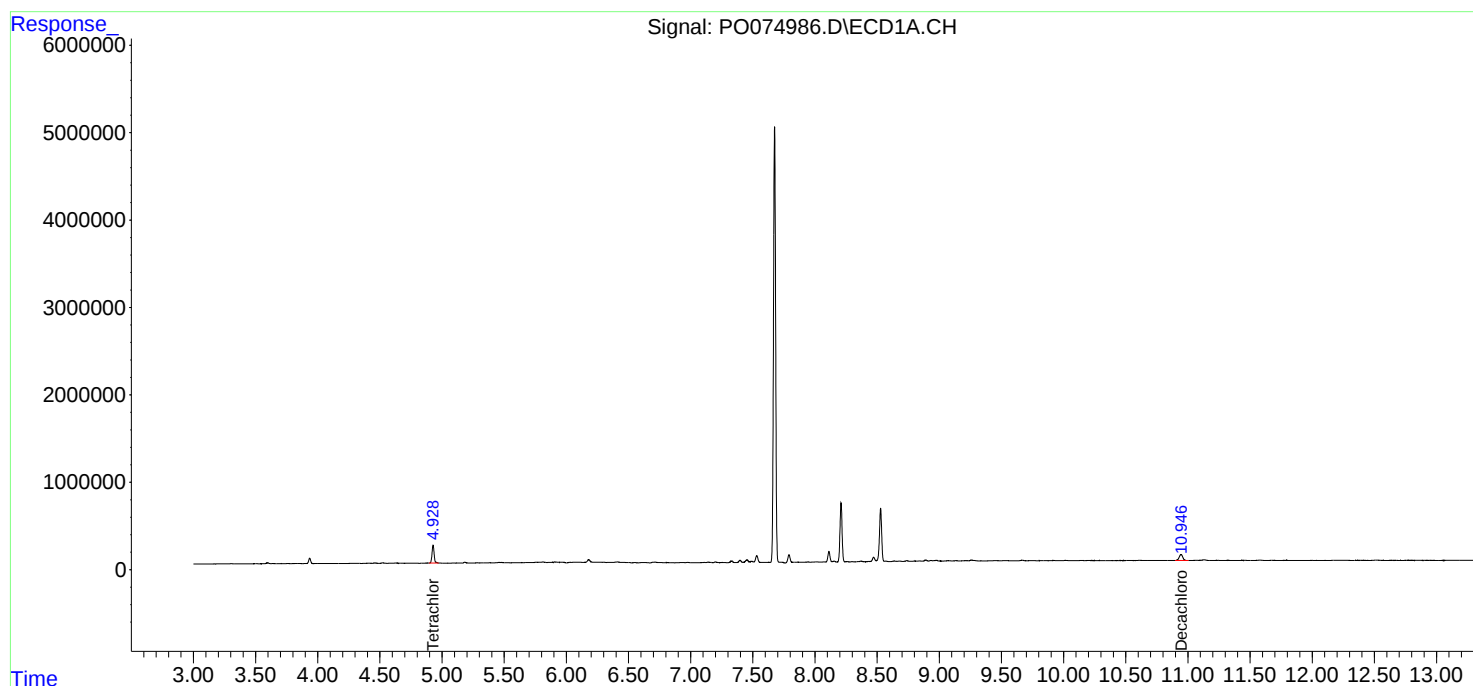

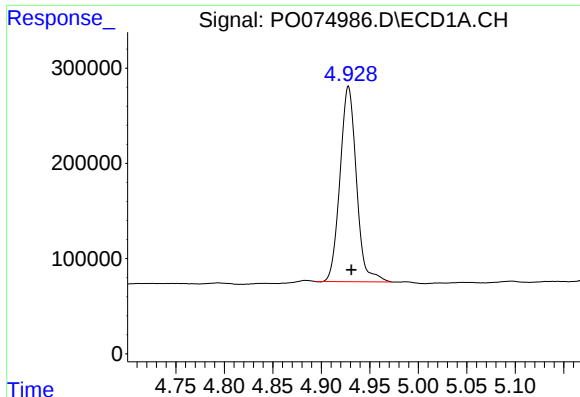


#1 Tetrachloro-m-xylene

R.T.: 4.928 min
Delta R.T.: -0.003 min
Response: 2419870
Conc: 22.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
PILE-1-(0.5-1.0)


Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:45 AM

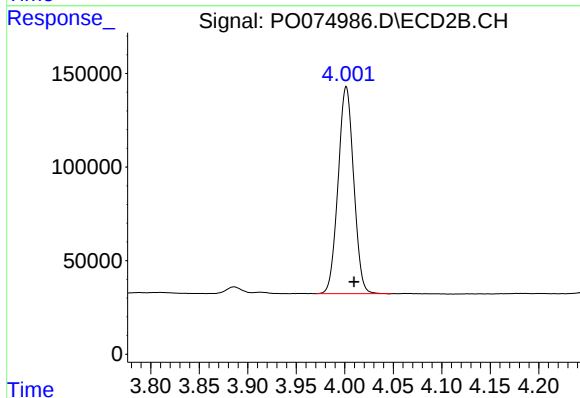


#1 Tetrachloro-m-xylene

R.T.: 4.002 min
Delta R.T.: -0.008 min
Response: 1236557
Conc: 21.98 ng/ml

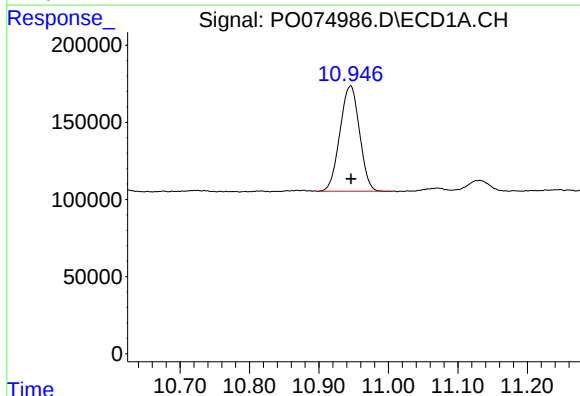

#2 Decachlorobiphenyl

R.T.: 10.946 min
Delta R.T.: 0.000 min
Response: 1334331
Conc: 13.15 ng/ml

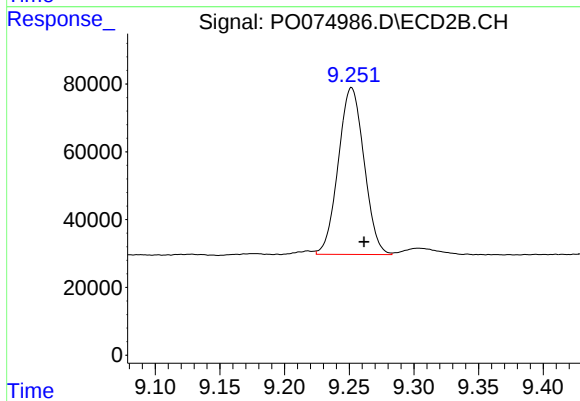

#2 Decachlorobiphenyl

R.T.: 9.251 min
Delta R.T.: -0.010 min
Response: 681788
Conc: 12.42 ng/ml m