

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012021\
 Data File : P0074992.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jan 2021 14:25
 Operator : AJ/MA
 Sample : M1086-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S3-03-D

Manual Integrations
 APPROVED

Ankita
 1/21/2021 10:38:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 05:23:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.928	4.002	2237690	1237745	21.207m	22.003
2) SA Decachlor...	10.944	9.245f	1384717	2312310	13.644	42.115m#
Target Compounds						
26) L6 AR-1254-1	7.164	6.111	5636066	3941388	1281.466	1091.191
27) L6 AR-1254-2	7.394	6.269	11463852	4787588	1683.194	1536.188
28) L6 AR-1254-3	7.778	6.685	15532902	9505893	2214.453	1938.427
29) L6 AR-1254-4	8.074	6.923	14005016	6549533	2309.278	1888.682
30) L6 AR-1254-5	8.503	7.349	22483438	18995527	3870.491	4197.033

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012021\
Data File : PO074992.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jan 2021 14:25
Operator : AJ/MA
Sample : M1086-09
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S3-03-D


Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:50 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 05:23:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

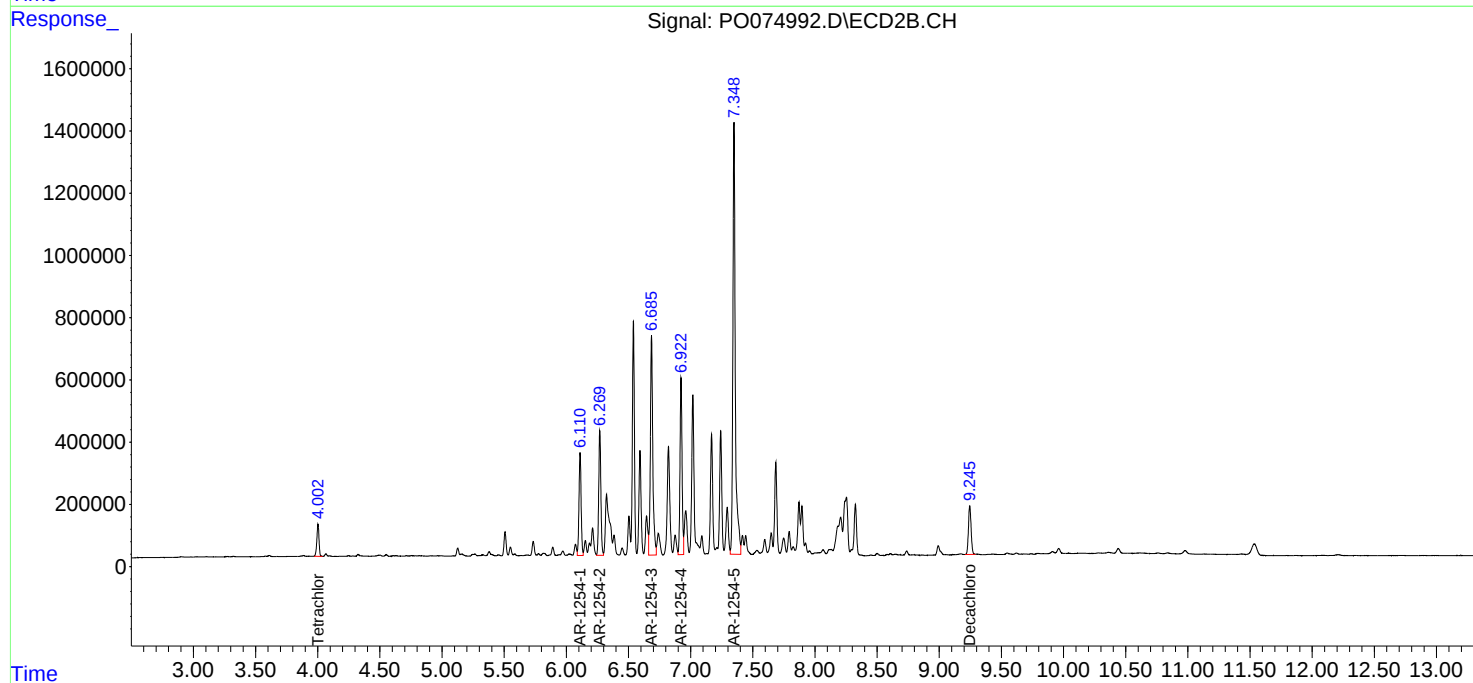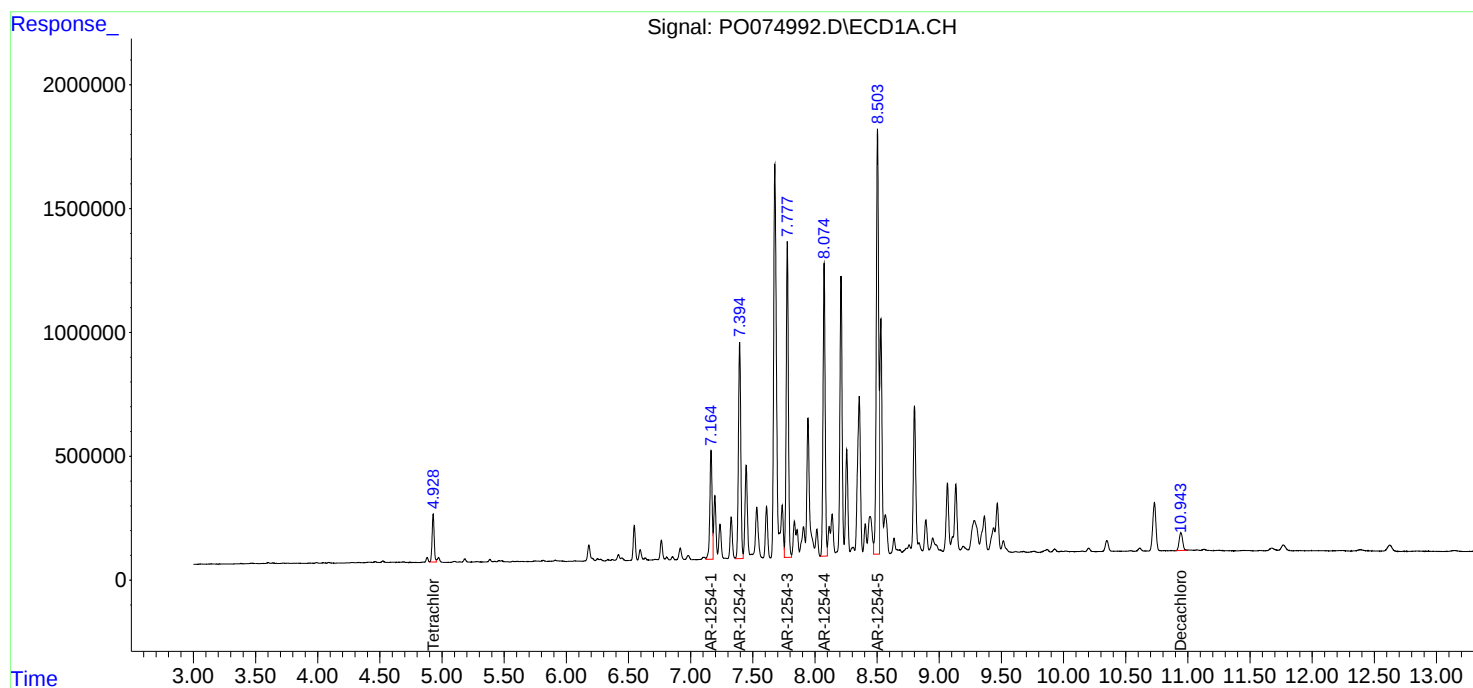

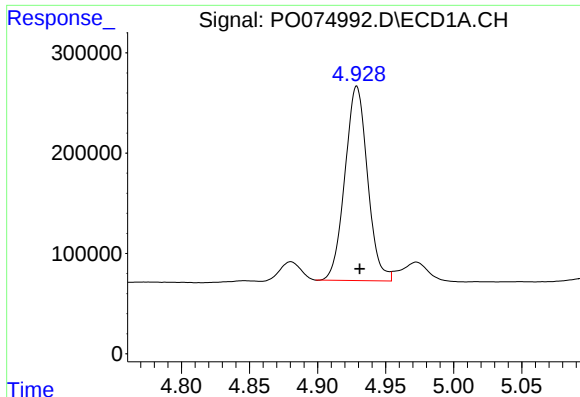


#1 Tetrachloro-m-xylene

R.T.: 4.928 min
Delta R.T.: -0.003 min
Response: 2237690
Conc: 21.21 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S3-03-D


Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:50 AM

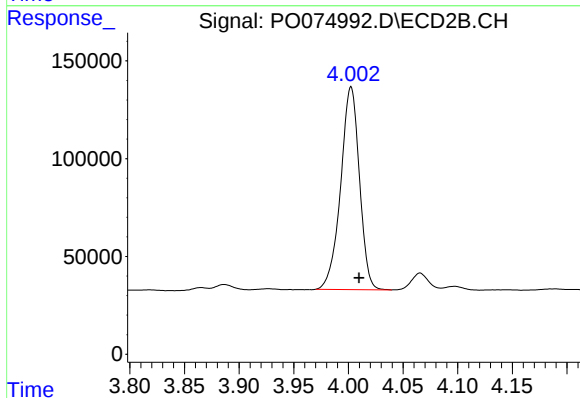


#1 Tetrachloro-m-xylene

R.T.: 4.002 min
Delta R.T.: -0.007 min
Response: 1237745
Conc: 22.00 ng/ml

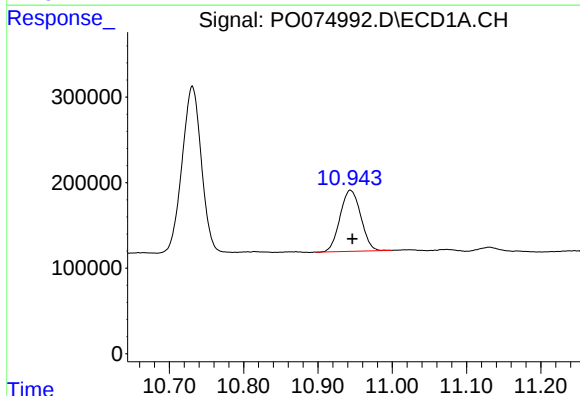


#2 Decachlorobiphenyl

R.T.: 10.944 min
Delta R.T.: -0.003 min
Response: 1384717
Conc: 13.64 ng/ml

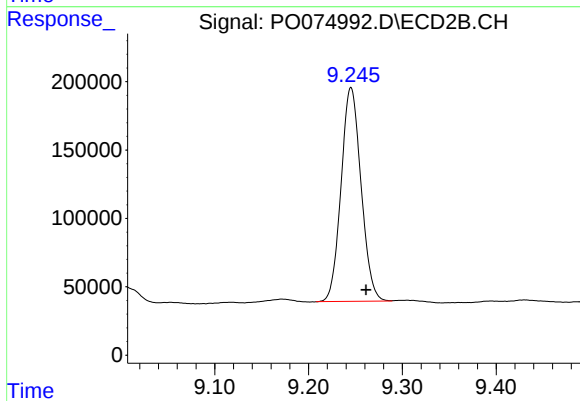

#2 Decachlorobiphenyl

R.T.: 9.245 min
Delta R.T.: -0.017 min
Response: 2312310
Conc: 42.12 ng/ml m

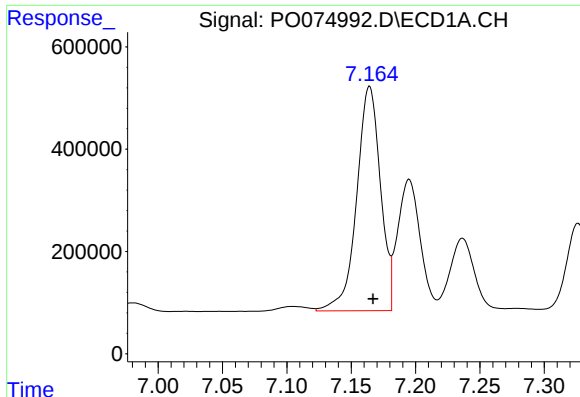


#26 AR-1254-1

R.T.: 7.164 min
Delta R.T.: -0.003 min
Response: 5636066
Conc: 1281.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-03-D


Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:50 AM

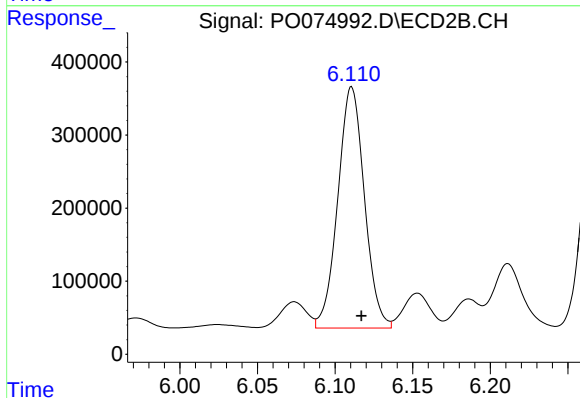


#26 AR-1254-1

R.T.: 6.111 min
Delta R.T.: -0.006 min
Response: 3941388
Conc: 1091.19 ng/ml

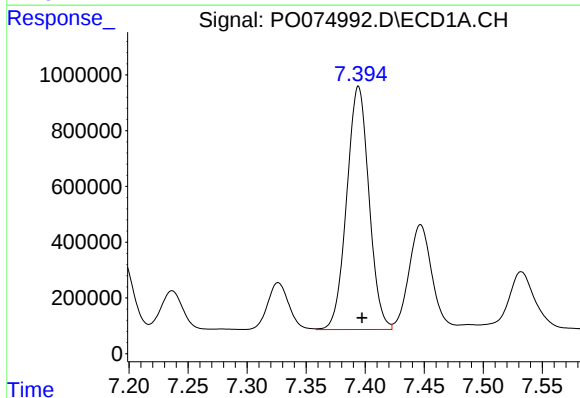


#27 AR-1254-2

R.T.: 7.394 min
Delta R.T.: -0.003 min
Response: 11463852
Conc: 1683.19 ng/ml

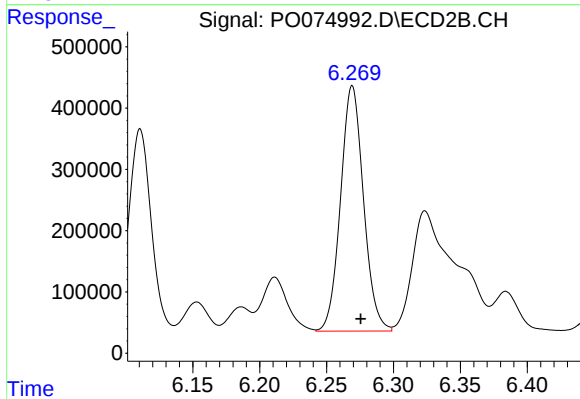

#27 AR-1254-2

R.T.: 6.269 min
Delta R.T.: -0.006 min
Response: 4787588
Conc: 1536.19 ng/ml

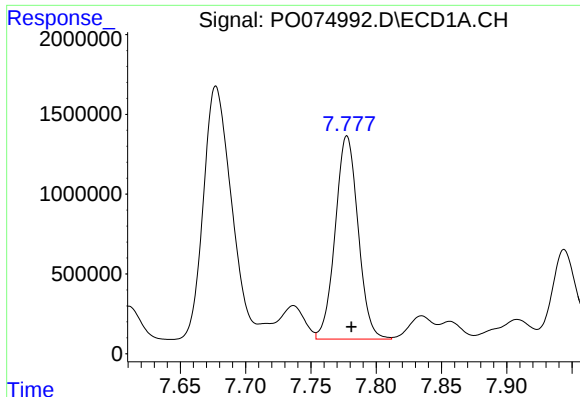


#28 AR-1254-3

R.T.: 7.778 min
Delta R.T.: -0.003 min
Response: 15532902
Conc: 2214.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-03-D


Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:50 AM

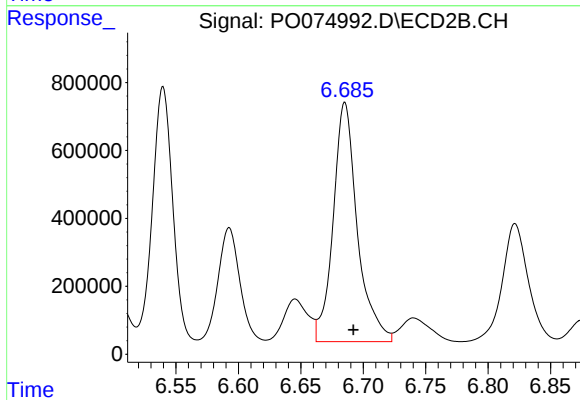


#28 AR-1254-3

R.T.: 6.685 min
Delta R.T.: -0.007 min
Response: 9505893
Conc: 1938.43 ng/ml

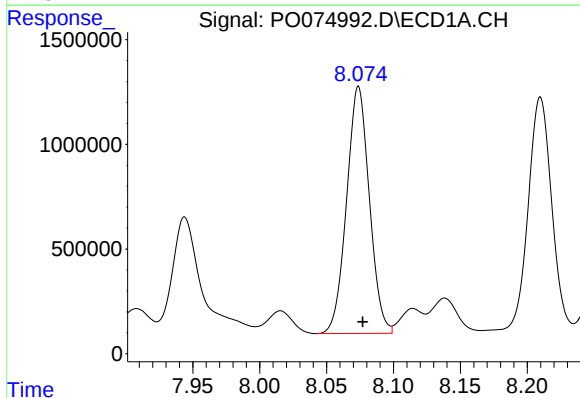


#29 AR-1254-4

R.T.: 8.074 min
Delta R.T.: -0.003 min
Response: 14005016
Conc: 2309.28 ng/ml

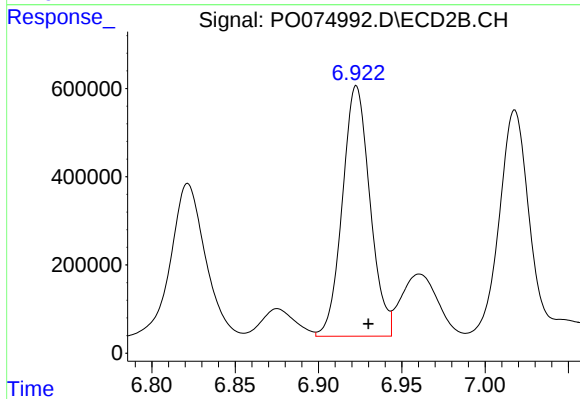

#29 AR-1254-4

R.T.: 6.923 min
Delta R.T.: -0.007 min
Response: 6549533
Conc: 1888.68 ng/ml

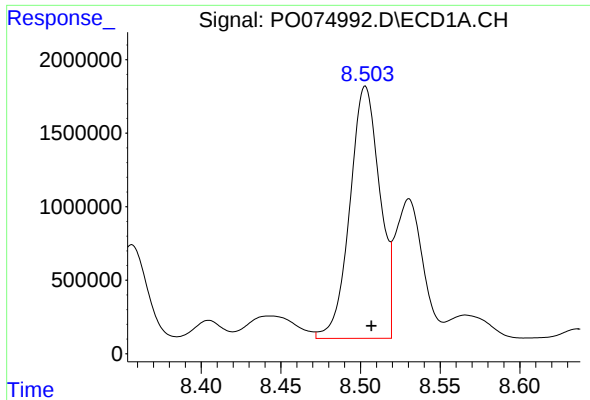


#30 AR-1254-5

R.T.: 8.503 min
Delta R.T.: -0.004 min
Response: 22483438
Conc: 3870.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-03-D

Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:50 AM

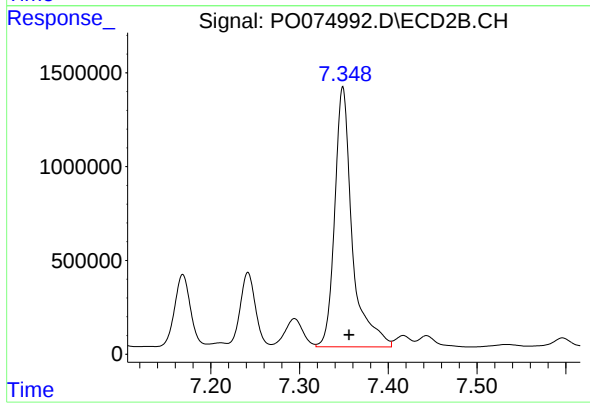

#30 AR-1254-5

R.T.: 7.349 min
Delta R.T.: -0.007 min
Response: 18995527
Conc: 4197.03 ng/ml