

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012021\
 Data File : P0075006.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jan 2021 18:27
 Operator : AJ/MA
 Sample : M1085-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S2-02-D

Manual Integrations
 APPROVED

Ankita
 1/21/2021 10:38:55 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 05:31:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.928	4.001	2180599	1147084	20.666	20.392
2) SA Decachlor...	10.942	9.250	1349543	895963	13.297	16.319m
Target Compounds						
26) L6 AR-1254-1	7.163	6.109	3821147	2471513	868.810	684.249
27) L6 AR-1254-2	7.393	6.269	7849888	3180249	1152.570	1020.443
28) L6 AR-1254-3	7.776	6.685	9904698	6077100	1412.067	1239.233
29) L6 AR-1254-4	8.073	6.922	9245552	4209366	1524.493	1213.850
30) L6 AR-1254-5	8.502	7.348	15453514	14476259	2660.300	3198.508

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012021\
Data File : PO075006.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jan 2021 18:27
Operator : AJ/MA
Sample : M1085-07
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S2-02-D


Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:55 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 05:31:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

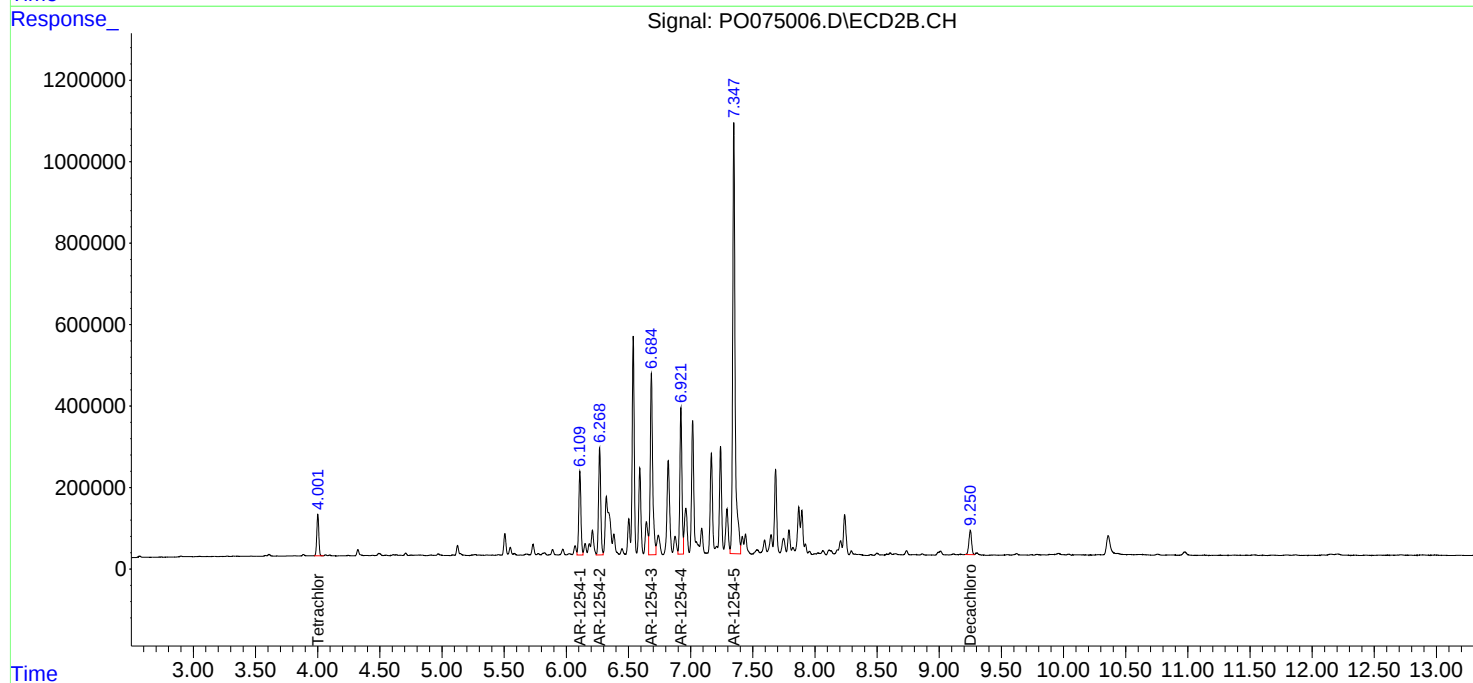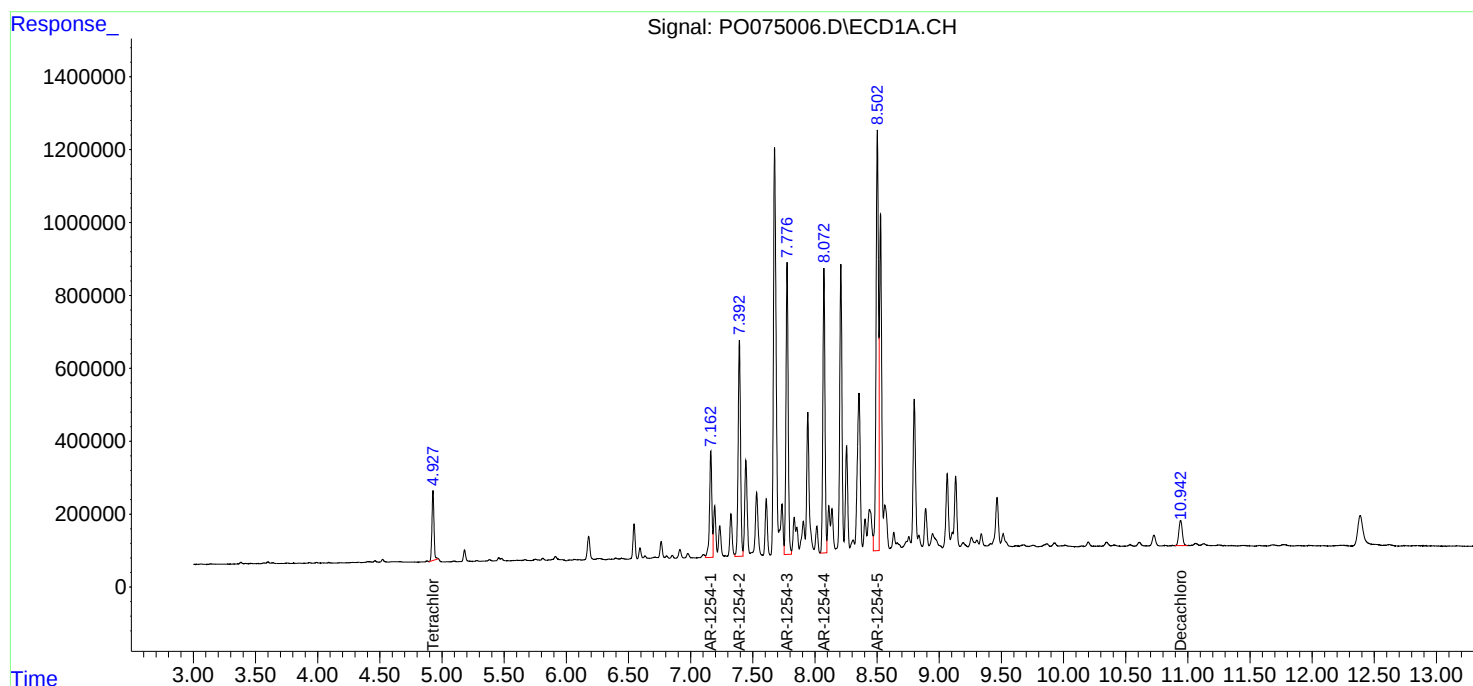

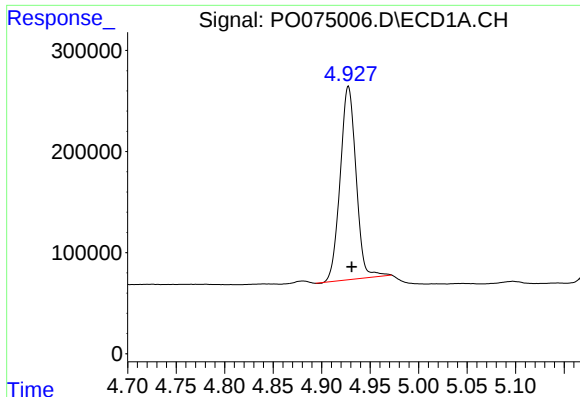


#1 Tetrachloro-m-xylene

R.T.: 4.928 min
Delta R.T.: -0.003 min
Response: 2180599
Conc: 20.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-02-D


Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:55 AM

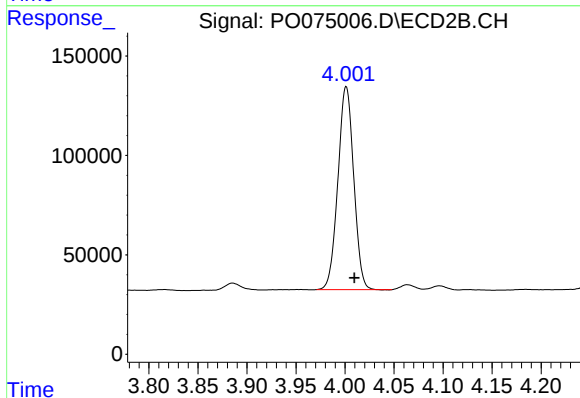


#1 Tetrachloro-m-xylene

R.T.: 4.001 min
Delta R.T.: -0.008 min
Response: 1147084
Conc: 20.39 ng/ml

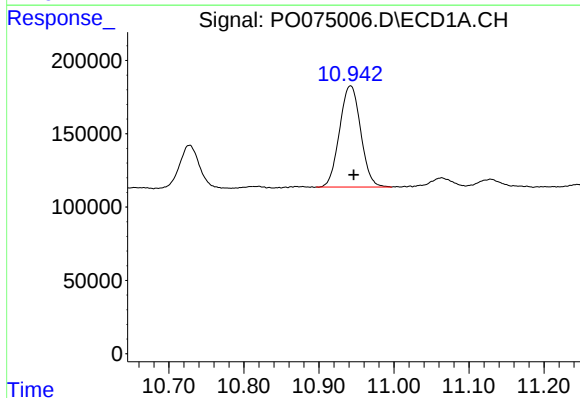


#2 Decachlorobiphenyl

R.T.: 10.942 min
Delta R.T.: -0.004 min
Response: 1349543
Conc: 13.30 ng/ml

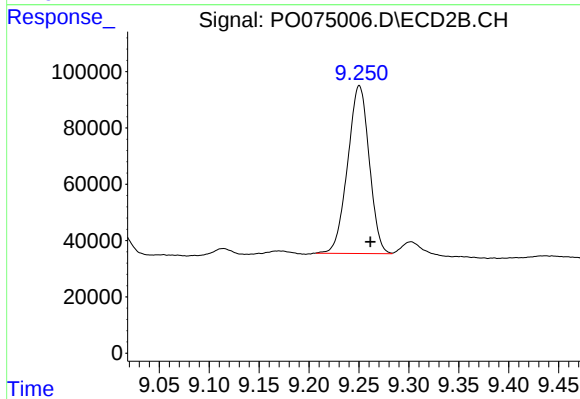

#2 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.012 min
Response: 895963
Conc: 16.32 ng/ml m

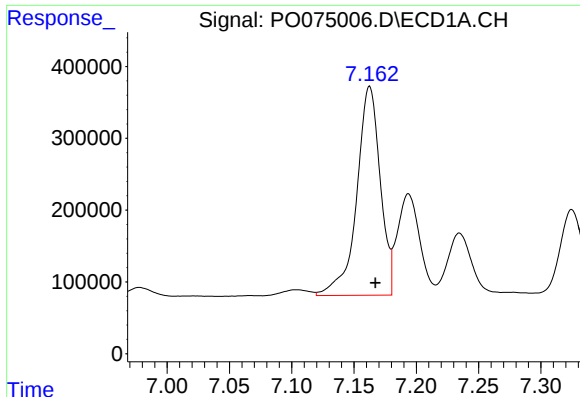


#26 AR-1254-1

R.T.: 7.163 min
Delta R.T.: -0.005 min
Response: 3821147
Conc: 868.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-02-D


Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:55 AM

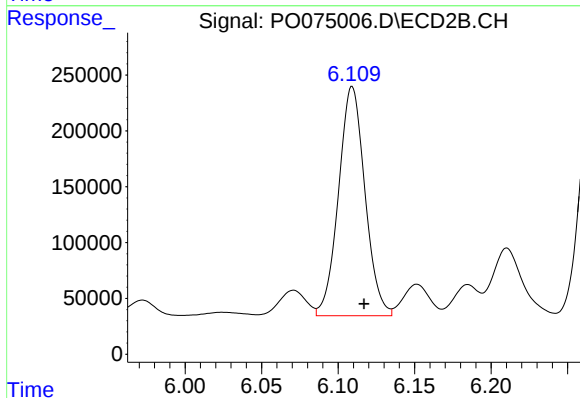


#26 AR-1254-1

R.T.: 6.109 min
Delta R.T.: -0.008 min
Response: 2471513
Conc: 684.25 ng/ml

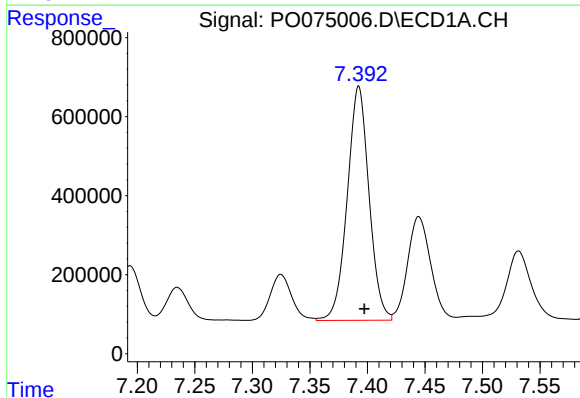


#27 AR-1254-2

R.T.: 7.393 min
Delta R.T.: -0.005 min
Response: 7849888
Conc: 1152.57 ng/ml

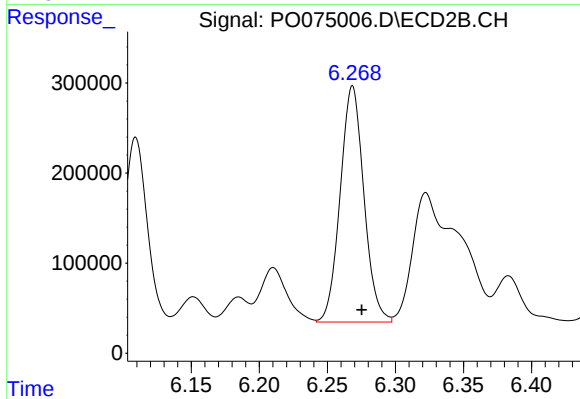

#27 AR-1254-2

R.T.: 6.269 min
Delta R.T.: -0.007 min
Response: 3180249
Conc: 1020.44 ng/ml

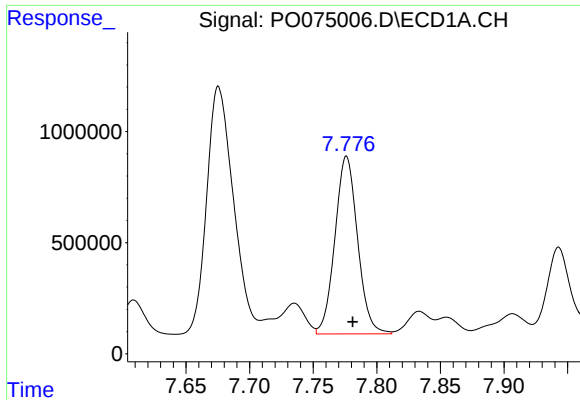


#28 AR-1254-3

R.T.: 7.776 min
Delta R.T.: -0.005 min
Response: 9904698
Conc: 1412.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-02-D


Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:55 AM

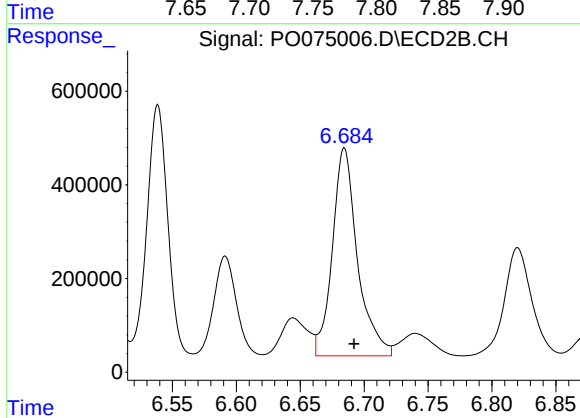


#28 AR-1254-3

R.T.: 6.685 min
Delta R.T.: -0.008 min
Response: 6077100
Conc: 1239.23 ng/ml

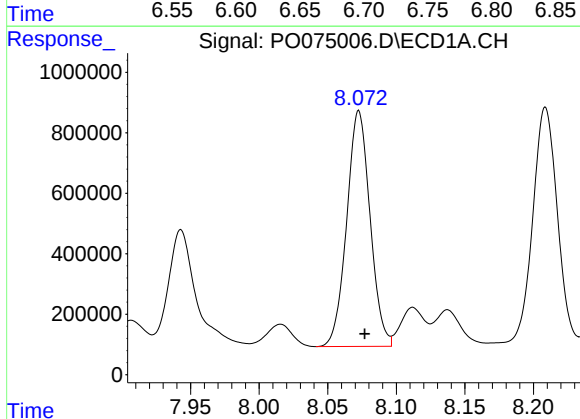


#29 AR-1254-4

R.T.: 8.073 min
Delta R.T.: -0.004 min
Response: 9245552
Conc: 1524.49 ng/ml

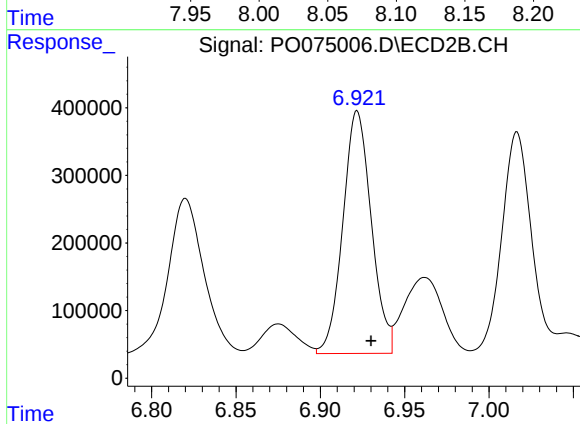

#29 AR-1254-4

R.T.: 6.922 min
Delta R.T.: -0.008 min
Response: 4209366
Conc: 1213.85 ng/ml

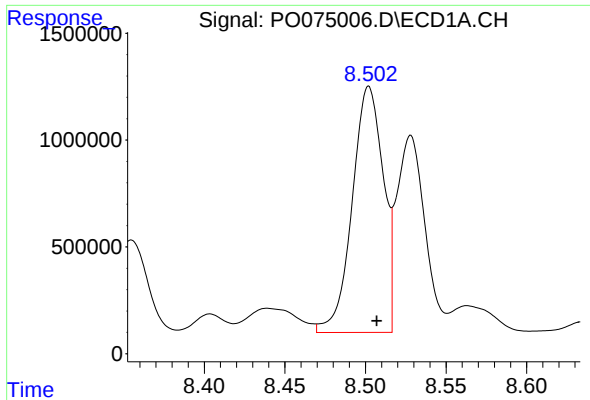


#30 AR-1254-5

R.T.: 8.502 min
Delta R.T.: -0.005 min
Response: 15453514
Conc: 2660.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-02-D

Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:55 AM

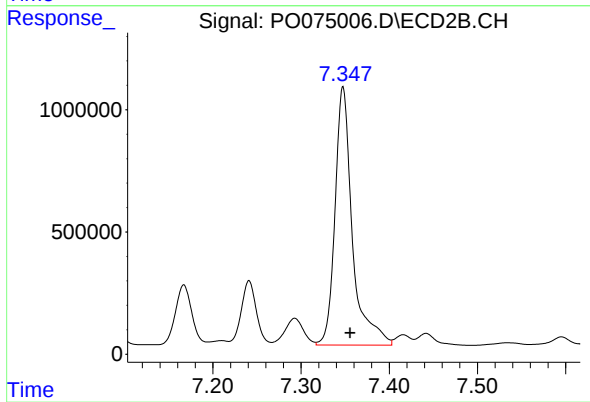

#30 AR-1254-5

R.T.: 7.348 min
Delta R.T.: -0.008 min
Response: 14476259
Conc: 3198.51 ng/ml