

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012021\
 Data File : P0075008.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jan 2021 19:02
 Operator : AJ/MA
 Sample : M1088-18
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S5-02-D

Manual Integrations
 APPROVED

Ankita
 1/21/2021 10:38:57 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 05:32:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.927	4.001	1311585	669141	12.430	11.895
2) SA Decachlor...	10.943	9.251	690052	366994	6.799	6.684
Target Compounds						
26) L6 AR-1254-1	7.162	6.109	129500	102280	29.444m	28.317
27) L6 AR-1254-2	7.391	6.267	523523	194054	76.867	62.266
28) L6 AR-1254-3	7.776	6.684	703876	465424	100.348	94.908
29) L6 AR-1254-4	8.073	6.922	603599	322752	99.527	93.072
30) L6 AR-1254-5	8.507	7.348	922389	3790499	158.788m	837.505 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012021\
Data File : PO075008.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jan 2021 19:02
Operator : AJ/MA
Sample : M1088-18
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S5-02-D


Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:57 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 05:32:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

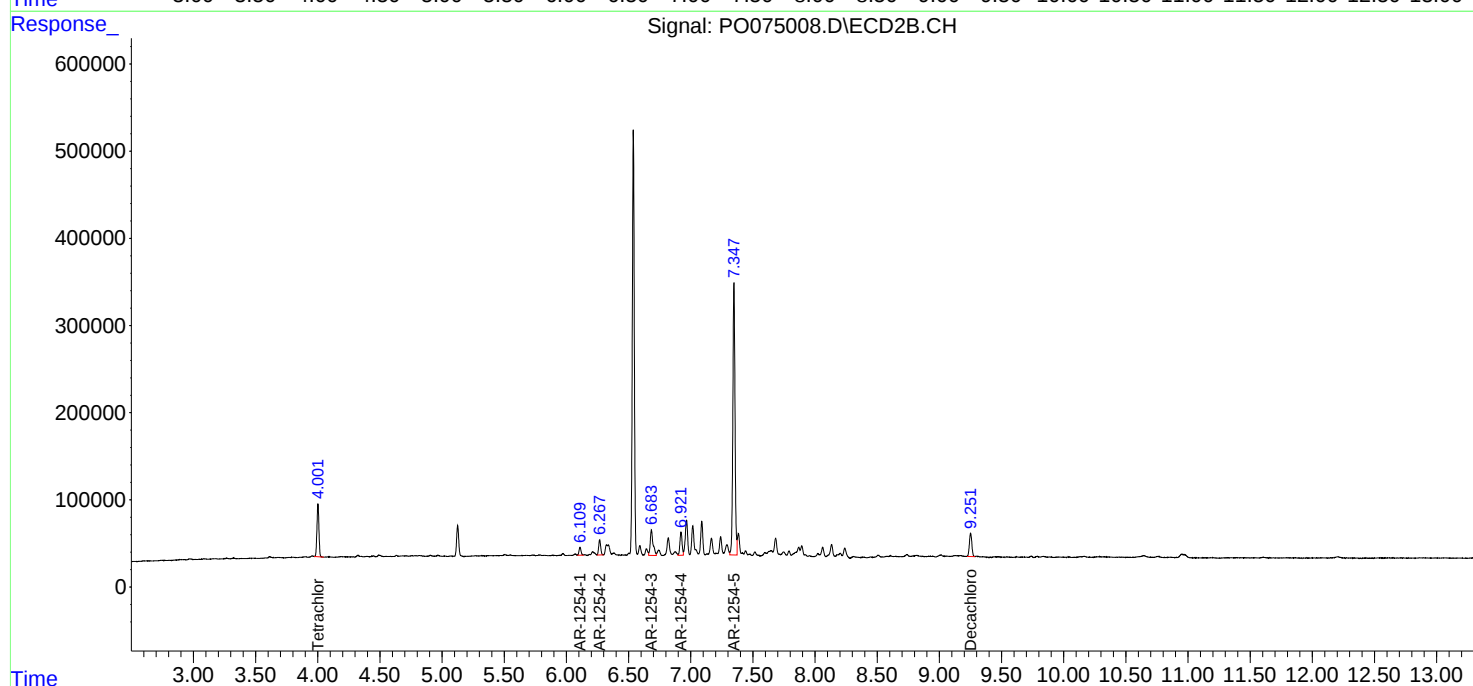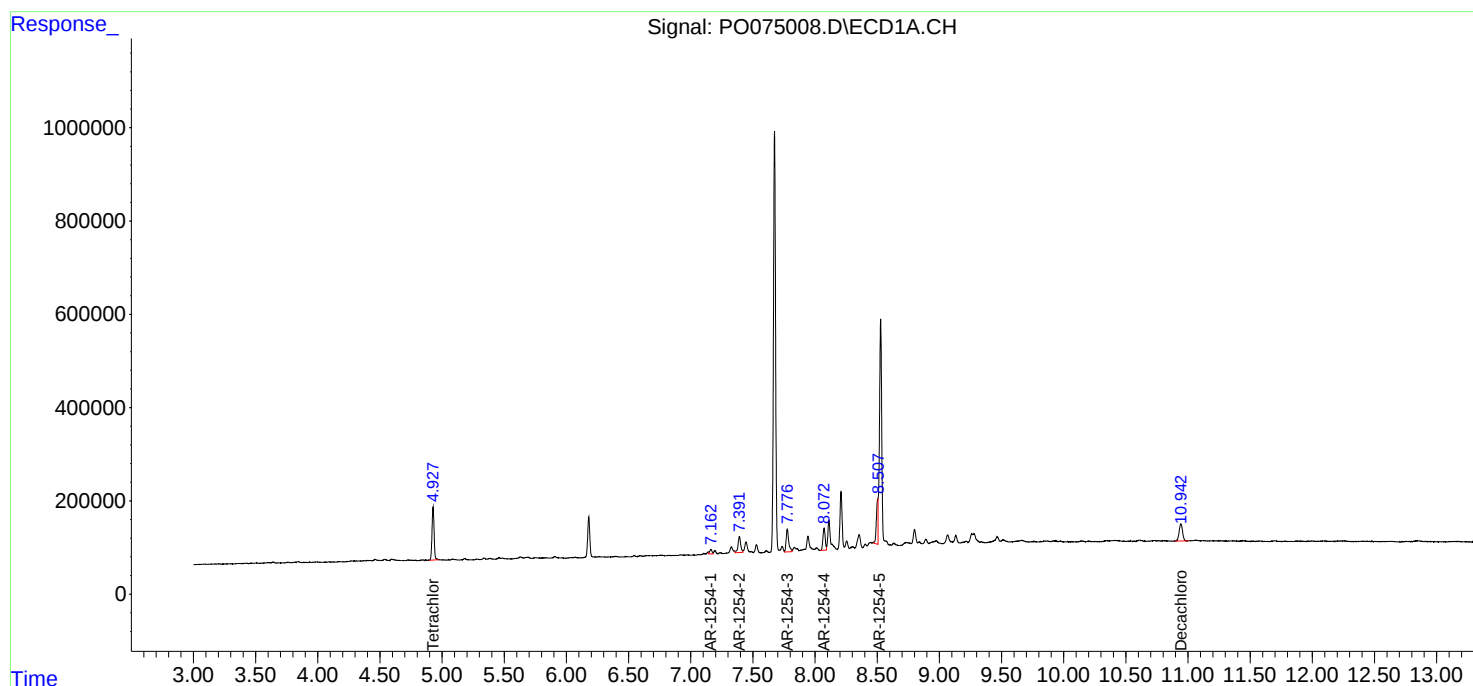

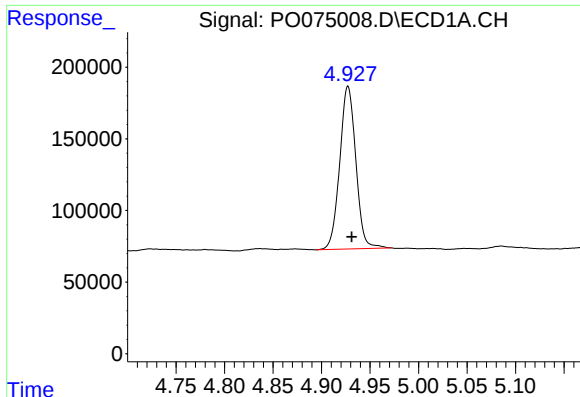


#1 Tetrachloro-m-xylene

R.T.: 4.927 min
Delta R.T.: -0.004 min
Response: 1311585
Conc: 12.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-02-D


Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:57 AM

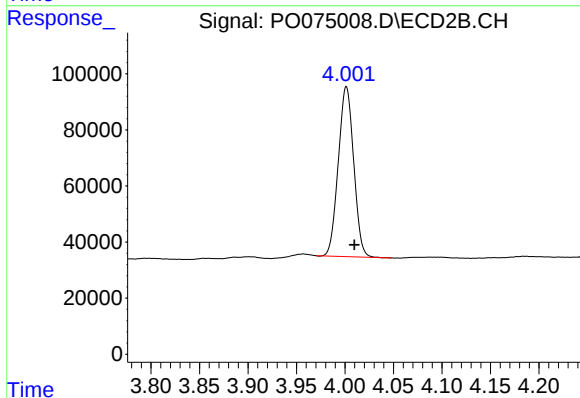


#1 Tetrachloro-m-xylene

R.T.: 4.001 min
Delta R.T.: -0.008 min
Response: 669141
Conc: 11.90 ng/ml

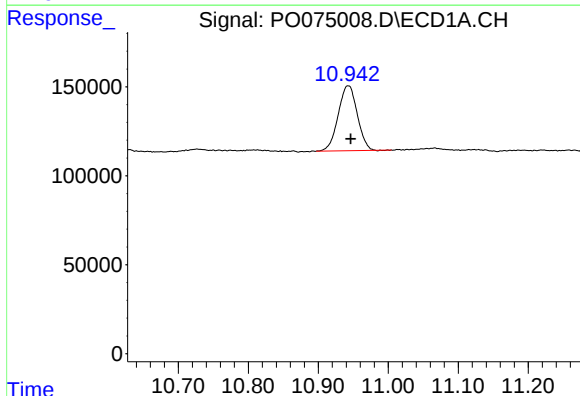


#2 Decachlorobiphenyl

R.T.: 10.943 min
Delta R.T.: -0.004 min
Response: 690052
Conc: 6.80 ng/ml

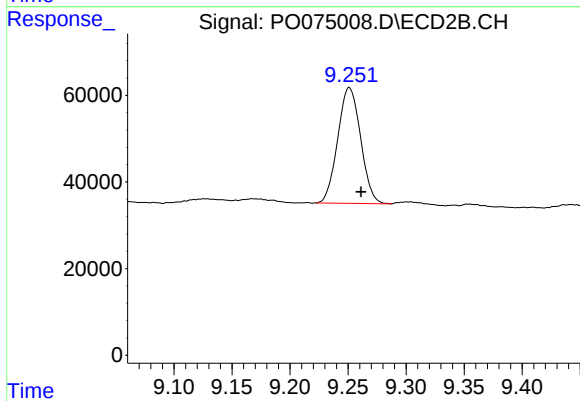

#2 Decachlorobiphenyl

R.T.: 9.251 min
Delta R.T.: -0.010 min
Response: 366994
Conc: 6.68 ng/ml

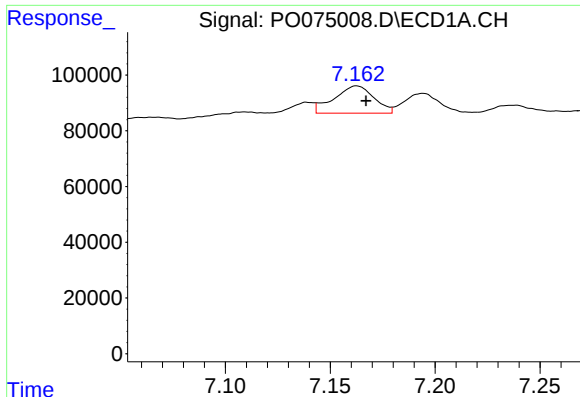


#26 AR-1254-1

R.T.: 7.162 min
Delta R.T.: -0.005 min
Response: 129500
Conc: 29.44 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S5-02-D


Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:57 AM

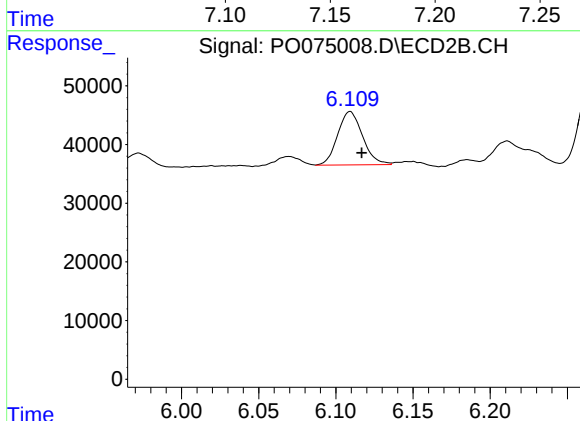


#26 AR-1254-1

R.T.: 6.109 min
Delta R.T.: -0.008 min
Response: 102280
Conc: 28.32 ng/ml

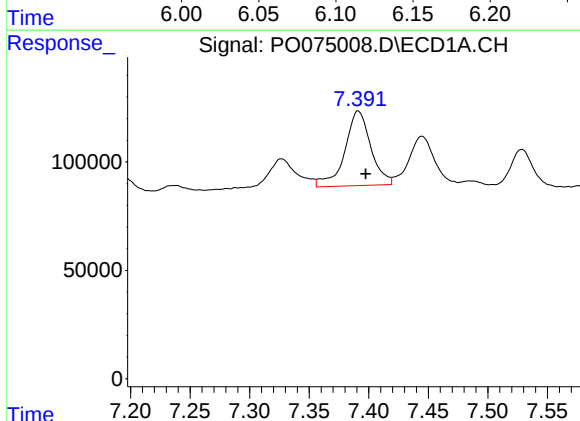


#27 AR-1254-2

R.T.: 7.391 min
Delta R.T.: -0.006 min
Response: 523523
Conc: 76.87 ng/ml

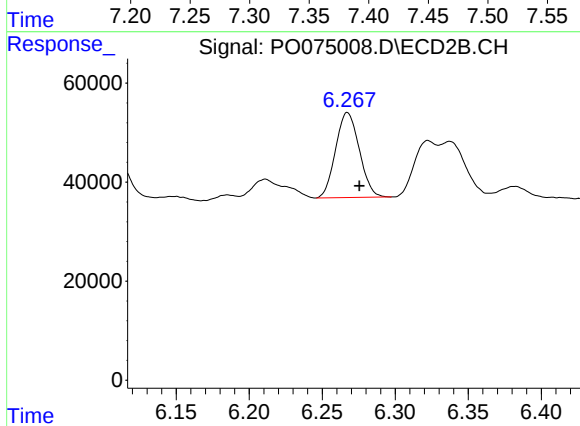

#27 AR-1254-2

R.T.: 6.267 min
Delta R.T.: -0.008 min
Response: 194054
Conc: 62.27 ng/ml

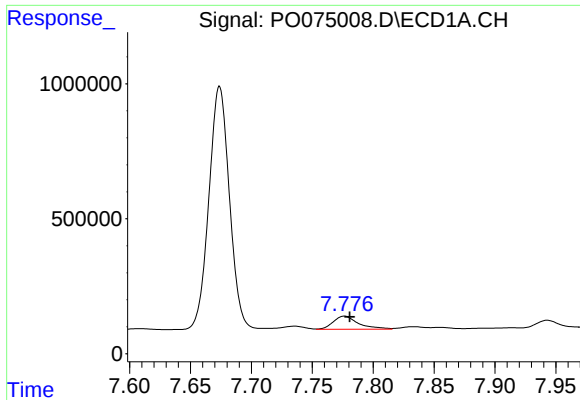


#28 AR-1254-3

R.T.: 7.776 min
Delta R.T.: -0.005 min
Response: 703876
Conc: 100.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-02-D


Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:57 AM

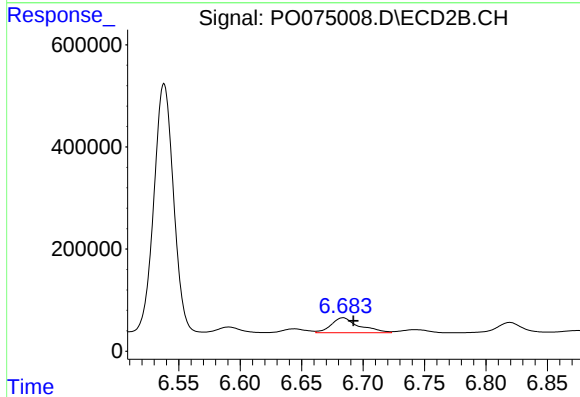


#28 AR-1254-3

R.T.: 6.684 min
Delta R.T.: -0.009 min
Response: 465424
Conc: 94.91 ng/ml

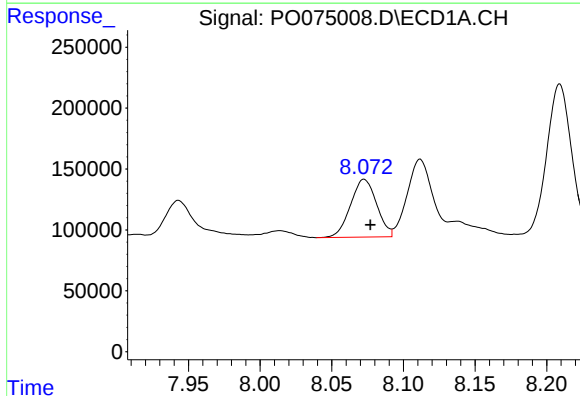


#29 AR-1254-4

R.T.: 8.073 min
Delta R.T.: -0.004 min
Response: 603599
Conc: 99.53 ng/ml

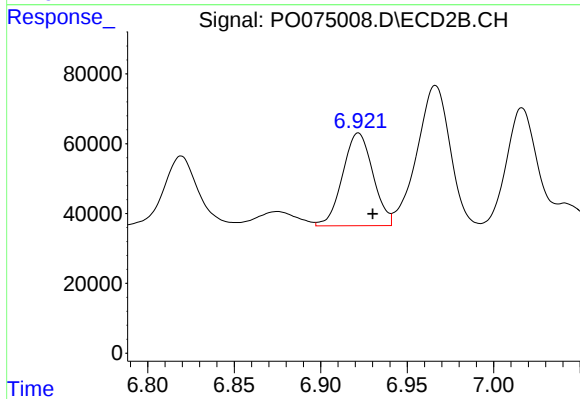

#29 AR-1254-4

R.T.: 6.922 min
Delta R.T.: -0.008 min
Response: 322752
Conc: 93.07 ng/ml

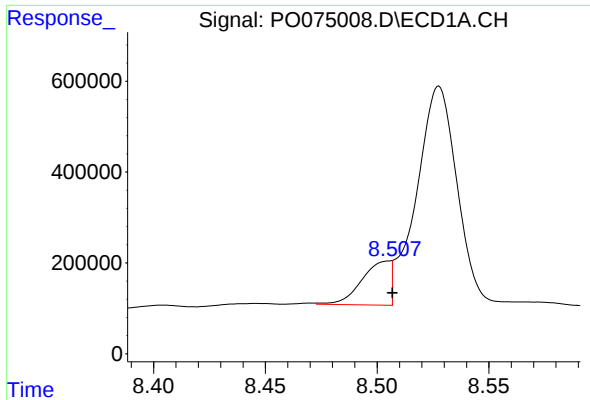


#30 AR-1254-5

R.T.: 8.507 min
Delta R.T.: 0.000 min
Response: 922389
Conc: 158.79 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S5-02-D

Manual Integrations
APPROVED

Ankita
1/21/2021 10:38:57 AM

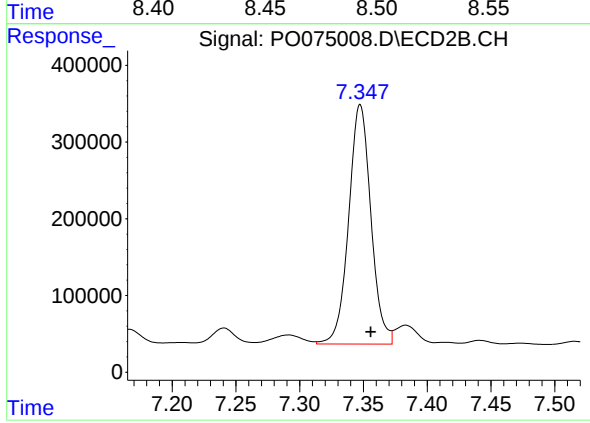

#30 AR-1254-5

R.T.: 7.348 min
Delta R.T.: -0.008 min
Response: 3790499
Conc: 837.51 ng/ml