

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012021\
 Data File : P0075017.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jan 2021 21:36
 Operator : AJ/MA
 Sample : M1089-08
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S6-01-D

Manual Integrations
 APPROVED

Ankita
 1/21/2021 10:39:01 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 05:37:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.927	4.001	2131208	1129761	20.198	20.084
2) SA Decachlor...	10.941	9.251	1139575	580881	11.228	10.580
Target Compounds						
26) L6 AR-1254-1	7.161	6.108	101470	127018	23.071m	35.166 #
27) L6 AR-1254-2	7.393	6.267	501770	217420	73.673	69.763
28) L6 AR-1254-3	7.777	6.683	557307	402271	79.453	82.030
29) L6 AR-1254-4	8.072	6.921	493480	263595	81.370	76.013
30) L6 AR-1254-5	8.502	7.346	1084756	1439567	186.739	318.070 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012021\
Data File : PO075017.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jan 2021 21:36
Operator : AJ/MA
Sample : M1089-08
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S6-01-D


Manual Integrations
APPROVED

Ankita
1/21/2021 10:39:01 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 05:37:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

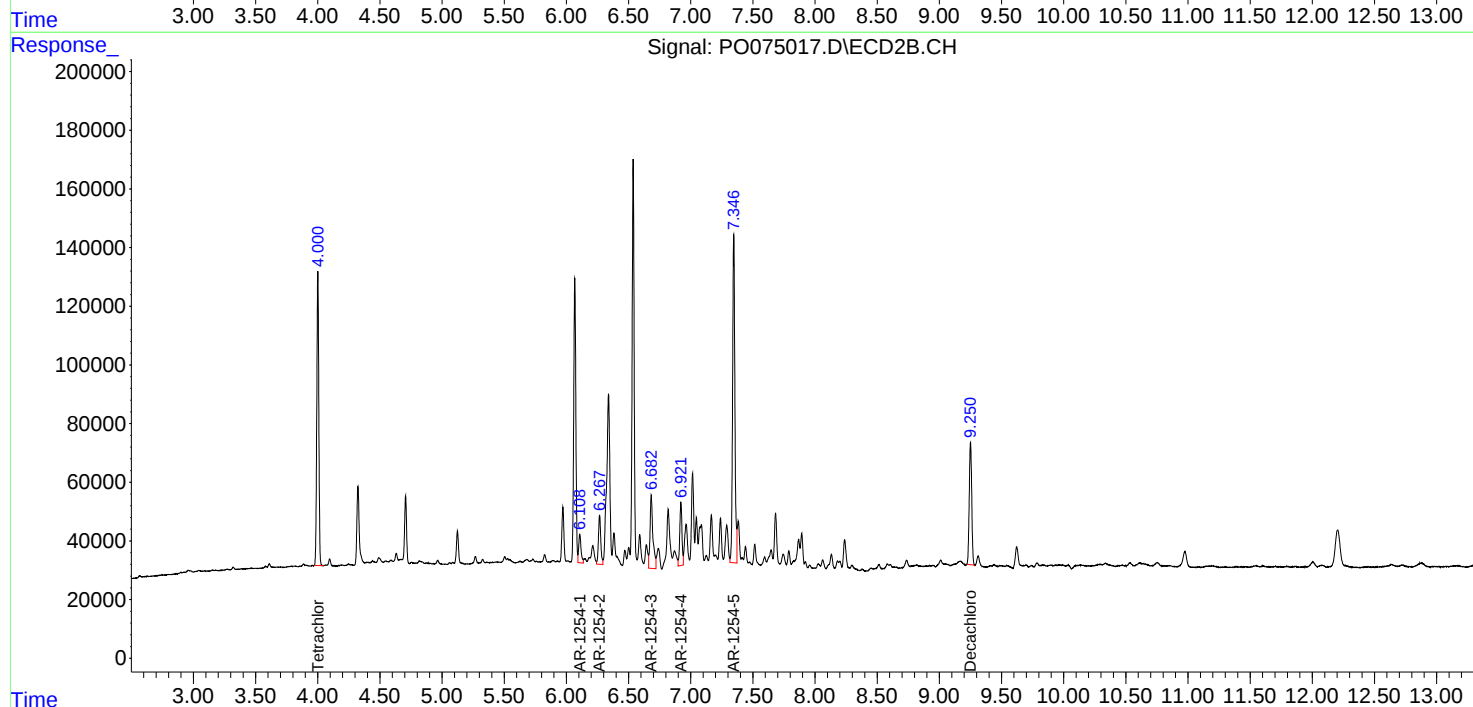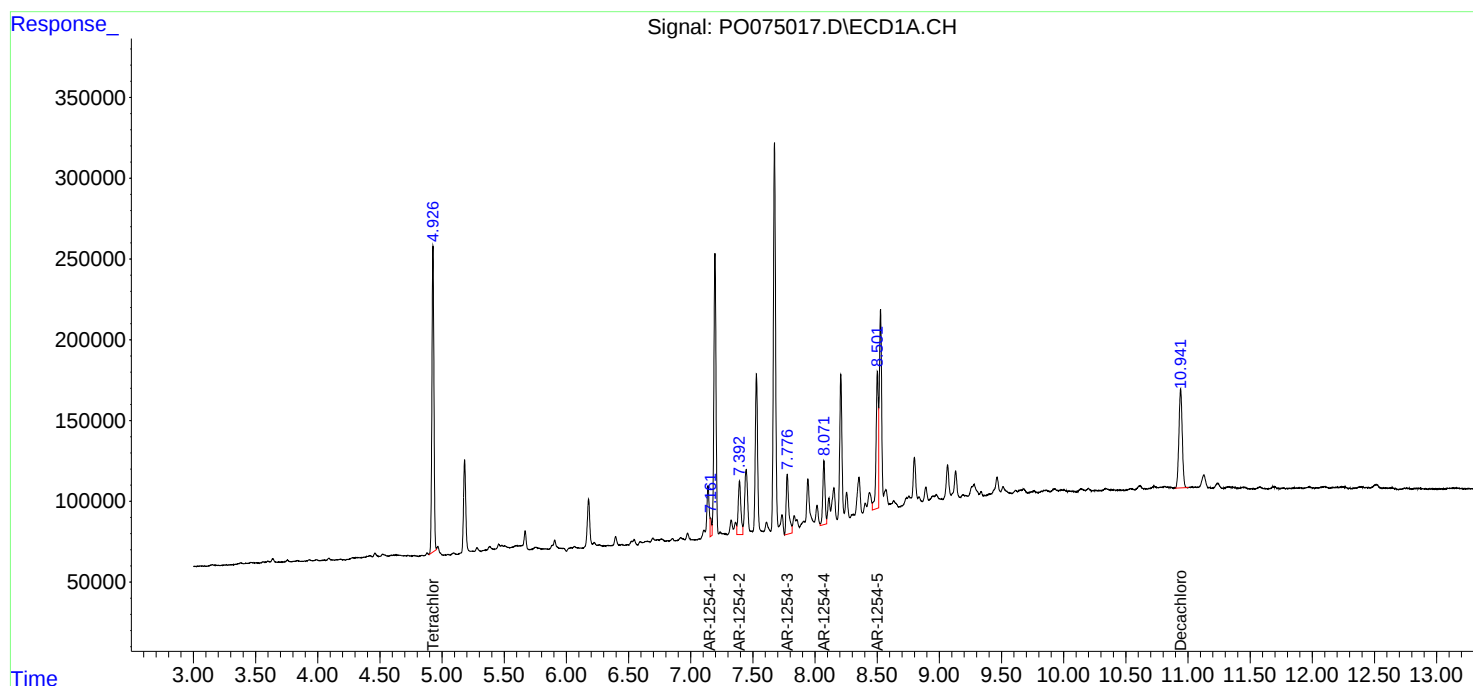

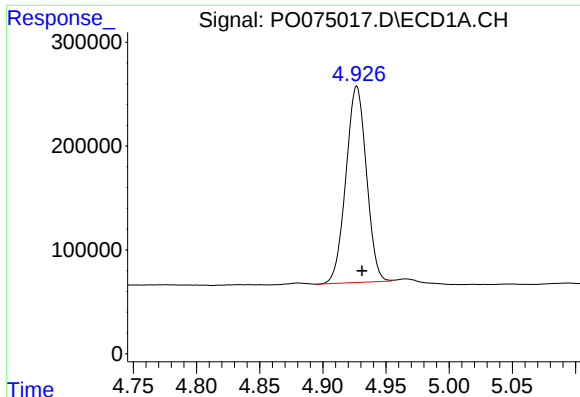


#1 Tetrachloro-m-xylene

R.T.: 4.927 min
Delta R.T.: -0.004 min
Response: 2131208
Conc: 20.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
S6-01-D


Manual Integrations
APPROVED

Ankita
1/21/2021 10:39:01 AM

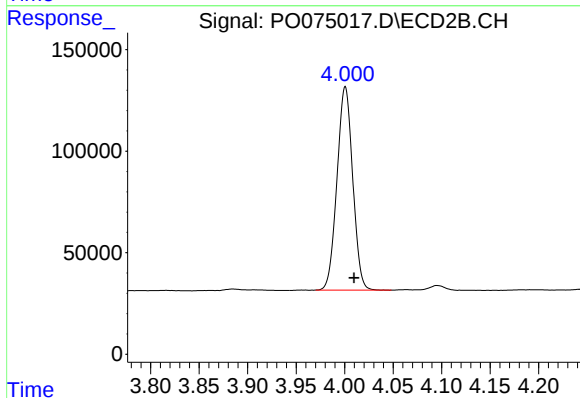


#1 Tetrachloro-m-xylene

R.T.: 4.001 min
Delta R.T.: -0.009 min
Response: 1129761
Conc: 20.08 ng/ml

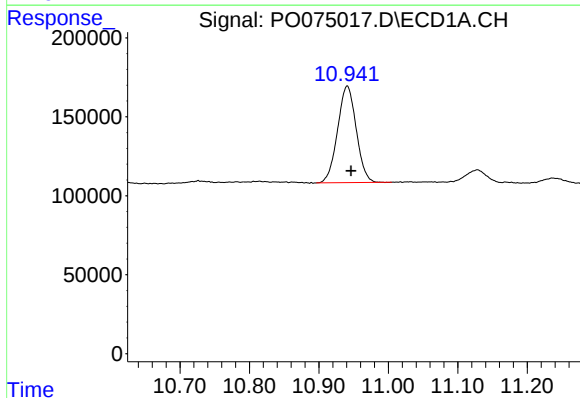


#2 Decachlorobiphenyl

R.T.: 10.941 min
Delta R.T.: -0.006 min
Response: 1139575
Conc: 11.23 ng/ml

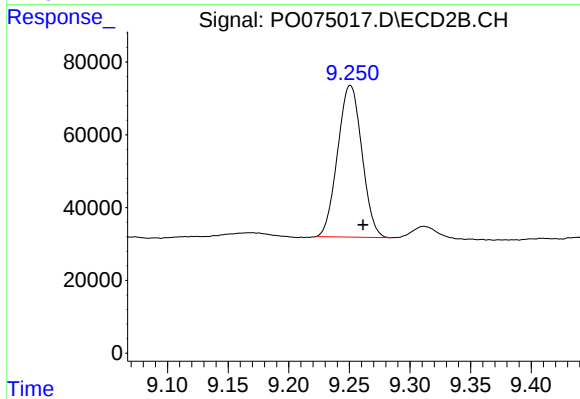

#2 Decachlorobiphenyl

R.T.: 9.251 min
Delta R.T.: -0.011 min
Response: 580881
Conc: 10.58 ng/ml

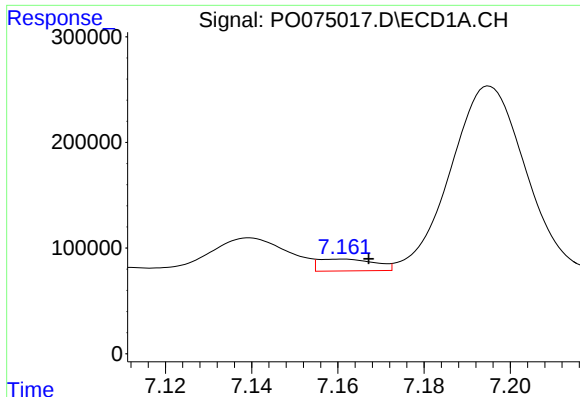


#26 AR-1254-1

R.T.: 7.161 min
Delta R.T.: -0.006 min
Response: 101470
Conc: 23.07 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S6-01-D


Manual Integrations
APPROVED

Ankita
1/21/2021 10:39:01 AM

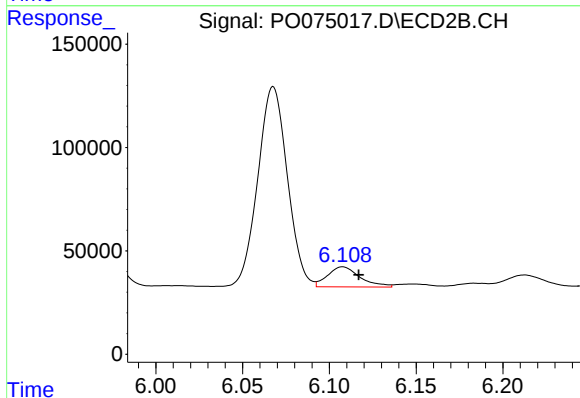


#26 AR-1254-1

R.T.: 6.108 min
Delta R.T.: -0.009 min
Response: 127018
Conc: 35.17 ng/ml

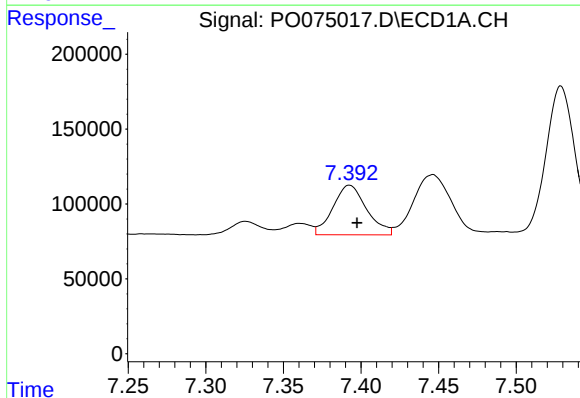


#27 AR-1254-2

R.T.: 7.393 min
Delta R.T.: -0.005 min
Response: 501770
Conc: 73.67 ng/ml

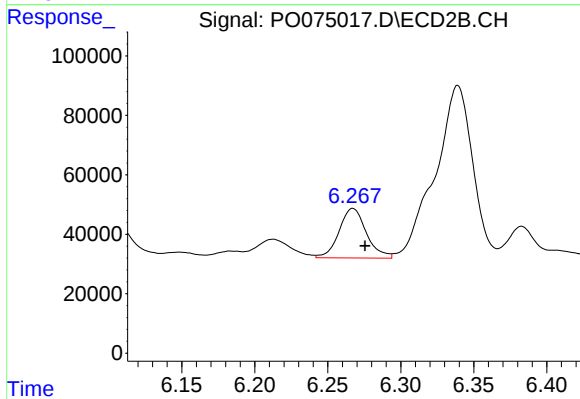

#27 AR-1254-2

R.T.: 6.267 min
Delta R.T.: -0.008 min
Response: 217420
Conc: 69.76 ng/ml

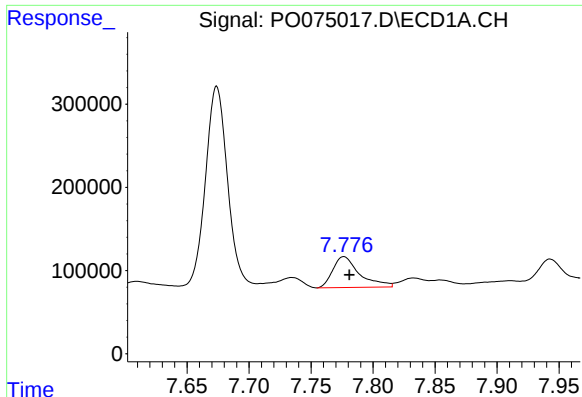


#28 AR-1254-3

R.T.: 7.777 min
Delta R.T.: -0.004 min
Response: 557307
Conc: 79.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
S6-01-D


Manual Integrations
APPROVED

Ankita
1/21/2021 10:39:01 AM

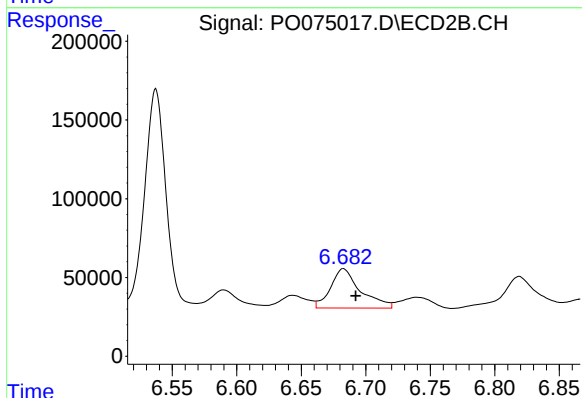


#28 AR-1254-3

R.T.: 6.683 min
Delta R.T.: -0.010 min
Response: 402271
Conc: 82.03 ng/ml

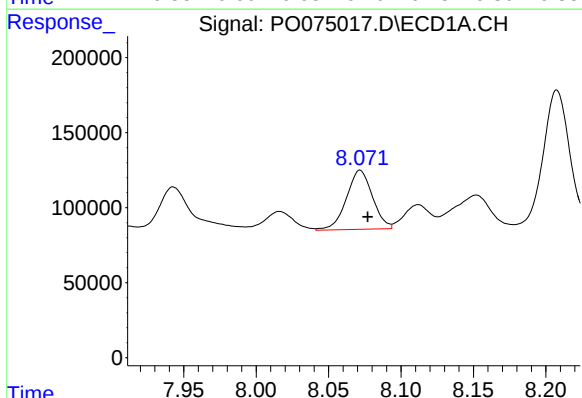


#29 AR-1254-4

R.T.: 8.072 min
Delta R.T.: -0.005 min
Response: 493480
Conc: 81.37 ng/ml

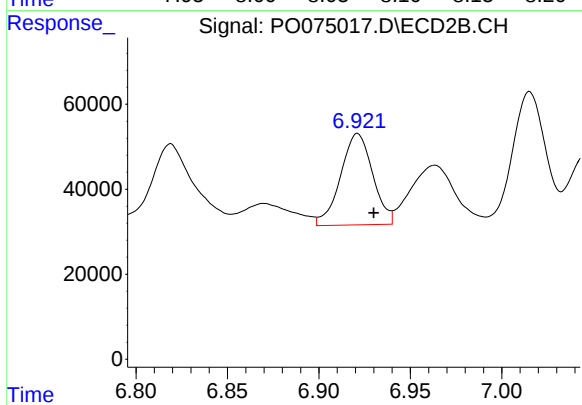

#29 AR-1254-4

R.T.: 6.921 min
Delta R.T.: -0.009 min
Response: 263595
Conc: 76.01 ng/ml

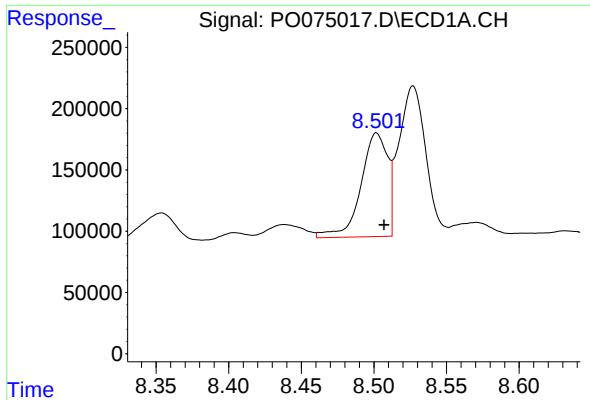


#30 AR-1254-5

R.T.: 8.502 min
Delta R.T.: -0.005 min
Response: 1084756
Conc: 186.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
S6-01-D

Manual Integrations
APPROVED

Ankita
1/21/2021 10:39:01 AM

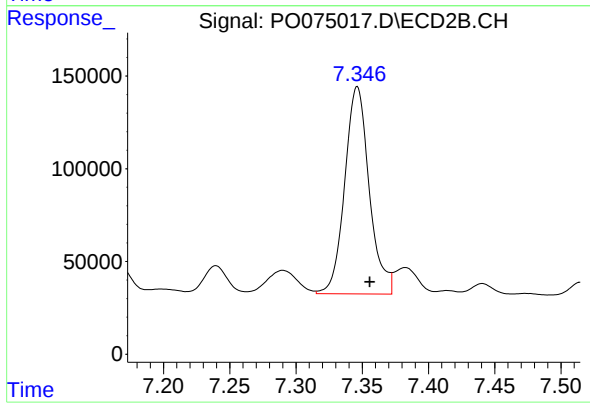

#30 AR-1254-5

R.T.: 7.346 min
Delta R.T.: -0.010 min
Response: 1439567
Conc: 318.07 ng/ml