

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012022\
 Data File : P0084380.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jan 2022 11:57
 Operator : AJ\MA
 Sample : PB142144BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 00:30:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 20 12:19:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	6.518	5.304	1726293	470190	21.126	20.760
2)	SA Decachlor...	13.784	11.306	1916585	702271	22.013	22.220
Target Compounds							
9)	L2 AR-1221-2	0.000	5.731	0	6193	N.D.	28.248 #
28)	L6 AR-1254-3	9.576	8.356	33208	7034	5.677	3.008 #
29)	L6 AR-1254-4	0.000	8.607	0	6872	N.D.	4.455 #
30)	L6 AR-1254-5	10.395	9.055	35828	14466	6.407	6.537
31)	L7 AR-1260-1	0.000	8.497	0	4894	N.D.	3.206 #
32)	L7 AR-1260-2	0.000	8.701	0	9143	N.D.	5.030 #
33)	L7 AR-1260-3	0.000	8.871	0	3505	N.D.	2.033 #
39)	L8 AR-1262-4	0.000	10.012	0	2093	N.D.	0.731 #
42)	L9 AR-1268-2	0.000	10.012	0	2093	N.D.	0.515 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012022\
Data File : P0084380.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jan 2022 11:57
Operator : AJ\MA
Sample : PB142144BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 00:30:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011922.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 20 12:19:51 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

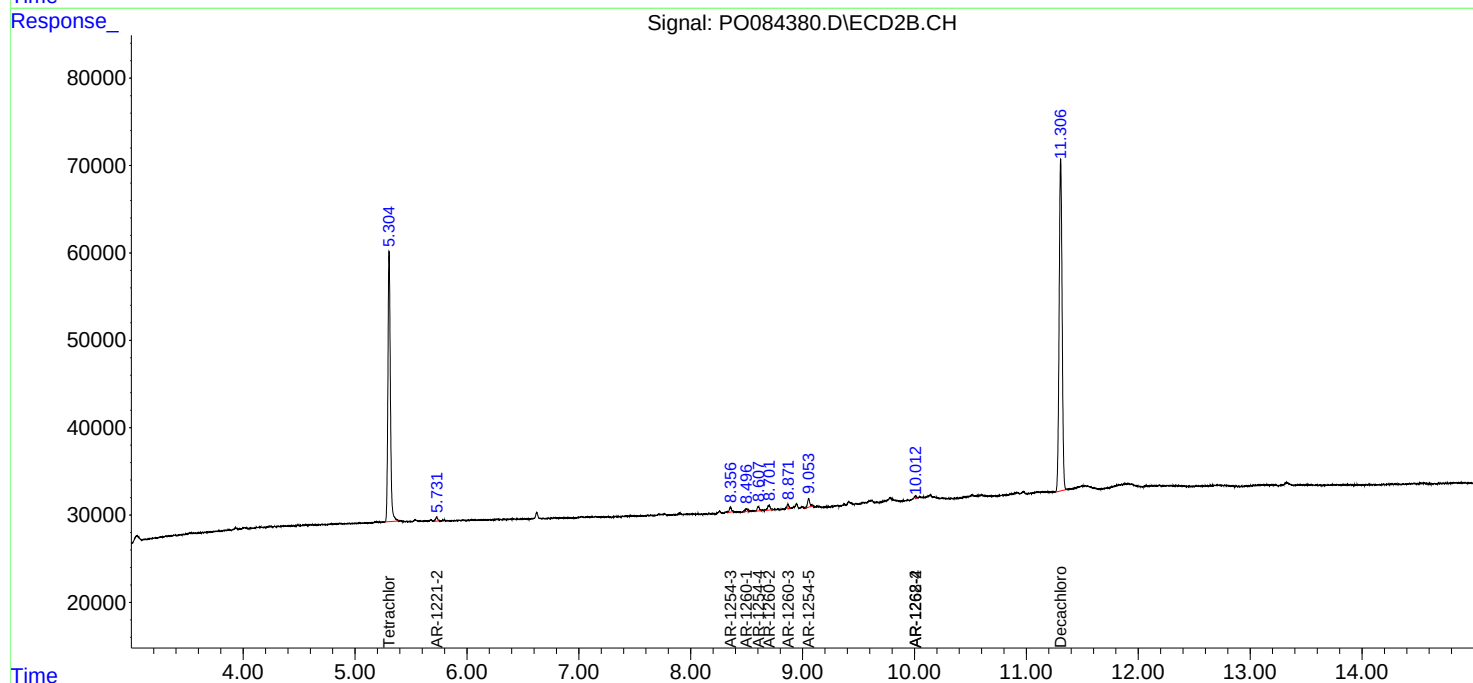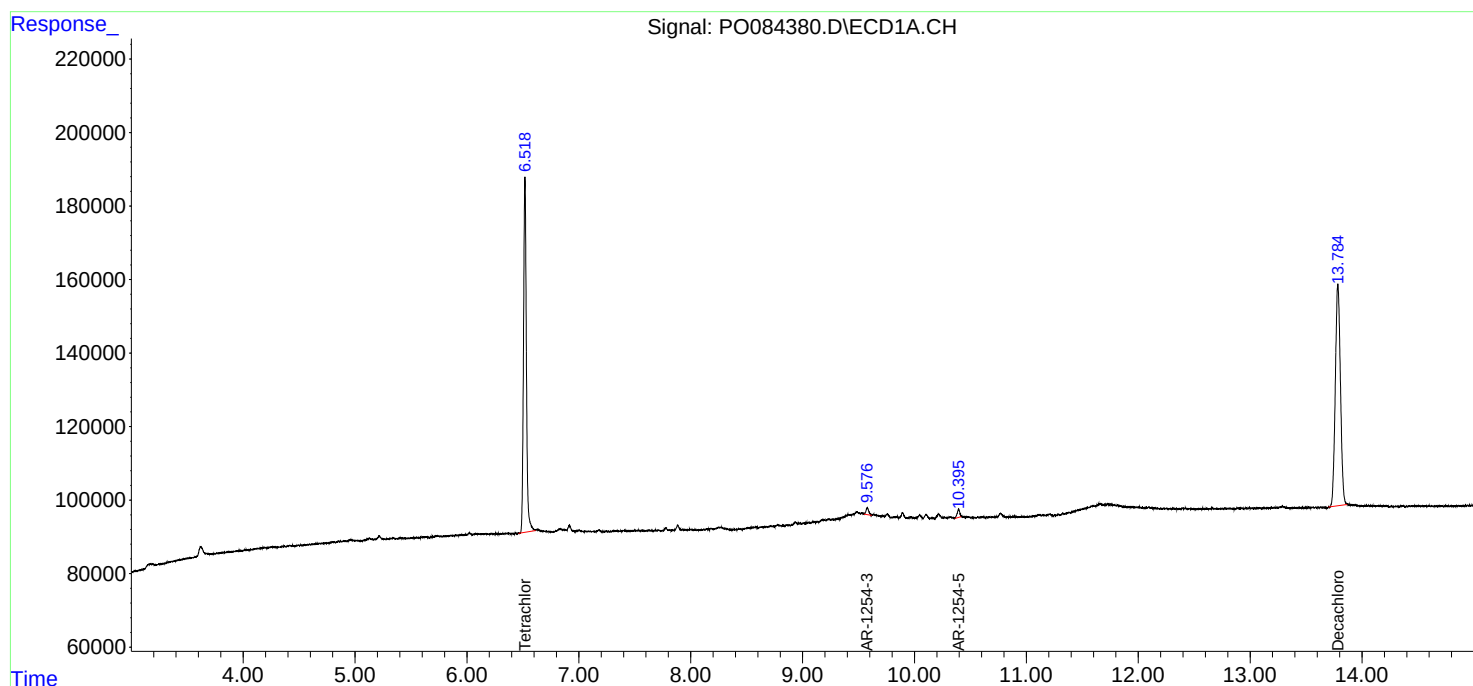


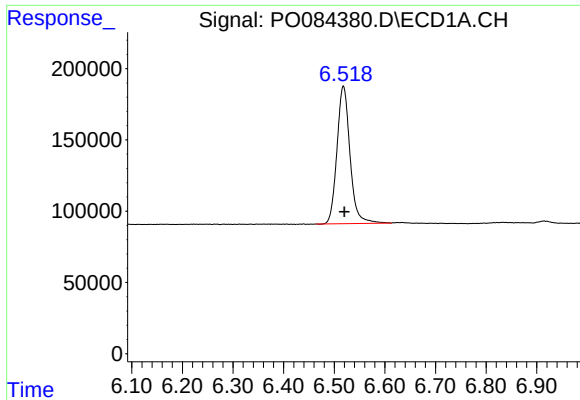

#1 Tetrachloro-m-xylene


R.T.: 6.518 min
Delta R.T.: -0.002 min
Response: 1726293
Conc: 21.13 ng/ml

Instrument :
ECD_O
ClientSampleId :

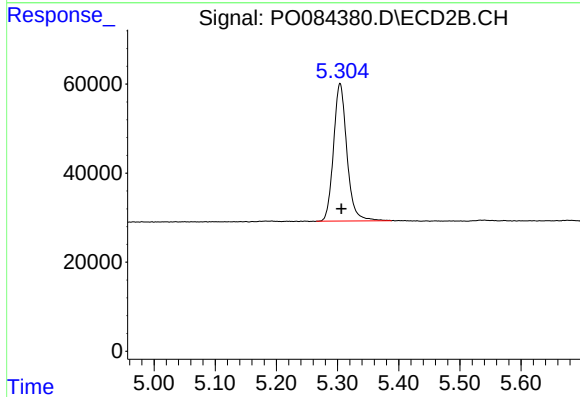


#1 Tetrachloro-m-xylene

R.T.: 5.304 min
Delta R.T.: -0.002 min
Response: 470190
Conc: 20.76 ng/ml

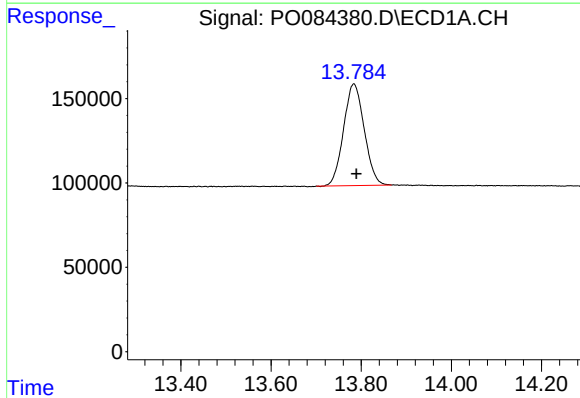


#2 Decachlorobiphenyl

R.T.: 13.784 min
Delta R.T.: -0.005 min
Response: 1916585
Conc: 22.01 ng/ml

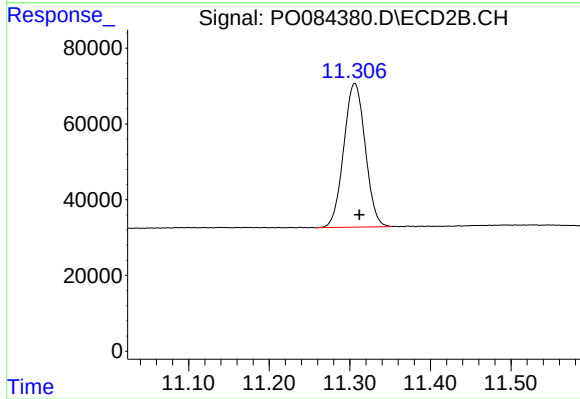

#2 Decachlorobiphenyl


R.T.: 11.306 min
Delta R.T.: -0.006 min
Response: 702271
Conc: 22.22 ng/ml

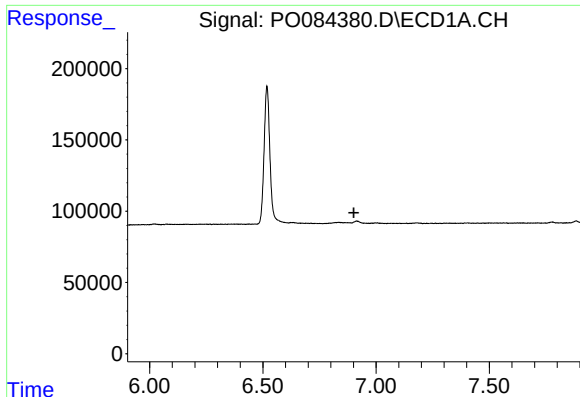

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 6.902 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

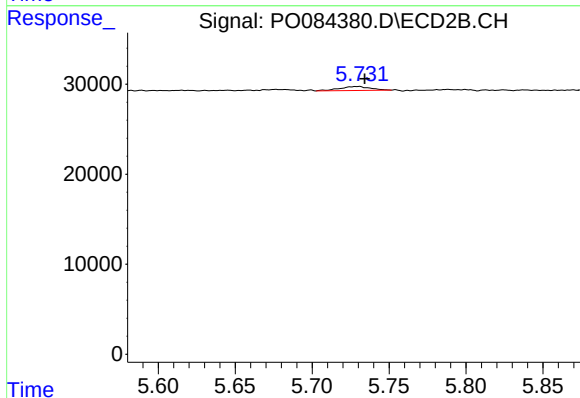


#9 AR-1221-2

R.T.: 5.731 min
Delta R.T.: -0.003 min
Response: 6193
Conc: 28.25 ng/ml

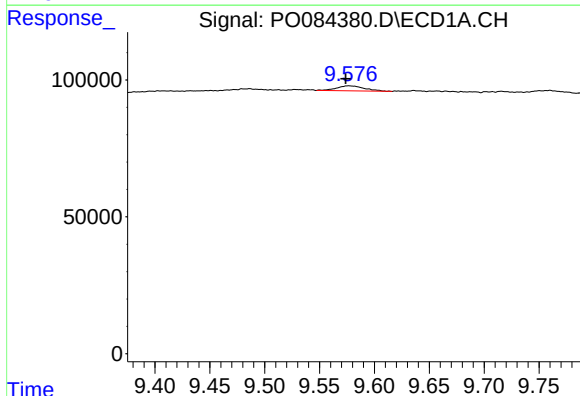


#28 AR-1254-3

R.T.: 9.576 min
Delta R.T.: 0.002 min
Response: 33208
Conc: 5.68 ng/ml

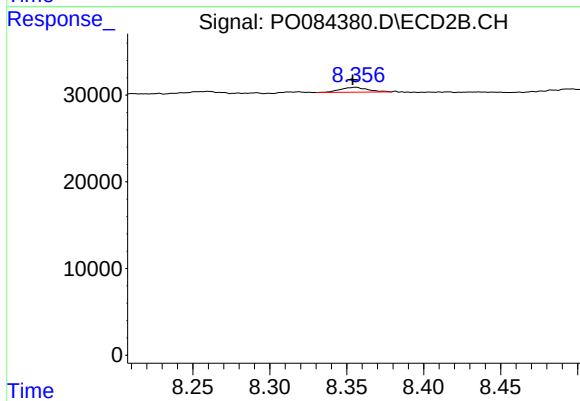

#28 AR-1254-3


R.T.: 8.356 min
Delta R.T.: 0.002 min
Response: 7034
Conc: 3.01 ng/ml

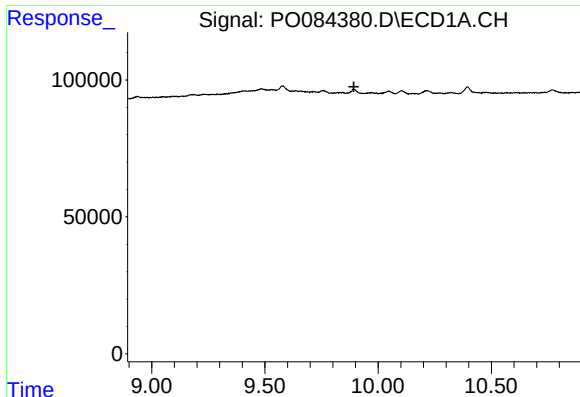

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 9.893 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

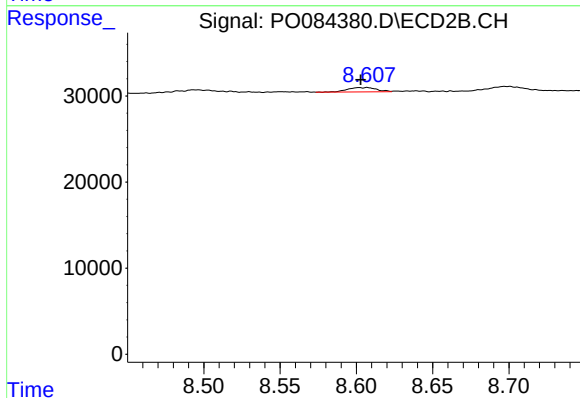


#29 AR-1254-4

R.T.: 8.607 min
Delta R.T.: 0.004 min
Response: 6872
Conc: 4.45 ng/ml

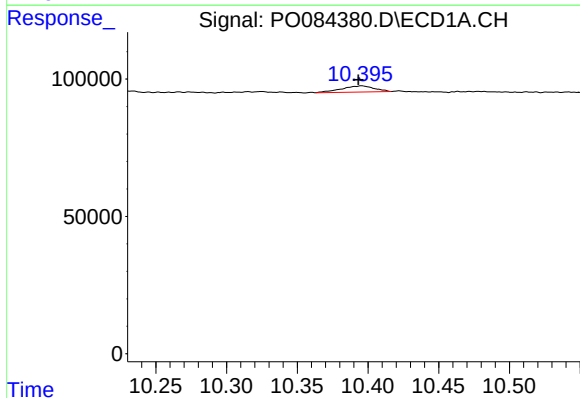


#30 AR-1254-5

R.T.: 10.395 min
Delta R.T.: 0.002 min
Response: 35828
Conc: 6.41 ng/ml

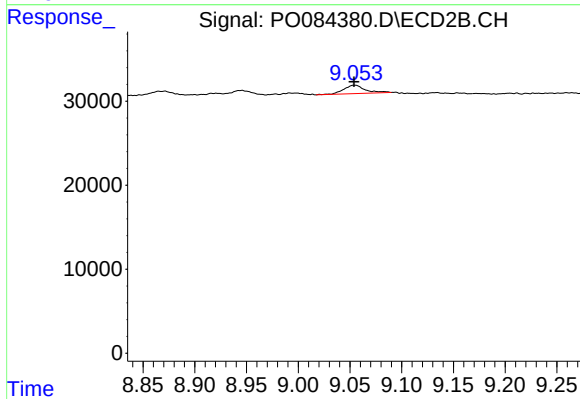

#30 AR-1254-5


R.T.: 9.055 min
Delta R.T.: 0.000 min
Response: 14466
Conc: 6.54 ng/ml

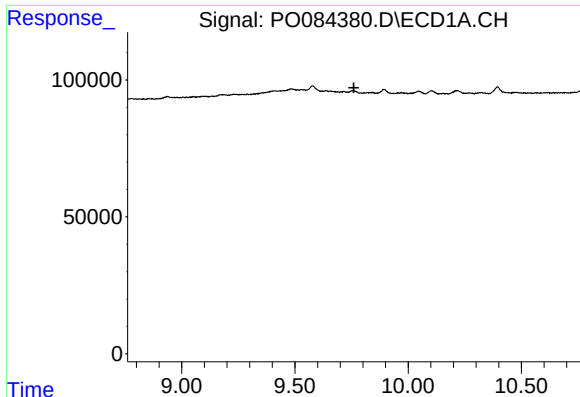

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 9.761 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

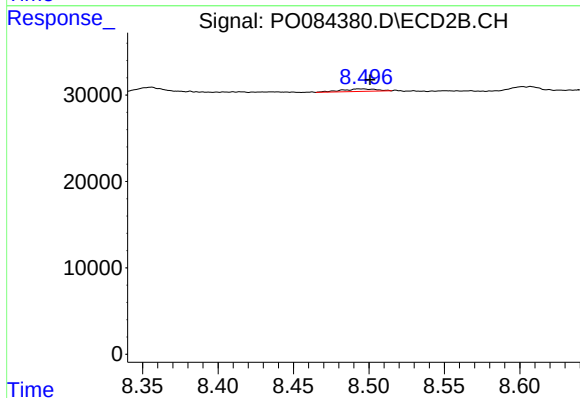


#31 AR-1260-1

R.T.: 8.497 min
Delta R.T.: -0.004 min
Response: 4894
Conc: 3.21 ng/ml

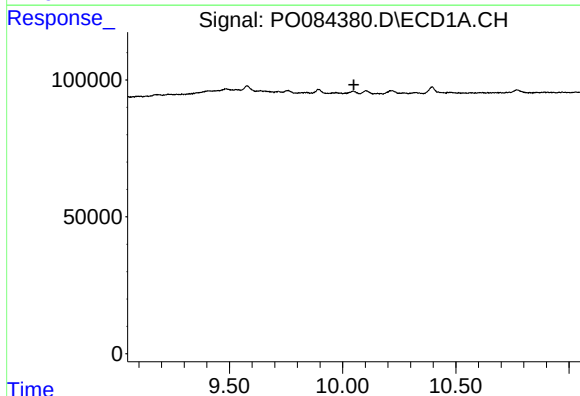


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 10.050 min
Response: 0
Conc: N.D.

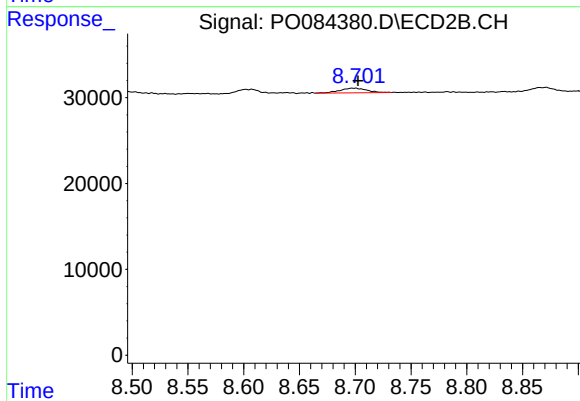

#32 AR-1260-2


R.T.: 8.701 min
Delta R.T.: -0.002 min
Response: 9143
Conc: 5.03 ng/ml

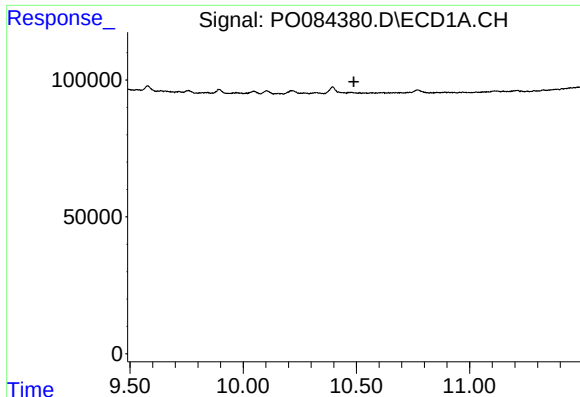

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 10.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

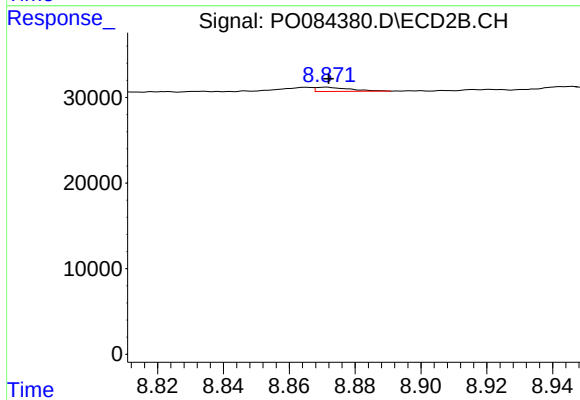


#33 AR-1260-3

R.T.: 8.871 min
Delta R.T.: 0.000 min
Response: 3505
Conc: 2.03 ng/ml

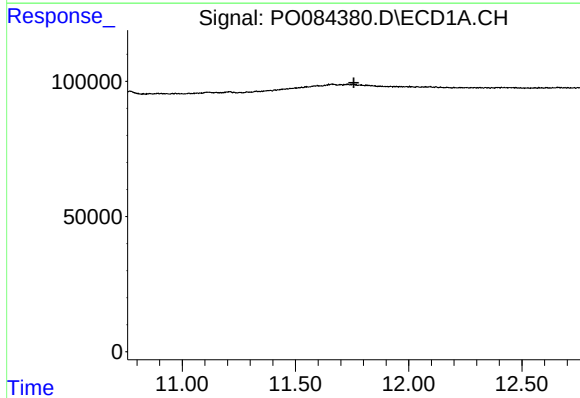


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 11.758 min
Response: 0
Conc: N.D.

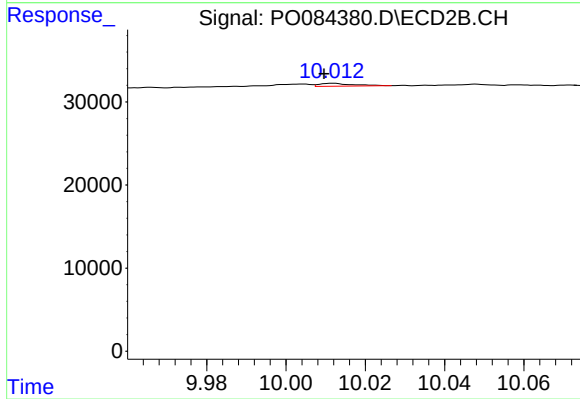

#39 AR-1262-4


R.T.: 10.012 min
Delta R.T.: 0.002 min
Response: 2093
Conc: 0.73 ng/ml

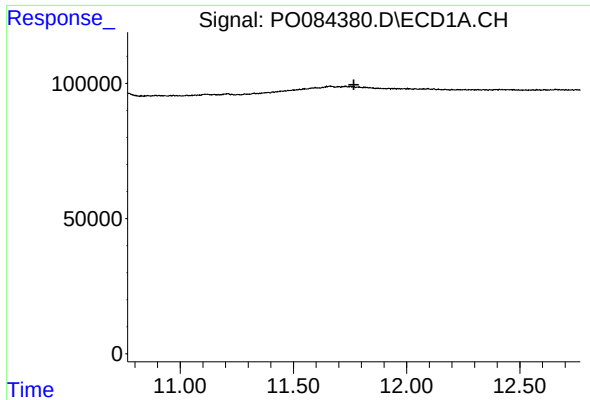

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 11.767 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

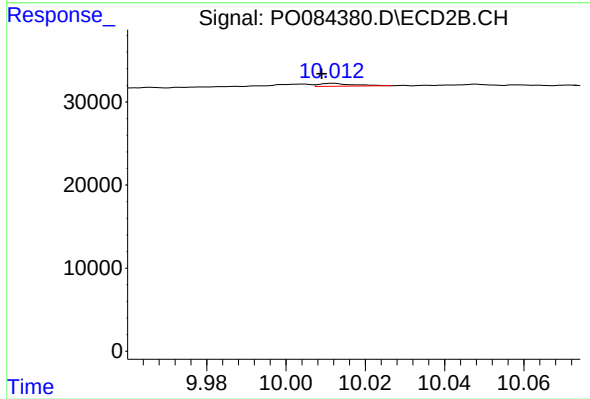

#42 AR-1268-2

R.T.: 10.012 min
Delta R.T.: 0.003 min
Response: 2093
Conc: 0.51 ng/ml