

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012022\
 Data File : P0084377.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jan 2022 10:41
 Operator : AJ\MA
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/21/2022
 Supervised By :Ankita Jodhani 01/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 00:29:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 20 12:19:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	6.517	5.302	4467844	1353019	54.676	59.738
2) SA Decachlor...	13.783	11.303	4682536	1759110	53.781	55.659
Target Compounds						
21) L5 AR-1248-1	7.966	6.770	1016185	326031	509.100	532.176
22) L5 AR-1248-2	8.282	7.063	1490972	452987	491.047	520.331
23) L5 AR-1248-3	8.516	7.113	1679586	478991	520.087	522.903
24) L5 AR-1248-4	8.964	7.319	1894190	644037	540.893	594.999
25) L5 AR-1248-5	9.008	7.777	1853796	646652	551.124	596.813m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012022\
Data File : PO084377.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jan 2022 10:41
Operator : AJ\MA
Sample : AR1248CCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 00:29:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011922.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 20 12:19:51 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

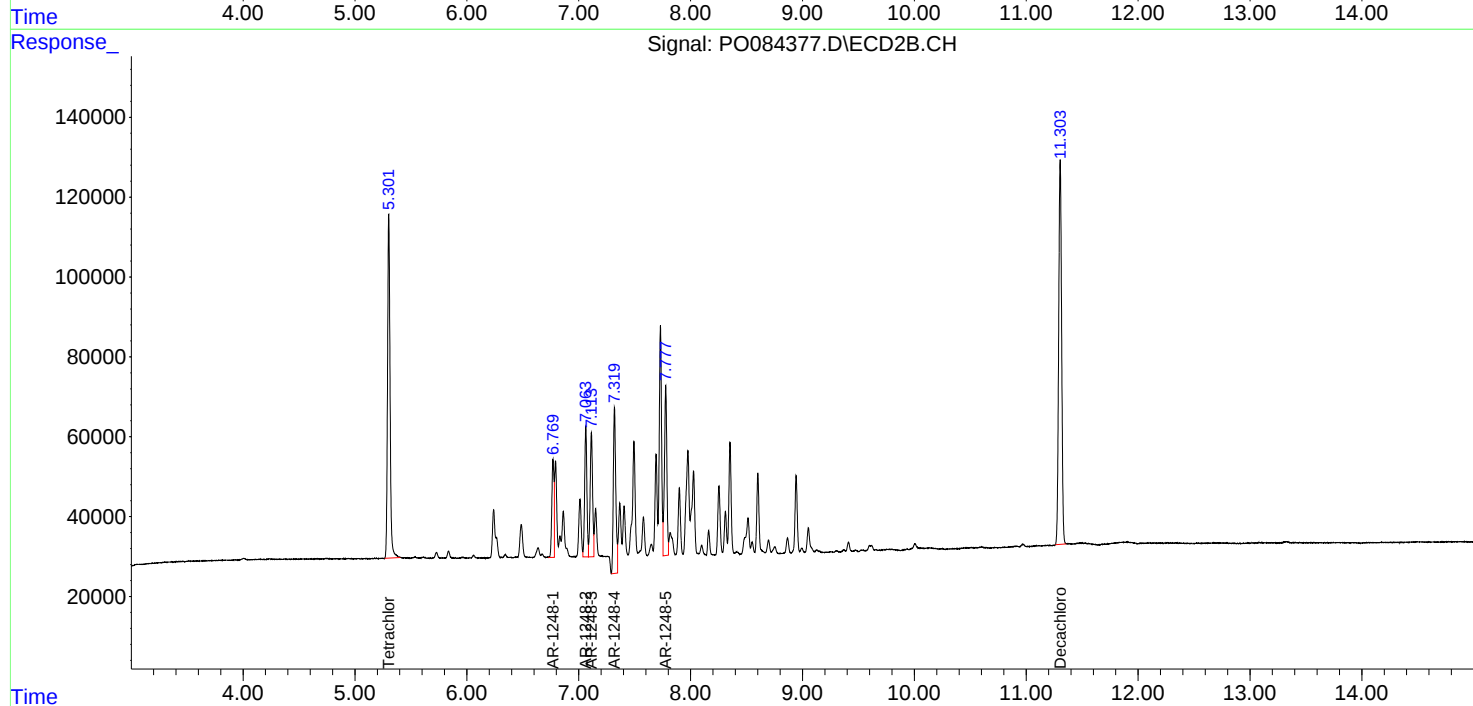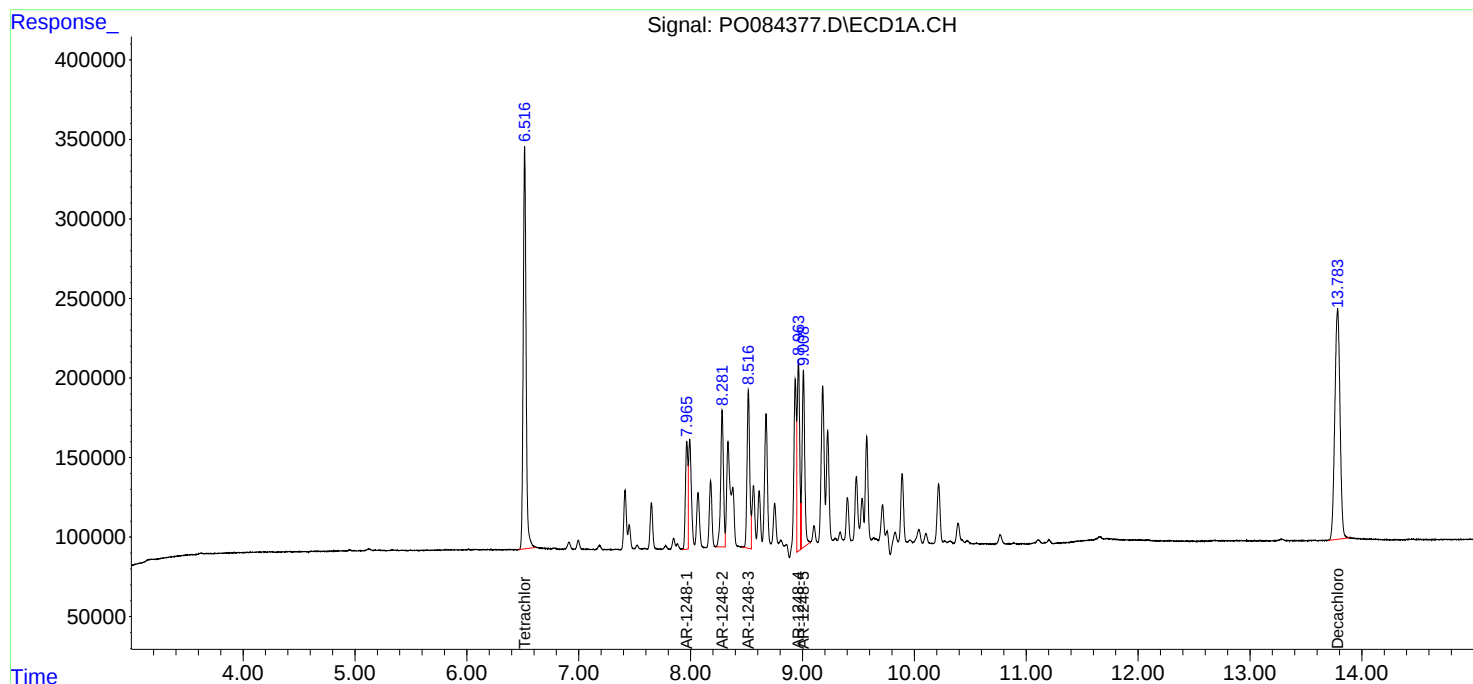

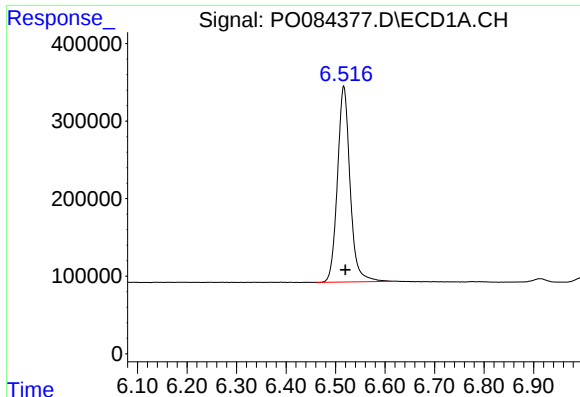


#1 Tetrachloro-m-xylene

R.T.: 6.517 min
Delta R.T.: -0.003 min
Response: 4467844
Conc: 54.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

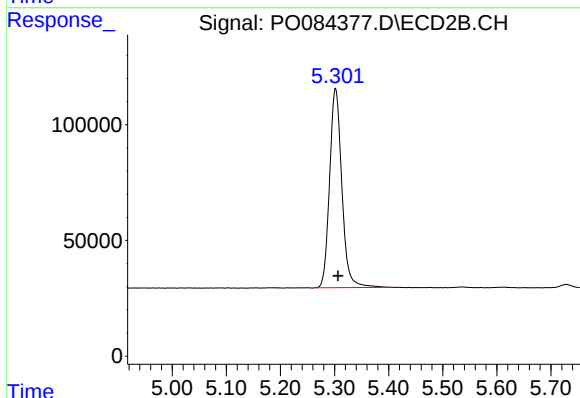


#1 Tetrachloro-m-xylene

R.T.: 5.302 min
Delta R.T.: -0.005 min
Response: 1353019
Conc: 59.74 ng/ml

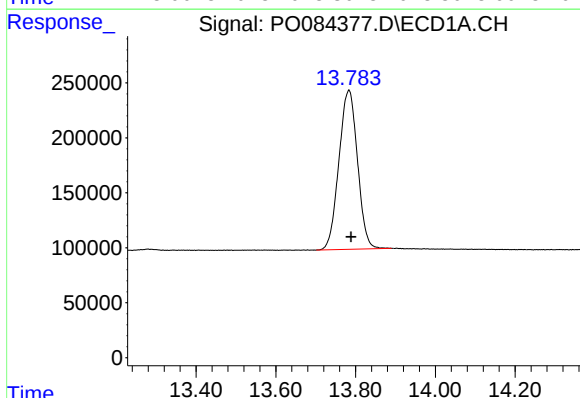


#2 Decachlorobiphenyl

R.T.: 13.783 min
Delta R.T.: -0.006 min
Response: 4682536
Conc: 53.78 ng/ml

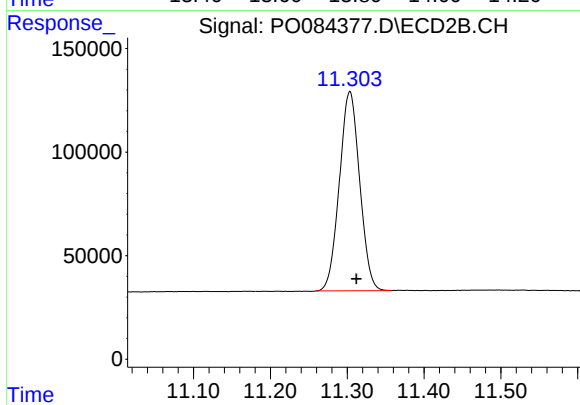

#2 Decachlorobiphenyl

R.T.: 11.303 min
Delta R.T.: -0.009 min
Response: 1759110
Conc: 55.66 ng/ml

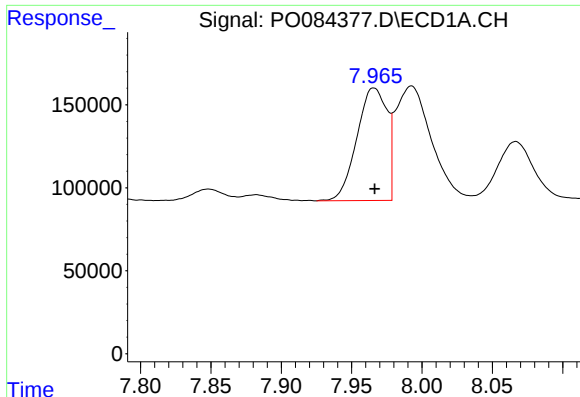


#21 AR-1248-1

R.T.: 7.966 min
Delta R.T.: 0.000 min
Response: 1016185
Conc: 509.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

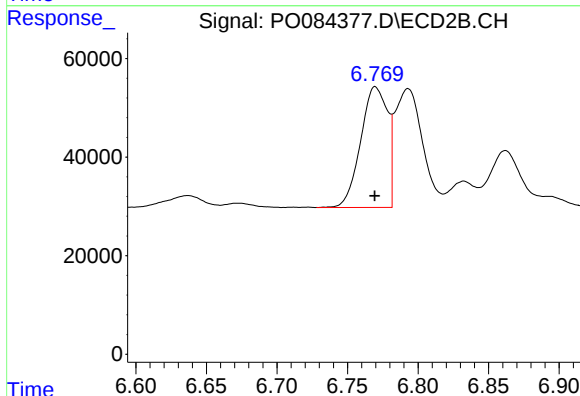


#21 AR-1248-1

R.T.: 6.770 min
Delta R.T.: 0.000 min
Response: 326031
Conc: 532.18 ng/ml

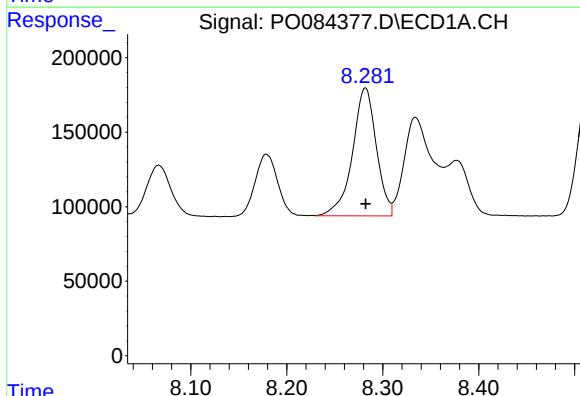


#22 AR-1248-2

R.T.: 8.282 min
Delta R.T.: 0.000 min
Response: 1490972
Conc: 491.05 ng/ml

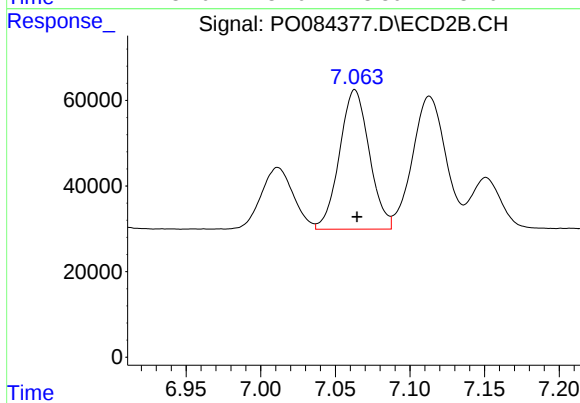

#22 AR-1248-2

R.T.: 7.063 min
Delta R.T.: -0.002 min
Response: 452987
Conc: 520.33 ng/ml

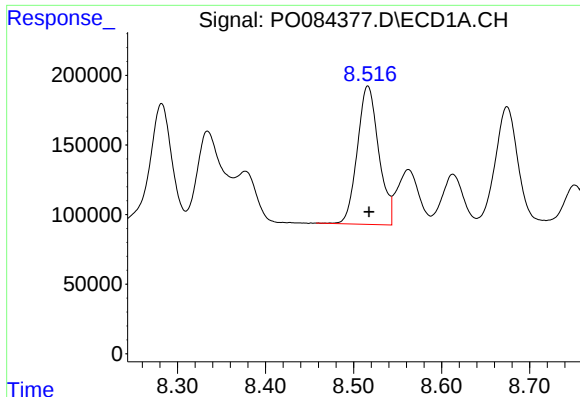


#23 AR-1248-3

R.T.: 8.516 min
Delta R.T.: -0.001 min
Response: 1679586
Conc: 520.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

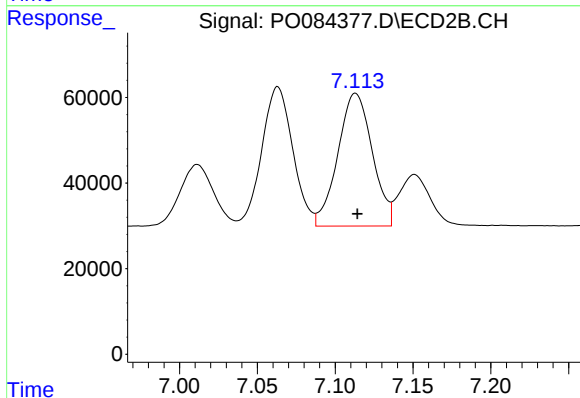


#23 AR-1248-3

R.T.: 7.113 min
Delta R.T.: -0.001 min
Response: 478991
Conc: 522.90 ng/ml

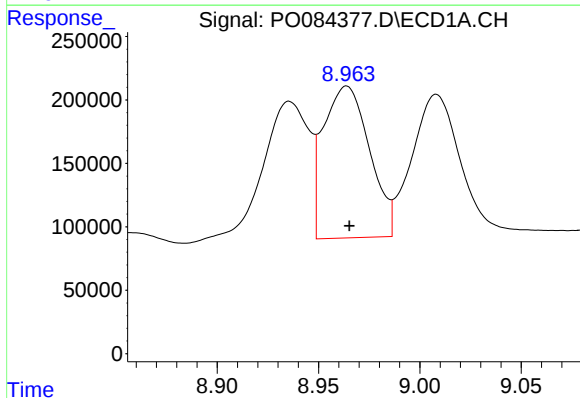


#24 AR-1248-4

R.T.: 8.964 min
Delta R.T.: -0.001 min
Response: 1894190
Conc: 540.89 ng/ml

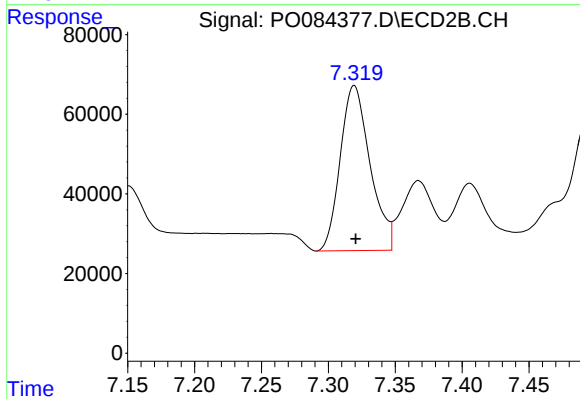

#24 AR-1248-4

R.T.: 7.319 min
Delta R.T.: -0.001 min
Response: 644037
Conc: 595.00 ng/ml

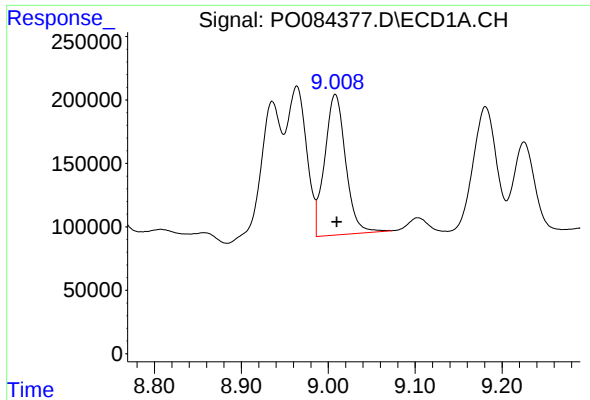


#25 AR-1248-5

R.T.: 9.008 min
Delta R.T.: -0.001 min
Response: 1853796
Conc: 551.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2022
Supervised By :Ankita Jodhani 01/21/2022

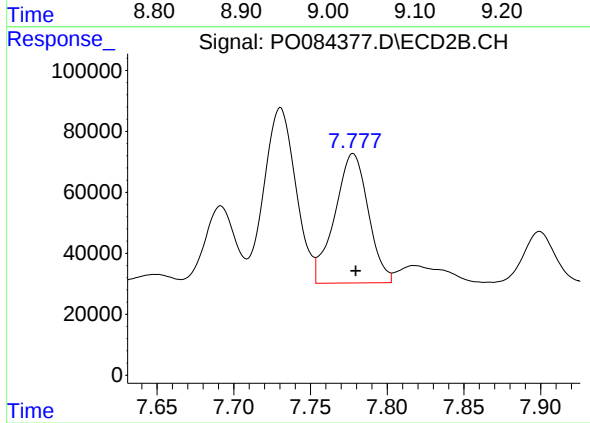

#25 AR-1248-5

R.T.: 7.777 min
Delta R.T.: -0.002 min
Response: 646652
Conc: 596.81 ng/ml m