

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012022\
 Data File : P0084380.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jan 2022 11:57
 Operator : AJ\MA
 Sample : PB142144BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB142144BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 00:30:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 20 12:19:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	6.518	5.304	1726293	470190	21.126	20.760
2) SA Decachlor...	13.784	11.306	1916585	702271	22.013	22.220

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012022\
Data File : P0084380.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jan 2022 11:57
Operator : AJ\MA
Sample : PB142144BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB142144BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 00:30:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011922.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 20 12:19:51 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

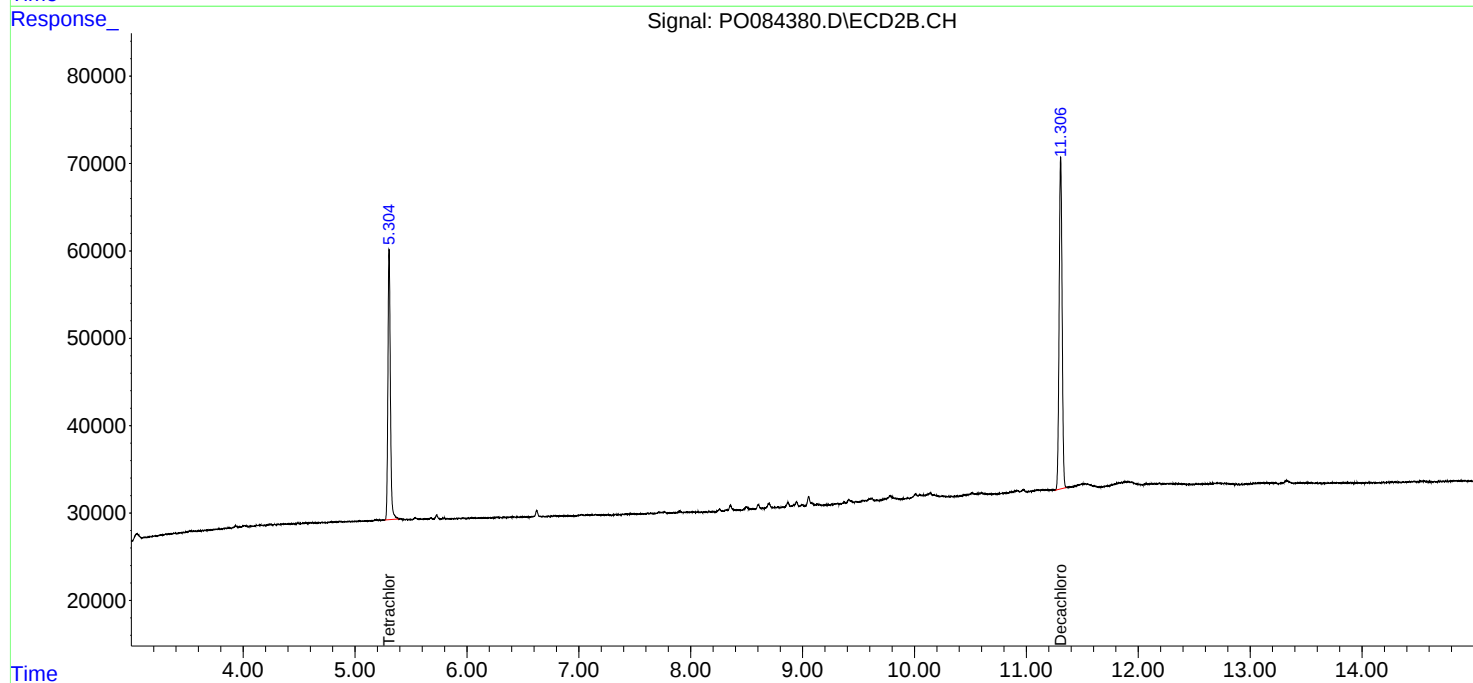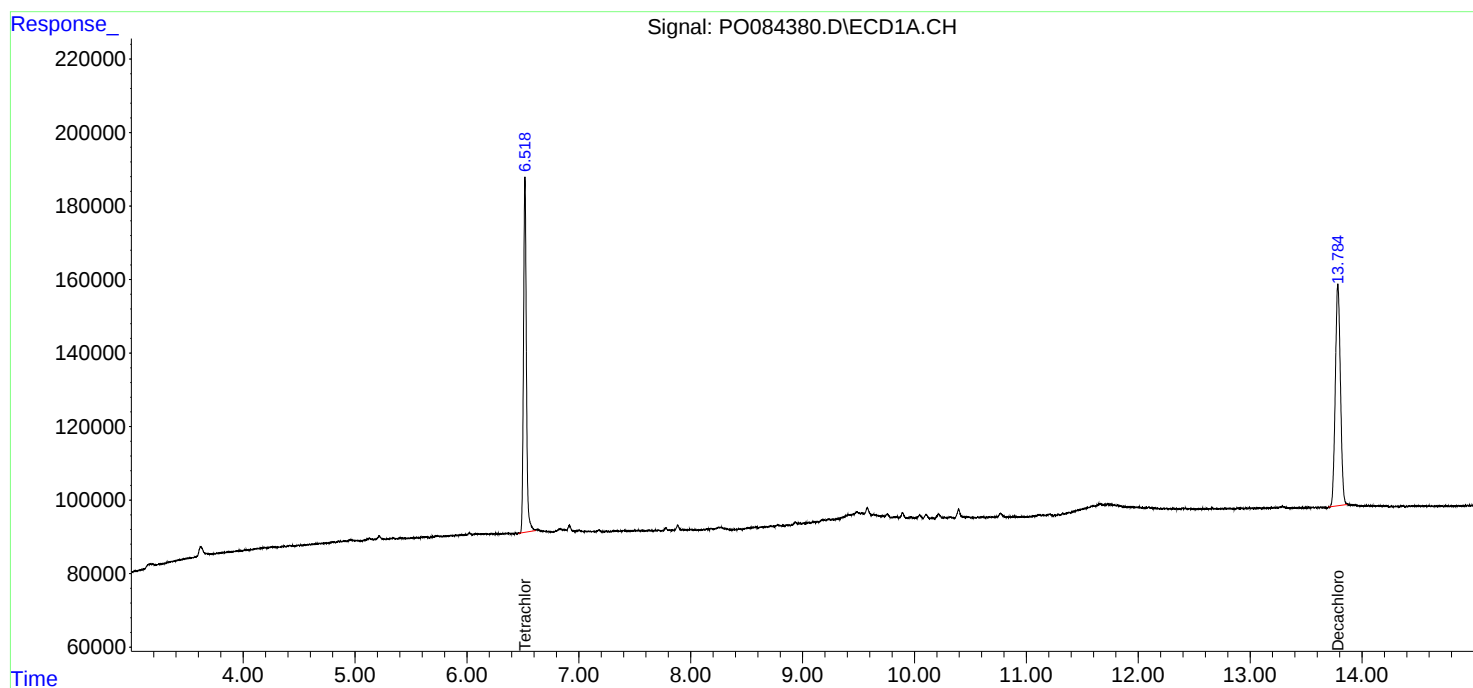


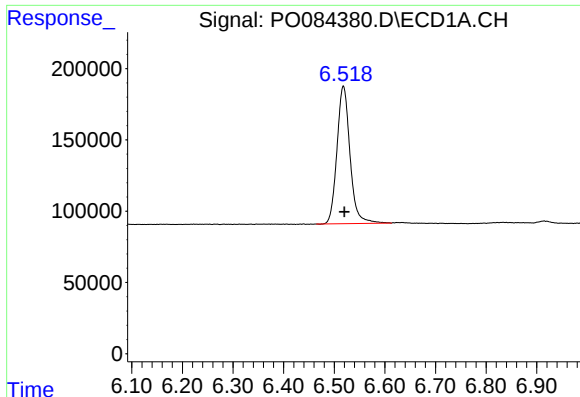

#1 Tetrachloro-m-xylene


R.T.: 6.518 min
Delta R.T.: -0.002 min
Response: 1726293
Conc: 21.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB142144BL

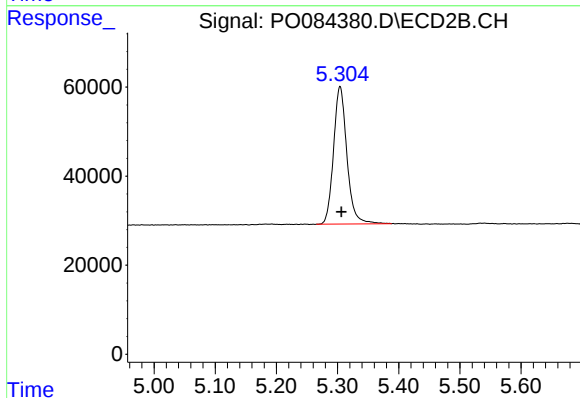


#1 Tetrachloro-m-xylene

R.T.: 5.304 min
Delta R.T.: -0.002 min
Response: 470190
Conc: 20.76 ng/ml

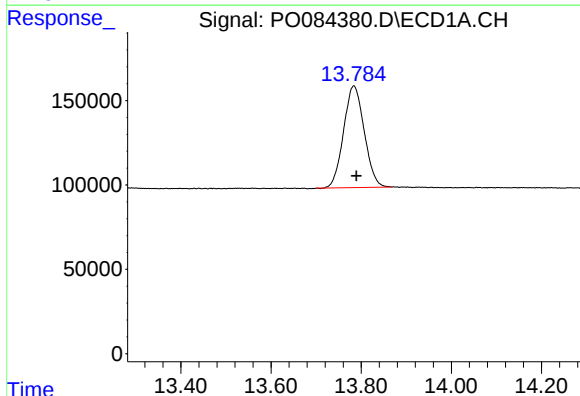

#2 Decachlorobiphenyl

R.T.: 13.784 min
Delta R.T.: -0.005 min
Response: 1916585
Conc: 22.01 ng/ml

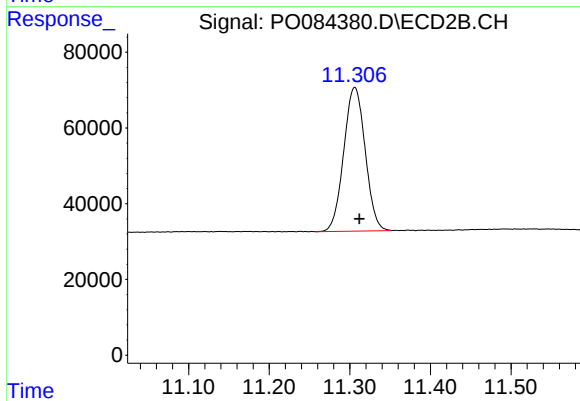

#2 Decachlorobiphenyl

R.T.: 11.306 min
Delta R.T.: -0.006 min
Response: 702271
Conc: 22.22 ng/ml