

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012023\
 Data File : P0092194.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2023 14:23
 Operator : YP/AJ
 Sample : PB150352BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 21:22:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 11 04:41:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.452	3.650	49064614	23042400	17.591	16.597
2)	SA Decachlor...	10.377	8.700	42279812	21890347	21.597	24.688
Target Compounds							
3)	L1 AR-1016-1	5.574f	0.000	2147606	0	25.268	N.D. #
9)	L2 AR-1221-2	0.000	3.950	0	402784	N.D.	30.838 #
16)	L4 AR-1242-1	5.574f	0.000	2147606	0	30.096	N.D. #
21)	L5 AR-1248-1	5.574f	0.000	2147606	0	39.240	N.D. #
32)	L7 AR-1260-2	7.481f	0.000	1126340	0	8.768	N.D. #
33)	L7 AR-1260-3	0.000	6.577	0	787920	N.D.	11.017 #
35)	L7 AR-1260-5	0.000	7.285	0	202982	N.D.	1.809 #
37)	L8 AR-1262-2	0.000	7.285	0	202982	N.D.	1.753 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012023\
Data File : PO092194.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2023 14:23
Operator : YP/AJ
Sample : PB150352BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 21:22:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 11 04:41:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

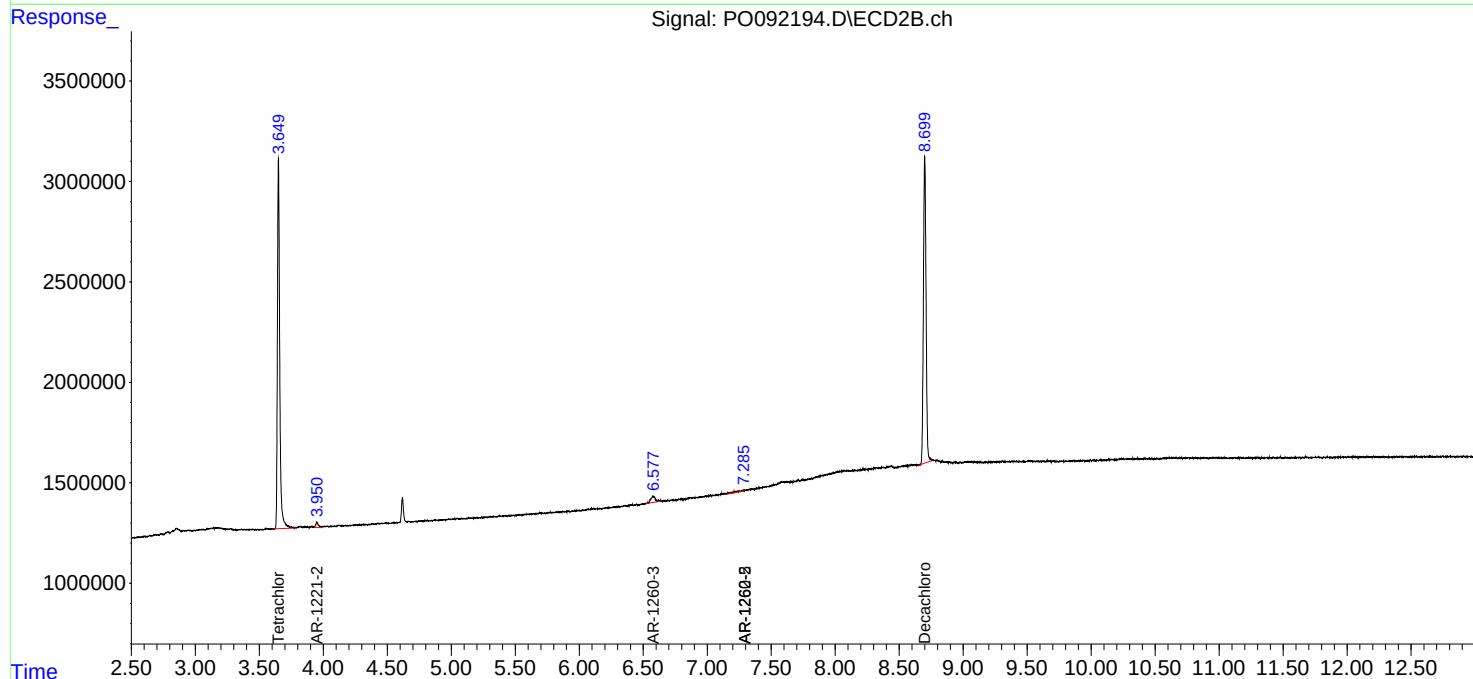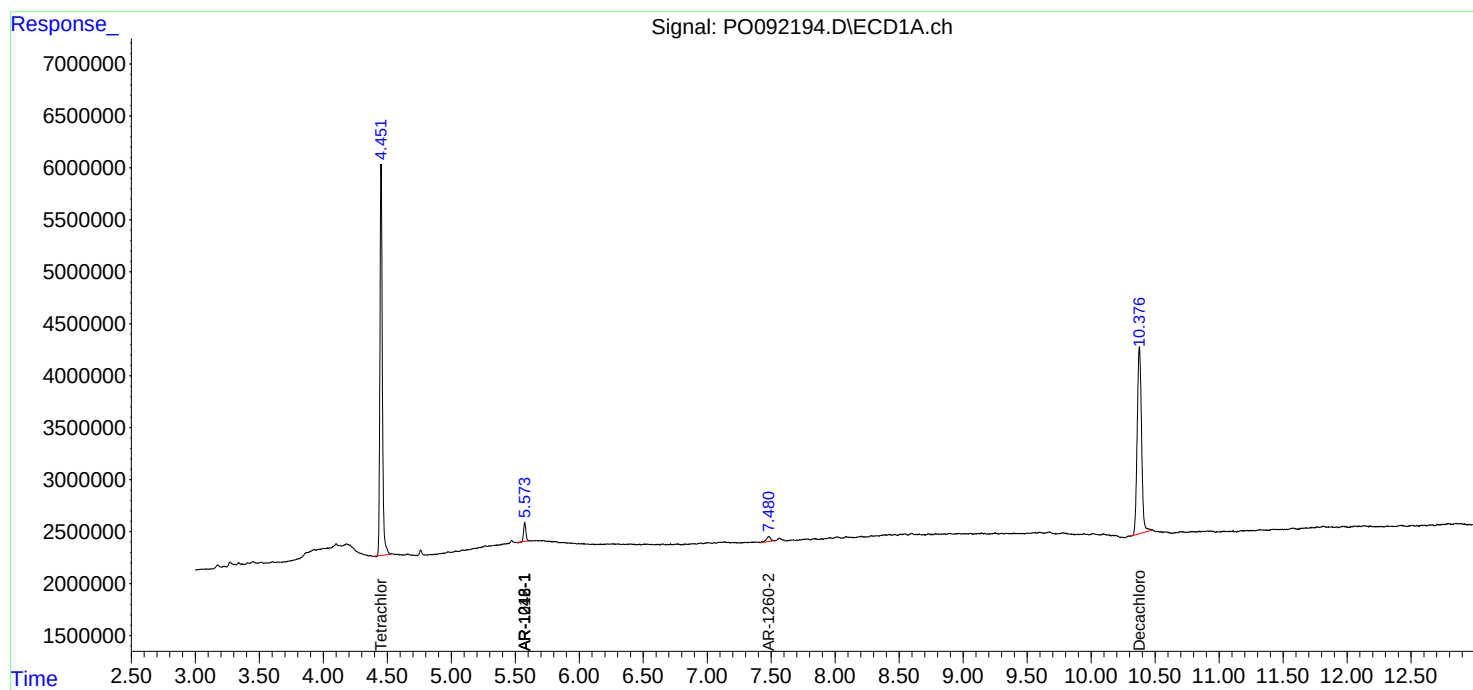


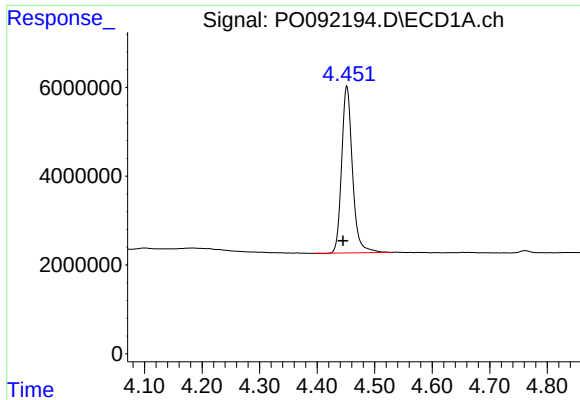

#1 Tetrachloro-m-xylene


R.T.: 4.452 min
Delta R.T.: 0.007 min
Response: 49064614
Conc: 17.59 ng/ml

Instrument :
ECD_O
ClientSampleId :

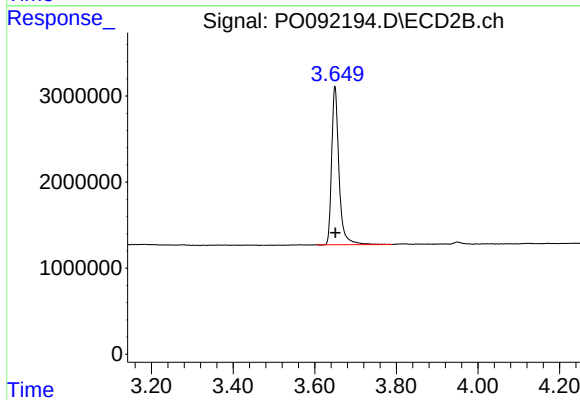


#1 Tetrachloro-m-xylene

R.T.: 3.650 min
Delta R.T.: 0.000 min
Response: 23042400
Conc: 16.60 ng/ml

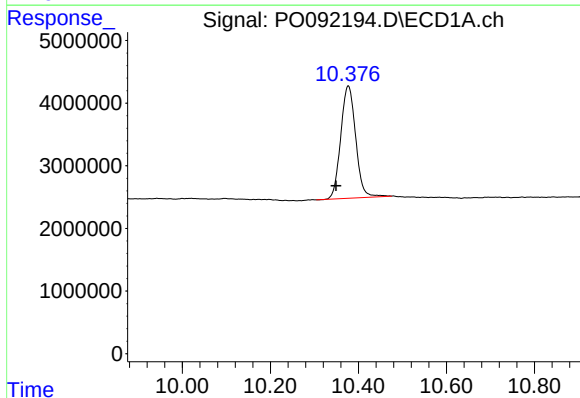


#2 Decachlorobiphenyl

R.T.: 10.377 min
Delta R.T.: 0.028 min
Response: 42279812
Conc: 21.60 ng/ml

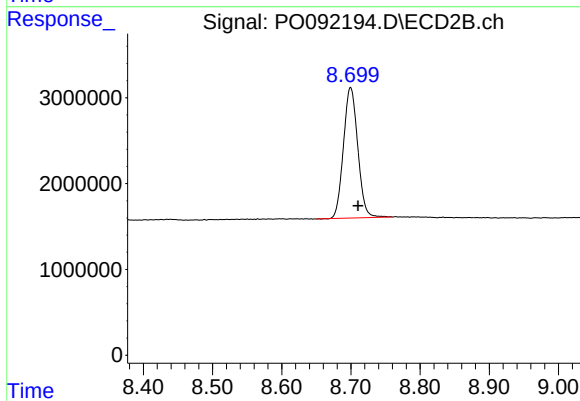

#2 Decachlorobiphenyl


R.T.: 8.700 min
Delta R.T.: -0.011 min
Response: 21890347
Conc: 24.69 ng/ml

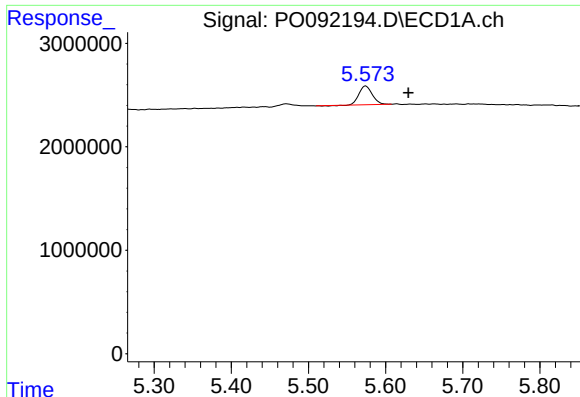

#3 AR-1016-1


R.T.: 5.574 min
Delta R.T.: -0.055 min
Response: 2147606
Conc: 25.27 ng/ml

Instrument :
ECD_O
ClientSampleId :

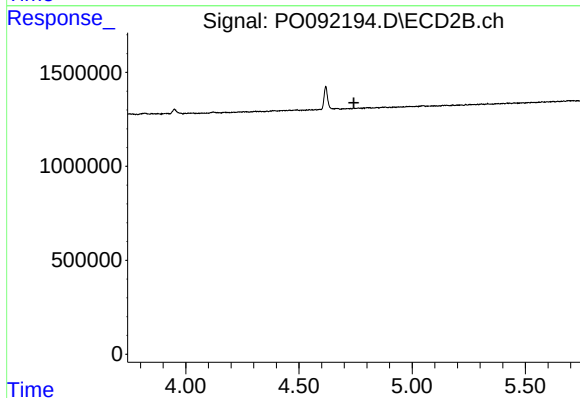


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.743 min
Response: 0
Conc: N.D.

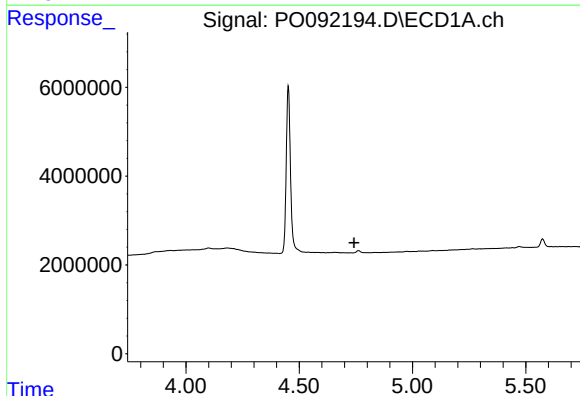


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.742 min
Response: 0
Conc: N.D.

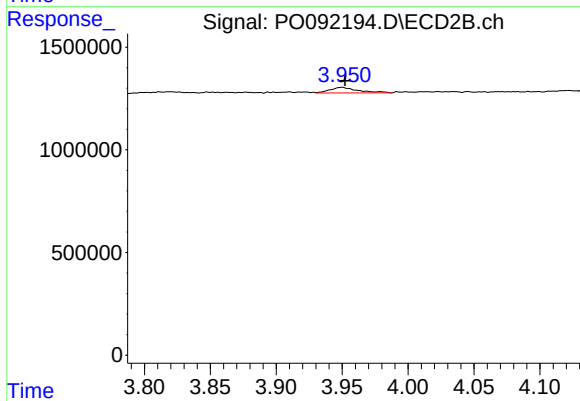

#9 AR-1221-2


R.T.: 3.950 min
Delta R.T.: -0.002 min
Response: 402784
Conc: 30.84 ng/ml

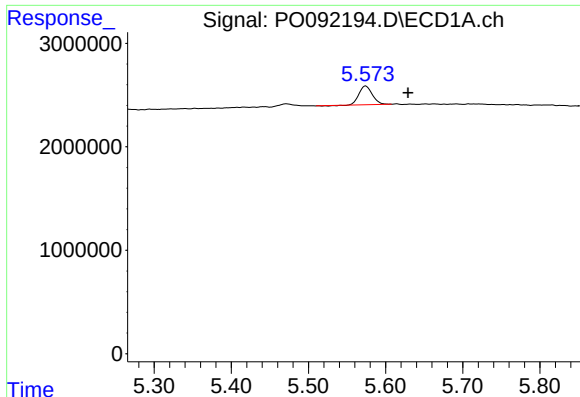

#16 AR-1242-1


R.T.: 5.574 min
Delta R.T.: -0.055 min
Response: 2147606
Conc: 30.10 ng/ml

Instrument :
ECD_O
ClientSampleId :

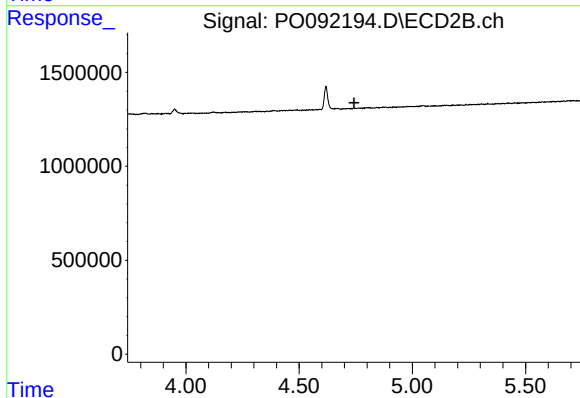


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 4.742 min
Response: 0
Conc: N.D.

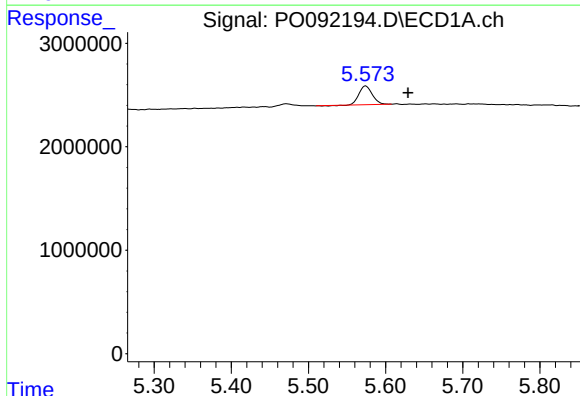


#21 AR-1248-1

R.T.: 5.574 min
Delta R.T.: -0.055 min
Response: 2147606
Conc: 39.24 ng/ml

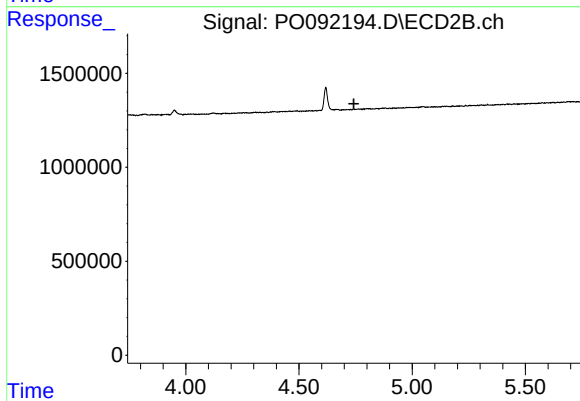

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T. : 4.743 min
Response: 0
Conc: N.D.

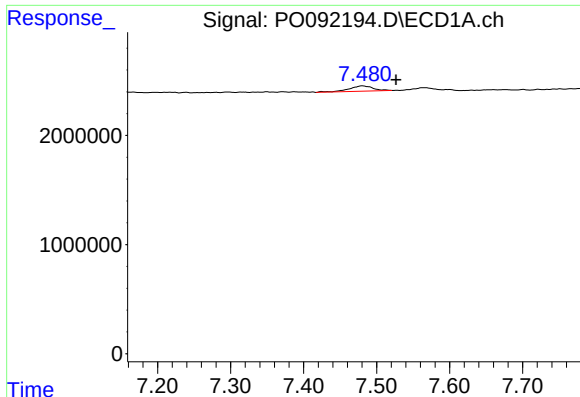

#32 AR-1260-2


R.T.: 7.481 min
Delta R.T.: -0.046 min
Response: 1126340
Conc: 8.77 ng/ml

Instrument :
ECD_O
ClientSampleId :

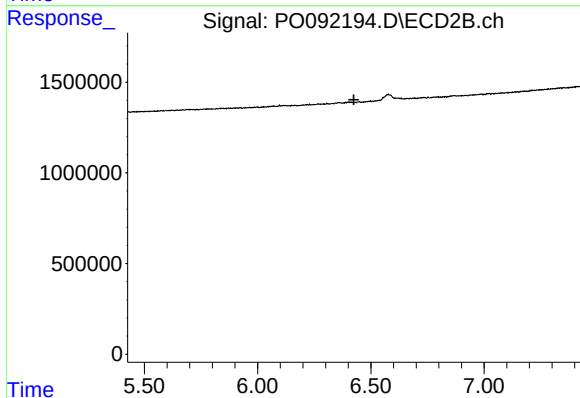


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.425 min
Response: 0
Conc: N.D.

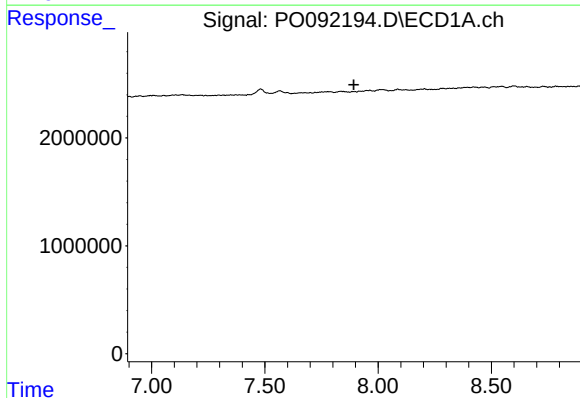


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.893 min
Response: 0
Conc: N.D.

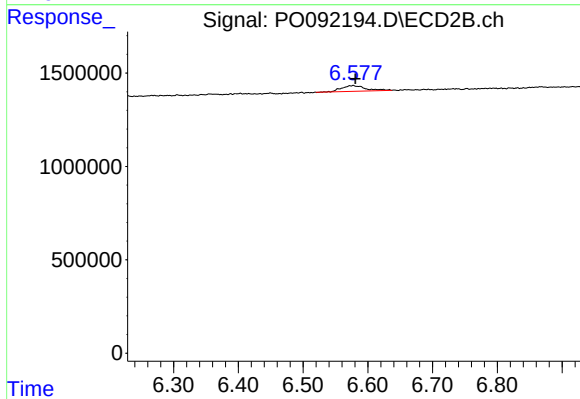

#33 AR-1260-3


R.T.: 6.577 min
Delta R.T.: -0.003 min
Response: 787920
Conc: 11.02 ng/ml

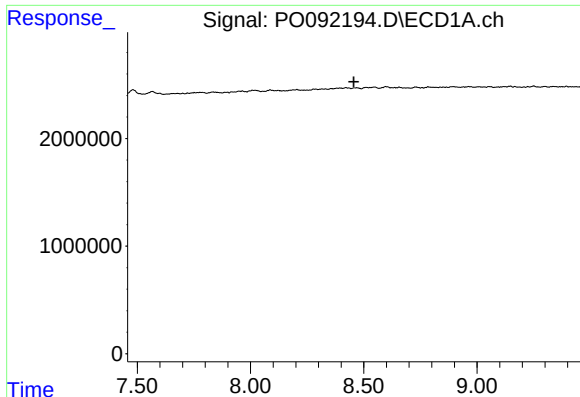

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

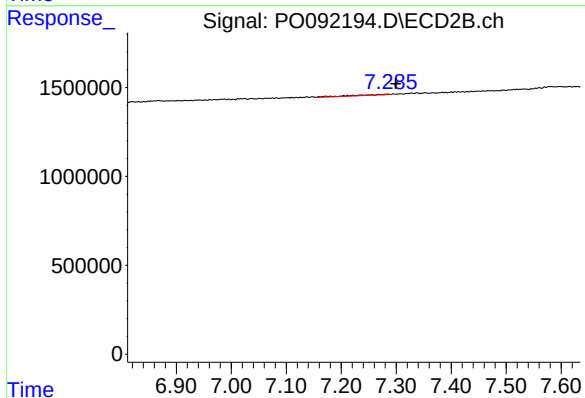


#35 AR-1260-5

R.T.: 7.285 min
Delta R.T.: -0.014 min
Response: 202982
Conc: 1.81 ng/ml

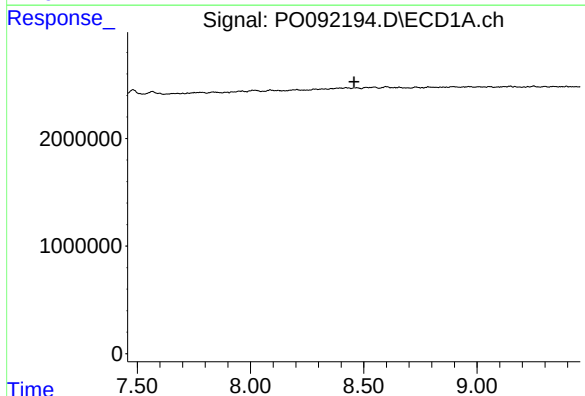

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.457 min
Response: 0
Conc: N.D.

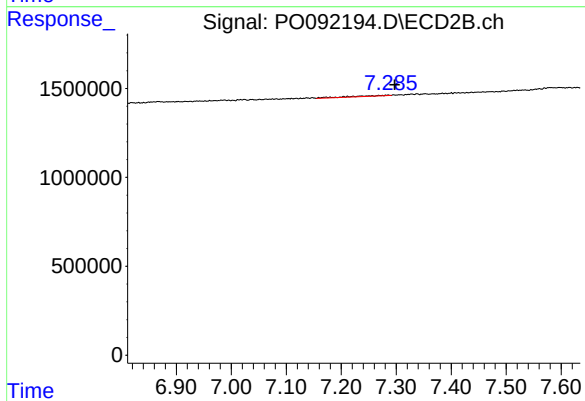

#37 AR-1262-2

R.T.: 7.285 min
Delta R.T.: -0.012 min
Response: 202982
Conc: 1.75 ng/ml