

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012023\
 Data File : P0092207.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2023 20:46
 Operator : YP/AJ
 Sample : 01235-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 12X54

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/23/2023
 Supervised By :Ankita Jodhani 01/23/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 00:03:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 11 04:41:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.448	3.646	14629801	7055562	5.245	5.082
2) SA Decachlor...	10.367	8.694	8102717	4527840	4.139m	5.106

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012023\
Data File : PO092207.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2023 20:46
Operator : YP/AJ
Sample : 01235-06
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
12X54


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/23/2023
Supervised By :Ankita Jodhani 01/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 00:03:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 11 04:41:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

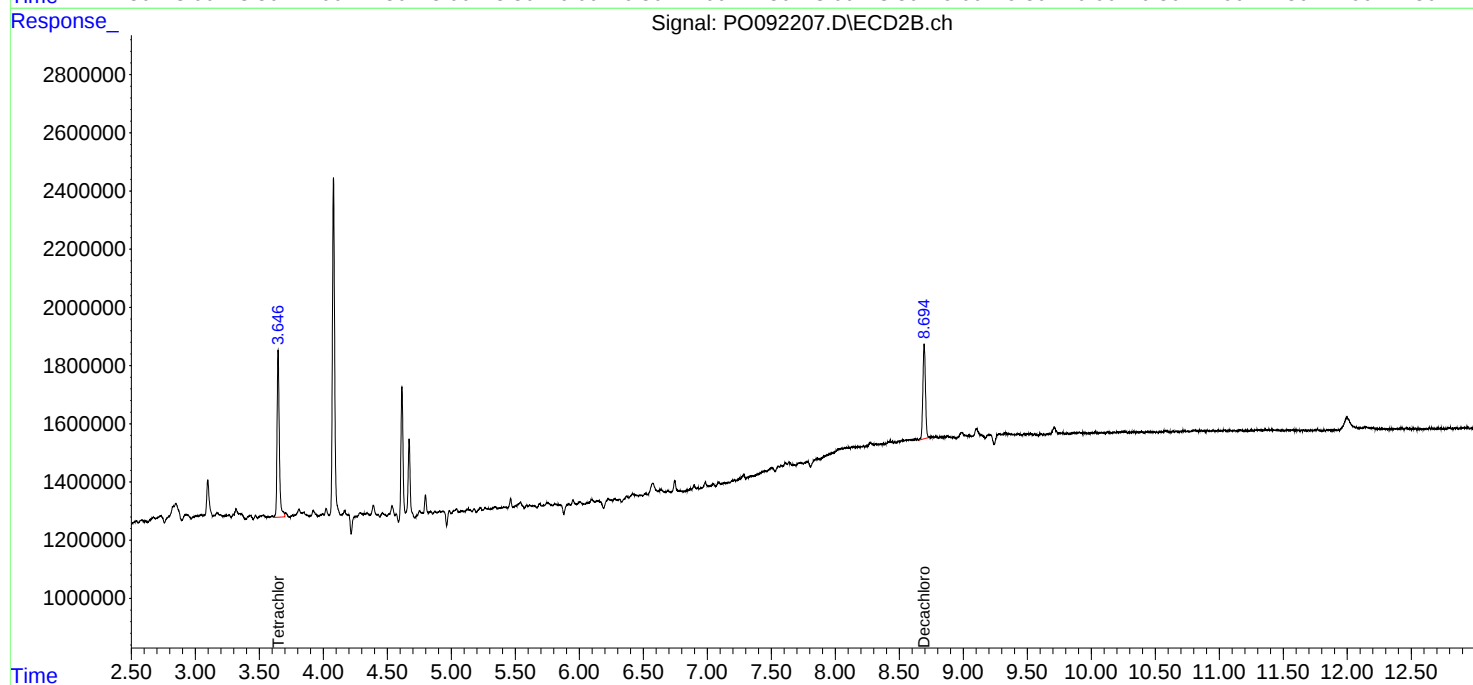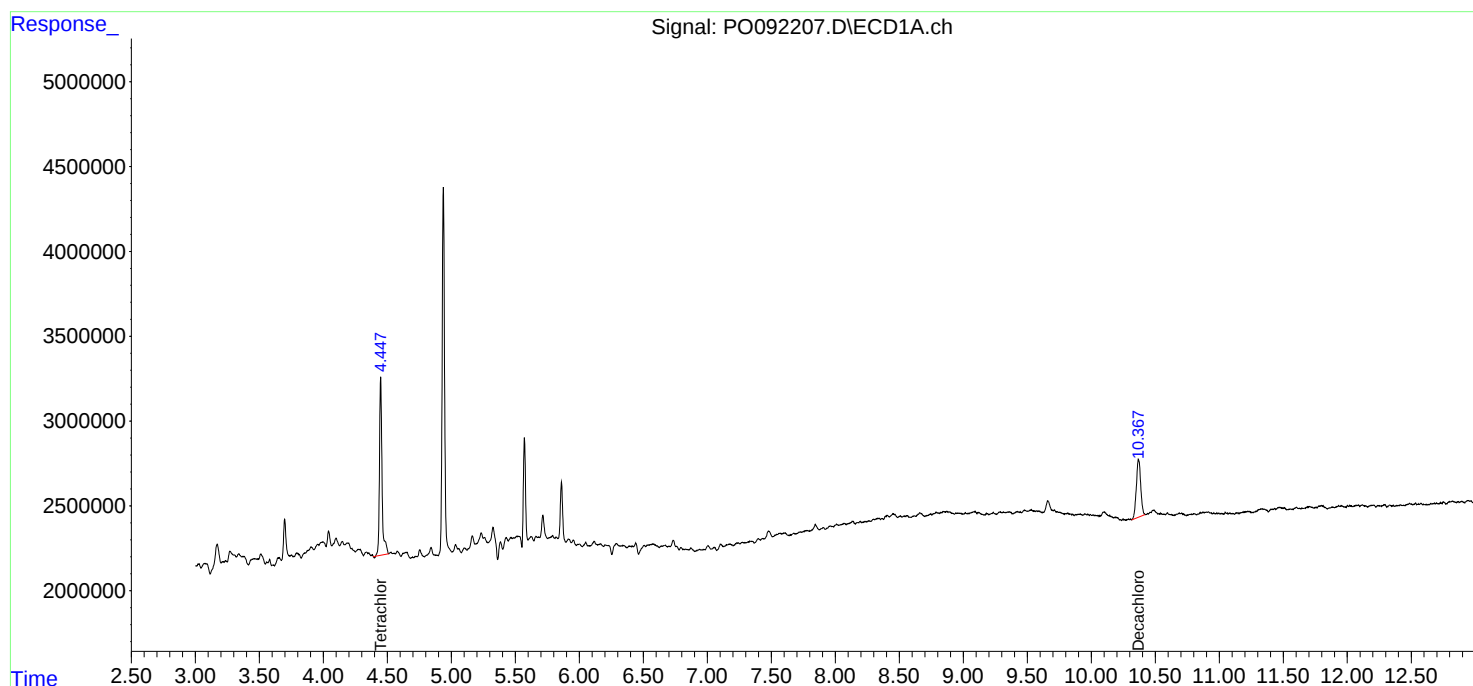

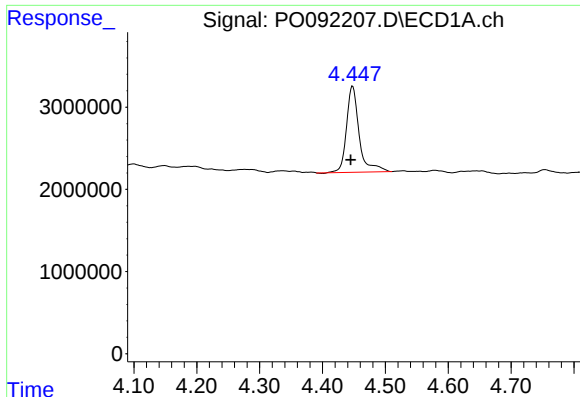


#1 Tetrachloro-m-xylene

R.T.: 4.448 min
Delta R.T.: 0.003 min
Response: 14629801
Conc: 5.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
12X54


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/23/2023
Supervised By :Ankita Jodhani 01/23/2023

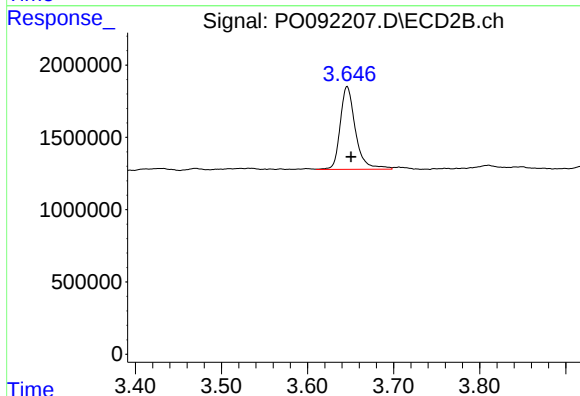


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: -0.004 min
Response: 7055562
Conc: 5.08 ng/ml

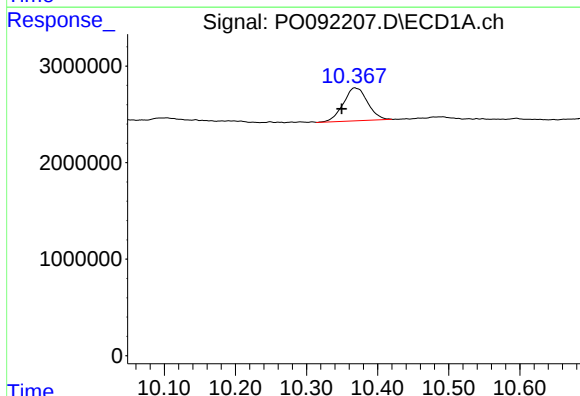

#2 Decachlorobiphenyl

R.T.: 10.367 min
Delta R.T.: 0.018 min
Response: 8102717
Conc: 4.14 ng/ml m

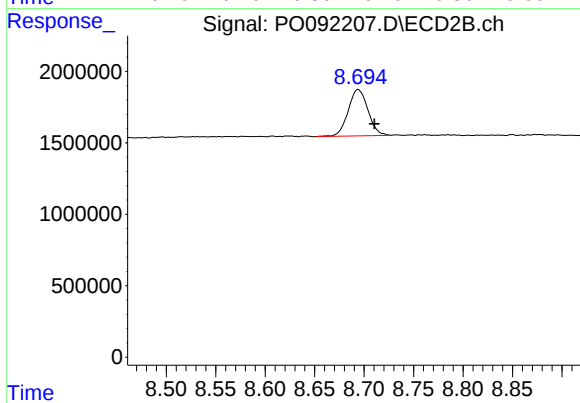

#2 Decachlorobiphenyl

R.T.: 8.694 min
Delta R.T.: -0.016 min
Response: 4527840
Conc: 5.11 ng/ml