

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012120\
 Data File : P0065727.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jan 2020 20:17
 Operator : DD\AJ
 Sample : L1161-08
 Misc : AR1221 LOQ 50 PPB
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOQ-WATER-02-QT1-2020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 04:26:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.155	3.430	390247	461606	21.371	20.985
2) SA Decachlor...	9.652	8.329	676214	801323	19.958	19.323
Target Compounds						
8) L2 AR-1221-1	4.365	3.640	14008	18821	67.572	72.590
9) L2 AR-1221-2	4.450	3.723	14325	16698	91.746	84.688
10) L2 AR-1221-3	4.523	3.796	34749	43511	66.541	67.532
11) L3 AR-1232-1	4.523	3.796	34749	43511	85.912	87.335
12) L3 AR-1232-2	4.998	0.000	4852	0	23.072	N.D. #
28) L6 AR-1254-3	6.733	0.000	7941	0	5.124	N.D. #
43) L9 AR-1268-3	8.599	0.000	4810	0	1.494	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012120\
Data File : P0065727.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jan 2020 20:17
Operator : DD\AJ
Sample : L1161-08
Misc : AR1221 LOQ 50 PPB
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOQ-WATER-02-QT1-2020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 04:26:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

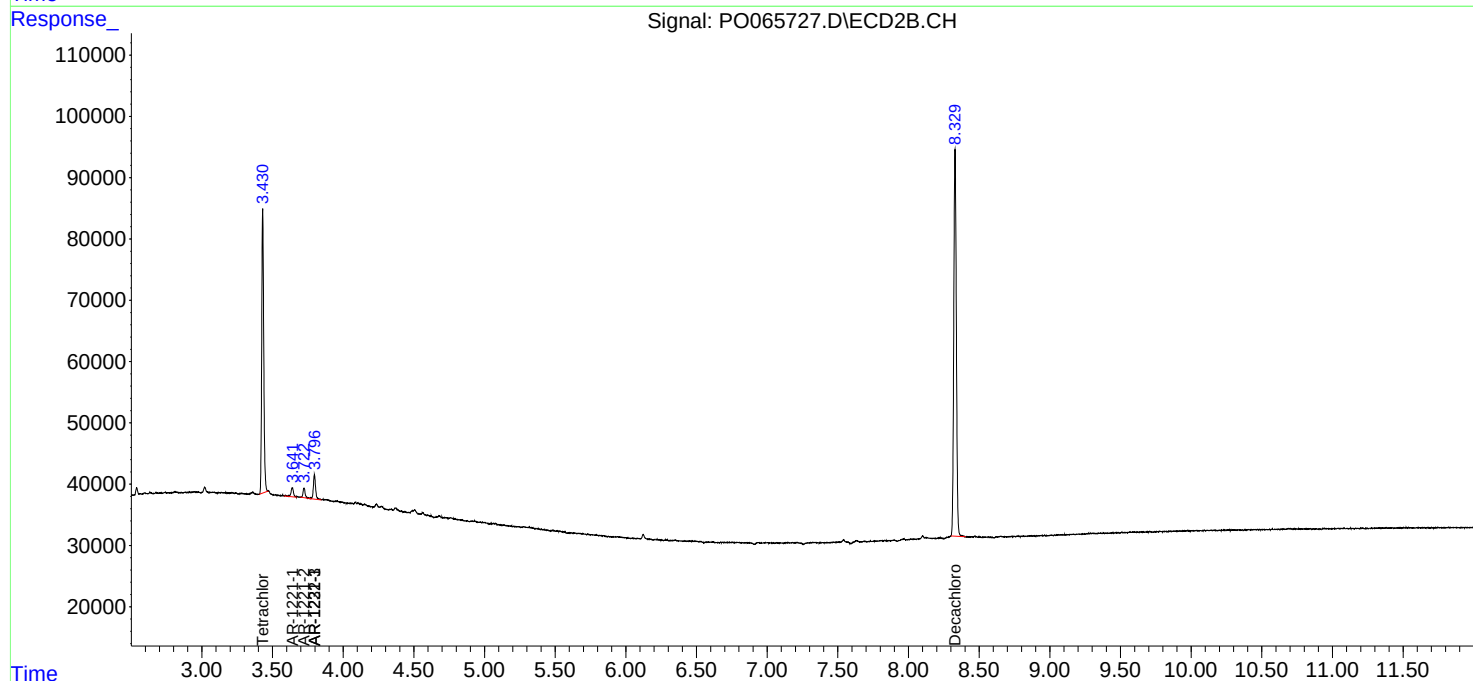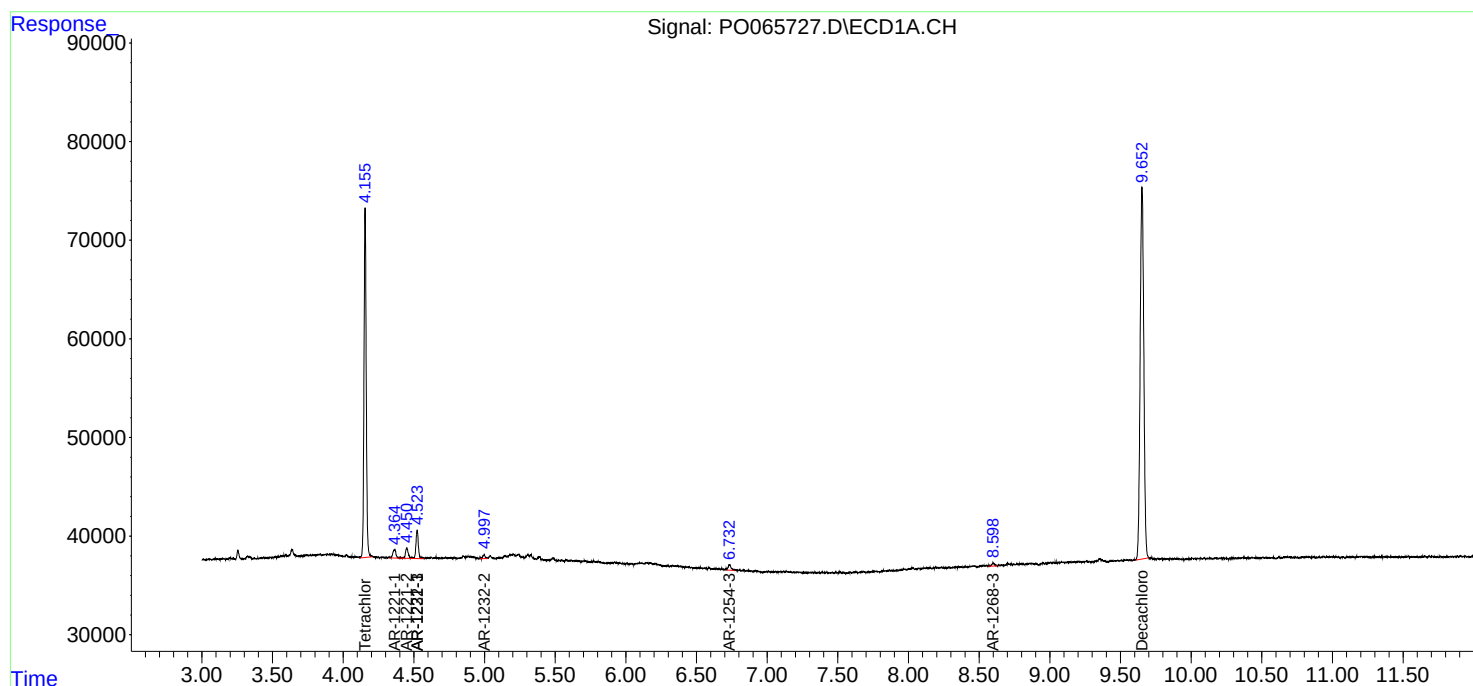


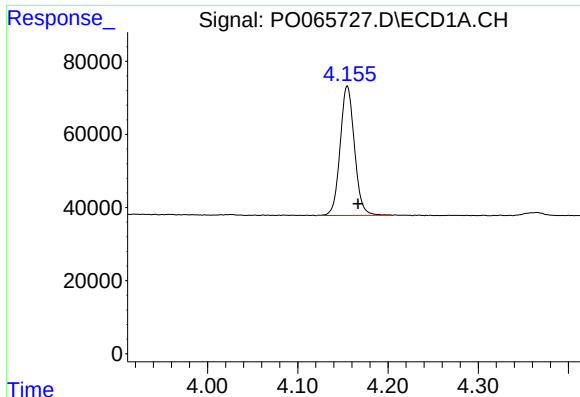

#1 Tetrachloro-m-xylene


R.T.: 4.155 min
Delta R.T.: -0.012 min
Response: 390247
Conc: 21.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOQ-WATER-02-QT1-2020

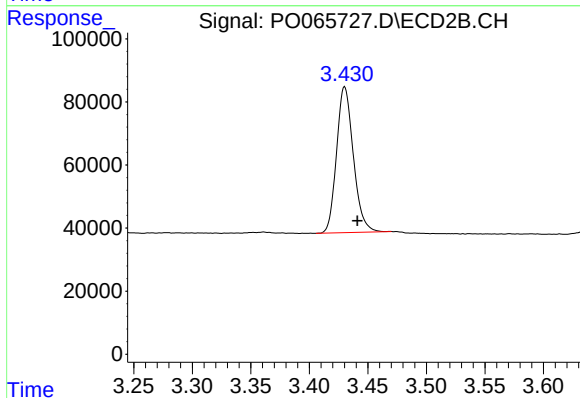


#1 Tetrachloro-m-xylene

R.T.: 3.430 min
Delta R.T.: -0.011 min
Response: 461606
Conc: 20.98 ng/ml

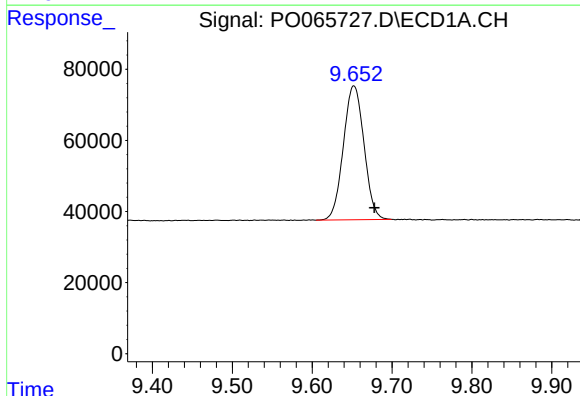


#2 Decachlorobiphenyl

R.T.: 9.652 min
Delta R.T.: -0.026 min
Response: 676214
Conc: 19.96 ng/ml

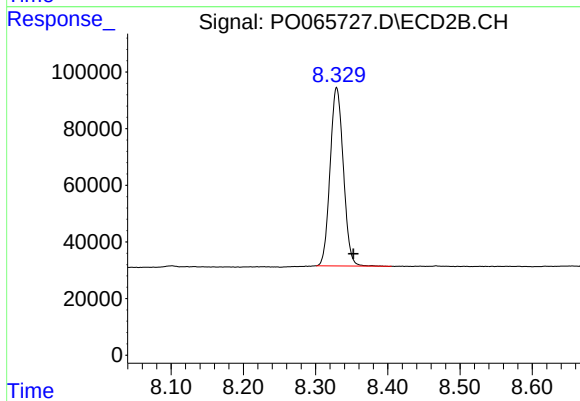

#2 Decachlorobiphenyl


R.T.: 8.329 min
Delta R.T.: -0.023 min
Response: 801323
Conc: 19.32 ng/ml

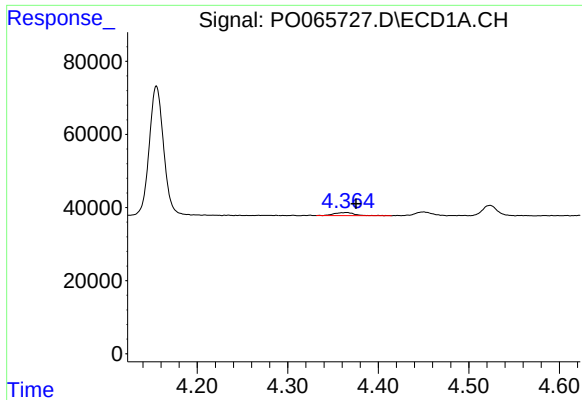

#8 AR-1221-1


R.T.: 4.365 min
Delta R.T.: -0.011 min
Response: 14008
Conc: 67.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOQ-WATER-02-QT1-2020

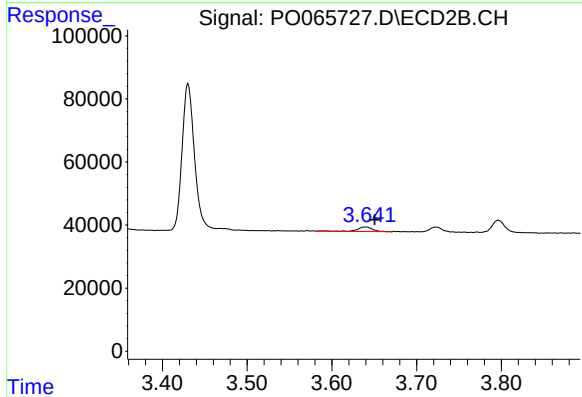


#8 AR-1221-1

R.T.: 3.640 min
Delta R.T.: -0.010 min
Response: 18821
Conc: 72.59 ng/ml

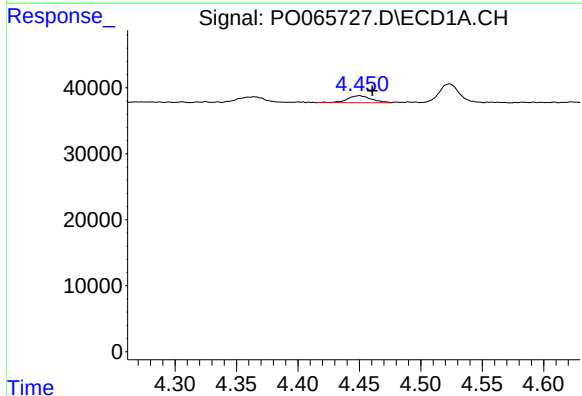


#9 AR-1221-2

R.T.: 4.450 min
Delta R.T.: -0.011 min
Response: 14325
Conc: 91.75 ng/ml

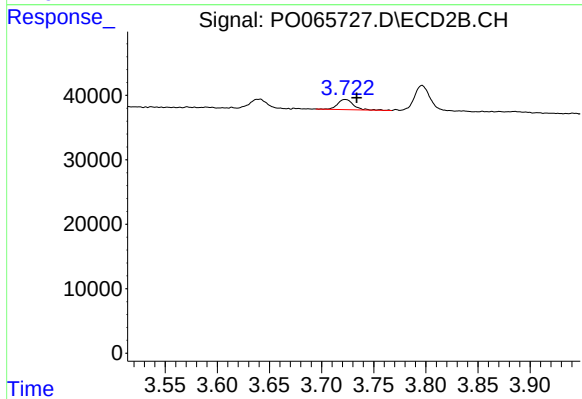

#9 AR-1221-2


R.T.: 3.723 min
Delta R.T.: -0.011 min
Response: 16698
Conc: 84.69 ng/ml

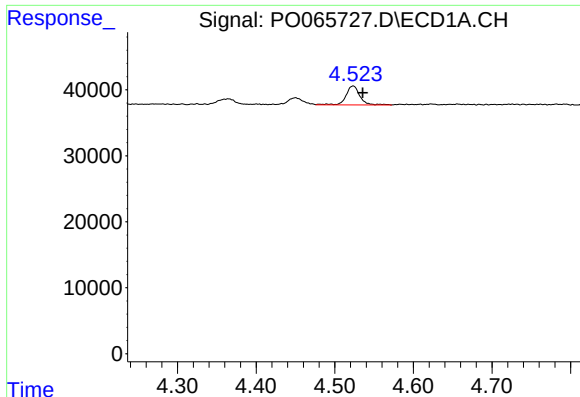

#10 AR-1221-3


R.T.: 4.523 min
Delta R.T.: -0.012 min
Response: 34749
Conc: 66.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOQ-WATER-02-QT1-2020

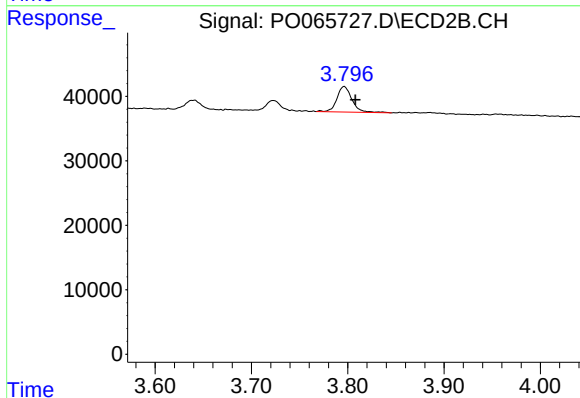


#10 AR-1221-3

R.T.: 3.796 min
Delta R.T.: -0.012 min
Response: 43511
Conc: 67.53 ng/ml

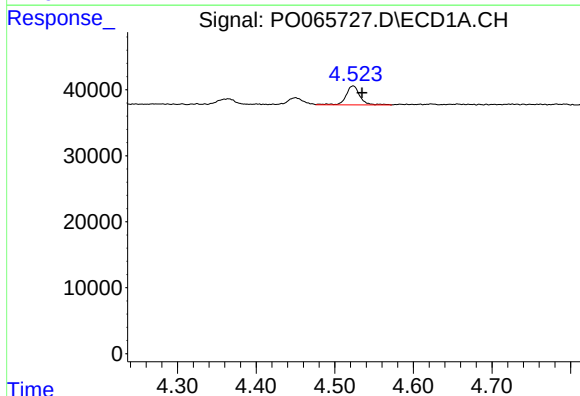


#11 AR-1232-1

R.T.: 4.523 min
Delta R.T.: -0.011 min
Response: 34749
Conc: 85.91 ng/ml

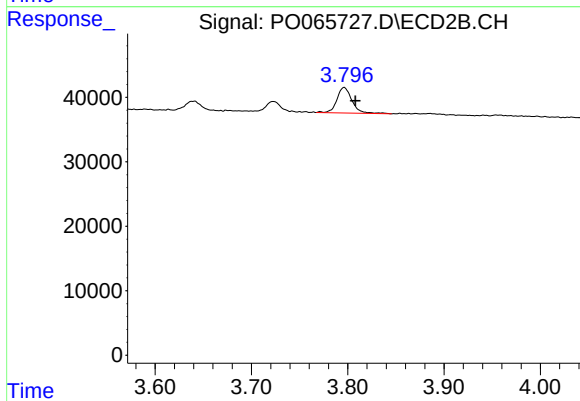

#11 AR-1232-1


R.T.: 3.796 min
Delta R.T.: -0.012 min
Response: 43511
Conc: 87.33 ng/ml

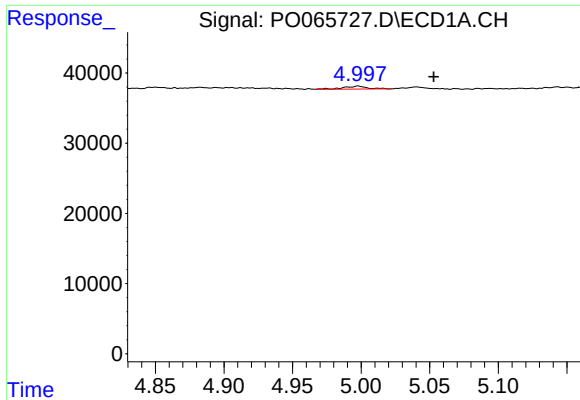

#12 AR-1232-2


R.T.: 4.998 min
Delta R.T.: -0.055 min
Response: 4852
Conc: 23.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOQ-WATER-02-QT1-2020

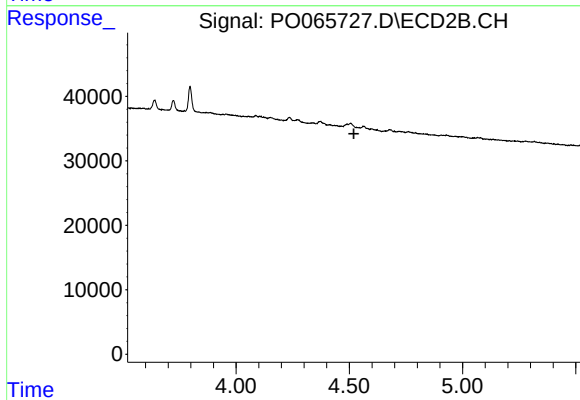


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 4.520 min
Response: 0
Conc: N.D.

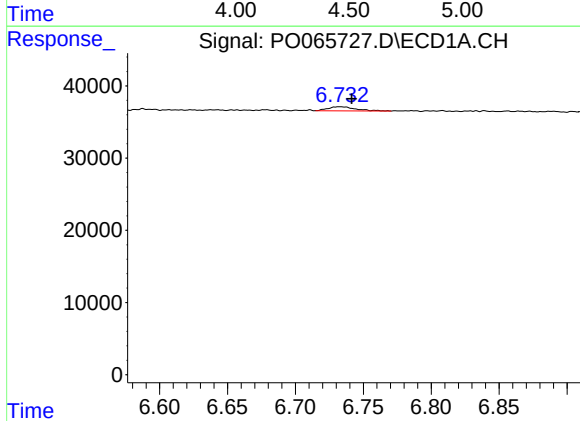


#28 AR-1254-3

R.T.: 6.733 min
Delta R.T.: -0.009 min
Response: 7941
Conc: 5.12 ng/ml

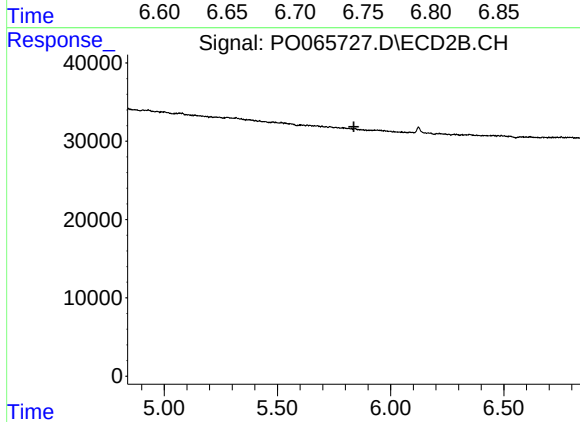

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 5.837 min
Response: 0
Conc: N.D.

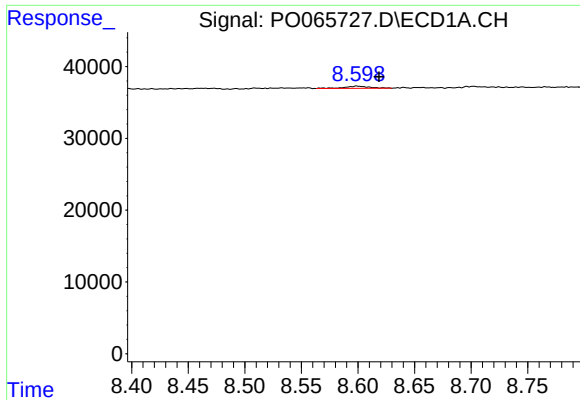

#43 AR-1268-3

R.T.: 8.599 min
Delta R.T.: -0.020 min
Response: 4810
Conc: 1.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOQ-WATER-02-QT1-2020

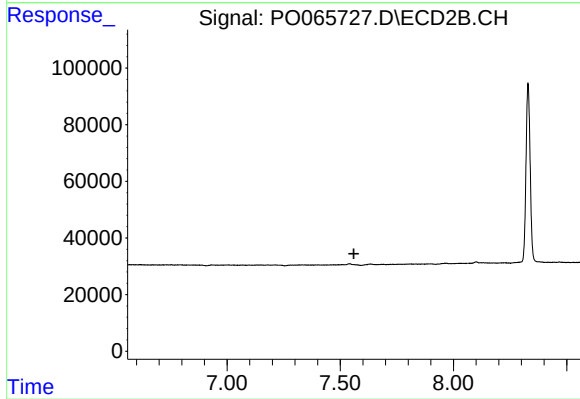

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.560 min
Response: 0
Conc: N.D.