

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012120\
 Data File : P0065746.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jan 2020 2:26
 Operator : DD\AJ
 Sample : L1161-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 07:09:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.155	3.430	390594	470814	21.390	21.403
2)	SA Decachlor...	9.650	8.329	711139	845525	20.988	20.389
Target Compounds							
3)	L1 AR-1016-1	5.306	4.489	35268	46970	40.439	45.586
4)	L1 AR-1016-2	5.327	4.506	51509	65389	40.158	45.123
5)	L1 AR-1016-3	5.387	4.679	32777	31075	41.602	39.970
6)	L1 AR-1016-4	5.484	4.721	25106	25758	38.910	38.527
7)	L1 AR-1016-5	5.775	4.930	25711	45732	38.784	53.748 #
9)	L2 AR-1221-2	4.451	3.723	8315	9838	53.256	49.894
10)	L2 AR-1221-3	4.524	3.796	17760	21053	34.009	32.677
11)	L3 AR-1232-1	4.524	3.796	17760	21053	43.910	42.258
12)	L3 AR-1232-2	5.040	4.506	23895	65389	113.630	121.261
13)	L3 AR-1232-3	5.327	4.679	51509	31075	110.309	109.240
14)	L3 AR-1232-4	5.484	4.761	25106	26884	107.609	100.565
15)	L3 AR-1232-5	5.574	4.930	23347	45732	132.052	159.521
16)	L4 AR-1242-1	5.306	4.489	35268	46970	60.580	68.911
17)	L4 AR-1242-2	5.327	4.506	51509	65389	60.239	68.233
18)	L4 AR-1242-3	5.387	4.679	32777	31075	62.505	60.626
19)	L4 AR-1242-4	5.484	4.761	25106	26884	59.260	51.437
20)	L4 AR-1242-5	6.212	5.276	7216	23287	13.251	32.041 #
21)	L5 AR-1248-1	5.327	4.506	51509	65389	110.699	117.954
22)	L5 AR-1248-2	5.574	4.721	23347	25758	35.382	33.572
23)	L5 AR-1248-3	5.775	4.761	25711	26884	34.123	34.170
24)	L5 AR-1248-4	6.212	4.930	7216	45732	7.617	47.712 #
25)	L5 AR-1248-5	6.212	5.276	7216	23287	7.888	23.004 #
26)	L6 AR-1254-1	6.148	5.276	37726	23287	44.471	16.074 #
27)	L6 AR-1254-2	6.362	5.422	24650	28607	17.937	21.627
28)	L6 AR-1254-3	6.728	5.834	25645	54593	16.546	24.226 #
29)	L6 AR-1254-4	7.008	6.077	19256	17174	15.106	11.392
30)	L6 AR-1254-5	7.454	6.496	10001	88255	7.122	39.648 #
31)	L7 AR-1260-1	6.887	5.948	68780	81398	49.869	43.235
32)	L7 AR-1260-2	7.142	6.136	82784	111029	47.183	45.701
33)	L7 AR-1260-3	7.497	6.286	65387	87972	46.262	40.643
34)	L7 AR-1260-4	7.720	6.752	66435	77992	38.048	38.875
35)	L7 AR-1260-5	8.026	6.995	143993	174248	42.937	35.198
36)	L8 AR-1262-1	7.497	6.550	65387	42271	39.526	44.838
37)	L8 AR-1262-2	8.026	6.995	143993	174248	44.964	38.779
38)	L8 AR-1262-3	8.323	7.273	89873	44799	39.480	26.618 #
39)	L8 AR-1262-4	8.374	7.337	62602	136190	35.414	39.602
40)	L8 AR-1262-5	8.986	7.830	47873	50011	35.987	29.328
41)	L9 AR-1268-1	8.323	7.273	89873	44799	22.091	8.435 #
42)	L9 AR-1268-2	8.374	7.337	62602	136190	16.266	26.812 #
43)	L9 AR-1268-3	8.597	0.000	9968	0	3.097	N.D. #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012120\
 Data File : P0065746.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jan 2020 2:26
 Operator : DD\AJ
 Sample : L1161-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 07:09:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44) L9	AR-1268-4	8.986	7.830	47873	50011	31.166	25.268
45) L9	AR-1268-5	9.353	8.100	21159	18387	1.910	1.279 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012120\
Data File : PO065746.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2020 2:26
Operator : DD\AJ
Sample : L1161-07
Misc : AR1660 LOD 40 PPB
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 07:09:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

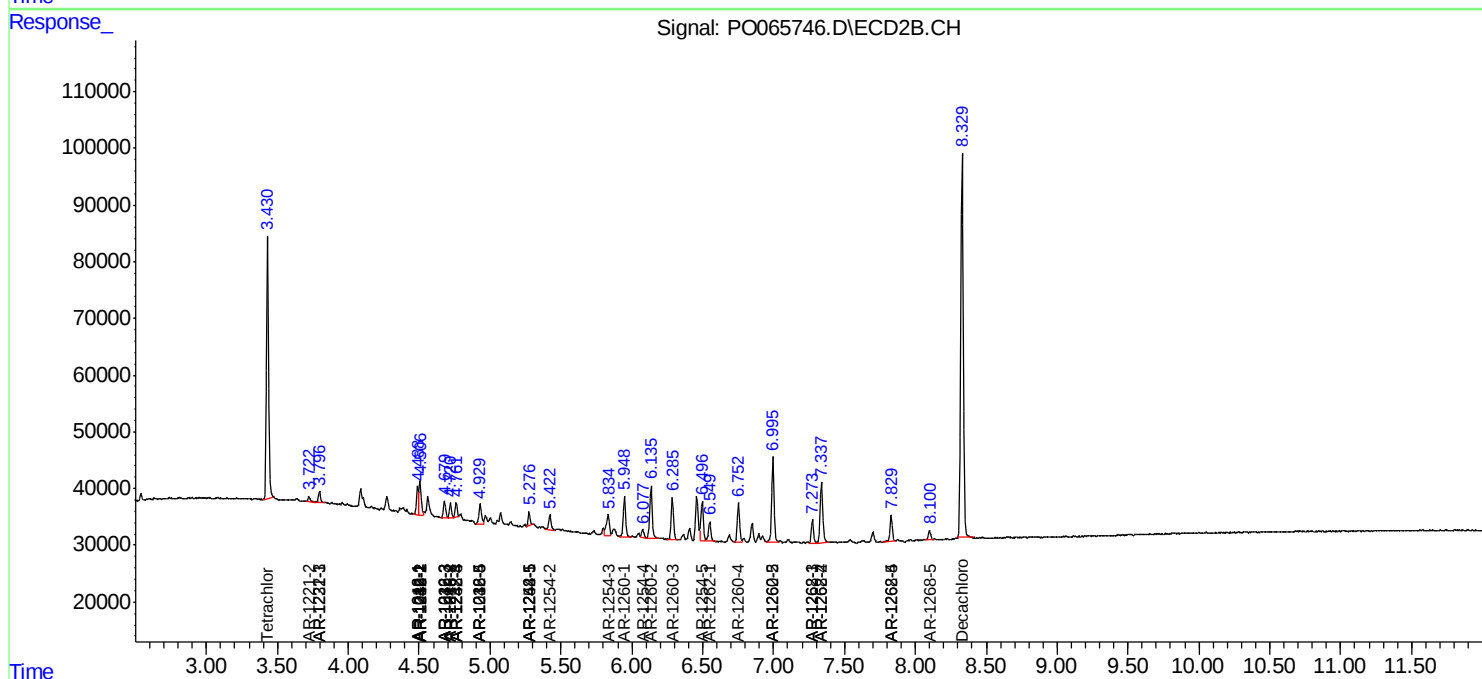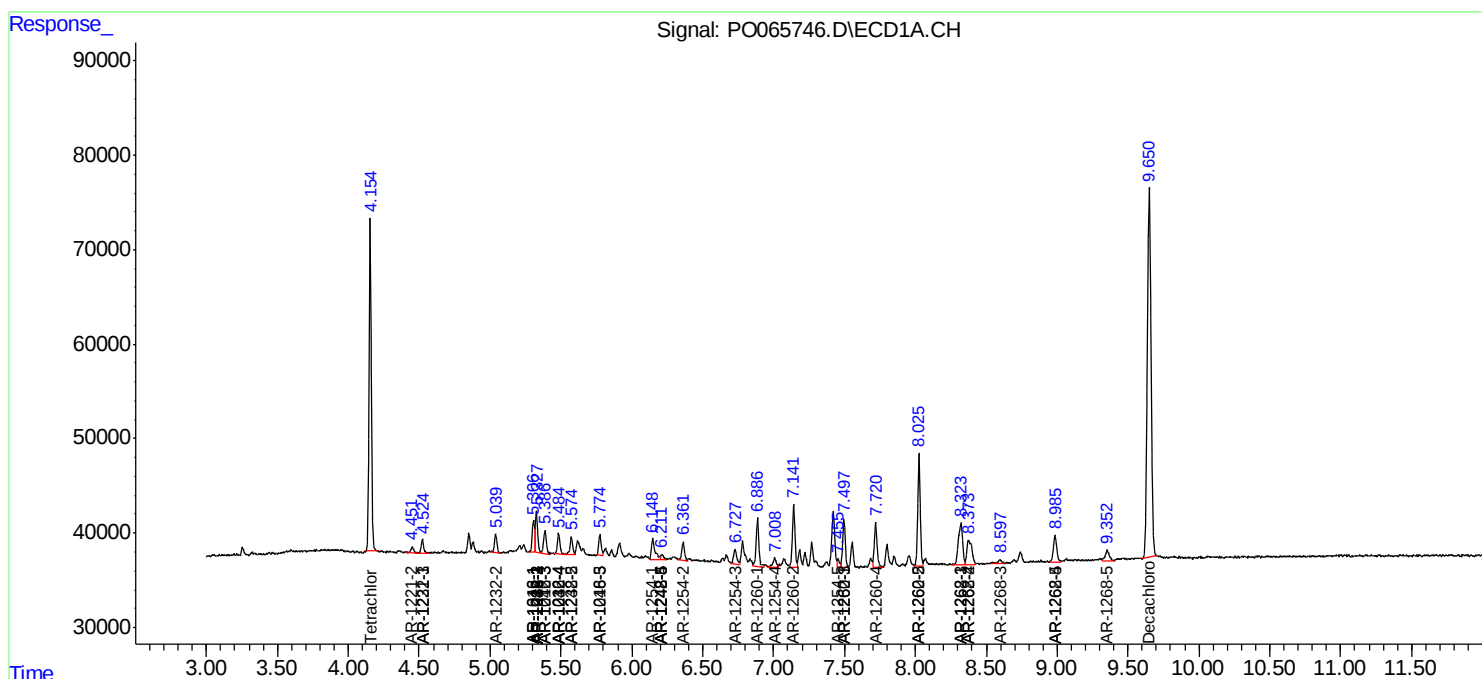


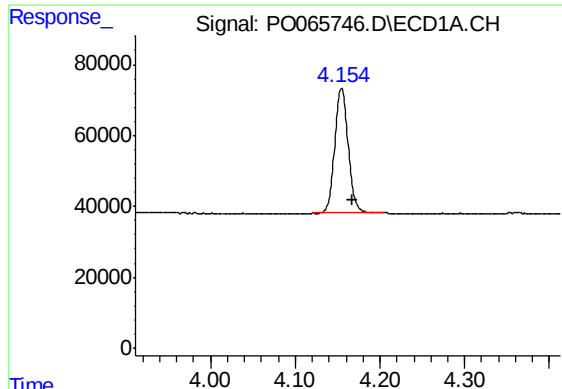

#1 Tetrachloro-m-xylene


R.T.: 4.155 min
Delta R.T.: -0.012 min
Response: 390594
Conc: 21.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020




#1 Tetrachloro-m-xylene

R.T.: 3.430 min
Delta R.T.: -0.011 min
Response: 470814
Conc: 21.40 ng/ml




#2 Decachlorobiphenyl

R.T.: 9.650 min
Delta R.T.: -0.028 min
Response: 711139
Conc: 20.99 ng/ml

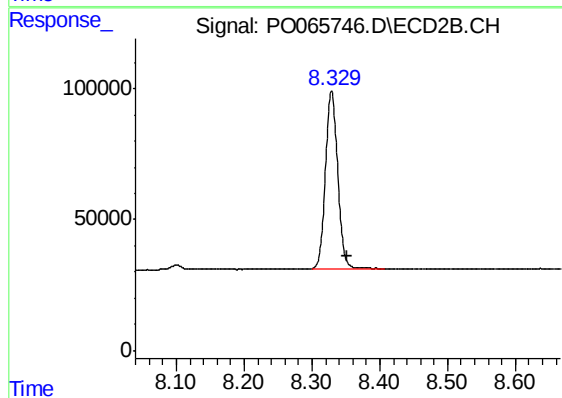

#2 Decachlorobiphenyl


R.T.: 8.329 min
Delta R.T.: -0.023 min
Response: 845525
Conc: 20.39 ng/ml

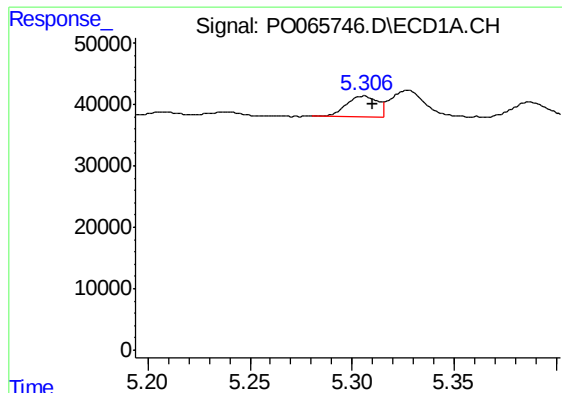

#3 AR-1016-1


R.T.: 5.306 min
Delta R.T.: -0.004 min
Response: 35268
Conc: 40.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

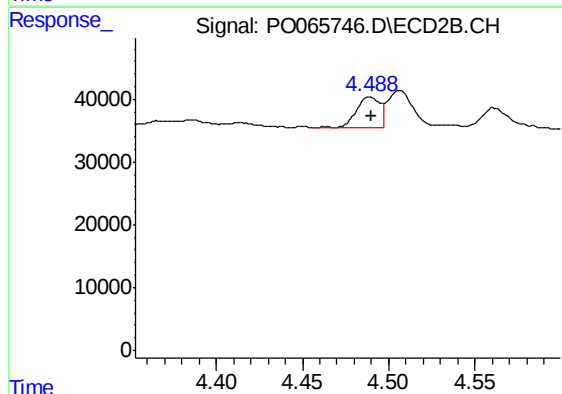


#3 AR-1016-1

R.T.: 4.489 min
Delta R.T.: -0.001 min
Response: 46970
Conc: 45.59 ng/ml




#4 AR-1016-2

R.T.: 5.327 min
Delta R.T.: -0.003 min
Response: 51509
Conc: 40.16 ng/ml

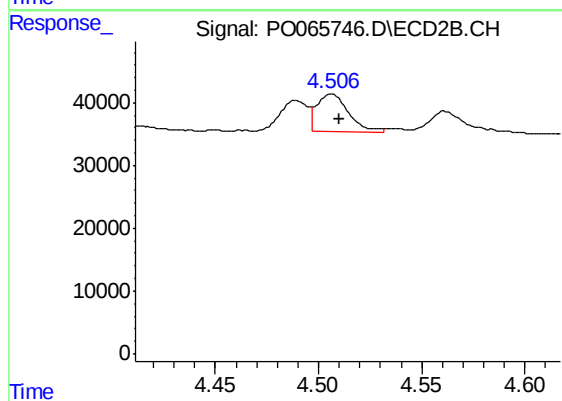

#4 AR-1016-2


R.T.: 4.506 min
Delta R.T.: -0.004 min
Response: 65389
Conc: 45.12 ng/ml

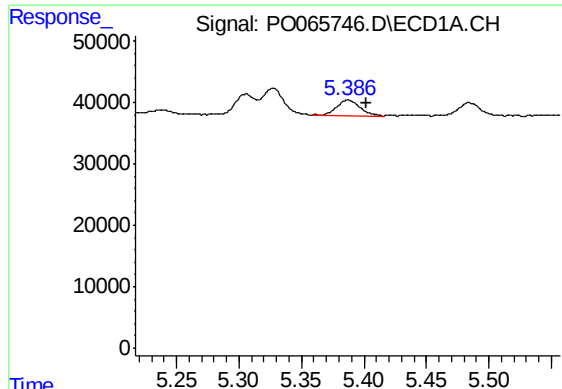

#5 AR-1016-3


R.T.: 5.387 min
Delta R.T.: -0.014 min
Response: 32777
Conc: 41.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020




#5 AR-1016-3

R.T.: 4.679 min
Delta R.T.: -0.015 min
Response: 31075
Conc: 39.97 ng/ml




#6 AR-1016-4

R.T.: 5.484 min
Delta R.T.: -0.014 min
Response: 25106
Conc: 38.91 ng/ml

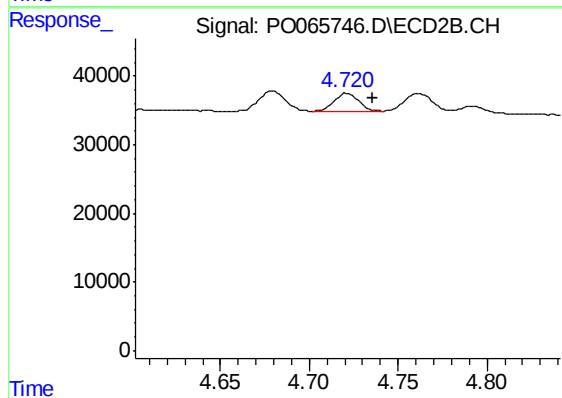

#6 AR-1016-4


R.T.: 4.721 min
Delta R.T.: -0.015 min
Response: 25758
Conc: 38.53 ng/ml

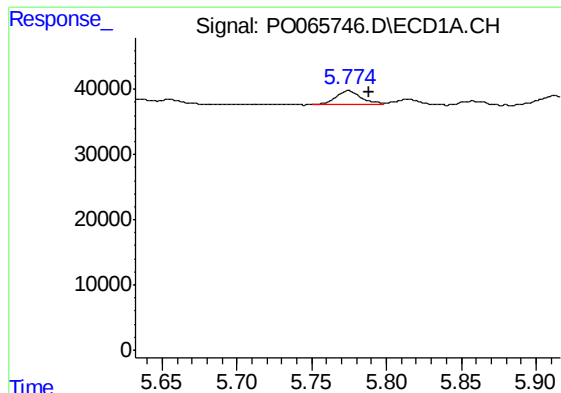

#7 AR-1016-5


R.T.: 5.775 min
Delta R.T.: -0.014 min
Response: 25711
Conc: 38.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

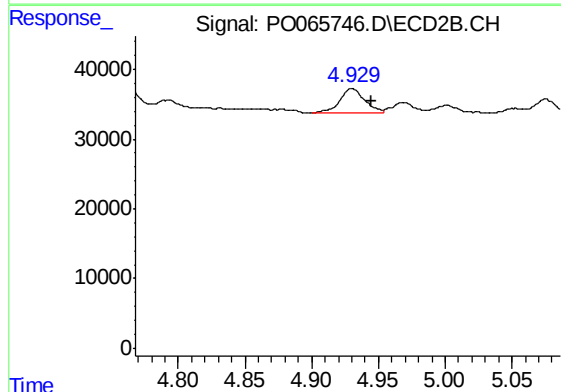


#7 AR-1016-5

R.T.: 4.930 min
Delta R.T.: -0.015 min
Response: 45732
Conc: 53.75 ng/ml

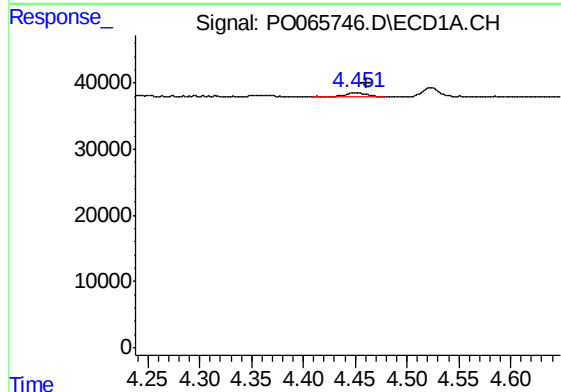


#9 AR-1221-2

R.T.: 4.451 min
Delta R.T.: -0.009 min
Response: 8315
Conc: 53.26 ng/ml

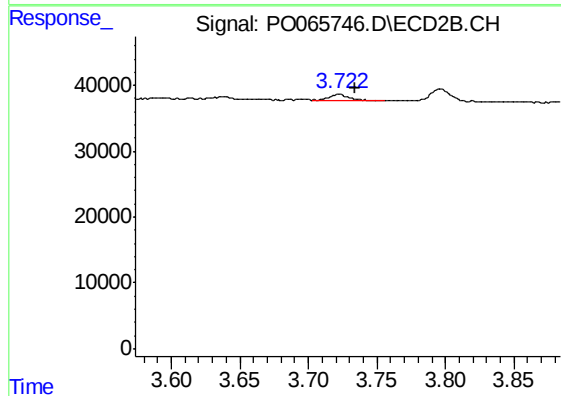

#9 AR-1221-2


R.T.: 3.723 min
Delta R.T.: -0.011 min
Response: 9838
Conc: 49.89 ng/ml



#10 AR-1221-3


R.T.: 4.524 min
Delta R.T.: -0.012 min
Response: 17760
Conc: 34.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020




#10 AR-1221-3

R.T.: 3.796 min
Delta R.T.: -0.012 min
Response: 21053
Conc: 32.68 ng/ml




#11 AR-1232-1

R.T.: 4.524 min
Delta R.T.: -0.011 min
Response: 17760
Conc: 43.91 ng/ml

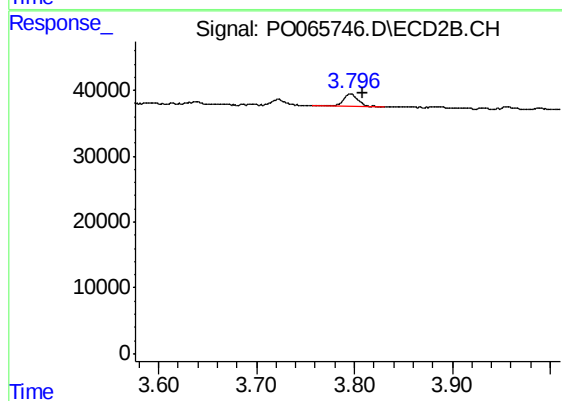

#11 AR-1232-1


R.T.: 3.796 min
Delta R.T.: -0.012 min
Response: 21053
Conc: 42.26 ng/ml

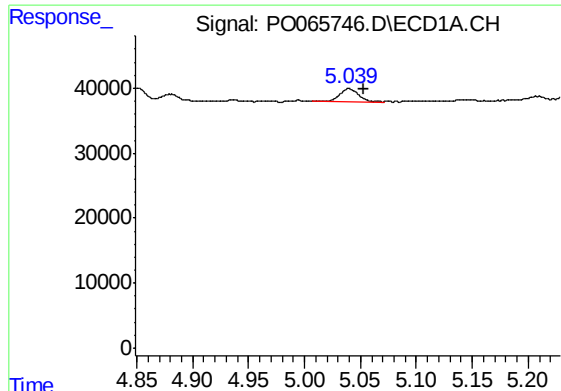

#12 AR-1232-2


R.T.: 5.040 min
Delta R.T.: -0.014 min
Response: 23895
Conc: 113.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

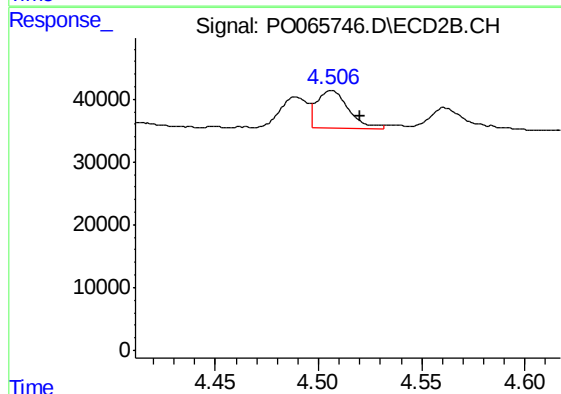


#12 AR-1232-2

R.T.: 4.506 min
Delta R.T.: -0.014 min
Response: 65389
Conc: 121.26 ng/ml

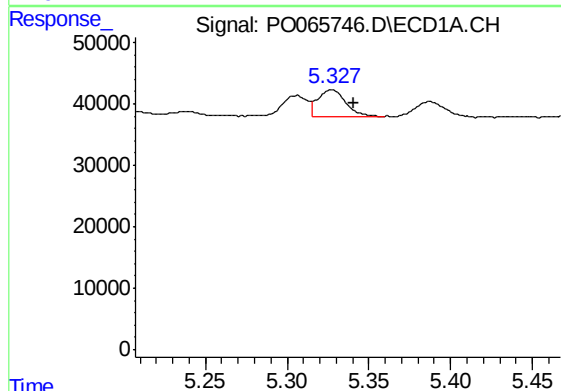


#13 AR-1232-3

R.T.: 5.327 min
Delta R.T.: -0.013 min
Response: 51509
Conc: 110.31 ng/ml

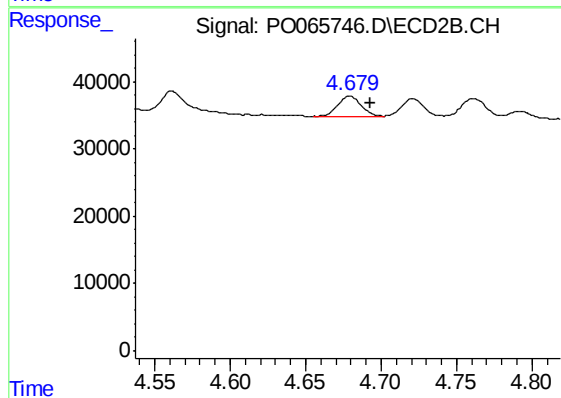

#13 AR-1232-3


R.T.: 4.679 min
Delta R.T.: -0.014 min
Response: 31075
Conc: 109.24 ng/ml

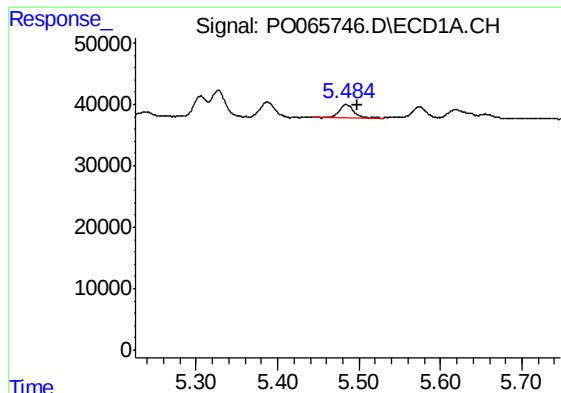

#14 AR-1232-4


R.T.: 5.484 min
Delta R.T.: -0.014 min
Response: 25106
Conc: 107.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

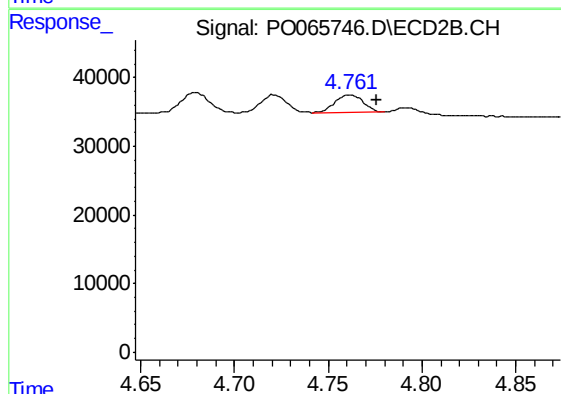


#14 AR-1232-4

R.T.: 4.761 min
Delta R.T.: -0.015 min
Response: 26884
Conc: 100.56 ng/ml

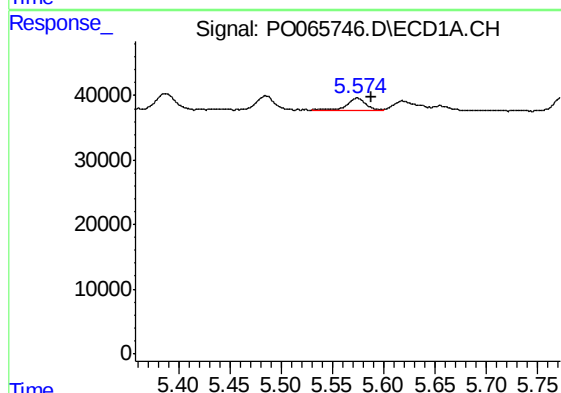


#15 AR-1232-5

R.T.: 5.574 min
Delta R.T.: -0.014 min
Response: 23347
Conc: 132.05 ng/ml

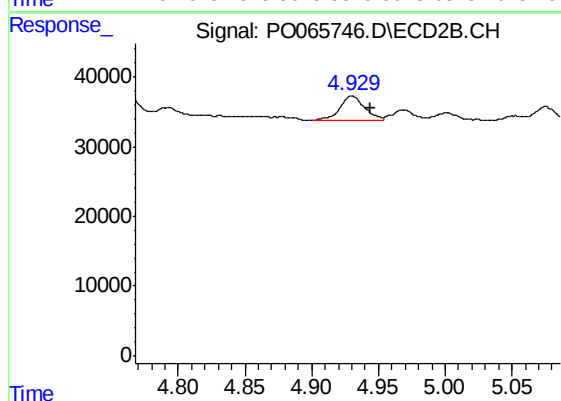

#15 AR-1232-5


R.T.: 4.930 min
Delta R.T.: -0.014 min
Response: 45732
Conc: 159.52 ng/ml



#16 AR-1242-1


R.T.: 5.306 min
Delta R.T.: -0.004 min
Response: 35268
Conc: 60.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020




#16 AR-1242-1

R.T.: 4.489 min
Delta R.T.: -0.001 min
Response: 46970
Conc: 68.91 ng/ml




#17 AR-1242-2

R.T.: 5.327 min
Delta R.T.: -0.003 min
Response: 51509
Conc: 60.24 ng/ml

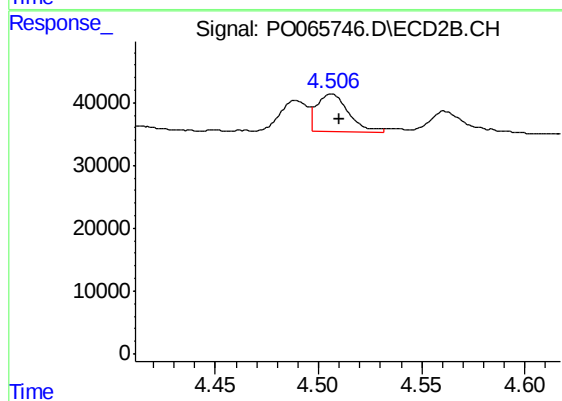

#17 AR-1242-2


R.T.: 4.506 min
Delta R.T.: -0.004 min
Response: 65389
Conc: 68.23 ng/ml

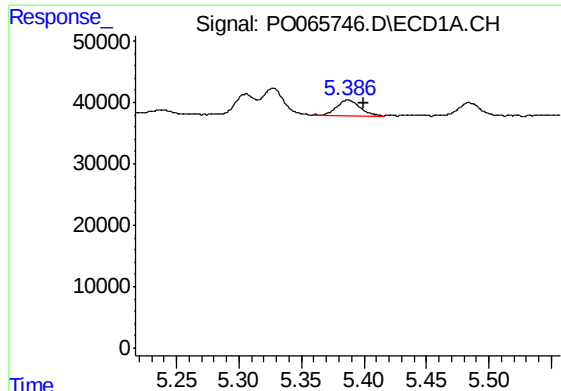

#18 AR-1242-3


R.T.: 5.387 min
Delta R.T.: -0.013 min
Response: 32777
Conc: 62.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

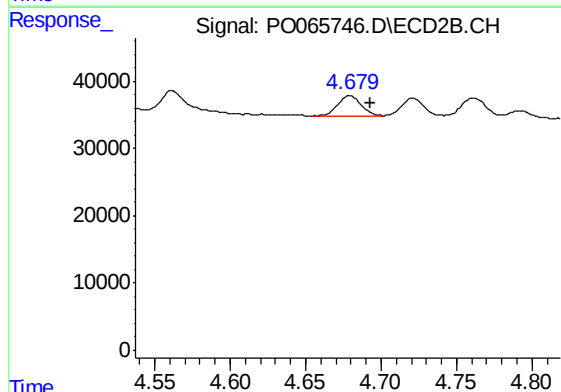


#18 AR-1242-3

R.T.: 4.679 min
Delta R.T.: -0.014 min
Response: 31075
Conc: 60.63 ng/ml

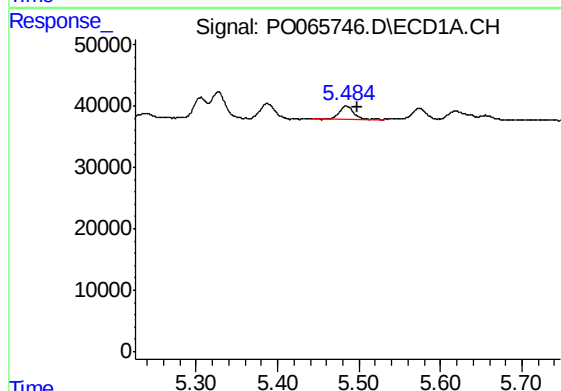


#19 AR-1242-4

R.T.: 5.484 min
Delta R.T.: -0.013 min
Response: 25106
Conc: 59.26 ng/ml

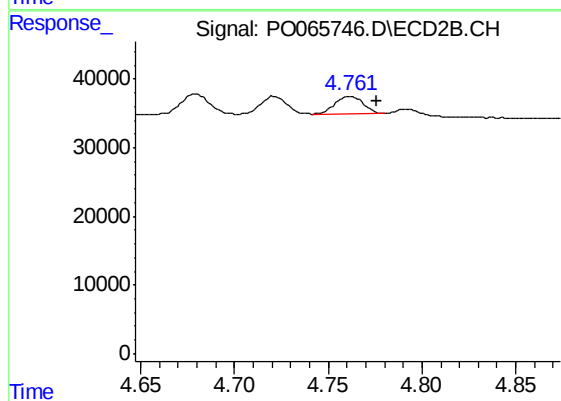

#19 AR-1242-4


R.T.: 4.761 min
Delta R.T.: -0.014 min
Response: 26884
Conc: 51.44 ng/ml



#20 AR-1242-5


R.T.: 6.212 min
Delta R.T.: -0.013 min
Response: 7216
Conc: 13.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020




#20 AR-1242-5

R.T.: 5.276 min
Delta R.T.: -0.016 min
Response: 23287
Conc: 32.04 ng/ml




#21 AR-1248-1

R.T.: 5.327 min
Delta R.T.: 0.008 min
Response: 51509
Conc: 110.70 ng/ml

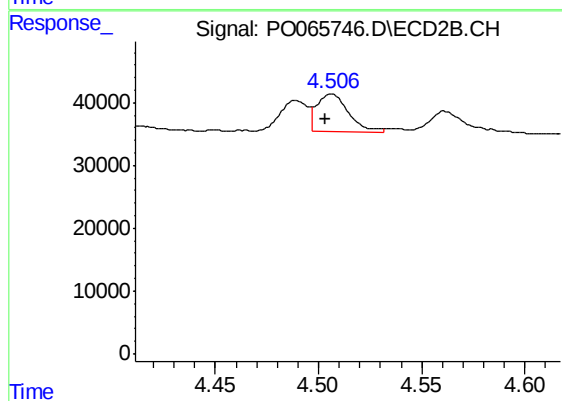

#21 AR-1248-1


R.T.: 4.506 min
Delta R.T.: 0.003 min
Response: 65389
Conc: 117.95 ng/ml



#22 AR-1248-2


R.T.: 5.574 min
Delta R.T.: -0.015 min
Response: 23347
Conc: 35.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020




#22 AR-1248-2

R.T.: 4.721 min
Delta R.T.: -0.015 min
Response: 25758
Conc: 33.57 ng/ml




#23 AR-1248-3

R.T.: 5.775 min
Delta R.T.: -0.015 min
Response: 25711
Conc: 34.12 ng/ml

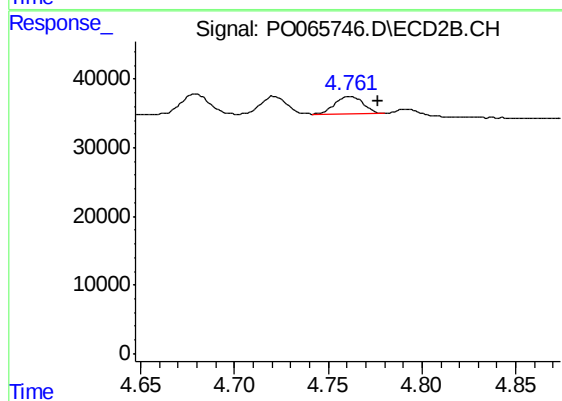

#23 AR-1248-3


R.T.: 4.761 min
Delta R.T.: -0.015 min
Response: 26884
Conc: 34.17 ng/ml

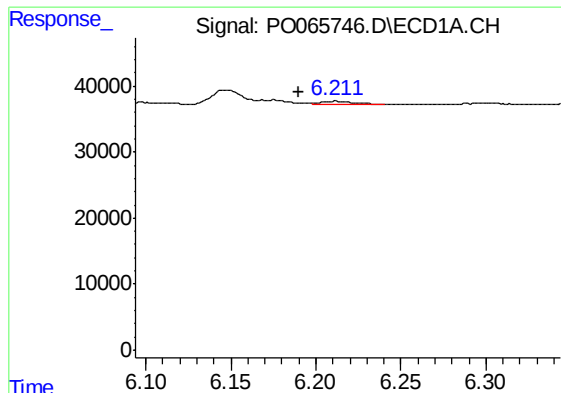

#24 AR-1248-4


R.T.: 6.212 min
Delta R.T.: 0.022 min
Response: 7216
Conc: 7.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

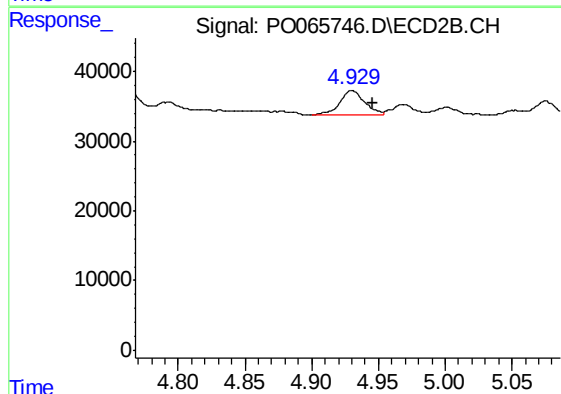


#24 AR-1248-4

R.T.: 4.930 min
Delta R.T.: -0.016 min
Response: 45732
Conc: 47.71 ng/ml

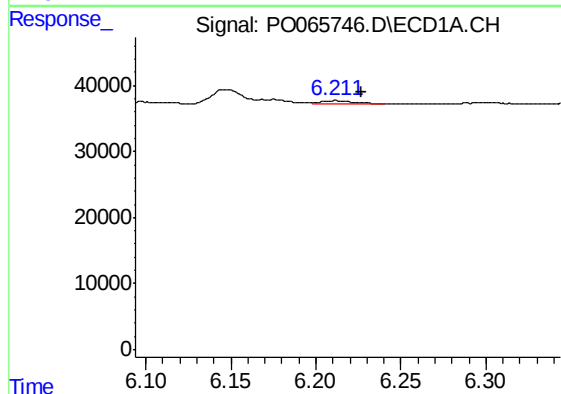


#25 AR-1248-5

R.T.: 6.212 min
Delta R.T.: -0.015 min
Response: 7216
Conc: 7.89 ng/ml

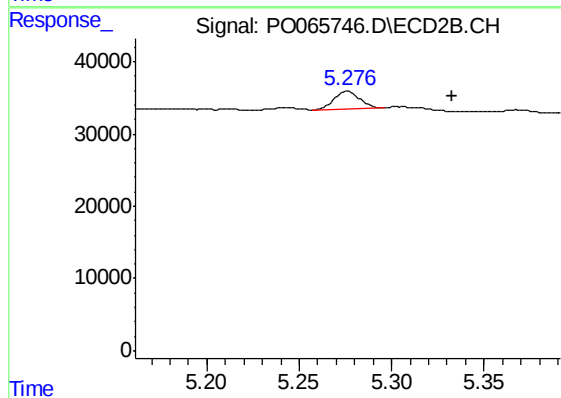

#25 AR-1248-5


R.T.: 5.276 min
Delta R.T.: -0.057 min
Response: 23287
Conc: 23.00 ng/ml



#26 AR-1254-1


R.T.: 6.148 min
Delta R.T.: -0.014 min
Response: 37726
Conc: 44.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020




#26 AR-1254-1

R.T.: 5.276 min
Delta R.T.: -0.016 min
Response: 23287
Conc: 16.07 ng/ml




#27 AR-1254-2

R.T.: 6.362 min
Delta R.T.: -0.016 min
Response: 24650
Conc: 17.94 ng/ml

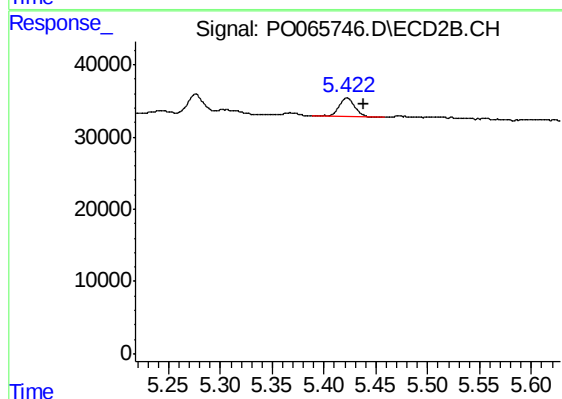

#27 AR-1254-2


R.T.: 5.422 min
Delta R.T.: -0.017 min
Response: 28607
Conc: 21.63 ng/ml

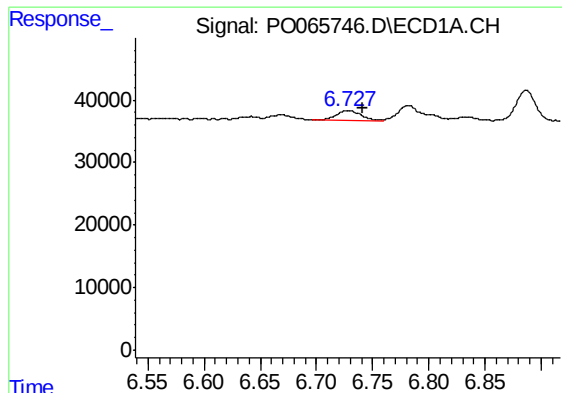

#28 AR-1254-3


R.T.: 6.728 min
Delta R.T.: -0.013 min
Response: 25645
Conc: 16.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

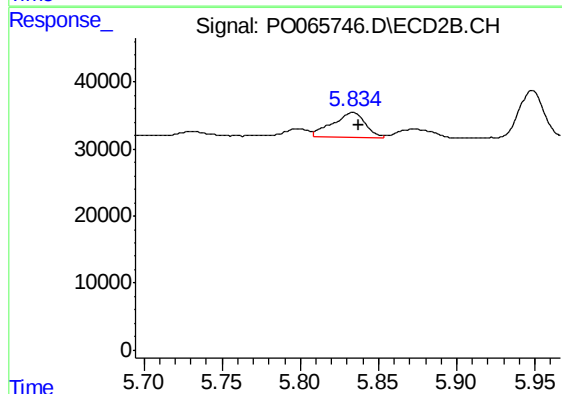


#28 AR-1254-3

R.T.: 5.834 min
Delta R.T.: -0.003 min
Response: 54593
Conc: 24.23 ng/ml

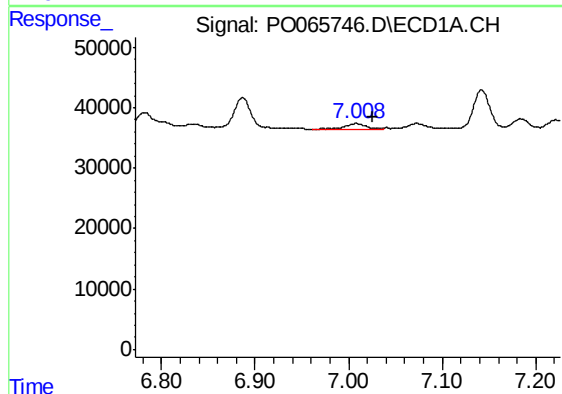


#29 AR-1254-4

R.T.: 7.008 min
Delta R.T.: -0.018 min
Response: 19256
Conc: 15.11 ng/ml

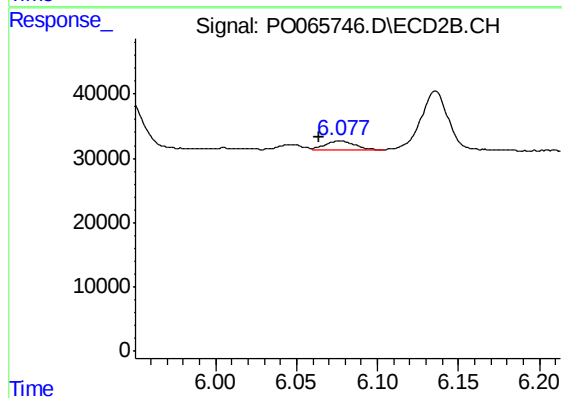

#29 AR-1254-4


R.T.: 6.077 min
Delta R.T.: 0.013 min
Response: 17174
Conc: 11.39 ng/ml

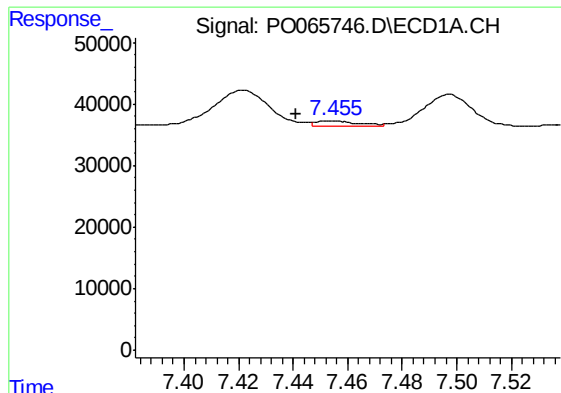

#30 AR-1254-5


R.T.: 7.454 min
Delta R.T.: 0.014 min
Response: 10001
Conc: 7.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

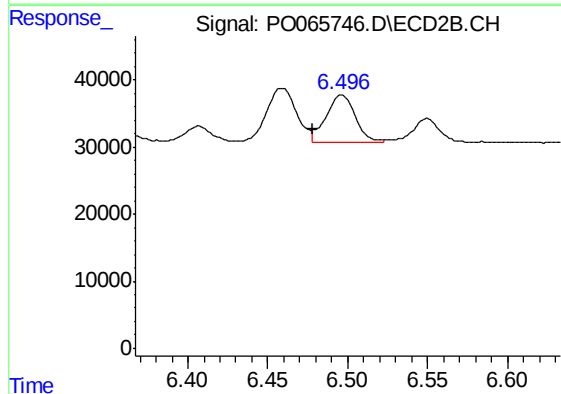


#30 AR-1254-5

R.T.: 6.496 min
Delta R.T.: 0.018 min
Response: 88255
Conc: 39.65 ng/ml

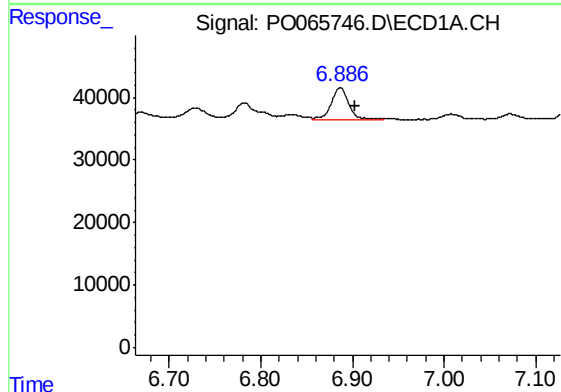


#31 AR-1260-1

R.T.: 6.887 min
Delta R.T.: -0.016 min
Response: 68780
Conc: 49.87 ng/ml

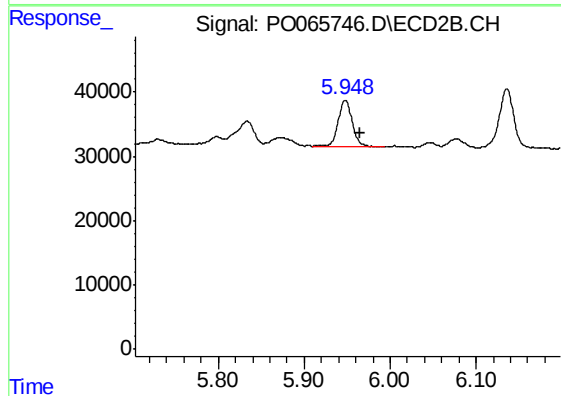

#31 AR-1260-1


R.T.: 5.948 min
Delta R.T.: -0.017 min
Response: 81398
Conc: 43.24 ng/ml



#32 AR-1260-2


R.T.: 7.142 min
Delta R.T.: -0.018 min
Response: 82784
Conc: 47.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

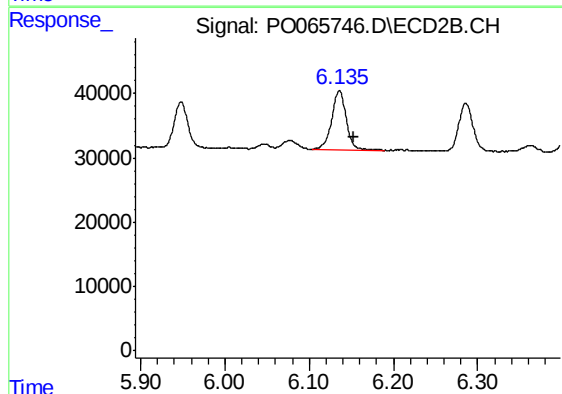


#32 AR-1260-2

R.T.: 6.136 min
Delta R.T.: -0.017 min
Response: 111029
Conc: 45.70 ng/ml

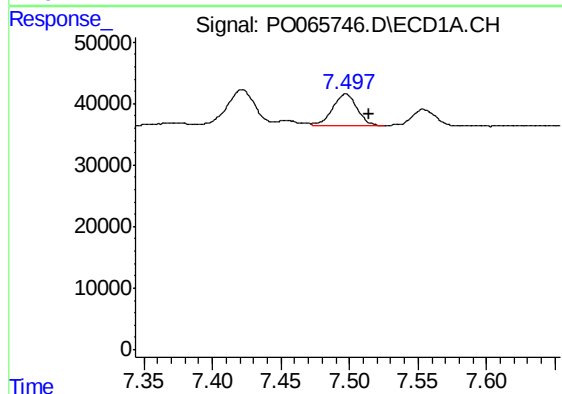


#33 AR-1260-3

R.T.: 7.497 min
Delta R.T.: -0.017 min
Response: 65387
Conc: 46.26 ng/ml

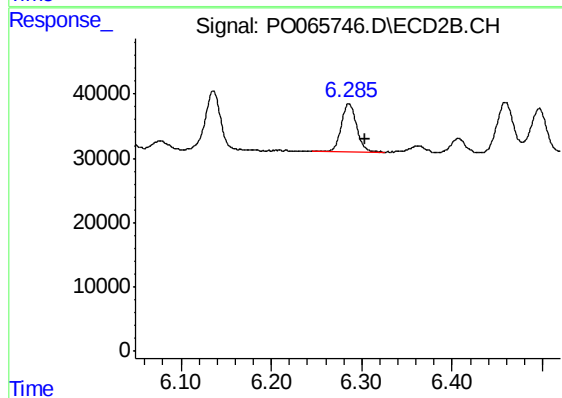

#33 AR-1260-3


R.T.: 6.286 min
Delta R.T.: -0.018 min
Response: 87972
Conc: 40.64 ng/ml

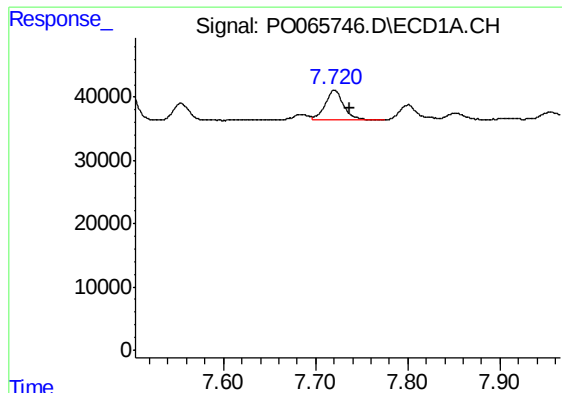

#34 AR-1260-4


R.T.: 7.720 min
Delta R.T.: -0.017 min
Response: 66435
Conc: 38.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

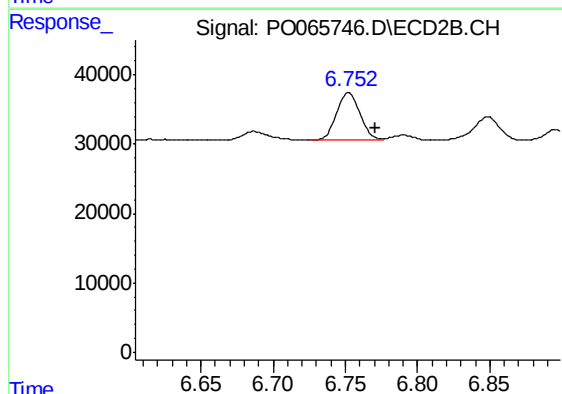


#34 AR-1260-4

R.T.: 6.752 min
Delta R.T.: -0.019 min
Response: 77992
Conc: 38.88 ng/ml

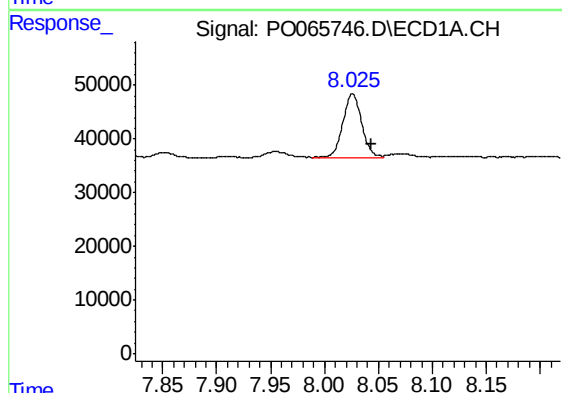


#35 AR-1260-5

R.T.: 8.026 min
Delta R.T.: -0.018 min
Response: 143993
Conc: 42.94 ng/ml

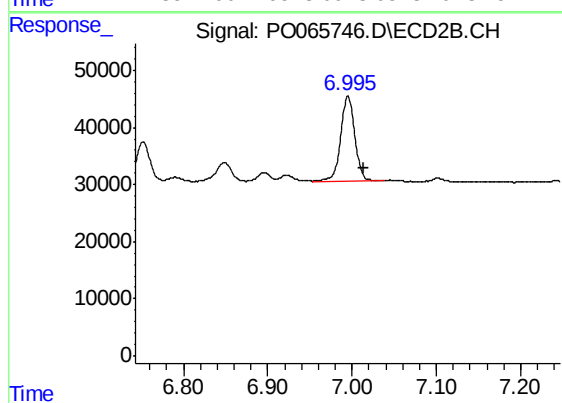

#35 AR-1260-5


R.T.: 6.995 min
Delta R.T.: -0.019 min
Response: 174248
Conc: 35.20 ng/ml



#36 AR-1262-1


R.T.: 7.497 min
Delta R.T.: -0.018 min
Response: 65387
Conc: 39.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020




#36 AR-1262-1

R.T.: 6.550 min
Delta R.T.: -0.018 min
Response: 42271
Conc: 44.84 ng/ml

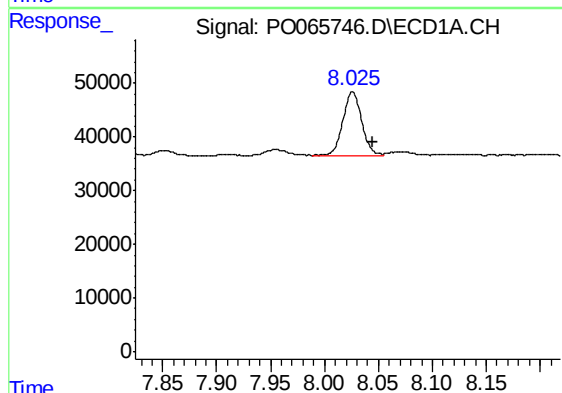


#37 AR-1262-2

R.T.: 8.026 min
Delta R.T.: -0.019 min
Response: 143993
Conc: 44.96 ng/ml

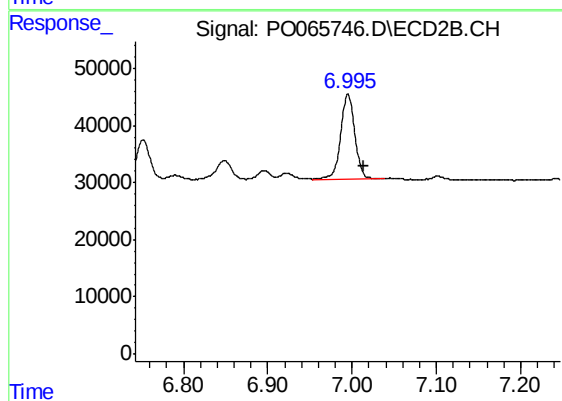

#37 AR-1262-2


R.T.: 6.995 min
Delta R.T.: -0.019 min
Response: 174248
Conc: 38.78 ng/ml

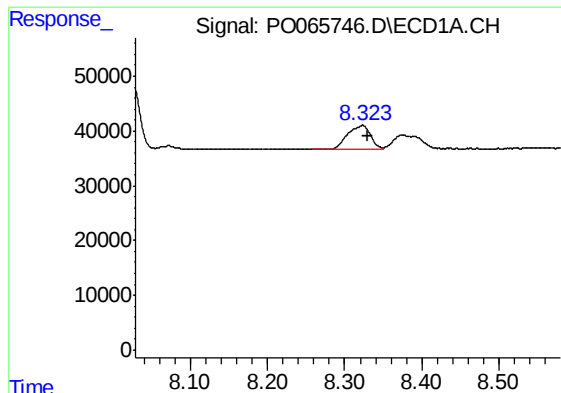

#38 AR-1262-3


R.T.: 8.323 min
Delta R.T.: -0.007 min
Response: 89873
Conc: 39.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

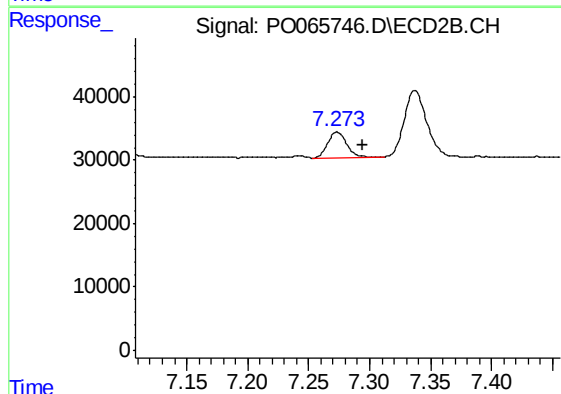


#38 AR-1262-3

R.T.: 7.273 min
Delta R.T.: -0.021 min
Response: 44799
Conc: 26.62 ng/ml

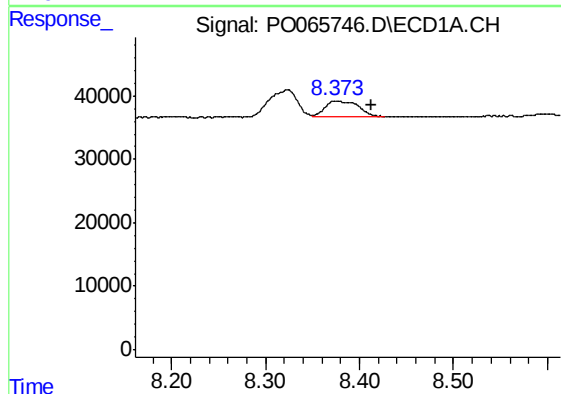


#39 AR-1262-4

R.T.: 8.374 min
Delta R.T.: -0.038 min
Response: 62602
Conc: 35.41 ng/ml

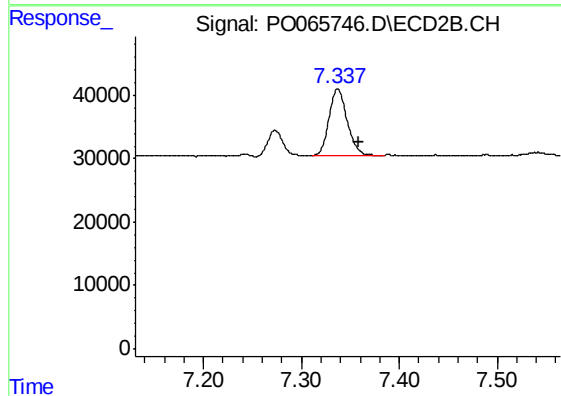

#39 AR-1262-4


R.T.: 7.337 min
Delta R.T.: -0.021 min
Response: 136190
Conc: 39.60 ng/ml



#40 AR-1262-5


R.T.: 8.986 min
Delta R.T.: -0.024 min
Response: 47873
Conc: 35.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020




#40 AR-1262-5

R.T.: 7.830 min
Delta R.T.: -0.021 min
Response: 50011
Conc: 29.33 ng/ml




#41 AR-1268-1

R.T.: 8.323 min
Delta R.T.: -0.004 min
Response: 89873
Conc: 22.09 ng/ml

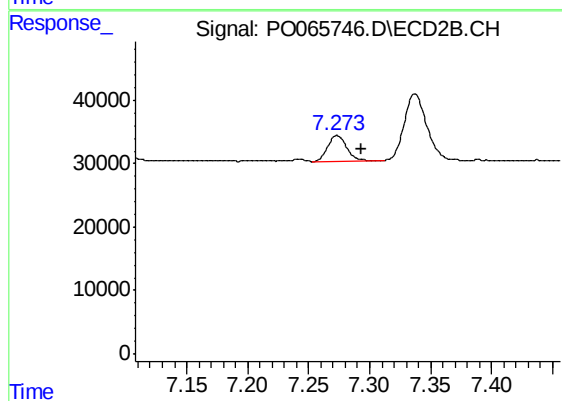

#41 AR-1268-1


R.T.: 7.273 min
Delta R.T.: -0.020 min
Response: 44799
Conc: 8.44 ng/ml



#42 AR-1268-2


R.T.: 8.374 min
Delta R.T.: -0.040 min
Response: 62602
Conc: 16.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020




#42 AR-1268-2

R.T.: 7.337 min
Delta R.T.: -0.021 min
Response: 136190
Conc: 26.81 ng/ml

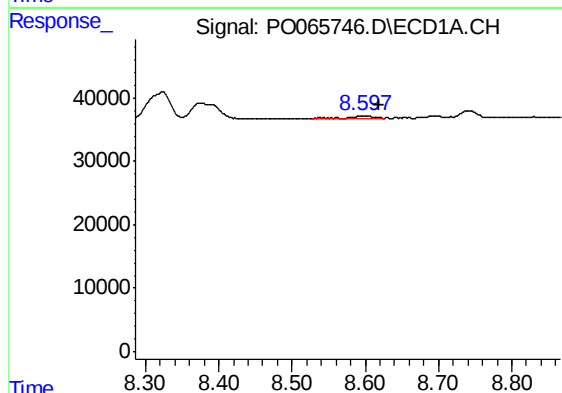


#43 AR-1268-3

R.T.: 8.597 min
Delta R.T.: -0.022 min
Response: 9968
Conc: 3.10 ng/ml

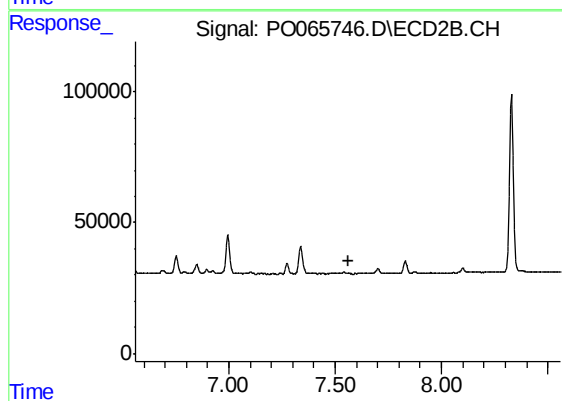

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 7.560 min
Response: 0
Conc: N.D.



#44 AR-1268-4


R.T.: 8.986 min
Delta R.T.: -0.024 min
Response: 47873
Conc: 31.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

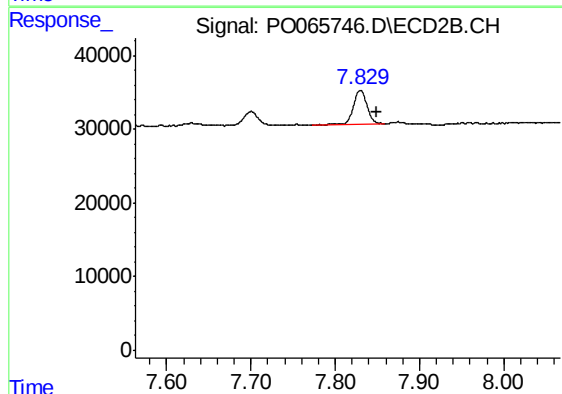


#44 AR-1268-4

R.T.: 7.830 min
Delta R.T.: -0.020 min
Response: 50011
Conc: 25.27 ng/ml



#45 AR-1268-5

R.T.: 9.353 min
Delta R.T.: -0.027 min
Response: 21159
Conc: 1.91 ng/ml

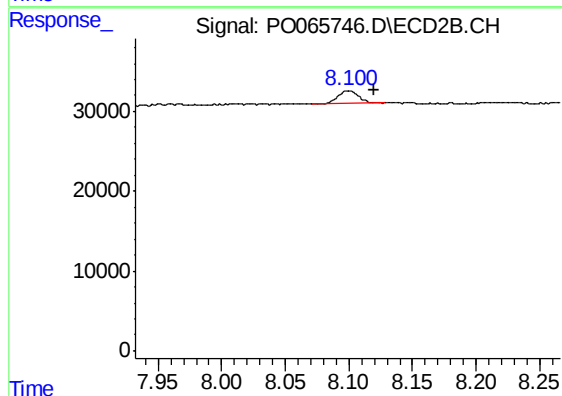

#45 AR-1268-5

R.T.: 8.100 min
Delta R.T.: -0.020 min
Response: 18387
Conc: 1.28 ng/ml