

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012120\
 Data File : P0065716.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jan 2020 17:13
 Operator : DD\AJ
 Sample : L1161-07
 Misc : AR1254 LOD 25 PPB
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2020

Manual Integrations
 APPROVED

mohammad
 1/22/2020 3:26:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 04:21:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.155	3.431	400865	489214	21.953	22.240
2) SA Decachlor...	9.652	8.331	743184	882709	21.934	21.285
Target Compounds						
26) L6 AR-1254-1	6.146	5.277	32844	57191	38.716m	39.477
27) L6 AR-1254-2	6.363	5.423	53787	54355	39.141	41.093
28) L6 AR-1254-3	6.726	5.821	64890	77723	41.867	34.489
29) L6 AR-1254-4	7.009	6.048	48680	53576	38.189	35.537
30) L6 AR-1254-5	7.424	6.461	49100	76460	34.964m	34.350

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012120\
Data File : PO065716.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jan 2020 17:13
Operator : DD\AJ
Sample : L1161-07
Misc : AR1254 LOD 25 PPB
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020


Manual Integrations
APPROVED

mohammad
1/22/2020 3:26:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 04:21:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

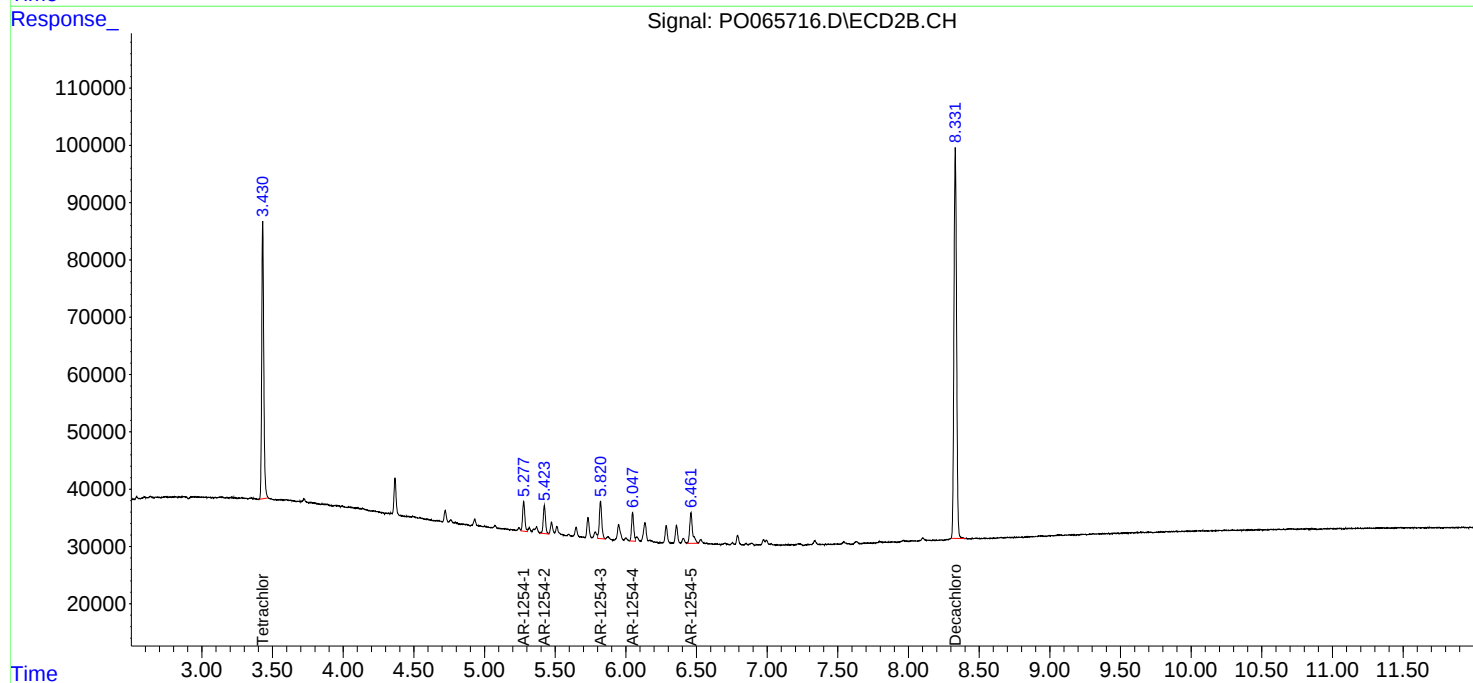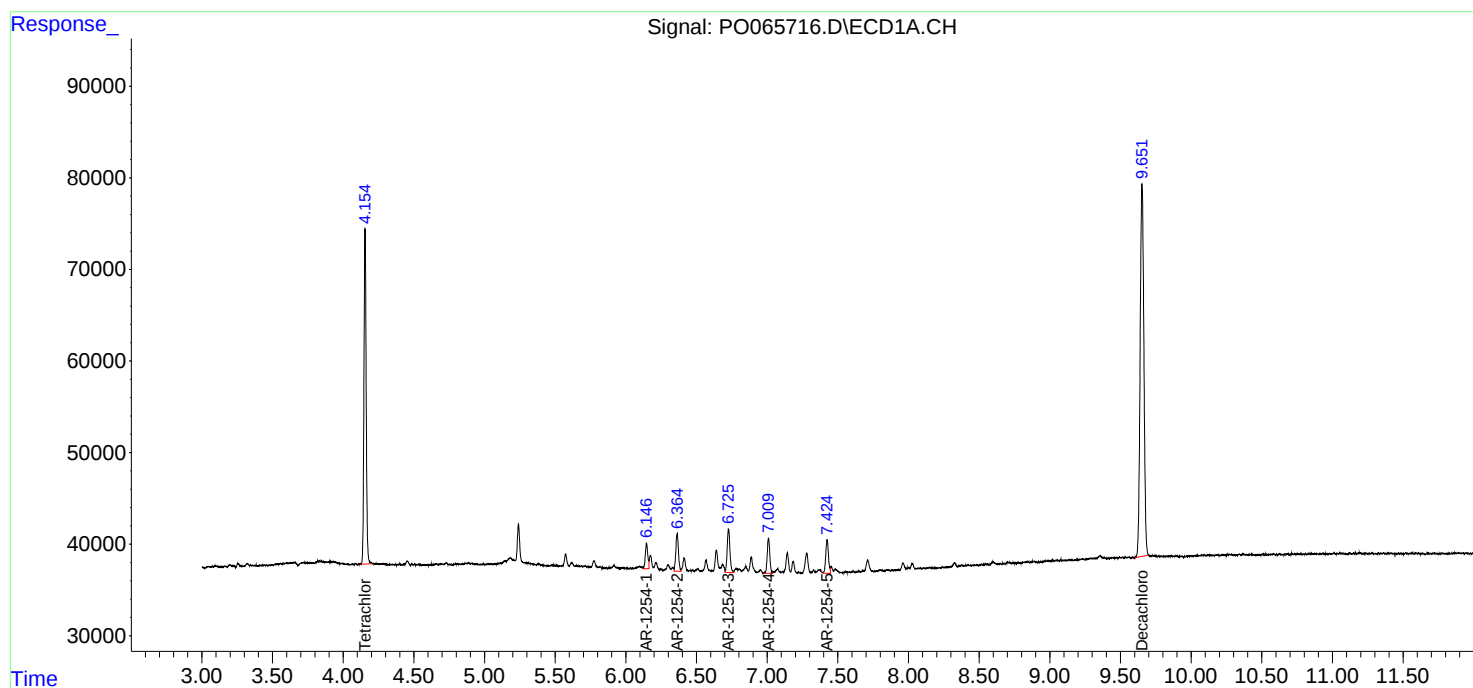

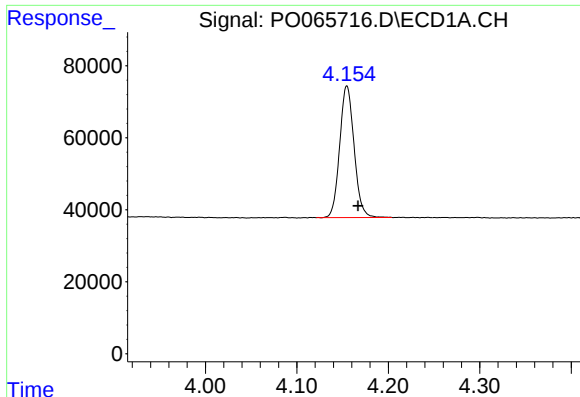


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: -0.012 min
Response: 400865
Conc: 21.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020


Manual Integrations
APPROVED

mohammad
1/22/2020 3:26:35 PM

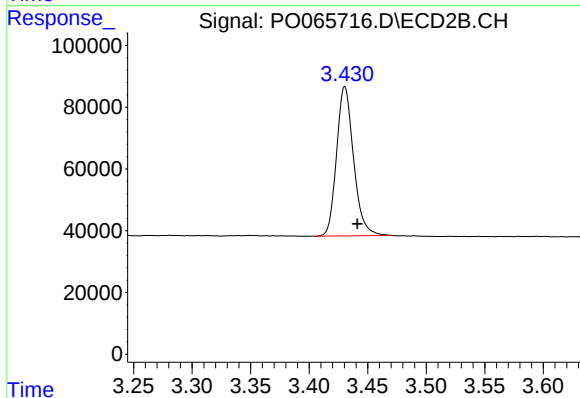


#1 Tetrachloro-m-xylene

R.T.: 3.431 min
Delta R.T.: -0.011 min
Response: 489214
Conc: 22.24 ng/ml

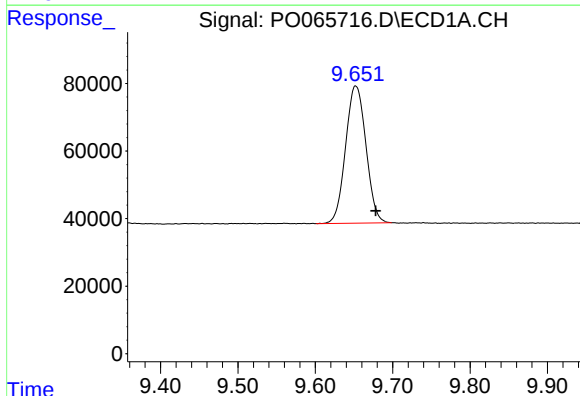


#2 Decachlorobiphenyl

R.T.: 9.652 min
Delta R.T.: -0.026 min
Response: 743184
Conc: 21.93 ng/ml

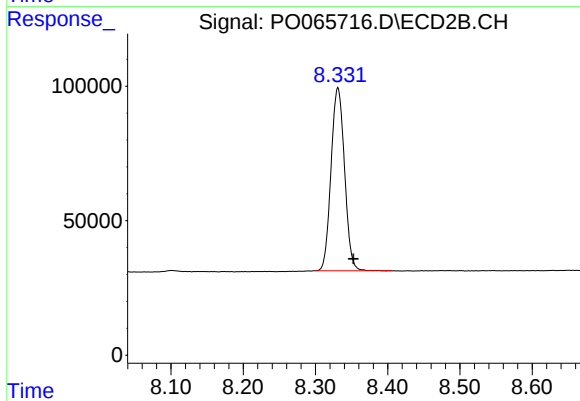

#2 Decachlorobiphenyl

R.T.: 8.331 min
Delta R.T.: -0.021 min
Response: 882709
Conc: 21.29 ng/ml

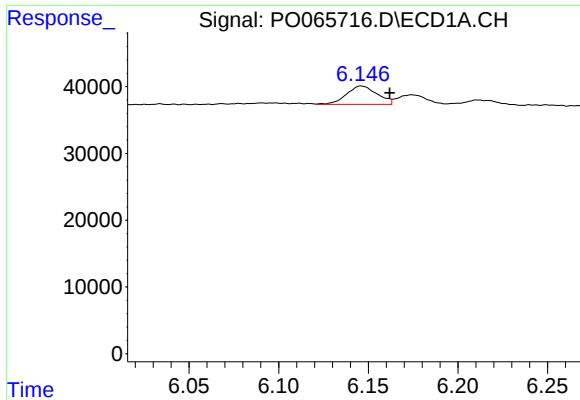


#26 AR-1254-1

R.T.: 6.146 min
Delta R.T.: -0.016 min
Response: 32844
Conc: 38.72 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020


Manual Integrations
APPROVED

mohammad
1/22/2020 3:26:35 PM

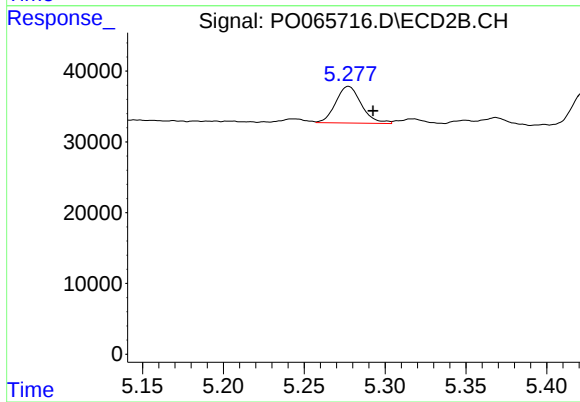


#26 AR-1254-1

R.T.: 5.277 min
Delta R.T.: -0.015 min
Response: 57191
Conc: 39.48 ng/ml

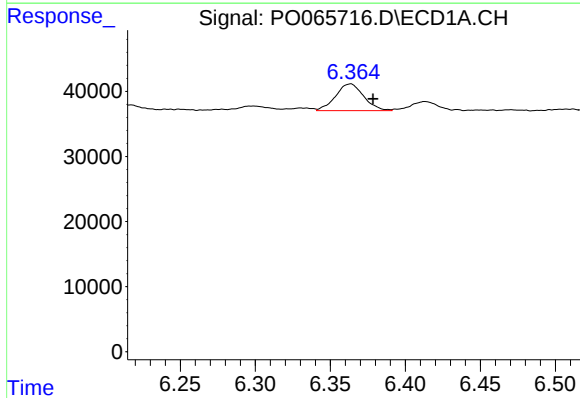


#27 AR-1254-2

R.T.: 6.363 min
Delta R.T.: -0.015 min
Response: 53787
Conc: 39.14 ng/ml

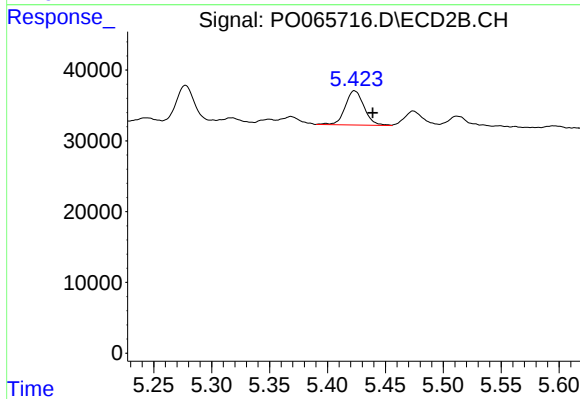

#27 AR-1254-2

R.T.: 5.423 min
Delta R.T.: -0.016 min
Response: 54355
Conc: 41.09 ng/ml

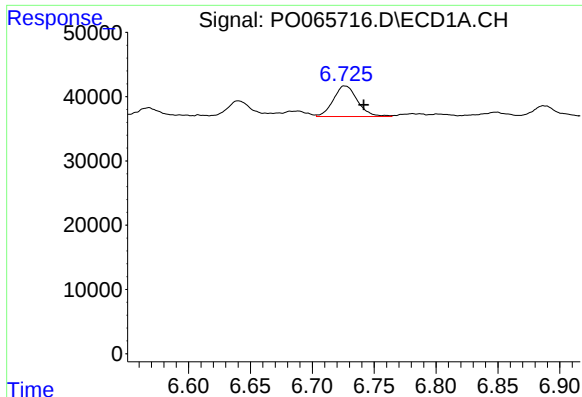


#28 AR-1254-3

R.T.: 6.726 min
Delta R.T.: -0.015 min
Response: 64890
Conc: 41.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020


Manual Integrations
APPROVED

mohammad
1/22/2020 3:26:35 PM

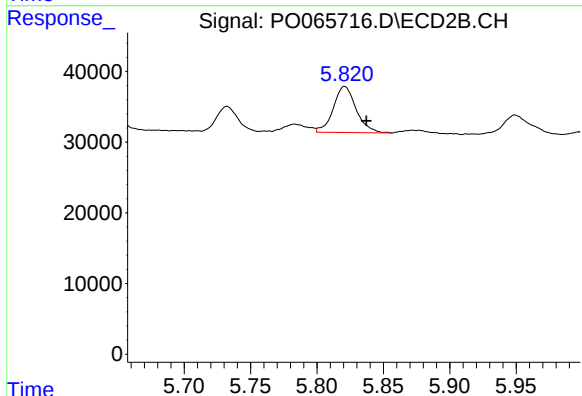


#28 AR-1254-3

R.T.: 5.821 min
Delta R.T.: -0.016 min
Response: 77723
Conc: 34.49 ng/ml

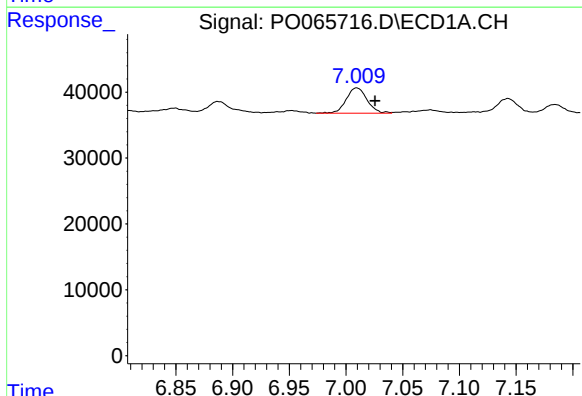


#29 AR-1254-4

R.T.: 7.009 min
Delta R.T.: -0.016 min
Response: 48680
Conc: 38.19 ng/ml

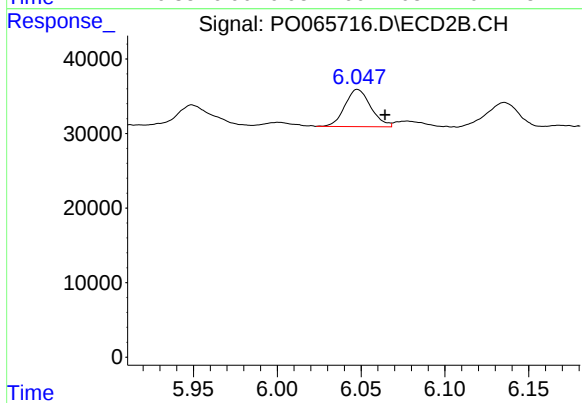

#29 AR-1254-4

R.T.: 6.048 min
Delta R.T.: -0.016 min
Response: 53576
Conc: 35.54 ng/ml

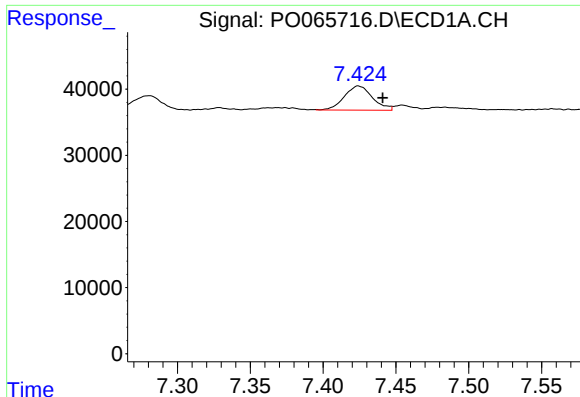


#30 AR-1254-5

R.T.: 7.424 min
Delta R.T.: -0.017 min
Response: 49100
Conc: 34.96 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

Manual Integrations
APPROVED

mohammad
1/22/2020 3:26:35 PM

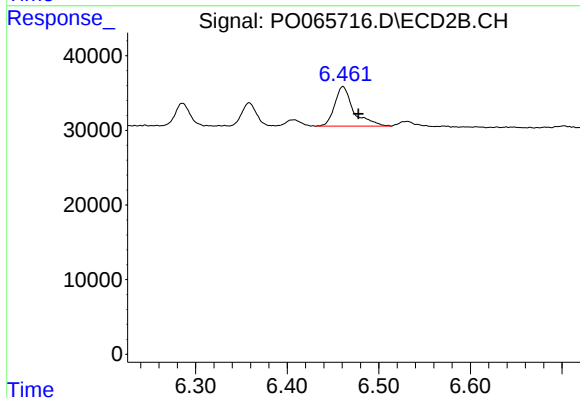

#30 AR-1254-5

R.T.: 6.461 min
Delta R.T.: -0.017 min
Response: 76460
Conc: 34.35 ng/ml