

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012120\
 Data File : P0065750.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jan 2020 3:33
 Operator : DD\AJ
 Sample : L1161-07
 Misc : AR1248 LOD 40 PPB
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2020

Manual Integrations
 APPROVED

mohammad
 1/22/2020 3:27:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 07:11:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.154	3.430	404146	483348	22.132	21.973
2) SA Decachlor...	9.651	8.329	735469	877525	21.706	21.160
Target Compounds						
21) L5 AR-1248-1	5.305	4.488	23186	28084	49.829m	50.660m
22) L5 AR-1248-2	5.574	4.721	32345	41676	49.018	54.319
23) L5 AR-1248-3	5.774	4.761	36447	38589	48.372	49.046m
24) L5 AR-1248-4	6.174	4.930	49366	50162	52.114	52.333
25) L5 AR-1248-5	6.211	5.316	45675	45863	49.933	45.306

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012120\
Data File : PO065750.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2020 3:33
Operator : DD\AJ
Sample : L1161-07
Misc : AR1248 LOD 40 PPB
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020


Manual Integrations
APPROVED

mohammad
1/22/2020 3:27:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 07:11:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

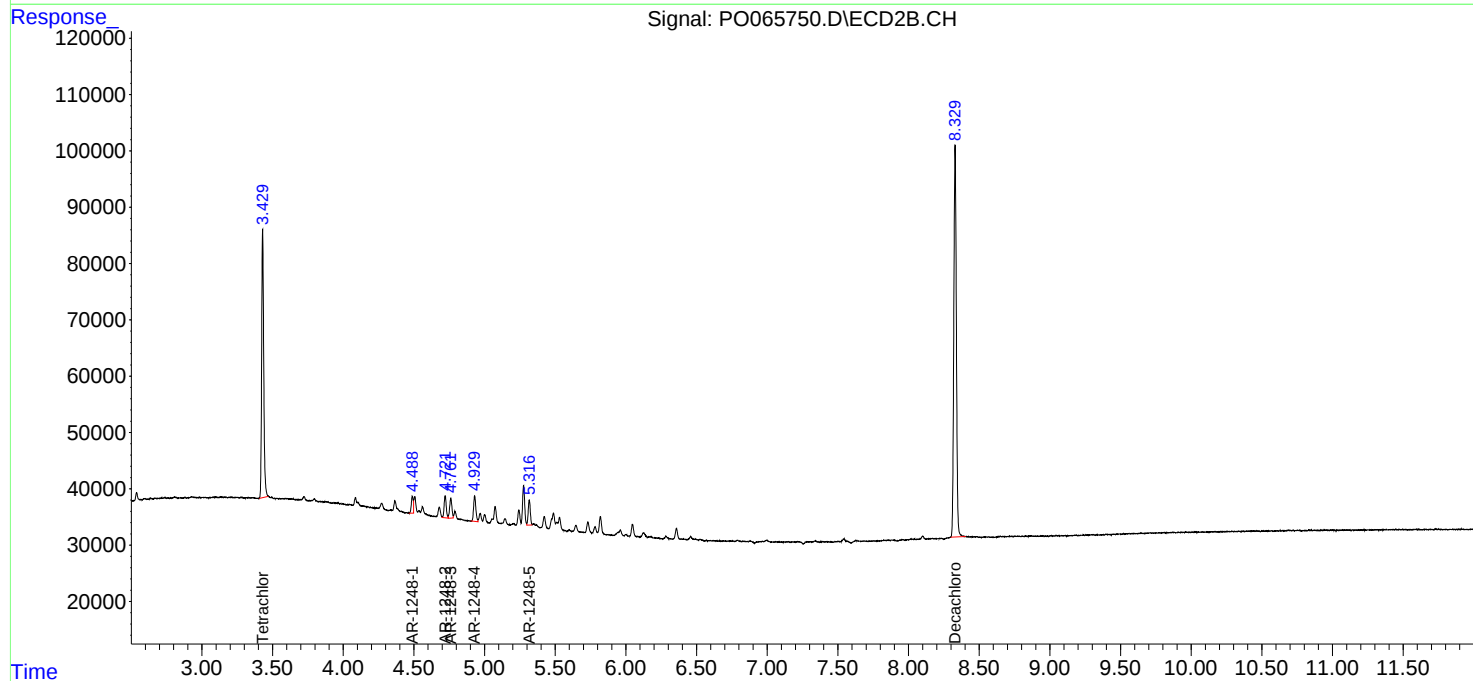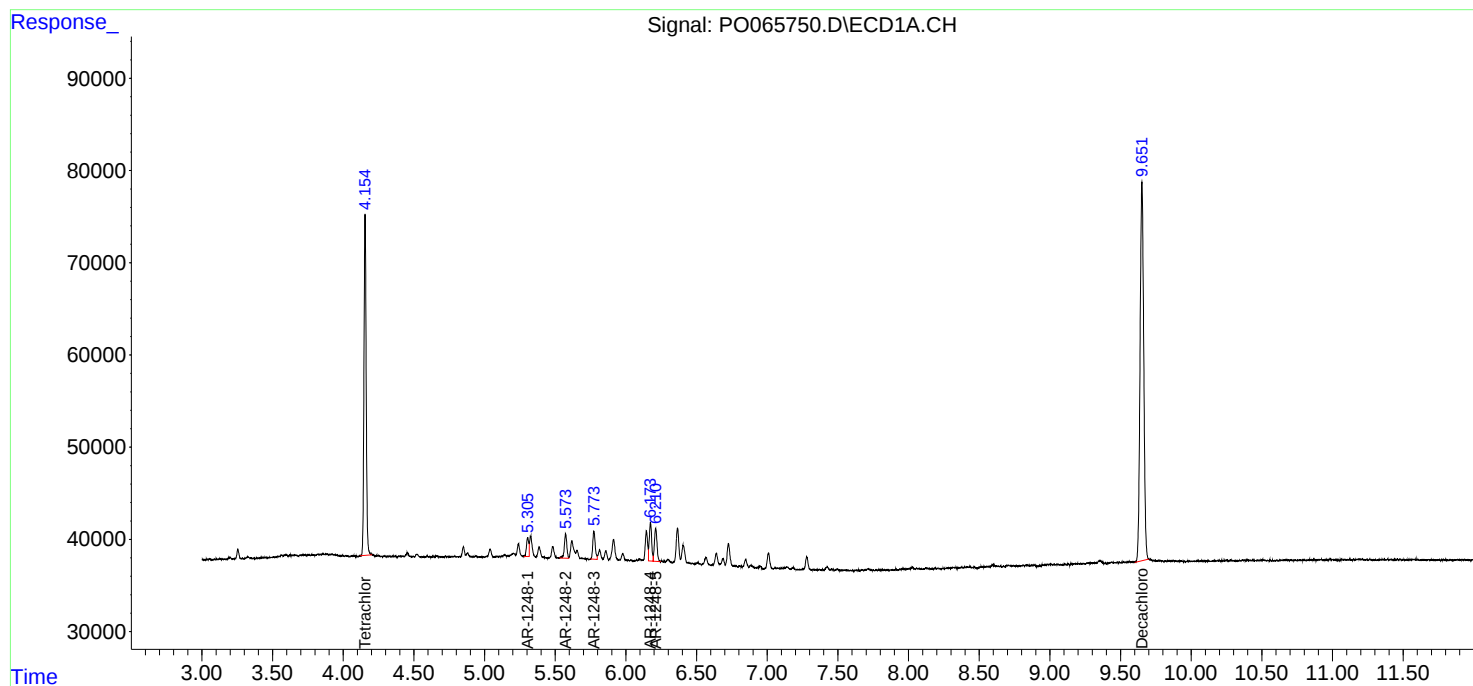

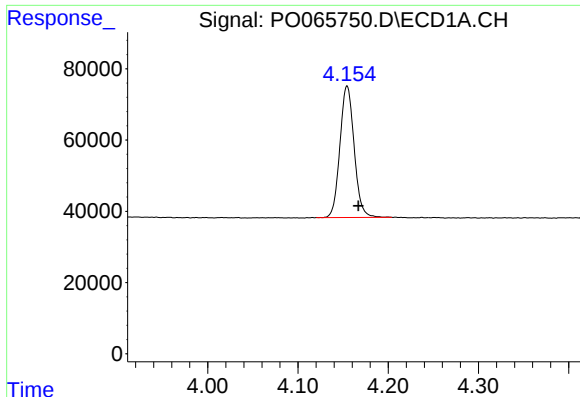


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: -0.013 min
Response: 404146
Conc: 22.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020


Manual Integrations
APPROVED

mohammad
1/22/2020 3:27:41 PM

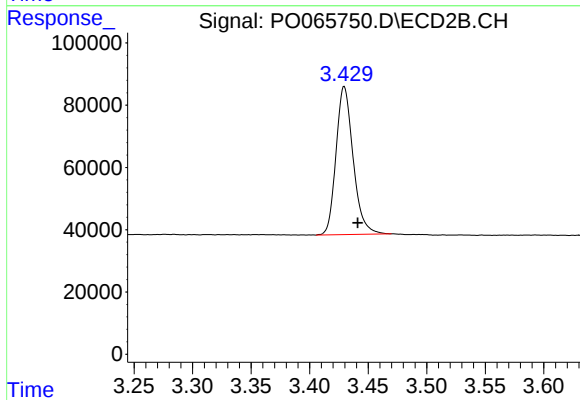


#1 Tetrachloro-m-xylene

R.T.: 3.430 min
Delta R.T.: -0.011 min
Response: 483348
Conc: 21.97 ng/ml

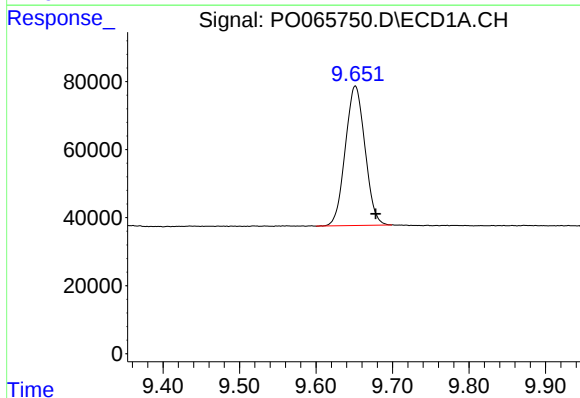


#2 Decachlorobiphenyl

R.T.: 9.651 min
Delta R.T.: -0.027 min
Response: 735469
Conc: 21.71 ng/ml

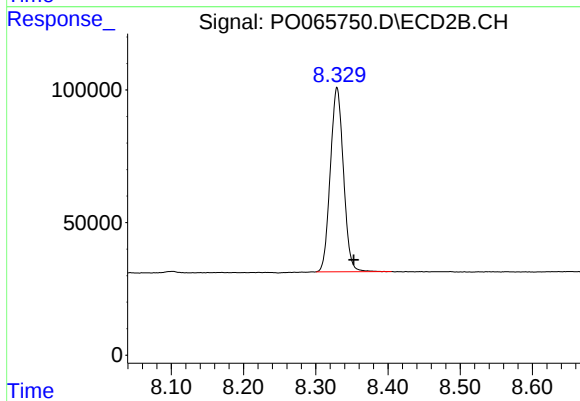

#2 Decachlorobiphenyl

R.T.: 8.329 min
Delta R.T.: -0.023 min
Response: 877525
Conc: 21.16 ng/ml

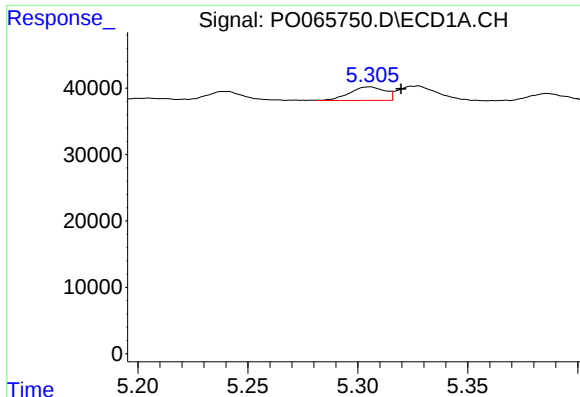


#21 AR-1248-1

R.T.: 5.305 min
Delta R.T.: -0.014 min
Response: 23186
Conc: 49.83 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020


Manual Integrations
APPROVED

mohammad
1/22/2020 3:27:41 PM

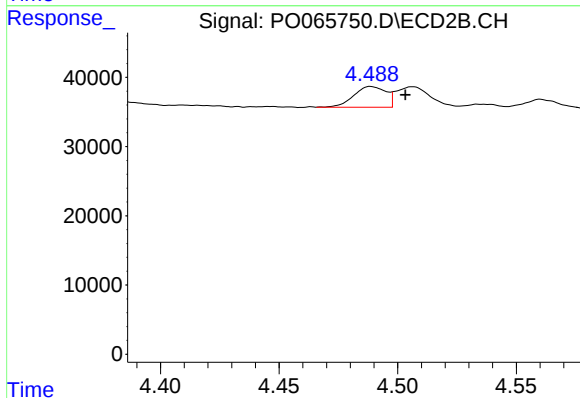


#21 AR-1248-1

R.T.: 4.488 min
Delta R.T.: -0.015 min
Response: 28084
Conc: 50.66 ng/ml m

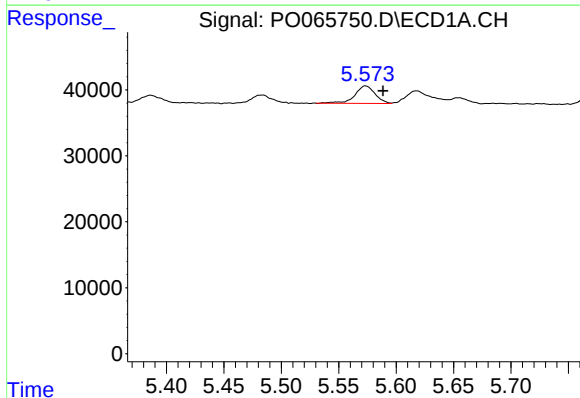


#22 AR-1248-2

R.T.: 5.574 min
Delta R.T.: -0.015 min
Response: 32345
Conc: 49.02 ng/ml

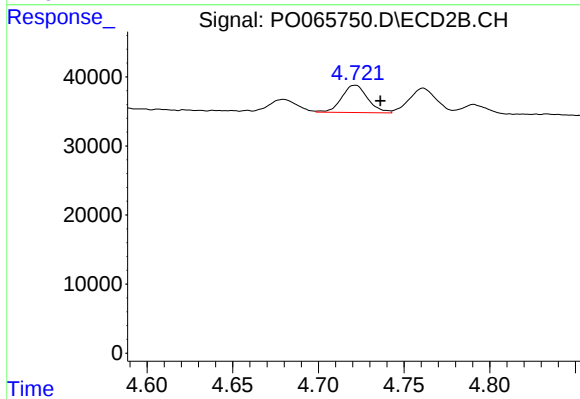

#22 AR-1248-2

R.T.: 4.721 min
Delta R.T.: -0.015 min
Response: 41676
Conc: 54.32 ng/ml

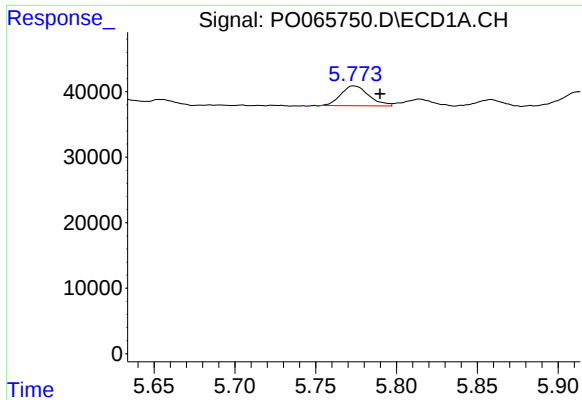


#23 AR-1248-3

R.T.: 5.774 min
Delta R.T.: -0.016 min
Response: 36447
Conc: 48.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020


Manual Integrations
APPROVED

mohammad
1/22/2020 3:27:41 PM

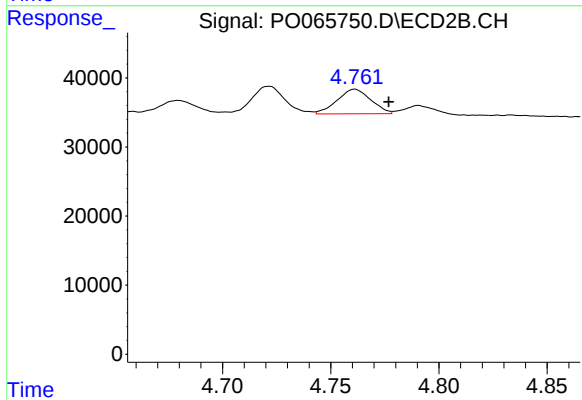


#23 AR-1248-3

R.T.: 4.761 min
Delta R.T.: -0.016 min
Response: 38589
Conc: 49.05 ng/ml m

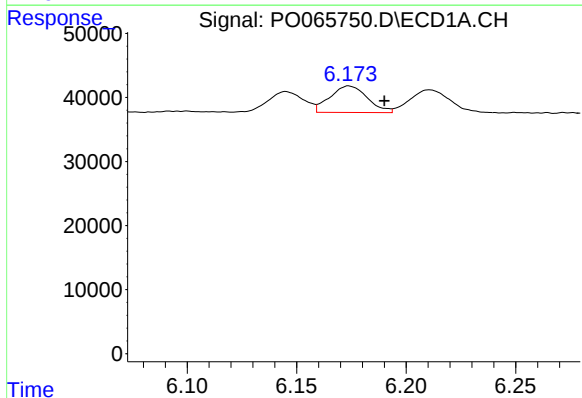


#24 AR-1248-4

R.T.: 6.174 min
Delta R.T.: -0.016 min
Response: 49366
Conc: 52.11 ng/ml

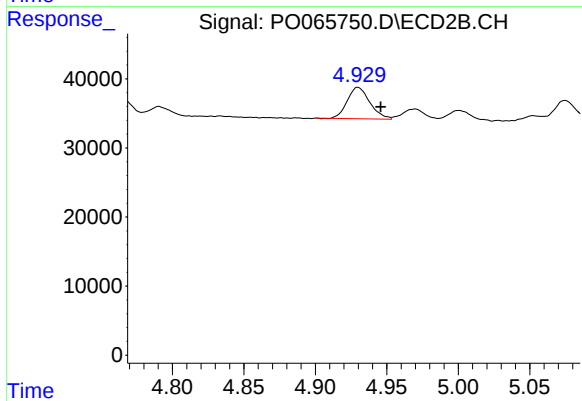

#24 AR-1248-4

R.T.: 4.930 min
Delta R.T.: -0.016 min
Response: 50162
Conc: 52.33 ng/ml

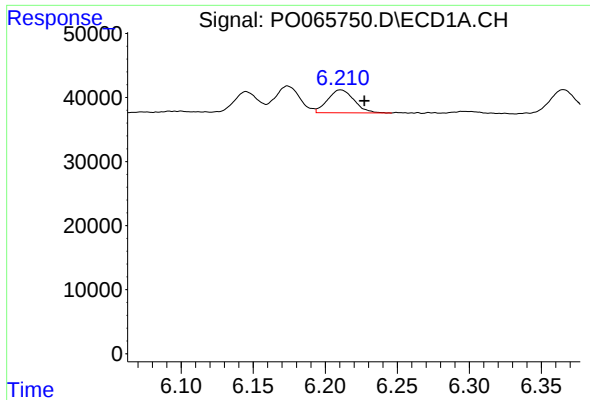


#25 AR-1248-5

R.T.: 6.211 min
Delta R.T.: -0.016 min
Response: 45675
Conc: 49.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

Manual Integrations
APPROVED

mohammad
1/22/2020 3:27:41 PM

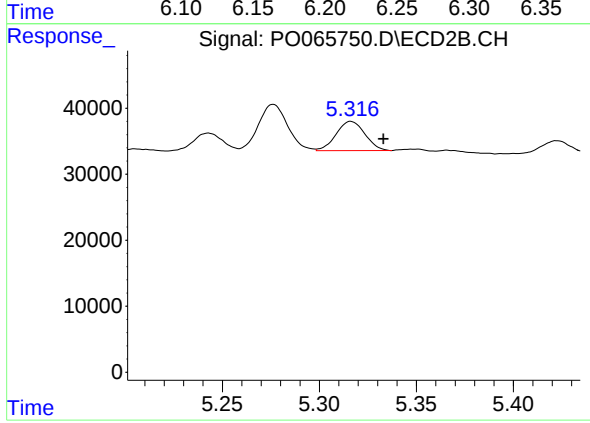

#25 AR-1248-5

R.T.: 5.316 min
Delta R.T.: -0.017 min
Response: 45863
Conc: 45.31 ng/ml