

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012120\
 Data File : P0065761.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jan 2020 7:27
 Operator : DD\AJ
 Sample : L1173-03
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 0052-DECANT-H2O-COMP-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 10:38:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.155	3.431	483514	587764	26.479	26.720
2) SA Decachlor...	9.650	8.329	671327	784579	19.813	18.919

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012120\
Data File : P0065761.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2020 7:27
Operator : DD\AJ
Sample : L1173-03
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
0052-DECANT-H2O-COMP-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 10:38:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

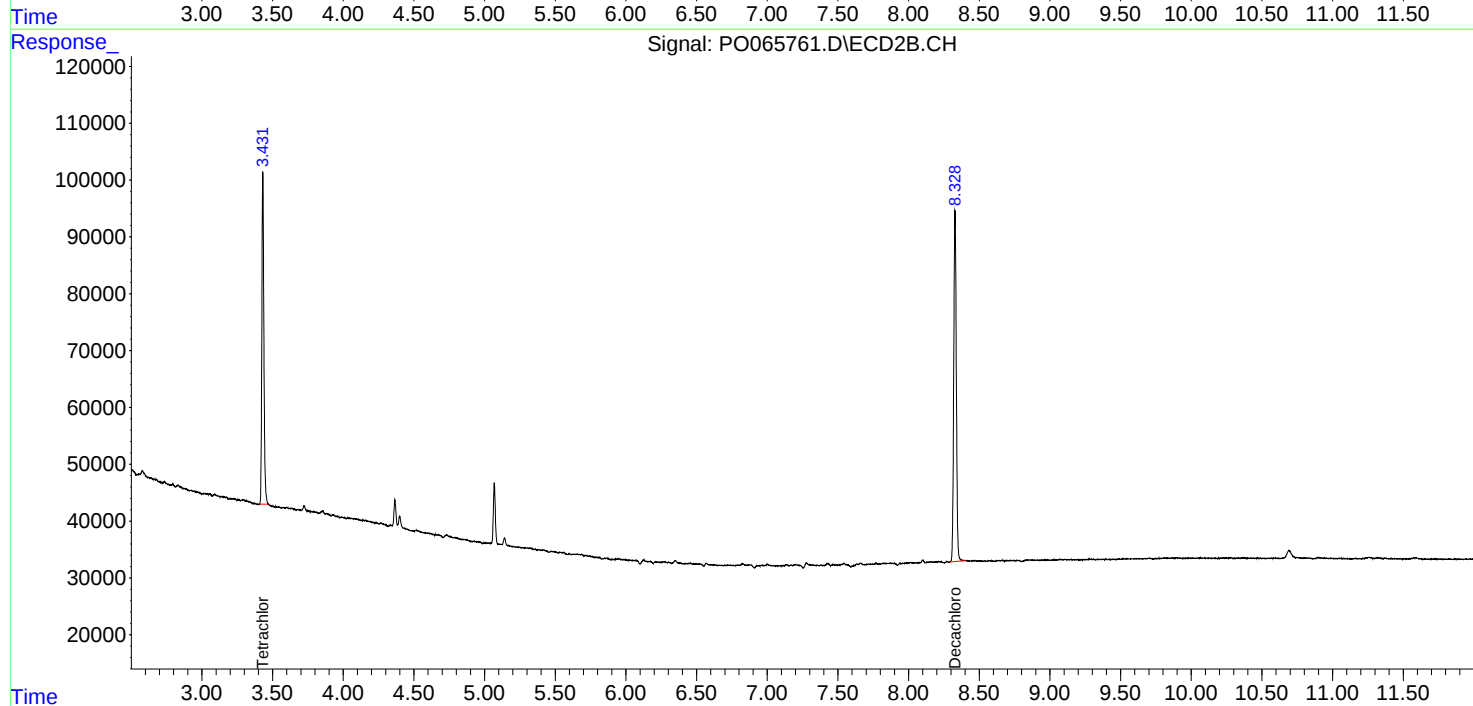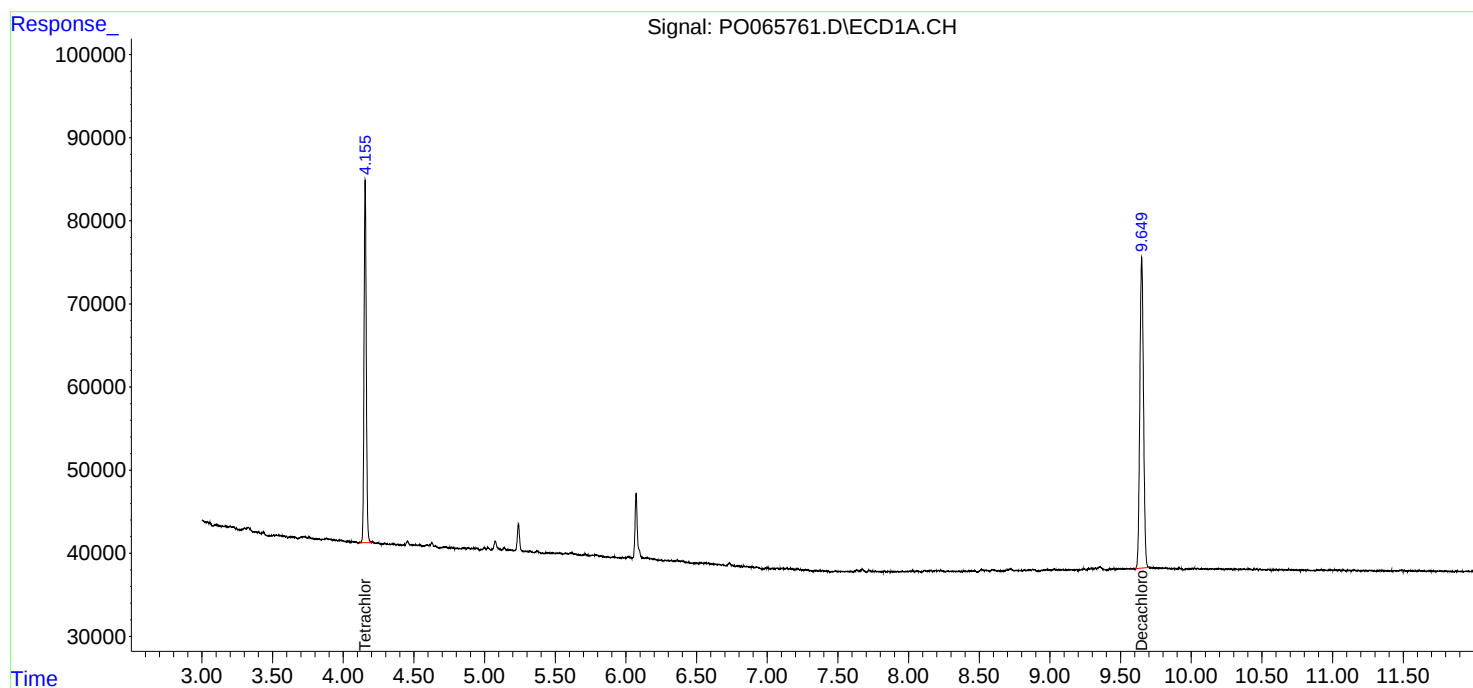


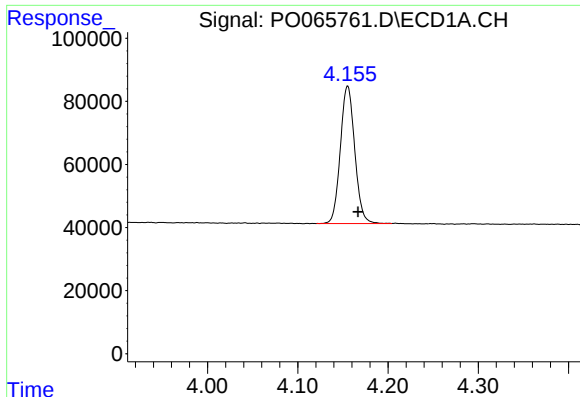

#1 Tetrachloro-m-xylene


R.T.: 4.155 min
Delta R.T.: -0.012 min
Response: 483514
Conc: 26.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
0052-DECANT-H2O-COMP-4

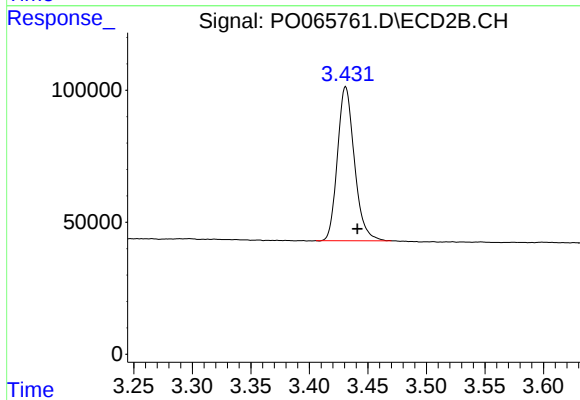


#1 Tetrachloro-m-xylene

R.T.: 3.431 min
Delta R.T.: -0.010 min
Response: 587764
Conc: 26.72 ng/ml

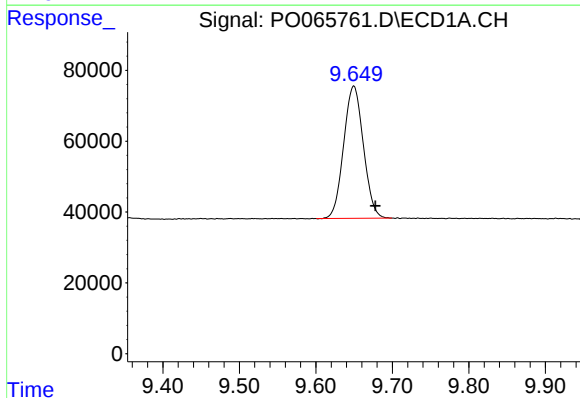

#2 Decachlorobiphenyl

R.T.: 9.650 min
Delta R.T.: -0.028 min
Response: 671327
Conc: 19.81 ng/ml

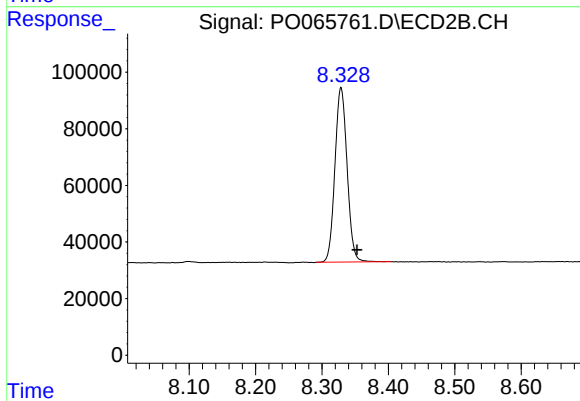

#2 Decachlorobiphenyl

R.T.: 8.329 min
Delta R.T.: -0.024 min
Response: 784579
Conc: 18.92 ng/ml