

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0012120\  
 Data File : P0065775.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 22 Jan 2020 11:22  
 Operator : DD\AJ  
 Sample : L1173-04RE  
 Misc :  
 ALS Vial : 50 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 0051-DECANT-H2O-COMP-3RE

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jan 22 12:52:13 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0010420.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Sat Jan 04 04:01:28 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1  | RT#2  | Resp#1 | Resp#2 | ng/ml  | ng/ml  |
|-----------------------------|-------|-------|--------|--------|--------|--------|
| -----                       |       |       |        |        |        |        |
| System Monitoring Compounds |       |       |        |        |        |        |
| 1) SA Tetrachlo...          | 4.155 | 3.432 | 673906 | 782851 | 36.905 | 35.588 |
| 2) SA Decachlor...          | 9.649 | 8.328 | 692627 | 784183 | 20.442 | 18.910 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0012120\  
Data File : P0065775.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 22 Jan 2020 11:22  
Operator : DD\AJ  
Sample : L1173-04RE  
Misc :  
ALS Vial : 50 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
0051-DECANT-H2O-COMP-3RE

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jan 22 12:52:13 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0010420.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Sat Jan 04 04:01:28 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

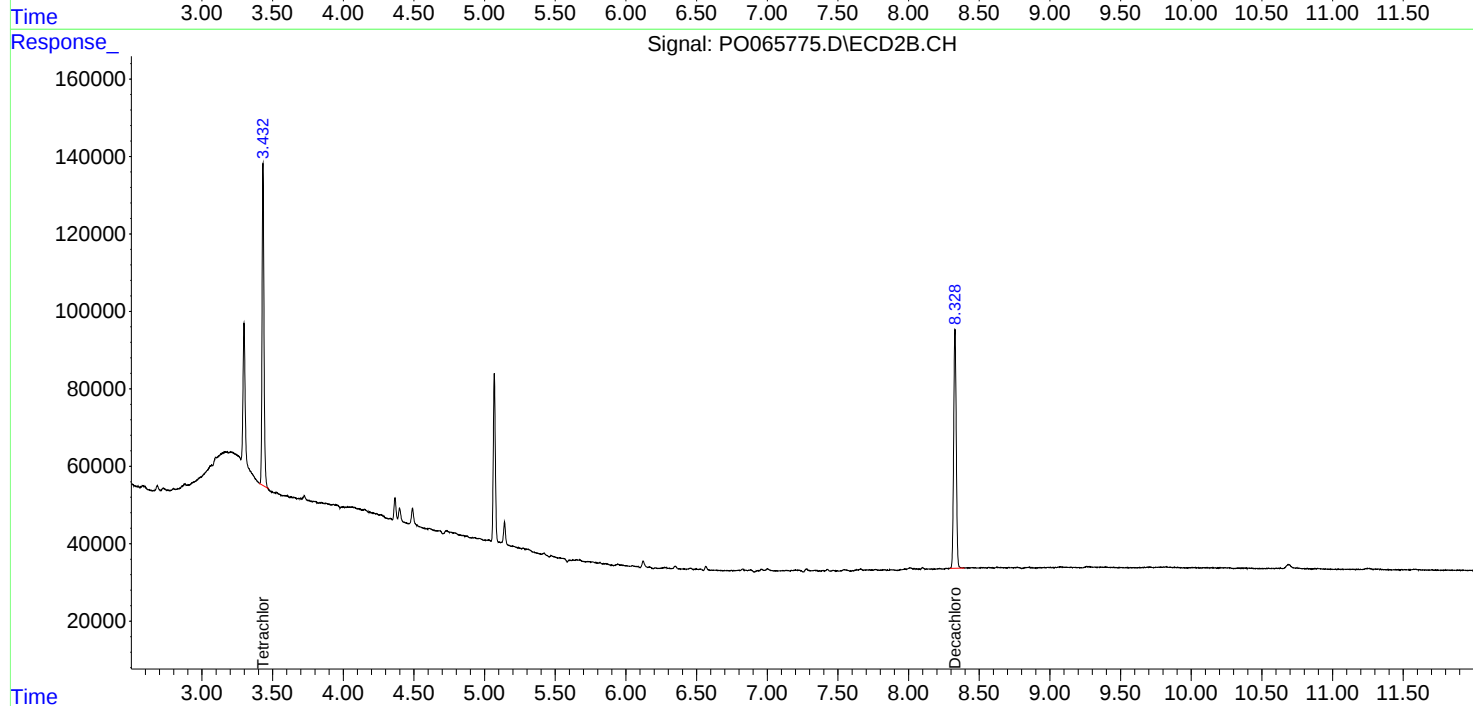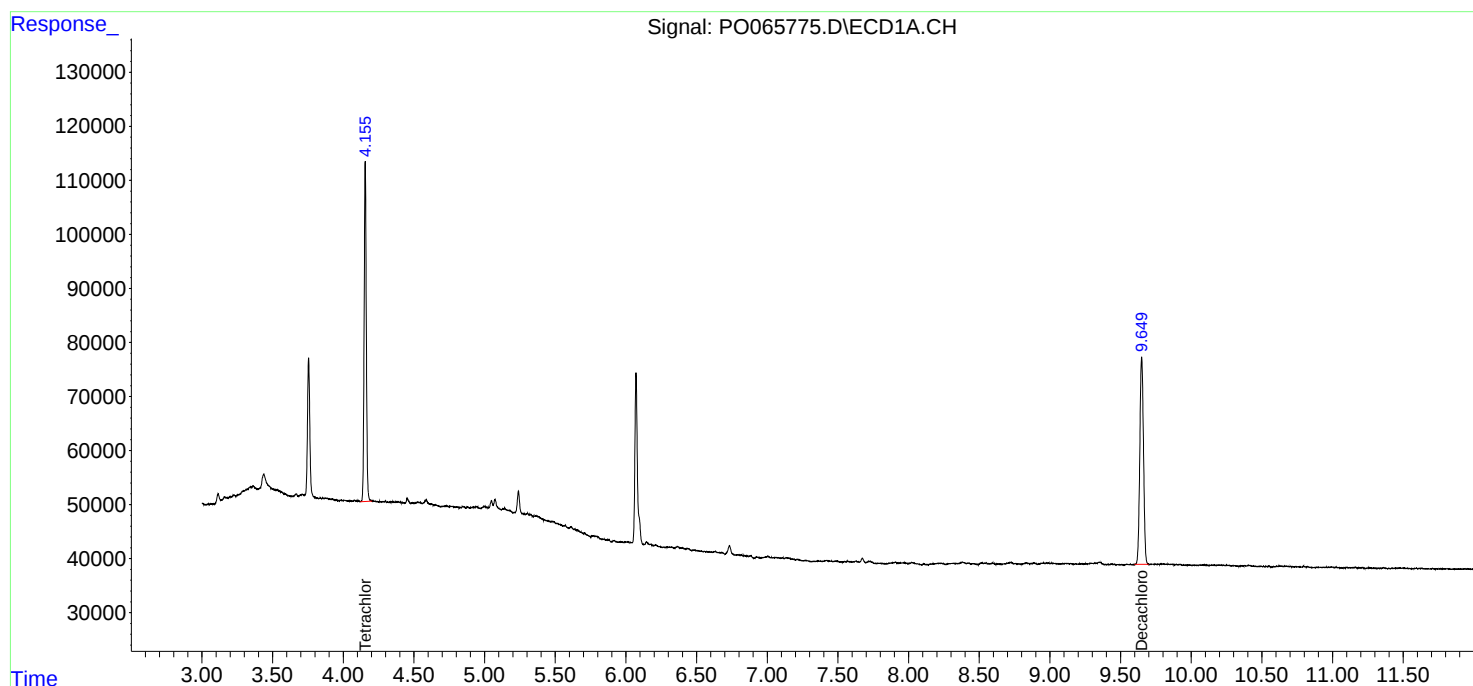


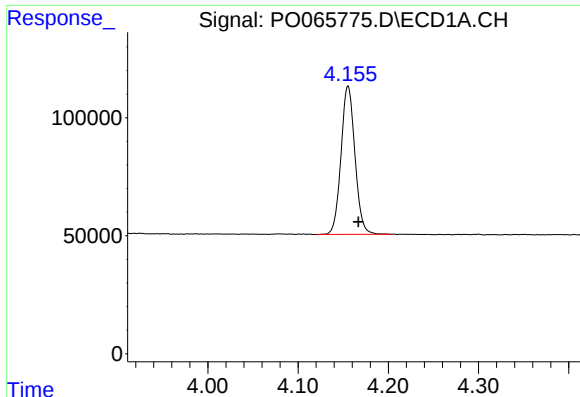

#1 Tetrachloro-m-xylene


R.T.: 4.155 min  
Delta R.T.: -0.012 min  
Response: 673906  
Conc: 36.91 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
0051-DECANT-H2O-COMP-3RE

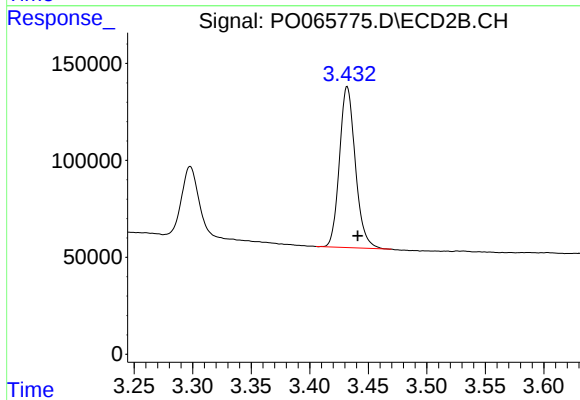


#1 Tetrachloro-m-xylene

R.T.: 3.432 min  
Delta R.T.: -0.009 min  
Response: 782851  
Conc: 35.59 ng/ml

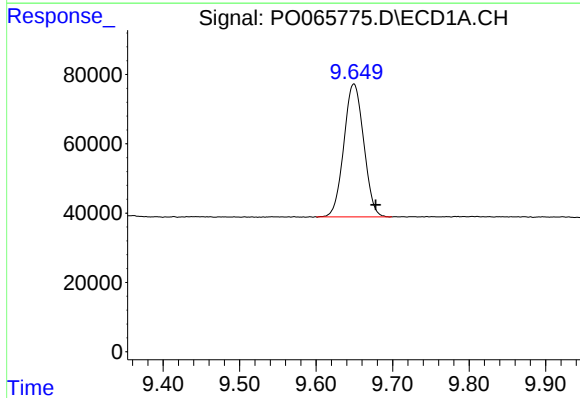

#2 Decachlorobiphenyl

R.T.: 9.649 min  
Delta R.T.: -0.029 min  
Response: 692627  
Conc: 20.44 ng/ml

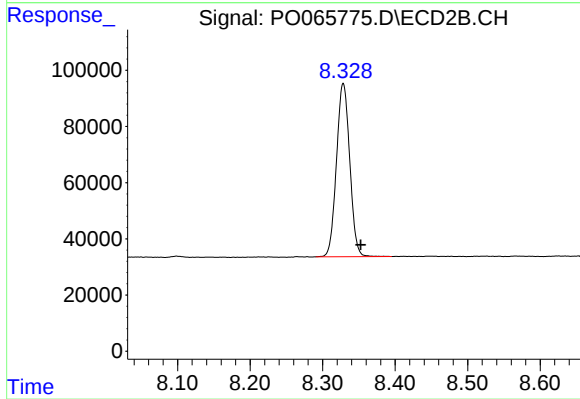

#2 Decachlorobiphenyl

R.T.: 8.328 min  
Delta R.T.: -0.024 min  
Response: 784183  
Conc: 18.91 ng/ml