

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012121\
 Data File : P0075036.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jan 2021 12:35
 Operator : AJ/MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 14:30:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.929	4.002	2761654	1395307	26.172	24.804
2)	SA Decachlor...	10.949	9.255	2585290	1294043	25.473	23.569
Target Compounds							
9)	L2 AR-1221-2	5.283	4.351	37563	19156	41.689	35.844
20)	L4 AR-1242-5	0.000	6.134	0	57175	N.D.	32.656 #
24)	L5 AR-1248-4	7.172f	0.000	174235	0	39.071	N.D. #
25)	L5 AR-1248-5	0.000	6.134f	0	57175	N.D.	24.319 #
26)	L6 AR-1254-1	7.172	6.134f	174235	57175	39.616	15.829 #
28)	L6 AR-1254-3	7.799f	0.000	55585	0	7.925	N.D. #
30)	L6 AR-1254-5	8.506	0.000	19525	0	3.361	N.D. #
34)	L7 AR-1260-4	8.813	0.000	16317	0	2.982	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012121\
Data File : PO075036.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jan 2021 12:35
Operator : AJ/MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 14:30:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

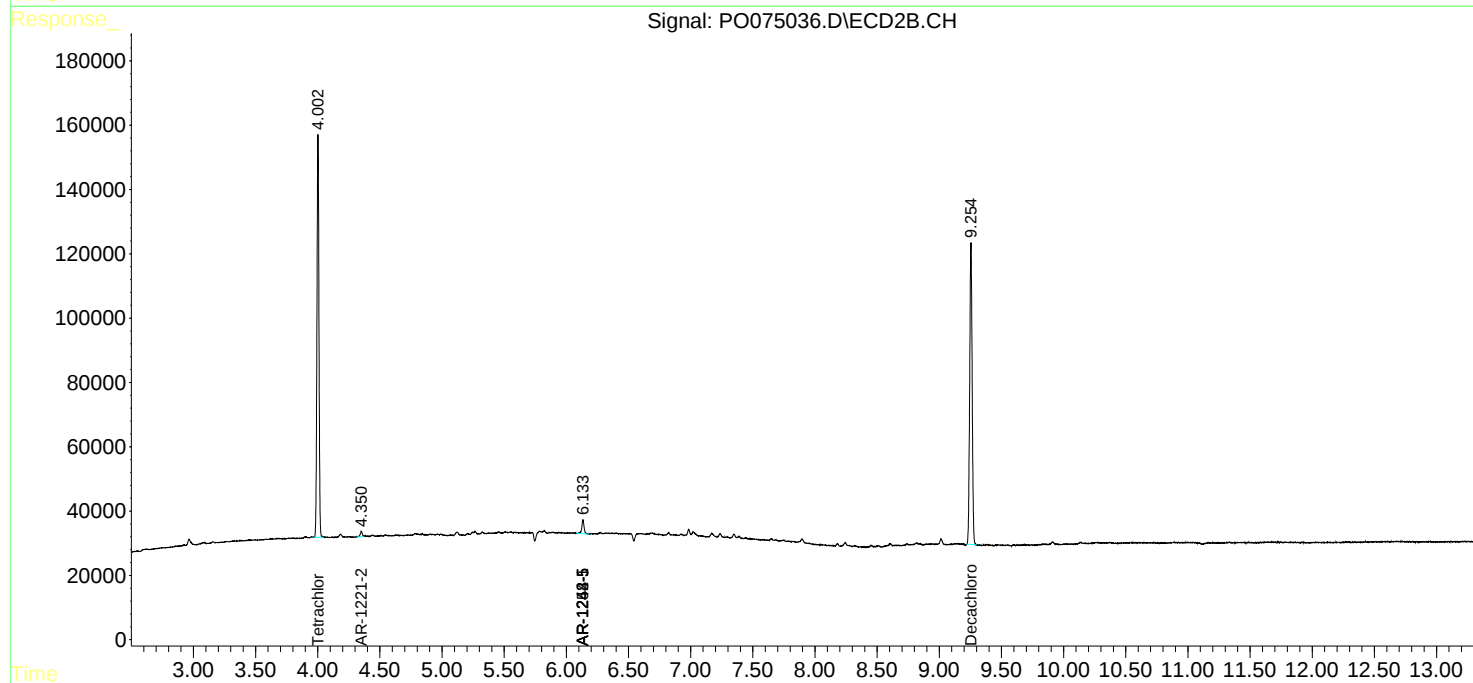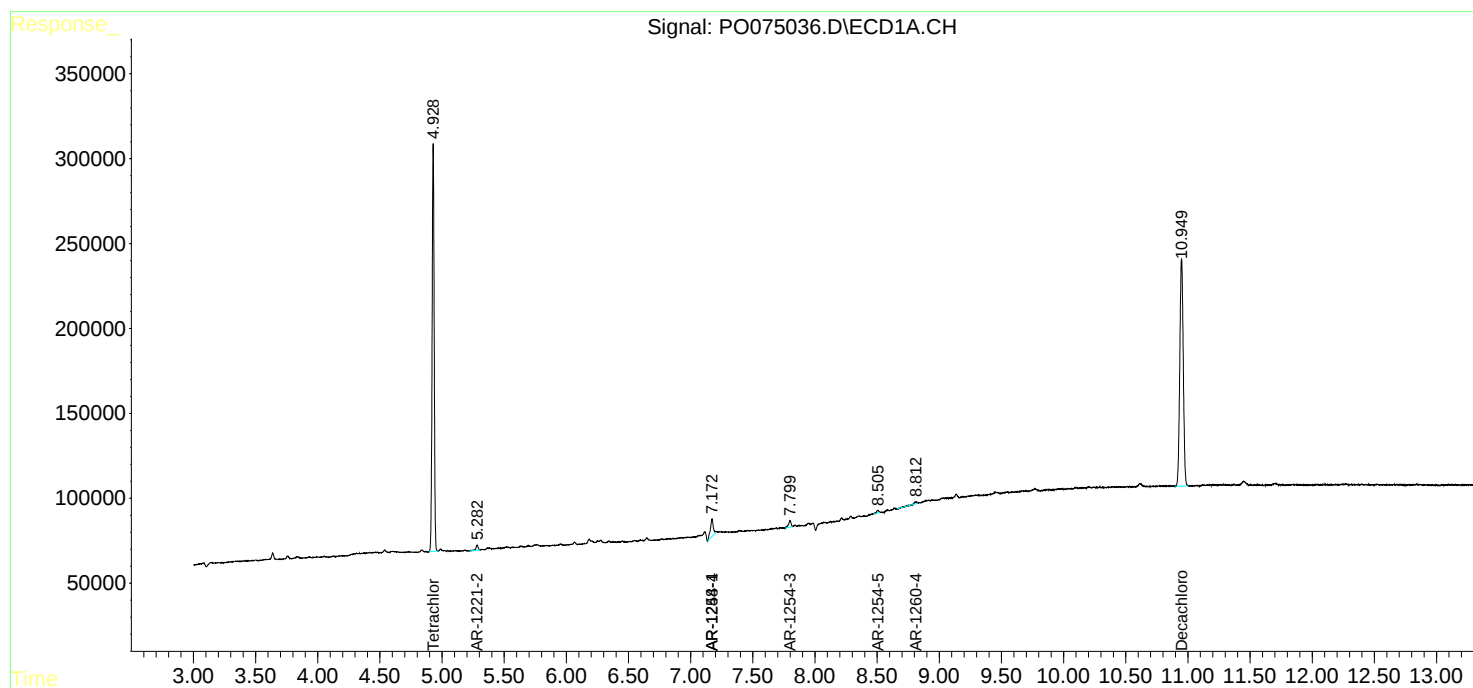


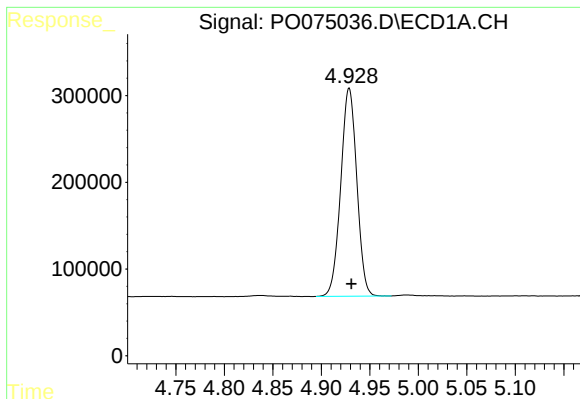

#1 Tetrachloro-m-xylene


R.T.: 4.929 min
Delta R.T.: -0.002 min
Response: 2761654
Conc: 26.17 ng/ml

Instrument :
ECD_O
ClientSampleId :

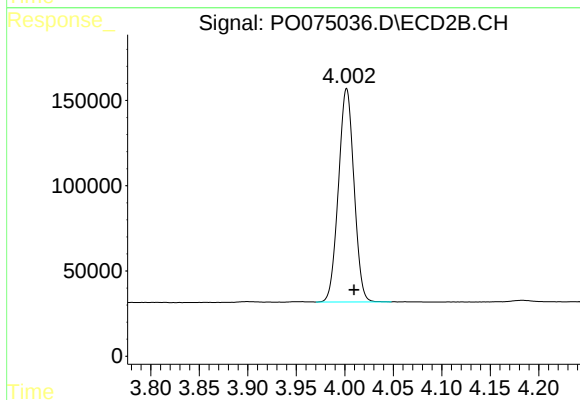


#1 Tetrachloro-m-xylene

R.T.: 4.002 min
Delta R.T.: -0.008 min
Response: 1395307
Conc: 24.80 ng/ml

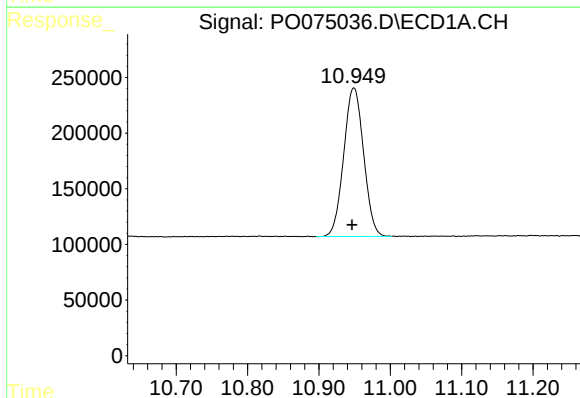


#2 Decachlorobiphenyl

R.T.: 10.949 min
Delta R.T.: 0.003 min
Response: 2585290
Conc: 25.47 ng/ml

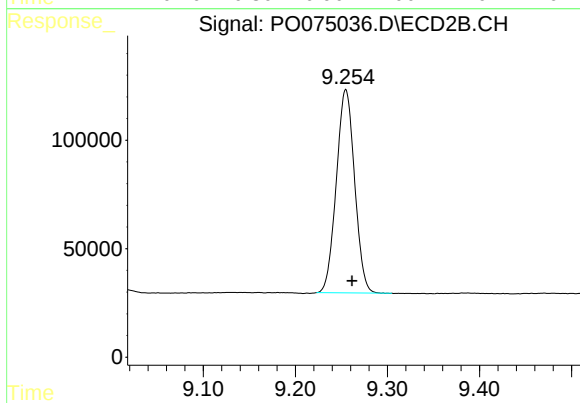

#2 Decachlorobiphenyl


R.T.: 9.255 min
Delta R.T.: -0.007 min
Response: 1294043
Conc: 23.57 ng/ml

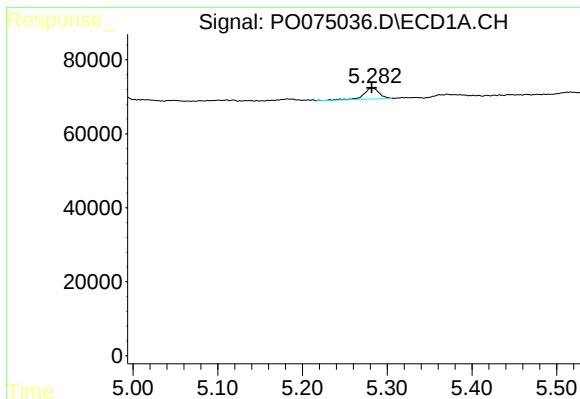

#9 AR-1221-2


R.T.: 5.283 min
Delta R.T.: 0.000 min
Response: 37563
Conc: 41.69 ng/ml

Instrument :
ECD_O
ClientSampleId :

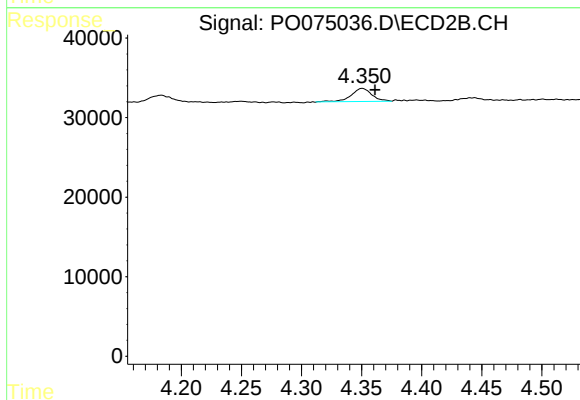


#9 AR-1221-2

R.T.: 4.351 min
Delta R.T.: -0.011 min
Response: 19156
Conc: 35.84 ng/ml

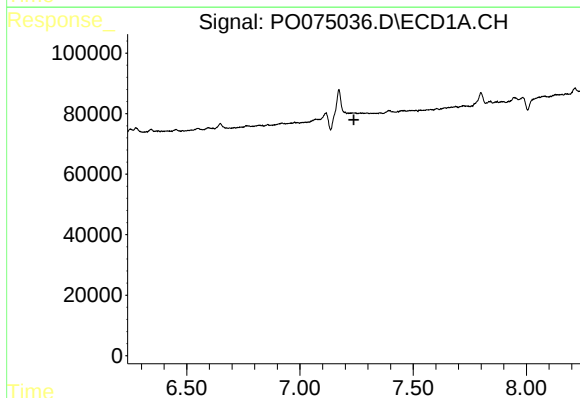


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 7.238 min
Response: 0
Conc: N.D.

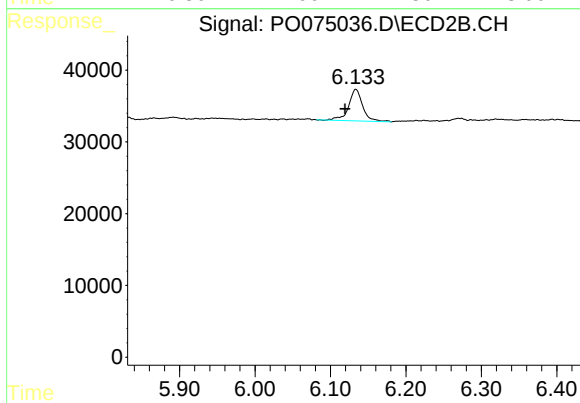

#20 AR-1242-5


R.T.: 6.134 min
Delta R.T.: 0.015 min
Response: 57175
Conc: 32.66 ng/ml

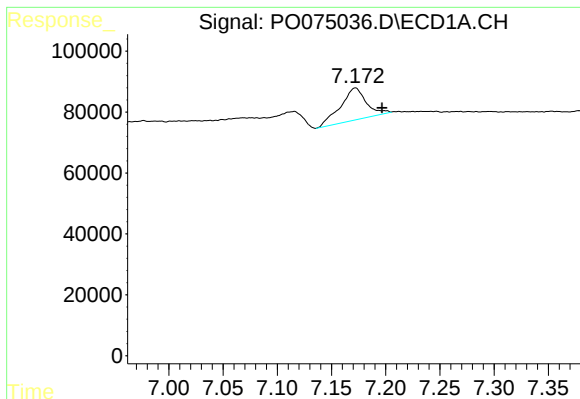

#24 AR-1248-4


R.T.: 7.172 min
Delta R.T.: -0.024 min
Response: 174235
Conc: 39.07 ng/ml

Instrument :
ECD_O
ClientSampleId :

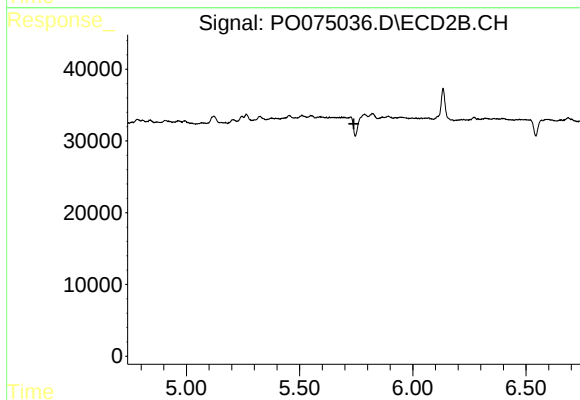


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.740 min
Response: 0
Conc: N.D.

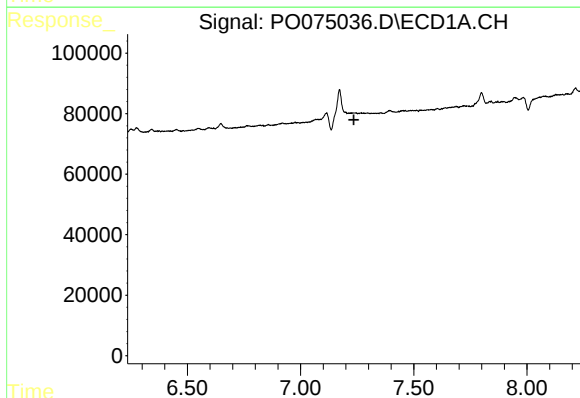


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 7.236 min
Response: 0
Conc: N.D.

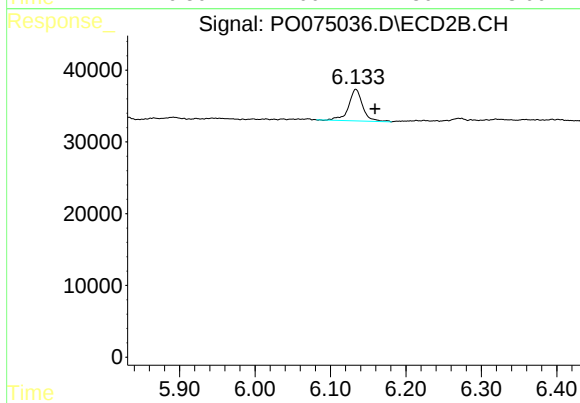

#25 AR-1248-5


R.T.: 6.134 min
Delta R.T.: -0.025 min
Response: 57175
Conc: 24.32 ng/ml

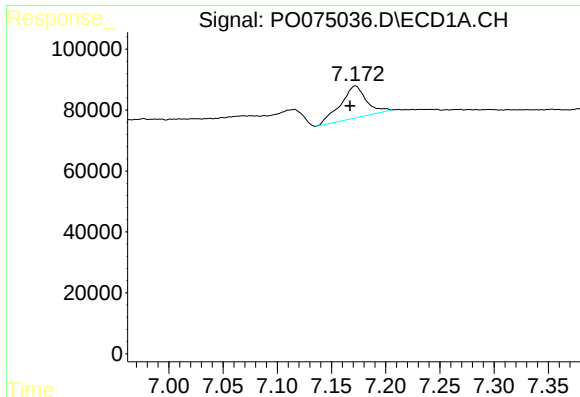

#26 AR-1254-1


R.T.: 7.172 min
Delta R.T.: 0.005 min
Response: 174235
Conc: 39.62 ng/ml

Instrument :
ECD_O
ClientSampleId :

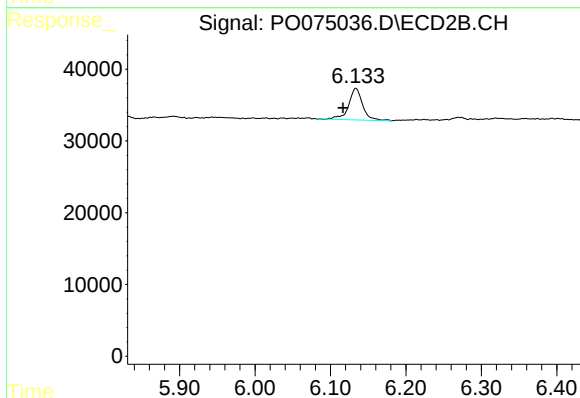


#26 AR-1254-1

R.T.: 6.134 min
Delta R.T.: 0.017 min
Response: 57175
Conc: 15.83 ng/ml

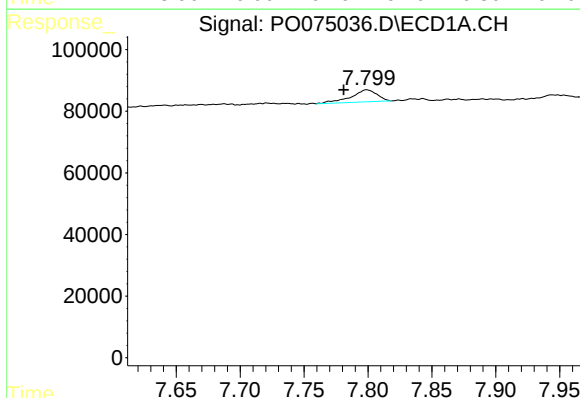


#28 AR-1254-3

R.T.: 7.799 min
Delta R.T.: 0.018 min
Response: 55585
Conc: 7.92 ng/ml

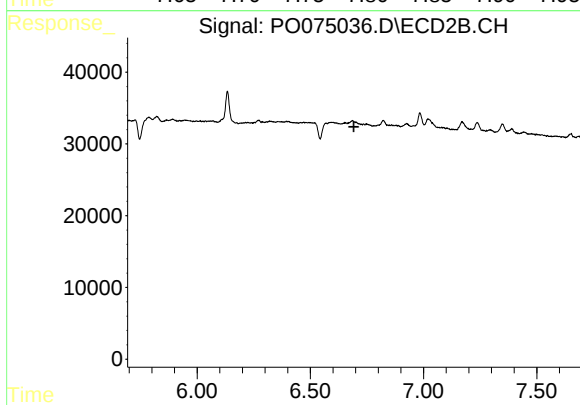

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.692 min
Response: 0
Conc: N.D.

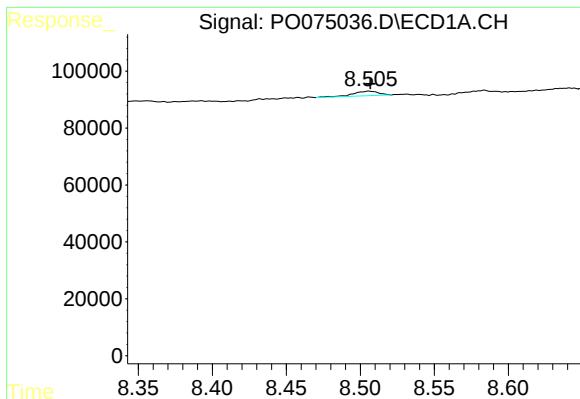

#30 AR-1254-5


R.T.: 8.506 min
Delta R.T.: -0.001 min
Response: 19525
Conc: 3.36 ng/ml

Instrument :
ECD_O
ClientSampleId :

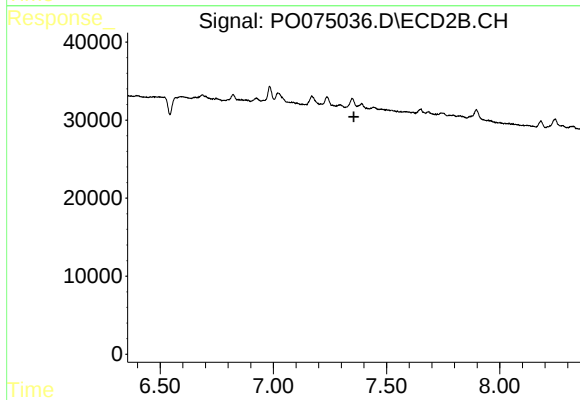


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.356 min
Response: 0
Conc: N.D.

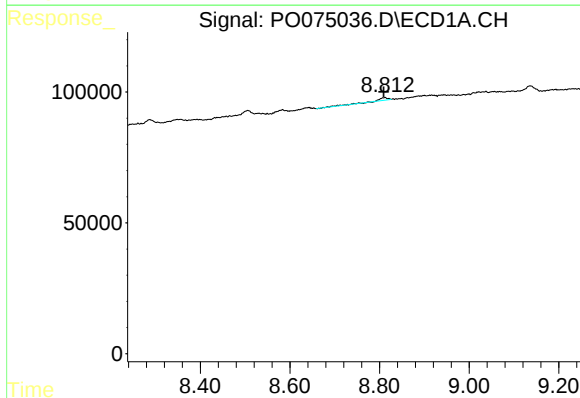

#34 AR-1260-4

R.T.: 8.813 min
Delta R.T.: 0.003 min
Response: 16317
Conc: 2.98 ng/ml

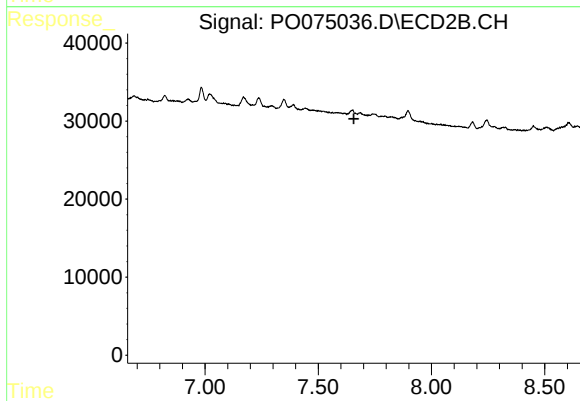

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.657 min
Response: 0
Conc: N.D.